




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040622\  
 Data File : BM034515.D  
 Acq On : 06 Apr 2022 13:45  
 Operator : CG/JU  
 Sample : N2166-05  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0R38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 14:48:30 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM040422.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Apr 05 11:50:53 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022  
 Supervised By :Yogesh Patel 04/09/2022

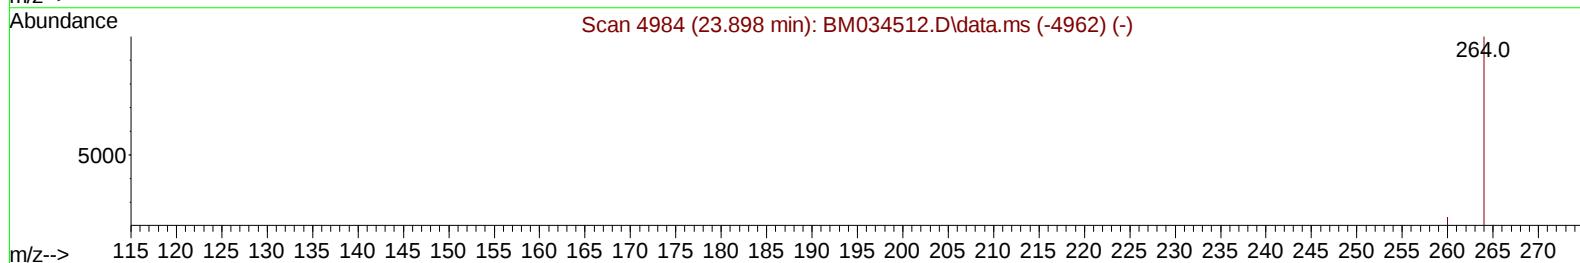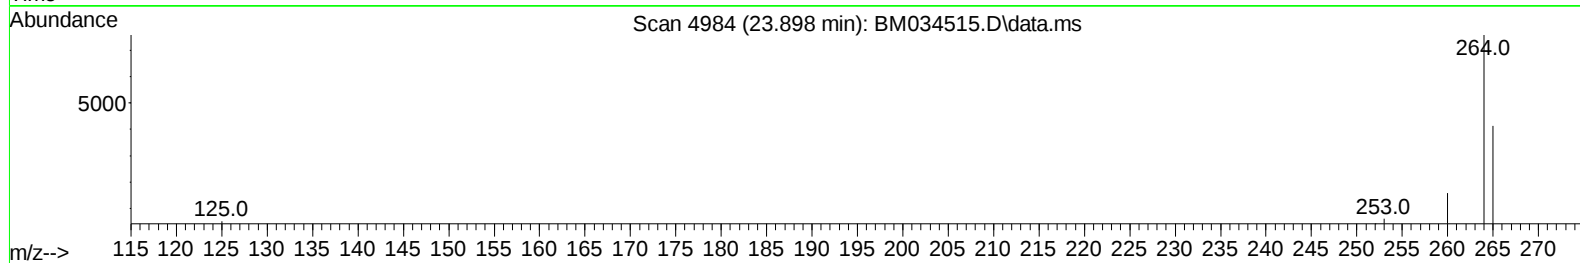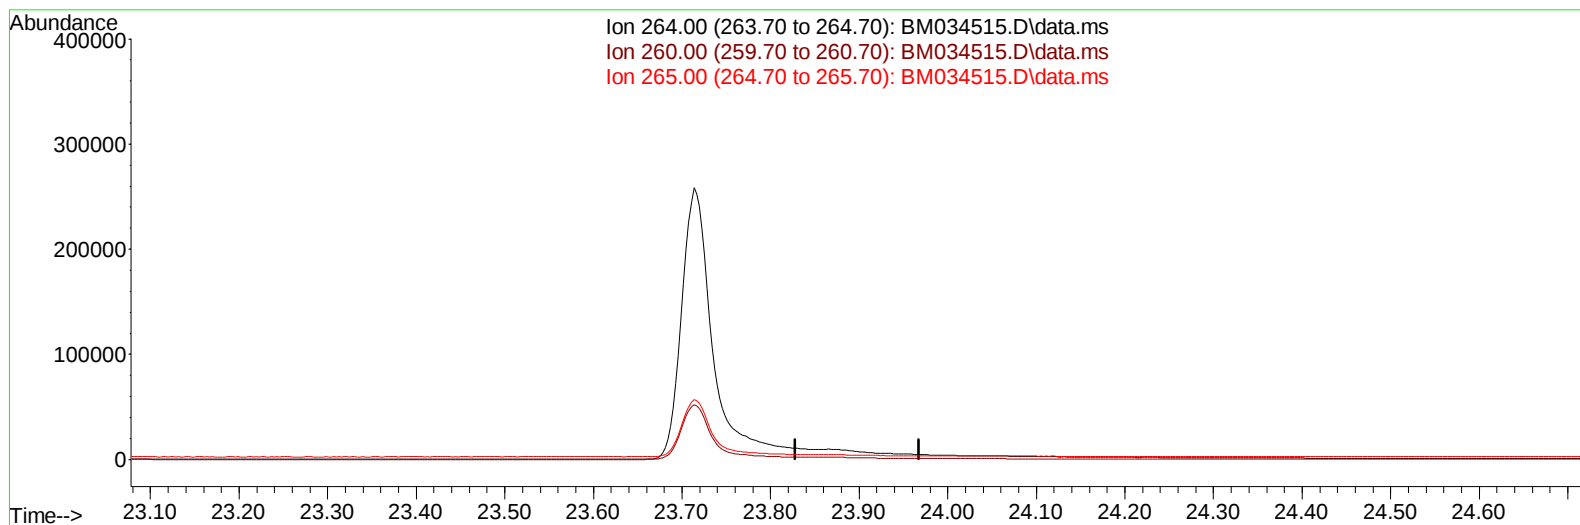

TIC: BM034515.D\data.ms

**(23) Perylene-d12 (I)**

**23.898min (-23.898) 0.00 ng/ul**

**response 0**

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 264.00 | 100.00 | 0.00  |
| 260.00 | 27.80  | 0.00# |
| 265.00 | 95.30  | 0.00# |
| 0.00   | 0.00   | 0.00  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040622\  
 Data File : BM034515.D  
 Acq On : 06 Apr 2022 13:45  
 Operator : CG/JU  
 Sample : N2166-05  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0R38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 14:48:30 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM040422.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Apr 05 11:50:53 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022  
 Supervised By :Yogesh Patel 04/09/2022

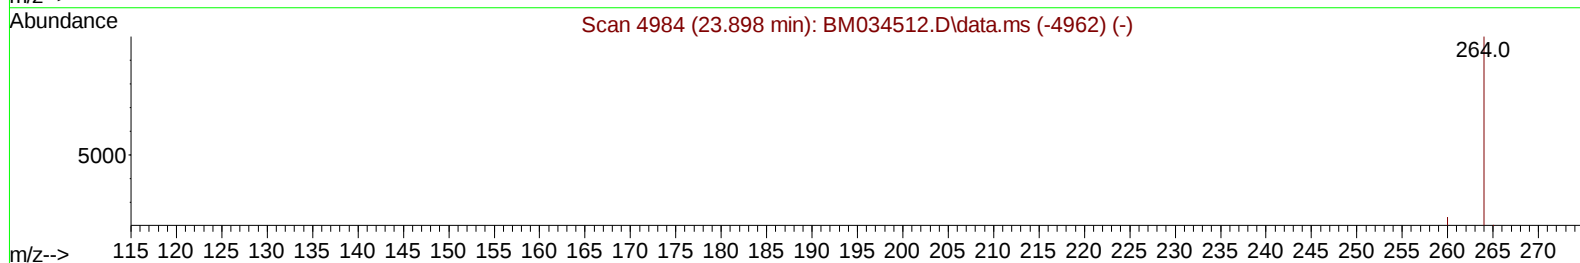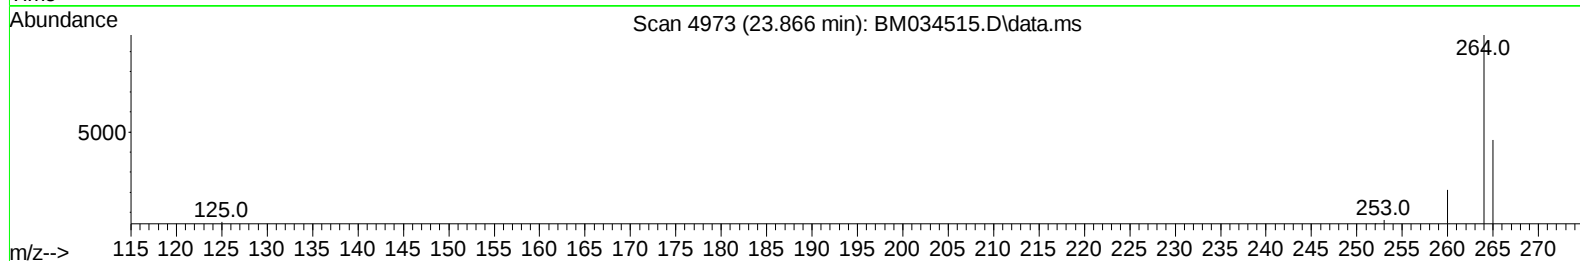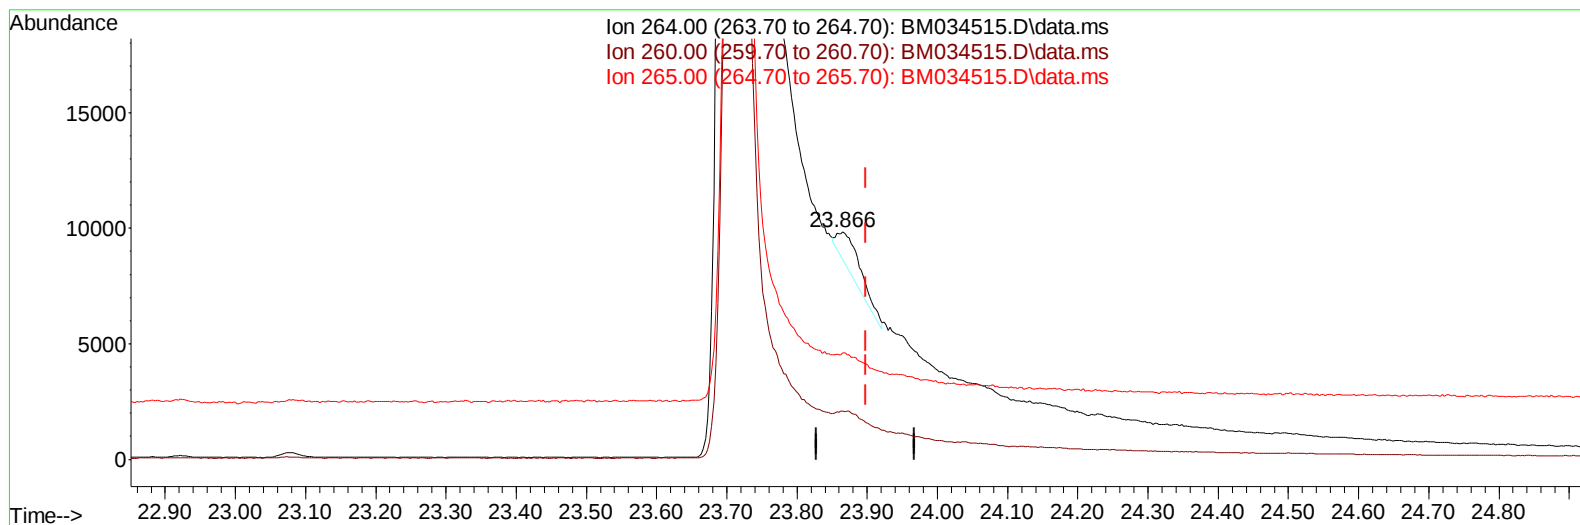

TIC: BM034515.D\data.ms

**(23) Perylene-d12 (I)**

23.866min (-0.032) 0.40 ng/ul m

response 3104

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 27.80  | 21.40# |
| 265.00 | 95.30  | 46.83# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040622\  
 Data File : BM034515.D  
 Acq On : 06 Apr 2022 13:45  
 Operator : CG/JU  
 Sample : N2166-05  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0R38

## Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/07/2022  
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 06 14:48:30 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM040422.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Apr 05 11:50:53 2022  
 Response via : Initial Calibration

| Compound                    | R.T.   | Q   | Ion | Response | Conc  | Units | Dev(Min) |
|-----------------------------|--------|-----|-----|----------|-------|-------|----------|
| -----                       |        |     |     |          |       |       |          |
| Internal Standards          |        |     |     |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.912  | 152 |     | 3018     | 0.400 | ng/ul | -0.02    |
| 4) Naphthalene-d8           | 10.719 | 136 |     | 8094     | 0.400 | ng/ul | #-0.02   |
| 9) Acenaphthene-d10         | 14.555 | 164 |     | 4484     | 0.400 | ng/ul | 0.00     |
| 13) Phenanthrene-d10        | 17.295 | 188 |     | 8184     | 0.400 | ng/ul | -0.02    |
| 17) Chrysene-d12            | 21.512 | 240 |     | 6050     | 0.400 | ng/ul | # 0.02   |
| 23) Perylene-d12            | 23.866 | 264 |     | 3104m    | 0.400 | ng/ul | -0.03    |
|                             |        |     |     |          |       |       |          |
| System Monitoring Compounds |        |     |     |          |       |       |          |
| 3) 1,4-Dioxane-d8           | 3.292  | 96  |     | 18342    | 3.629 | ng/ul | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.319 | 152 |     | 3358     | 0.316 | ng/ul | -0.02    |
| 18) Fluoranthene-d10        | 19.324 | 212 |     | 7442     | 0.419 | ng/ul | 0.00     |

Target Compounds Qvalue

-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040622\  
Data File : BM034515.D  
Acq On : 06 Apr 2022 13:45  
Operator : CG/JU  
Sample : N2166-05  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0R38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 14:48:30 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM040422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 05 11:50:53 2022  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022  
Supervised By :Yogesh Patel 04/09/2022

