




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034524.D
 Acq On : 06 Apr 2022 19:50
 Operator : CG/JU
 Sample : N2182-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R19

Manual IntegrationsAPPROVED

Quant Time: Apr 07 01:29:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

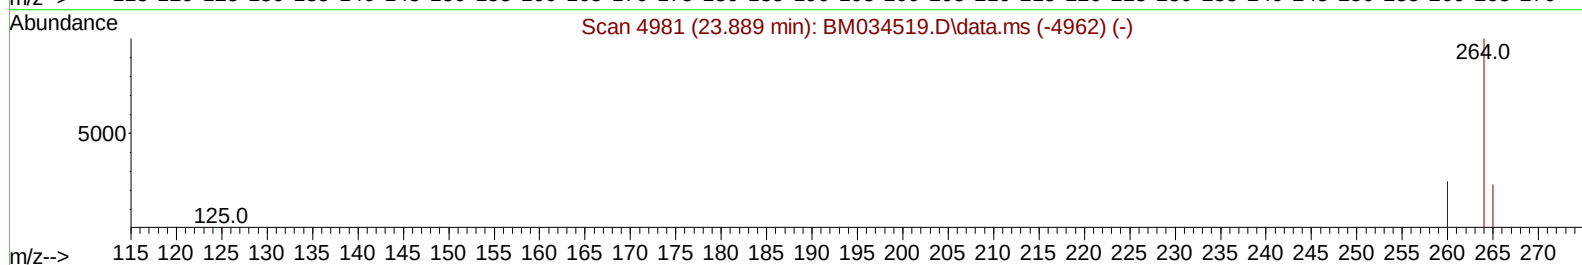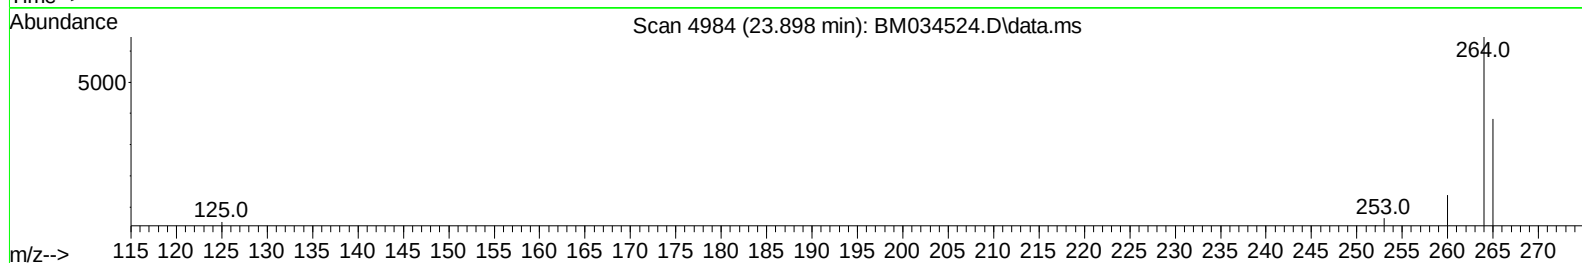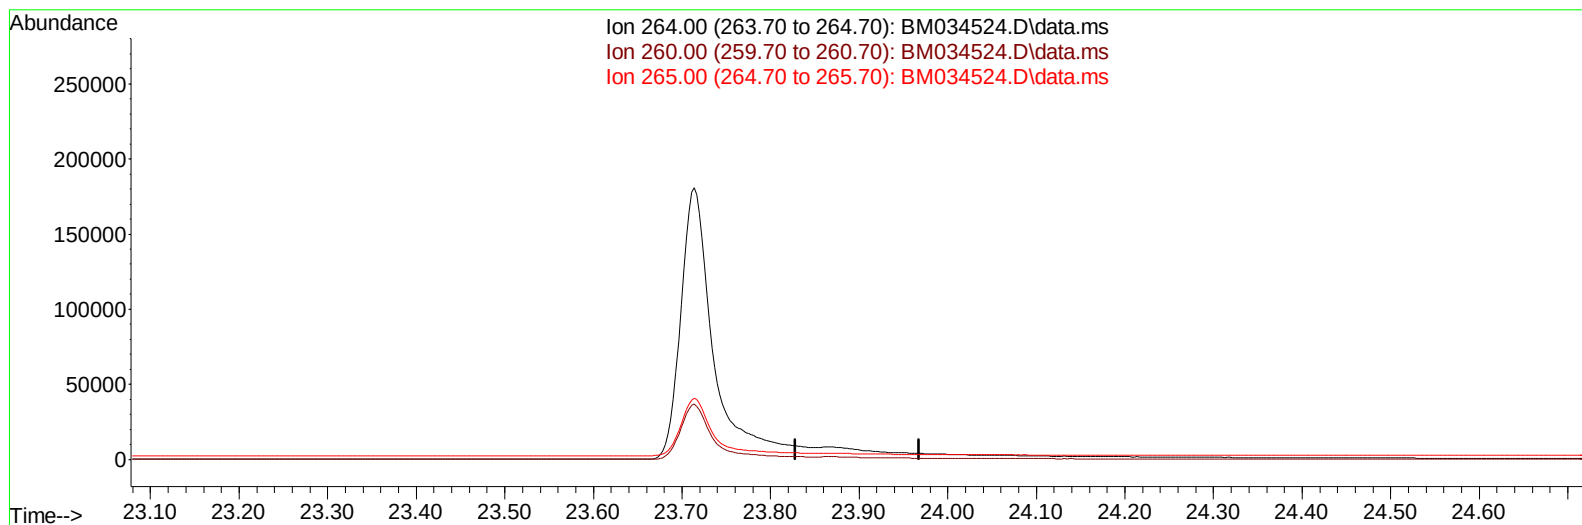

TIC: BM034524.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034524.D
 Acq On : 06 Apr 2022 19:50
 Operator : CG/JU
 Sample : N2182-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R19

Manual IntegrationsAPPROVED

Quant Time: Apr 07 01:29:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

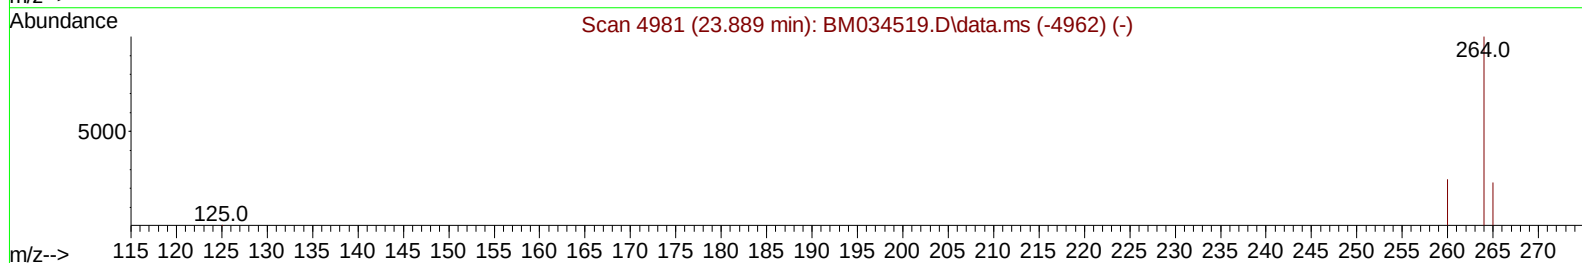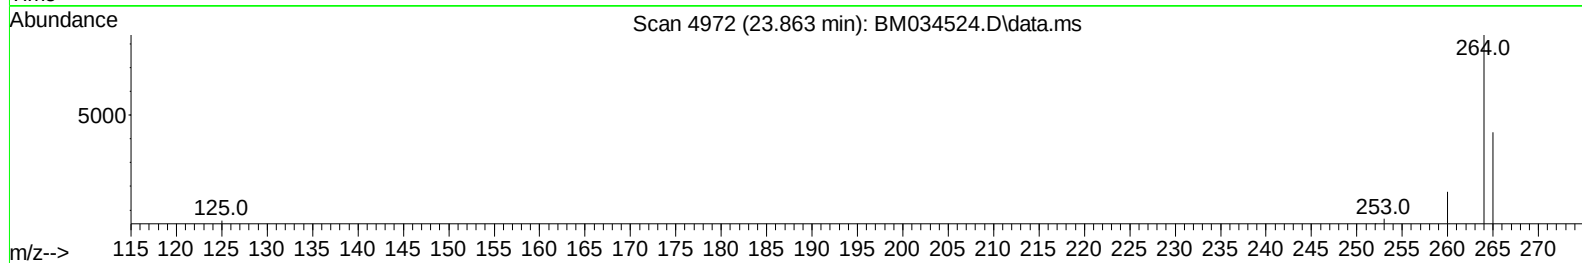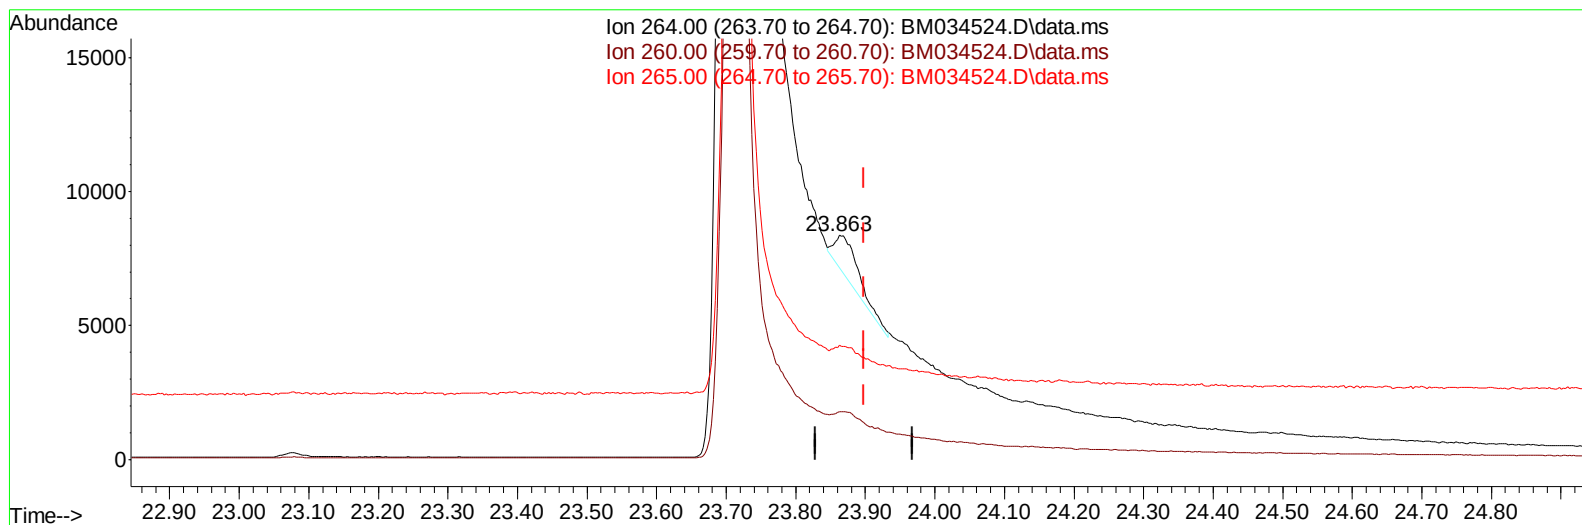

TIC: BM034524.D\data.ms

(23) Perylene-d12 (I)

23.863min (-0.035) 0.40 ng/ul m

response 3268

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.18#
265.00	95.30	50.96#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034524.D
 Acq On : 06 Apr 2022 19:50
 Operator : CG/JU
 Sample : N2182-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R19

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 07 01:29:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.912	152		2771	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.719	136		7501	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.555	164		3947	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188		7125	0.400	ng/ul	-0.02
17) Chrysene-d12	21.513	240		5200	0.400	ng/ul	# 0.02
23) Perylene-d12	23.863	264		3268m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.292	96		18602	4.008	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.336	152		2933	0.298	ng/ul	0.00
18) Fluoranthene-d10	19.325	212		5740	0.376	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.768	128		611	0.026	ng/ul#	79
15) Phenanthrene	17.337	178		1034	0.045	ng/ul#	84
19) Fluoranthene	19.357	202		443	0.020	ng/ul#	28

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
Data File : BM034524.D
Acq On : 06 Apr 2022 19:50
Operator : CG/JU
Sample : N2182-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R19

Manual IntegrationsAPPROVED

Quant Time: Apr 07 01:29:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
Supervised By :Yogesh Patel 04/09/2022

