




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034537.D
 Acq On : 07 Apr 2022 04:17
 Operator : CG/JU
 Sample : SP5859
 Misc : SFAM SURROGATE
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5859

Manual IntegrationsAPPROVED

Quant Time: Apr 07 05:00:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

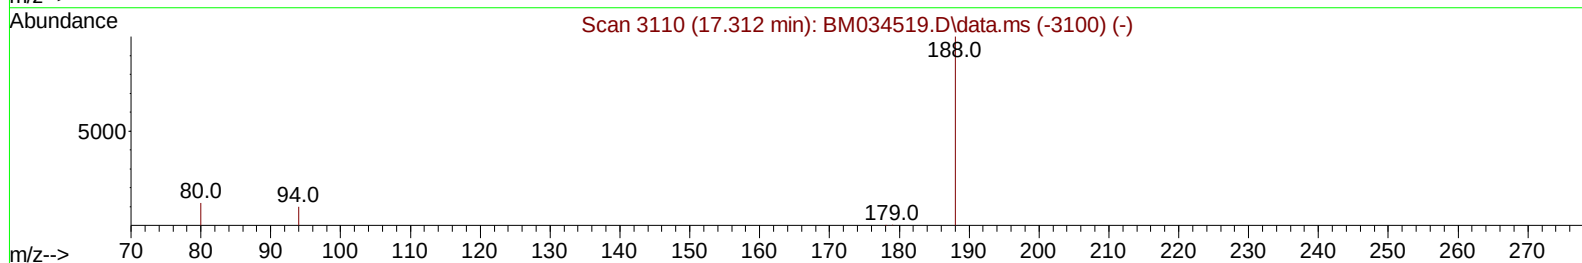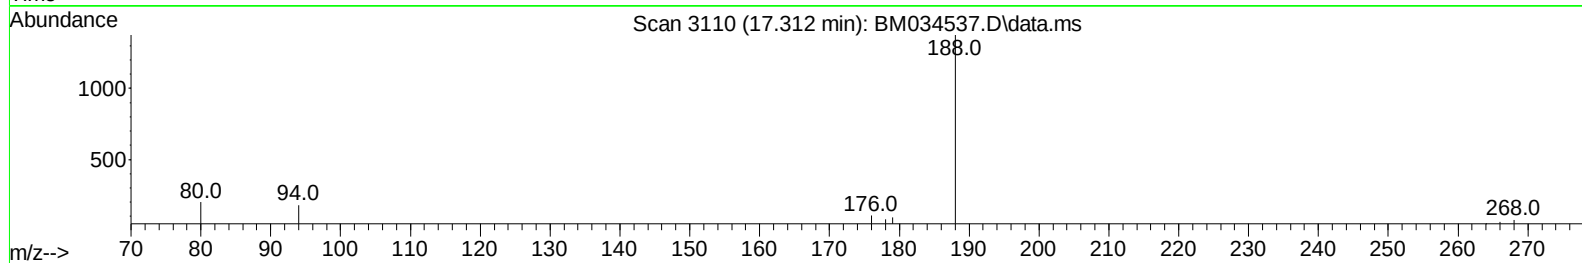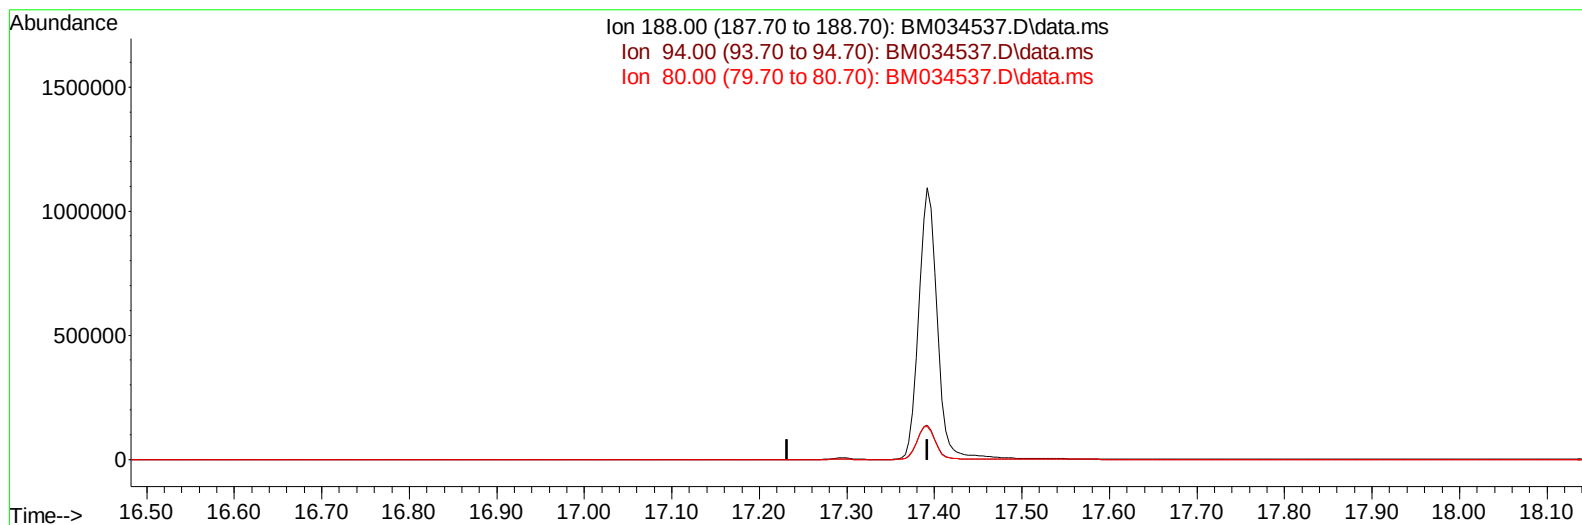

TIC: BM034537.D\data.ms

(13) Phenanthrene-d10 (I)

17.312min (-17.312) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.30	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034537.D
 Acq On : 07 Apr 2022 04:17
 Operator : CG/JU
 Sample : SP5859
 Misc : SFAM SURROGATE
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5859

Manual IntegrationsAPPROVED

Quant Time: Apr 07 05:00:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

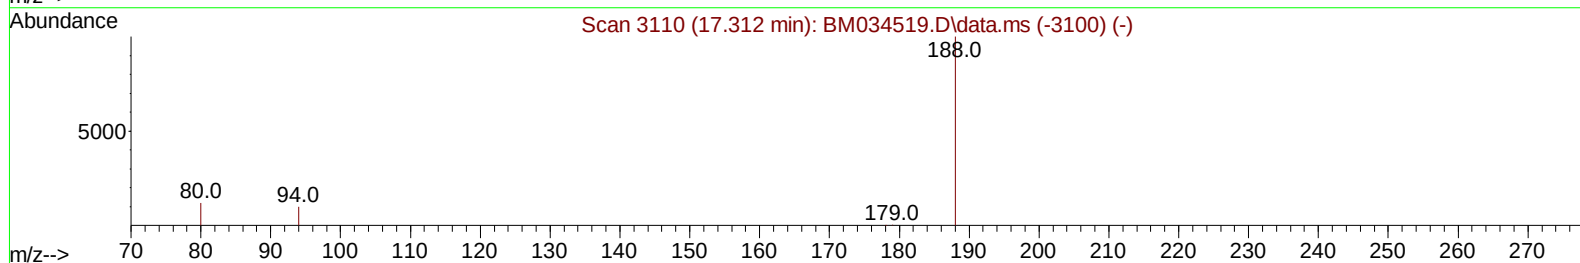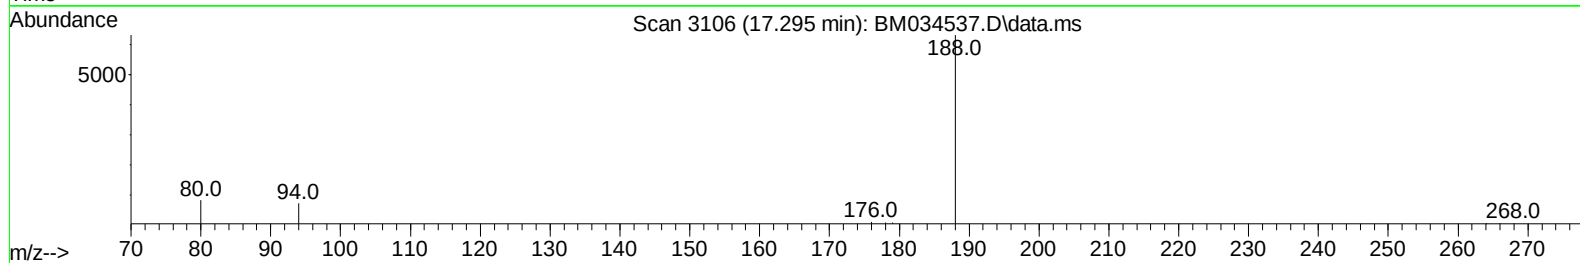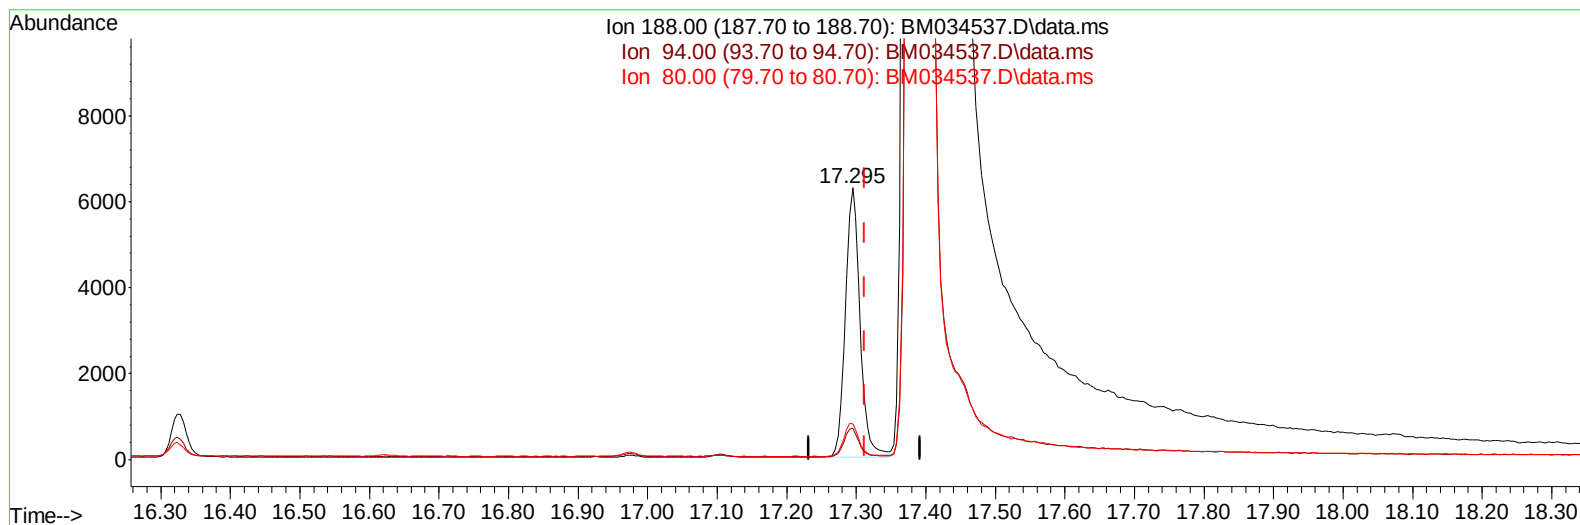

TIC: BM034537.D\data.ms

(13) Phenanthrene-d10 (I)

17.295min (-0.017) 0.40 ng/ul m

response 9139

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.30	11.42
80.00	15.50	13.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034537.D
 Acq On : 07 Apr 2022 04:17
 Operator : CG/JU
 Sample : SP5859
 Misc : SFAM SURROGATE
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5859

Manual IntegrationsAPPROVED

Quant Time: Apr 07 05:00:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

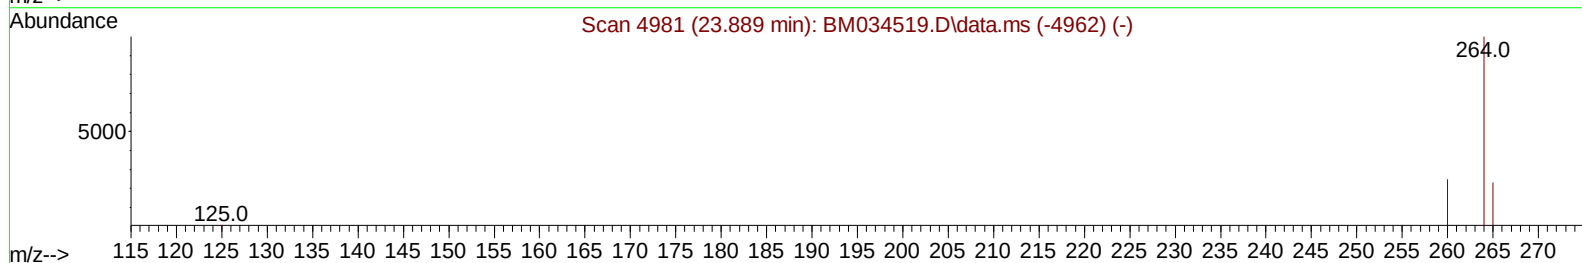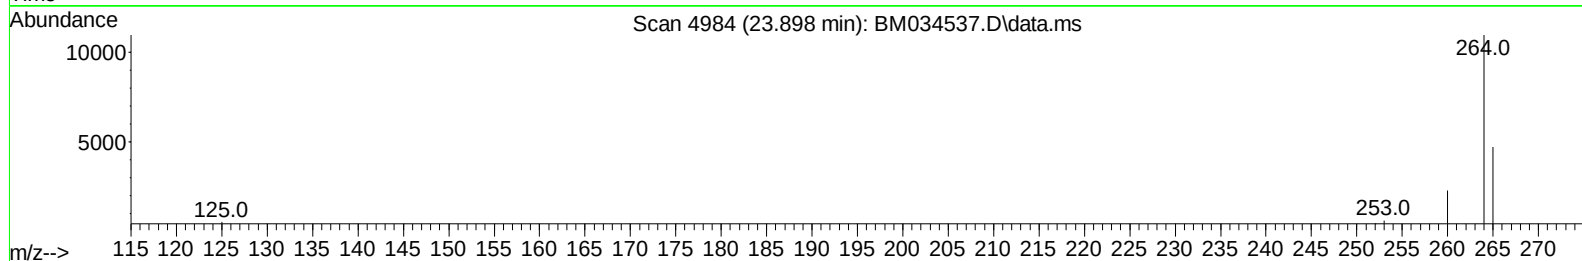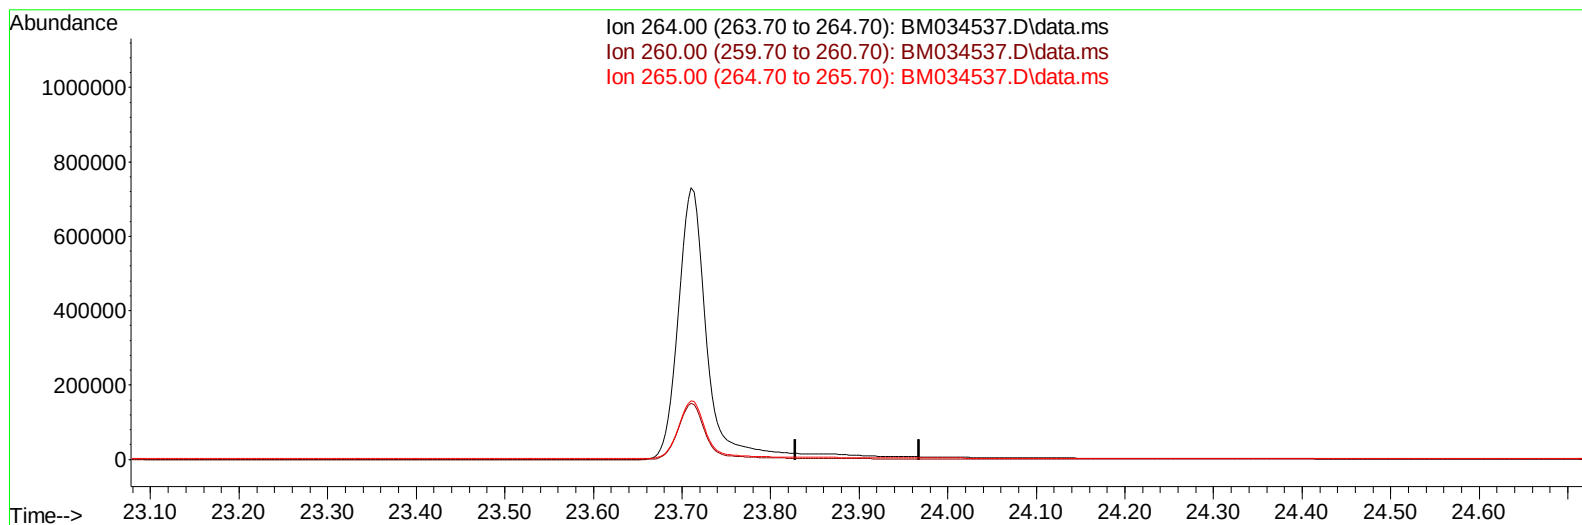

TIC: BM034537.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034537.D
 Acq On : 07 Apr 2022 04:17
 Operator : CG/JU
 Sample : SP5859
 Misc : SFAM SURROGATE
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5859

Manual IntegrationsAPPROVED

Quant Time: Apr 07 05:00:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

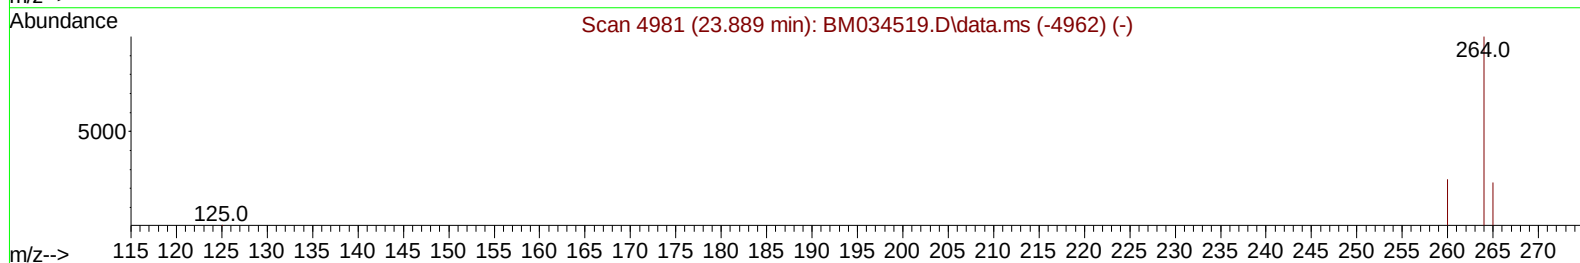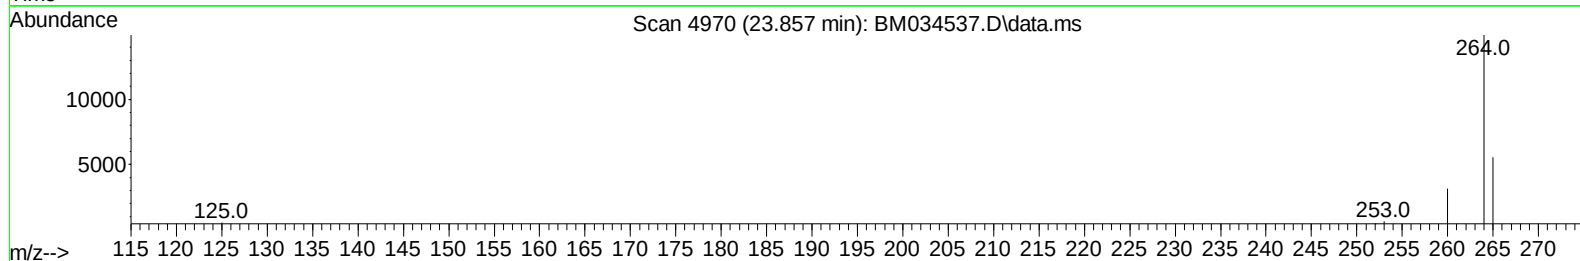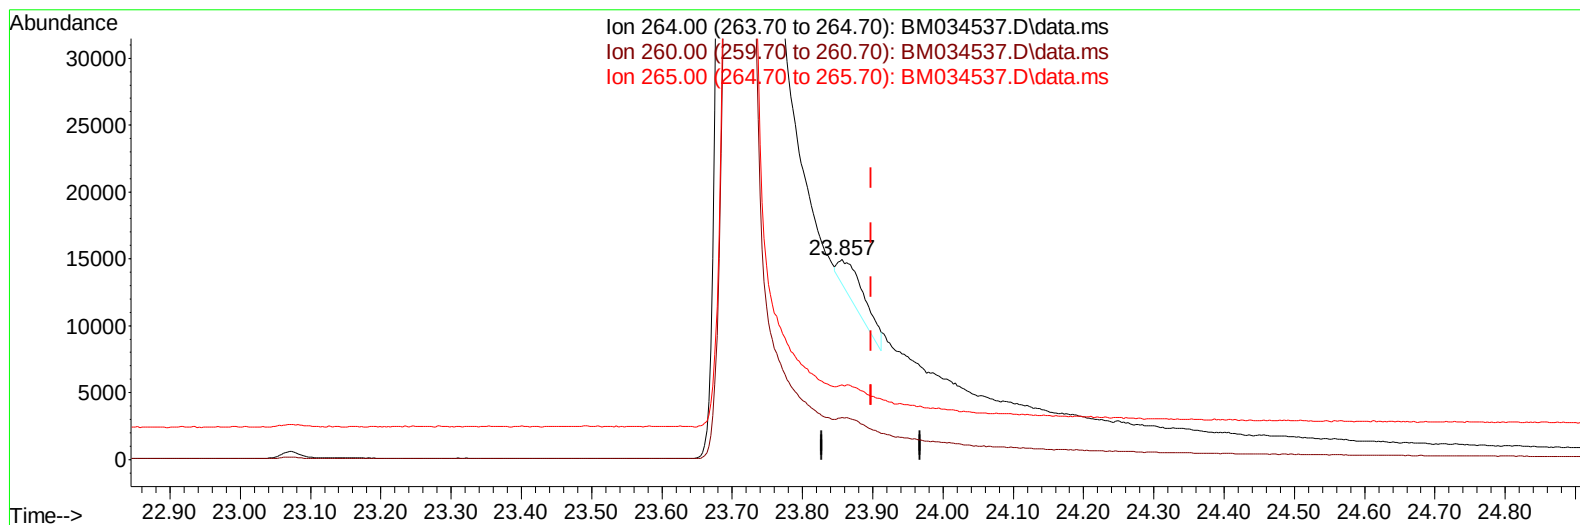

TIC: BM034537.D\data.ms

(23) Perylene-d12 (I)

23.857min (-0.041) 0.40 ng/ul m

response 6902

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.09#
265.00	95.30	37.29#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034537.D
 Acq On : 07 Apr 2022 04:17
 Operator : CG/JU
 Sample : SP5859
 Misc : SFAM SURROGATE
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5859

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 07 05:00:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.912	152		3218	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.719	136		9045	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.555	164		5169	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188		9139m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.512	240		6692	0.400	ng/ul	# 0.02
23) Perylene-d12	23.857	264		6902m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.292	96		66332	12.307	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.324	152		9767	0.822	ng/ul	-0.01
18) Fluoranthene-d10	19.324	212		17417	0.887	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
Data File : BM034537.D
Acq On : 07 Apr 2022 04:17
Operator : CG/JU
Sample : SP5859
Misc : SFAM SURROGATE
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP5859

Manual IntegrationsAPPROVED

Quant Time: Apr 07 05:00:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
Supervised By :Yogesh Patel 04/09/2022

