

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039324.D
 Acq On : 06 Apr 2023 19:52
 Operator : CG/JU
 Sample : PB151753BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK753

Quant Time: Apr 07 02:17:21 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 23:58:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	5987	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.691	136	23461	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.532	164	14488	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.282	188	26789	0.400	ng/ul	0.00
17) Chrysene-d12	21.480	240	16891	0.400	ng/ul	# 0.00
23) Perylene-d12	23.860	264	25090	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.259	96	46917	4.233	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.302	152	8966	0.331	ng/ul	0.01
18) Fluoranthene-d10	19.315	212	20865	0.396	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.527	166	3674	0.083	ng/ul#	17
20) Pyrene	19.678	202	3469	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.705	252	5741	0.072	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039324.D
Acq On : 06 Apr 2023 19:52
Operator : CG/JU
Sample : PB151753BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK753

Quant Time: Apr 07 02:17:21 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 23:58:10 2023
Response via : Initial Calibration




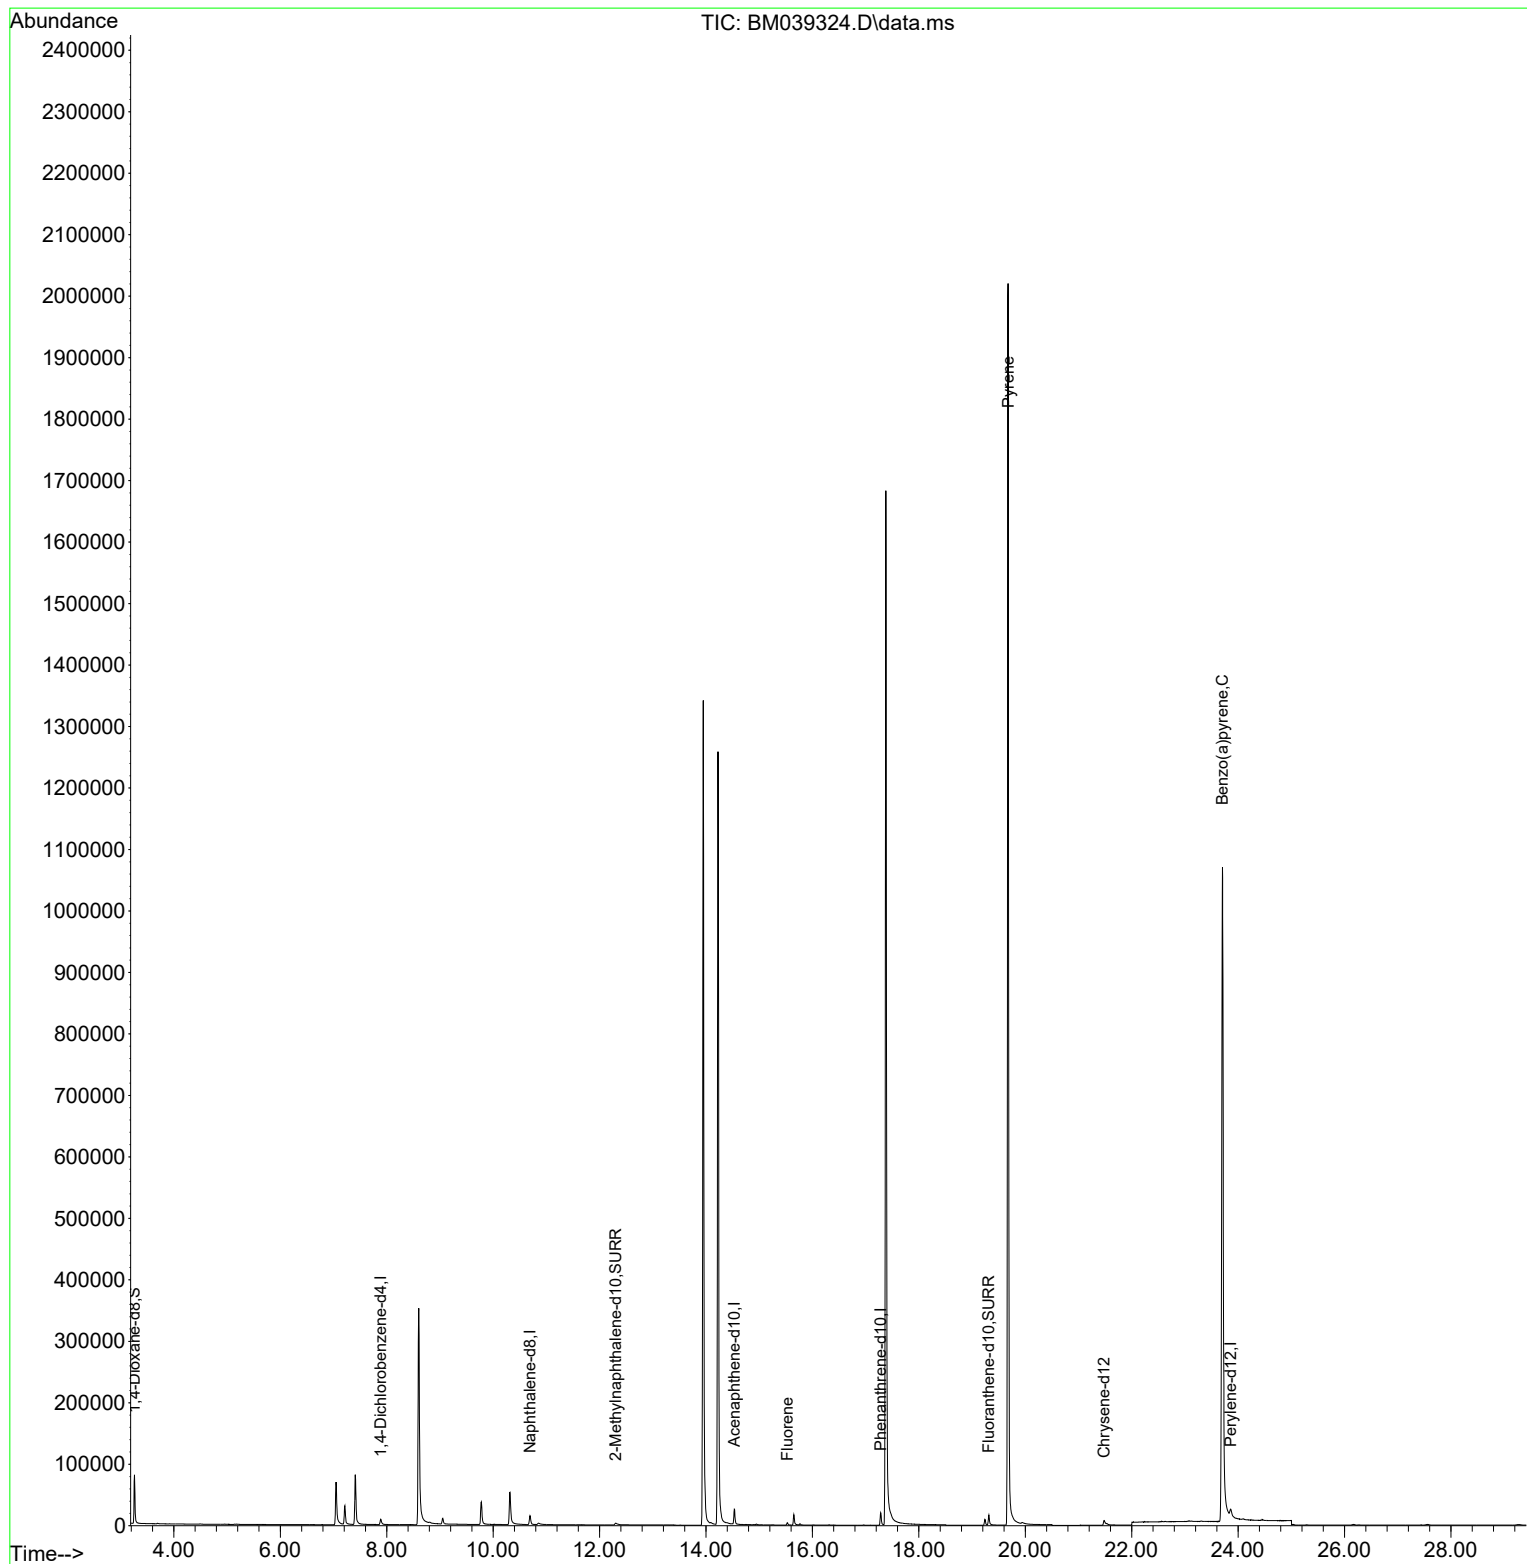


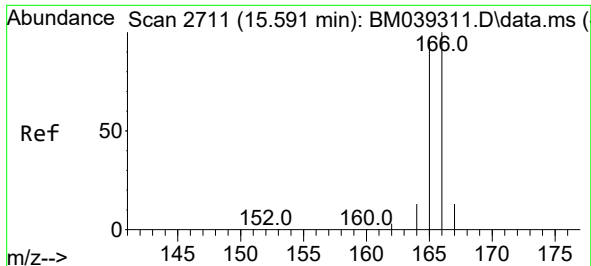

#12
Fluorene
Concen: 0.083 ng/ul
RT: 15.527 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM039324.D
Acq: 06 Apr 2023 19:52




Instrument :
BNA_M
ClientSampleId :
SBLK753


Tgt Ion:166 Resp: 3674
Ion Ratio Lower Upper
166 100
165 9.1 77.8 116.8#
167 31.5 11.8 17.6#

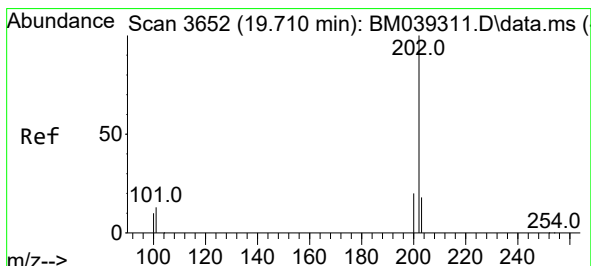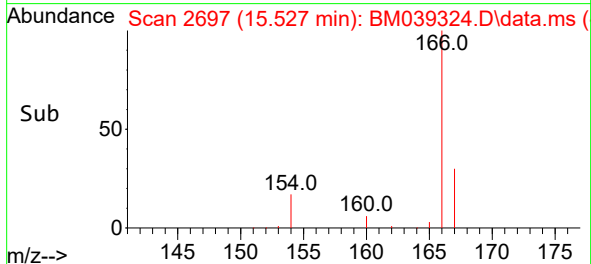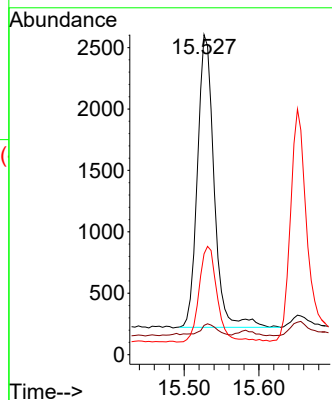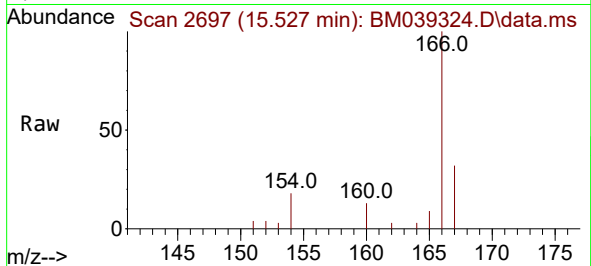

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.678 min Scan# 3645
Delta R.T. -0.033 min
Lab File: BM039324.D
Acq: 06 Apr 2023 19:52


Tgt Ion:202 Resp: 3469
Ion Ratio Lower Upper
202 100
101 150.8 11.1 16.7#
100 1086.2 8.8 13.2#

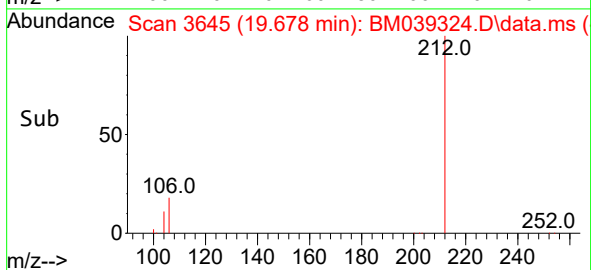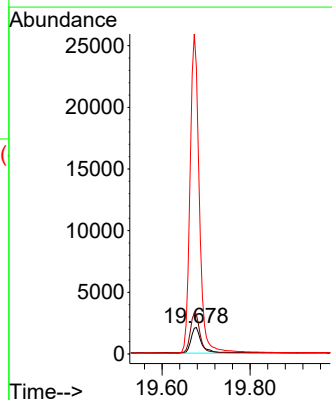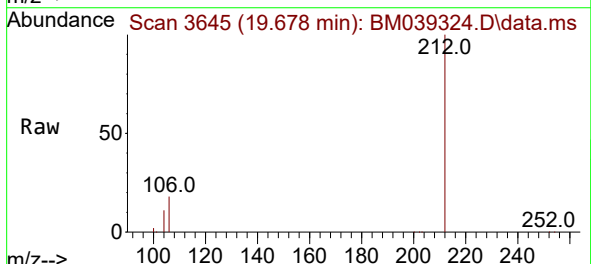

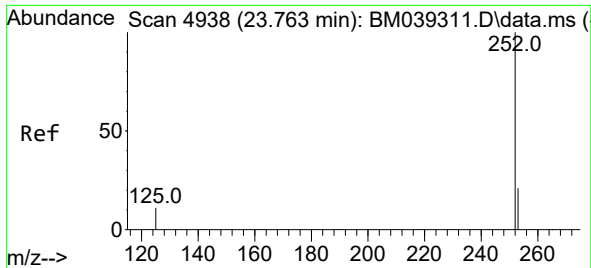

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.705 min Scan# 4918
Delta R.T. -0.058 min
Lab File: BM039324.D
Acq: 06 Apr 2023 19:52

Instrument :
BNA_M
ClientSampleId :
SBLK753

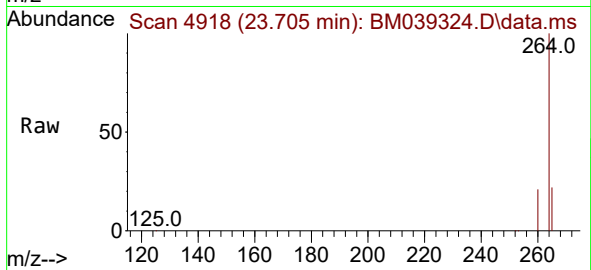

Tgt Ion:252 Resp: 5741
Ion Ratio Lower Upper
252 100
253 48.3 31.0 46.4#
125 46.6 28.2 42.4#

