

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039352.D
 Acq On : 07 Apr 2023 13:47
 Operator : CG/JU
 Sample : PB151828BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK828

Quant Time: Apr 07 23:13:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 07 23:05:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	7516	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.686	136	28763	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.527	164	16447	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.278	188	30824	0.400	ng/ul	0.00
17) Chrysene-d12	21.472	240	18628	0.400	ng/ul	# 0.00
23) Perylene-d12	23.854	264	21016	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	52755	3.791	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	10594	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.311	212	21233	0.366	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.522	166	3820	0.076	ng/ul#	16
20) Pyrene	19.673	202	3108	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.699	252	4770	0.071	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039352.D
Acq On : 07 Apr 2023 13:47
Operator : CG/JU
Sample : PB151828BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Quant Time: Apr 07 23:13:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 07 23:05:01 2023
Response via : Initial Calibration




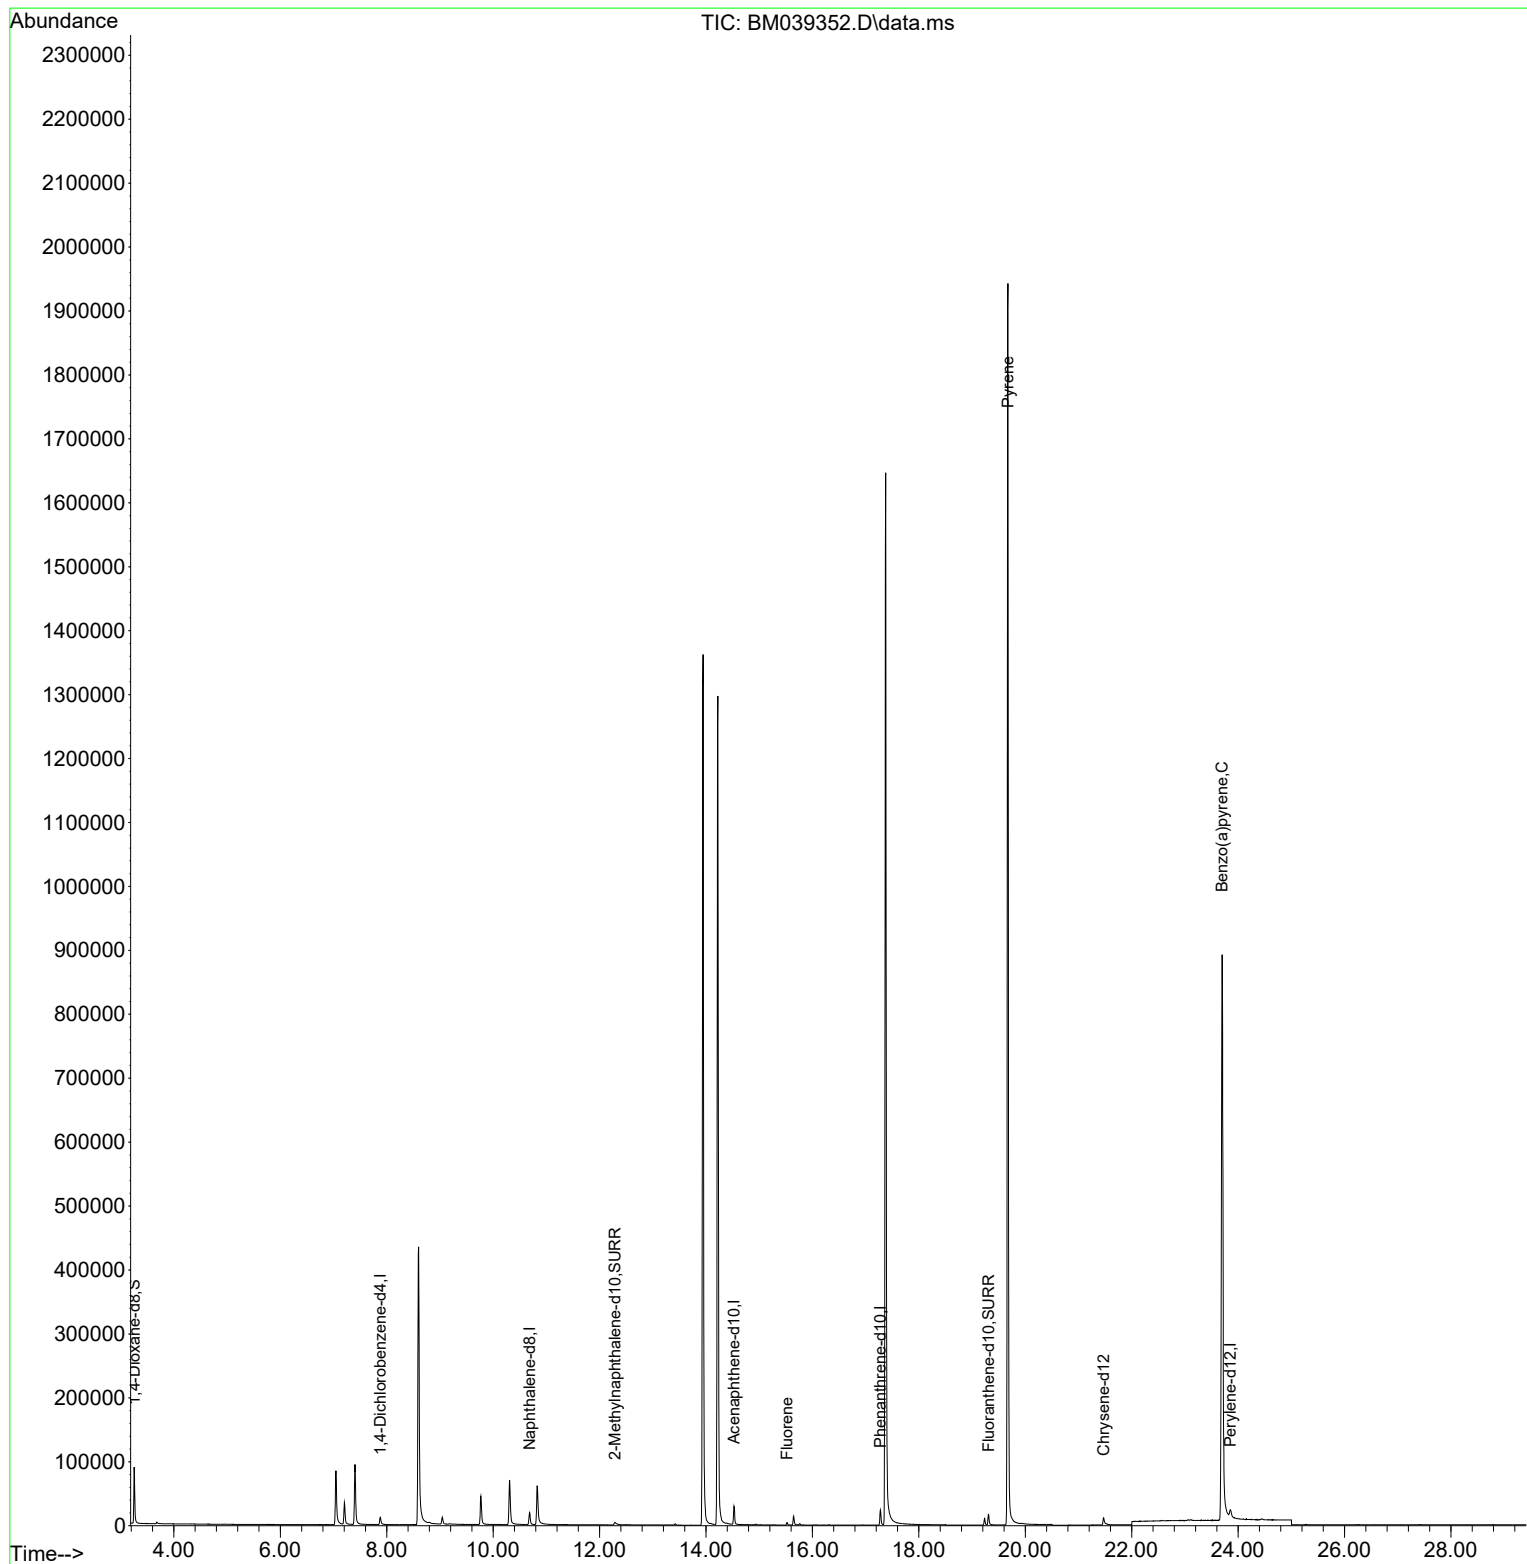


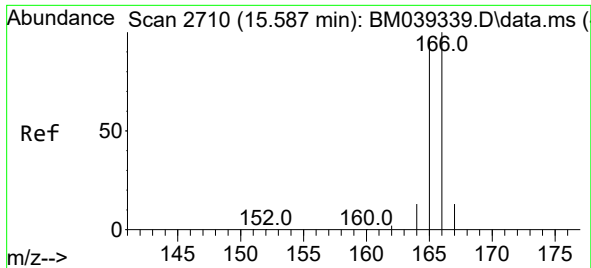

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.522 min Scan# 20
Delta R.T. -0.060 min
Lab File: BM039352.D
Acq: 07 Apr 2023 13:47




Instrument :
BNA_M
ClientSampleId :
SBLK828


Tgt Ion:166 Resp: 3820
Ion Ratio Lower Upper
166 100
165 8.6 77.8 116.8#
167 33.0 11.8 17.6#

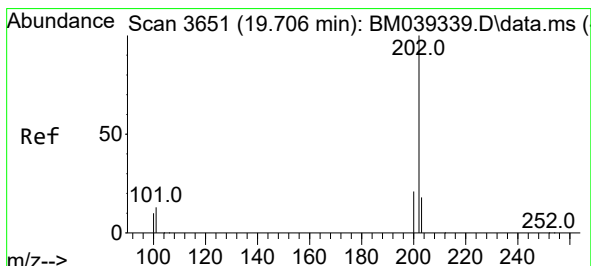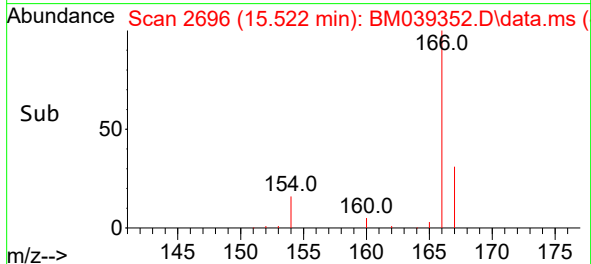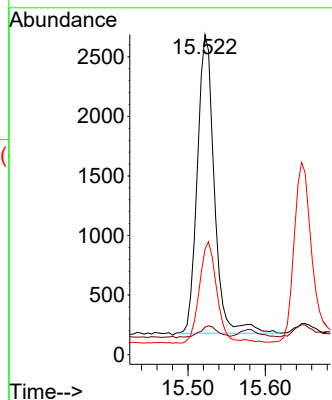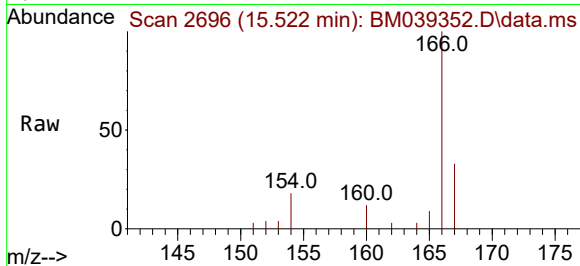

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.673 min Scan# 3644
Delta R.T. -0.028 min
Lab File: BM039352.D
Acq: 07 Apr 2023 13:47


Tgt Ion:202 Resp: 3108
Ion Ratio Lower Upper
202 100
101 149.9 11.1 16.7#
100 1070.9 8.8 13.2#

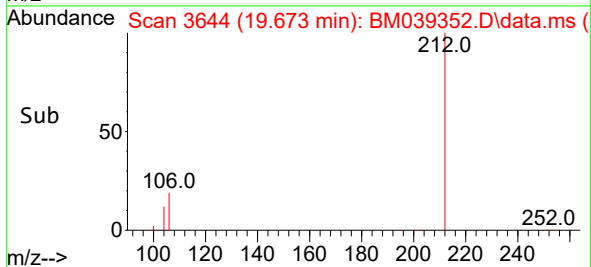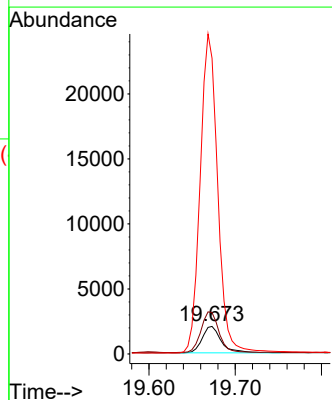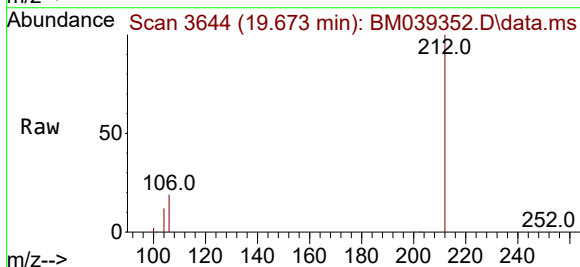

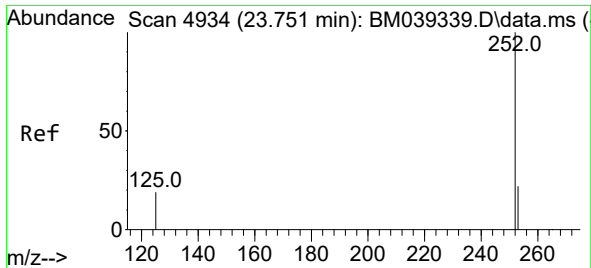

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.699 min Scan# 4916
Delta R.T. -0.050 min
Lab File: BM039352.D
Acq: 07 Apr 2023 13:47

Instrument :
BNA_M
ClientSampleId :
SBLK828

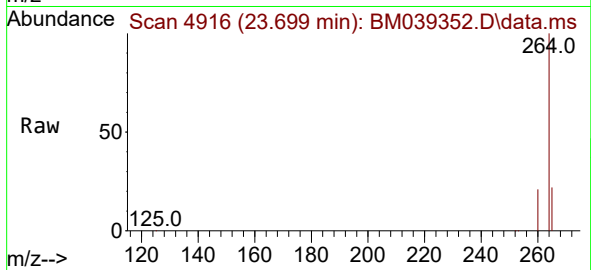

Tgt Ion:252 Resp: 4770
Ion Ratio Lower Upper
252 100
253 58.4 31.0 46.4#
125 56.5 28.2 42.4#

