

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039357.D
 Acq On : 07 Apr 2023 17:28
 Operator : CG/JU
 Sample : PB151828BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK828

Quant Time: Apr 07 23:14:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 07 23:05:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	6829	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.686	136	26025	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.527	164	15367	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	28251	0.400	ng/ul	0.00
17) Chrysene-d12	21.474	240	15058	0.400	ng/ul	# 0.00
23) Perylene-d12	23.854	264	19341	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	50424	3.988	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	9579	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	18388	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.668	202	2745	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.696	252	4388	0.071	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039357.D
Acq On : 07 Apr 2023 17:28
Operator : CG/JU
Sample : PB151828BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Quant Time: Apr 07 23:14:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 07 23:05:01 2023
Response via : Initial Calibration




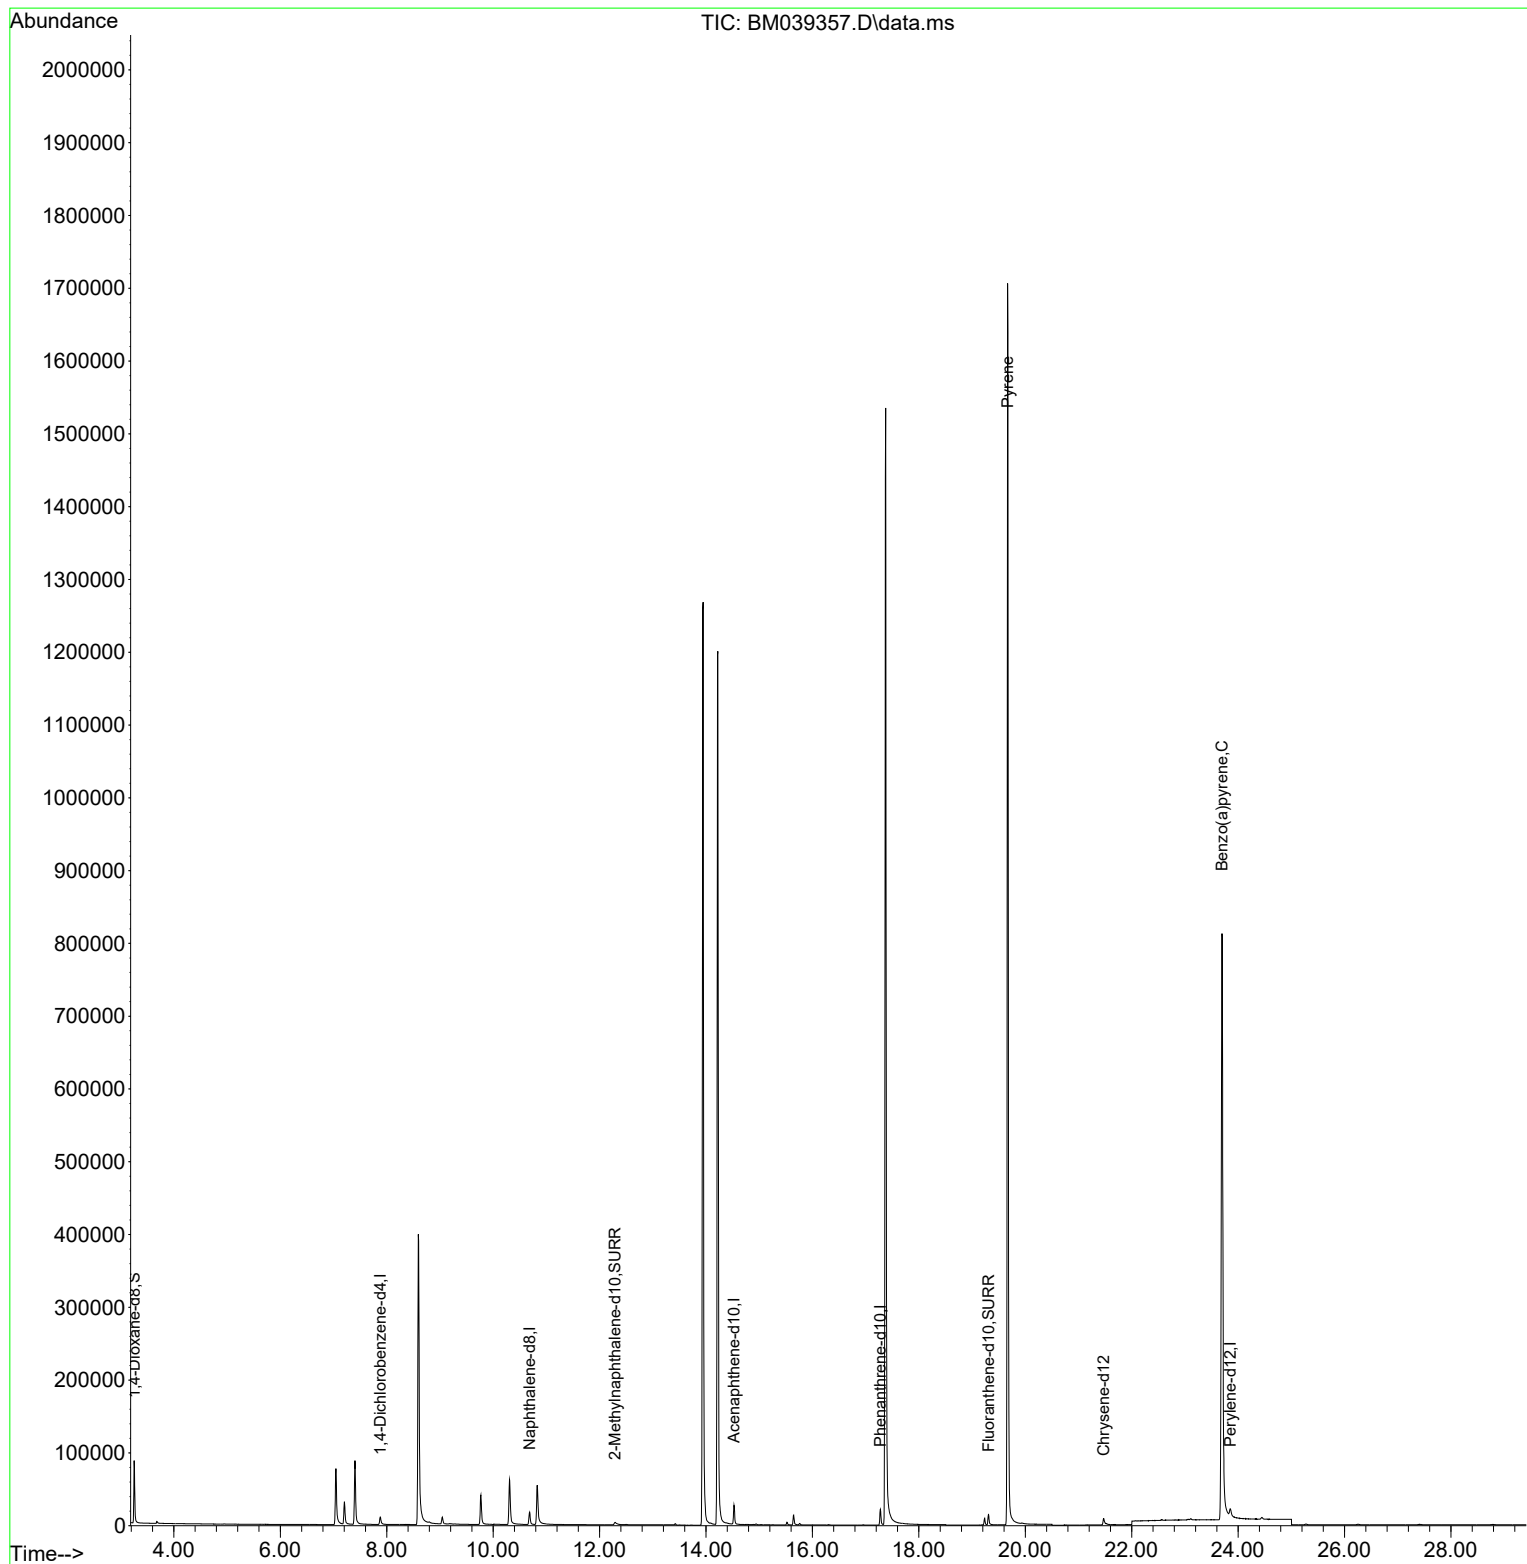


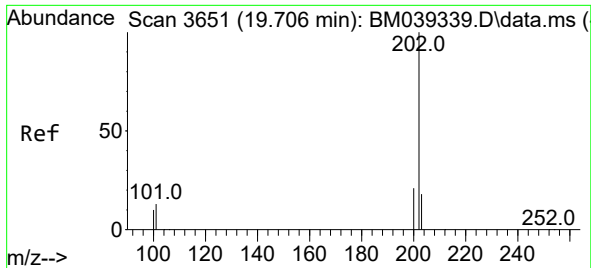

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.668 min Scan# 3643
Delta R.T. -0.033 min
Lab File: BM039357.D
Acq: 07 Apr 2023 17:28

Instrument :
BNA_M
ClientSampleId :
SBLK828

Tgt Ion:202 Resp: 2745
Ion Ratio Lower Upper
202 100
101 157.2 11.1 16.7#
100 1185.9 8.8 13.2#

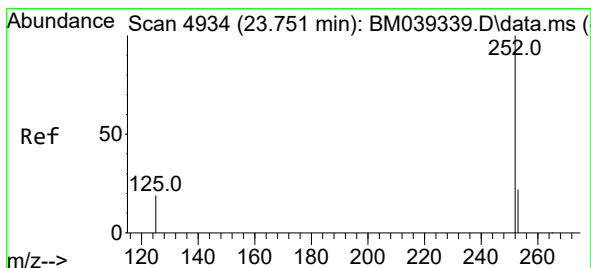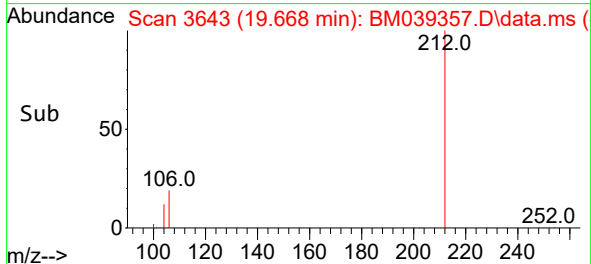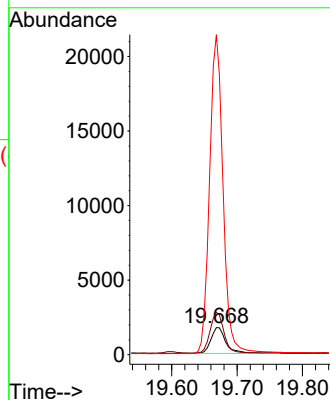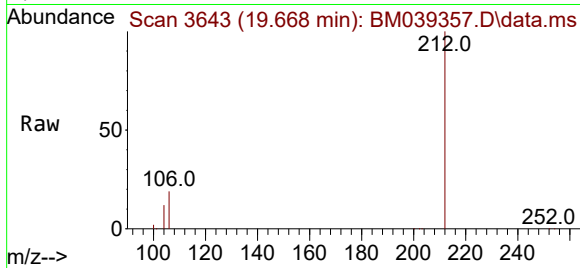

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.696 min Scan# 4915
Delta R.T. -0.053 min
Lab File: BM039357.D
Acq: 07 Apr 2023 17:28

Tgt Ion:252 Resp: 4388
Ion Ratio Lower Upper
252 100
253 59.3 31.0 46.4#
125 58.3 28.2 42.4#

