

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039320.D
 Acq On : 06 Apr 2023 16:40
 Operator : CG/JU
 Sample : 02122-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB9C3

Quant Time: Apr 07 02:16:45 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 23:58:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	5450	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.691	136	21105	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.532	164	13272	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.282	188	24761	0.400	ng/u1	0.00
17) Chrysene-d12	21.472	240	17459	0.400	ng/u1	# 0.00
23) Perylene-d12	23.857	264	24132	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	34430	3.412	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.297	152	8764	0.359	ng/u1	0.00
18) Fluoranthene-d10	19.310	212	22413	0.412	ng/u1	0.00
Target Compounds						
					Qvalue	
11) Acenaphthene	14.597	153	3659	0.090	ng/u1	99
19) Fluoranthene	19.343	202	3527	0.049	ng/u1#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039320.D
Acq On : 06 Apr 2023 16:40
Operator : CG/JU
Sample : 02122-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB9C3

Quant Time: Apr 07 02:16:45 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 23:58:10 2023
Response via : Initial Calibration




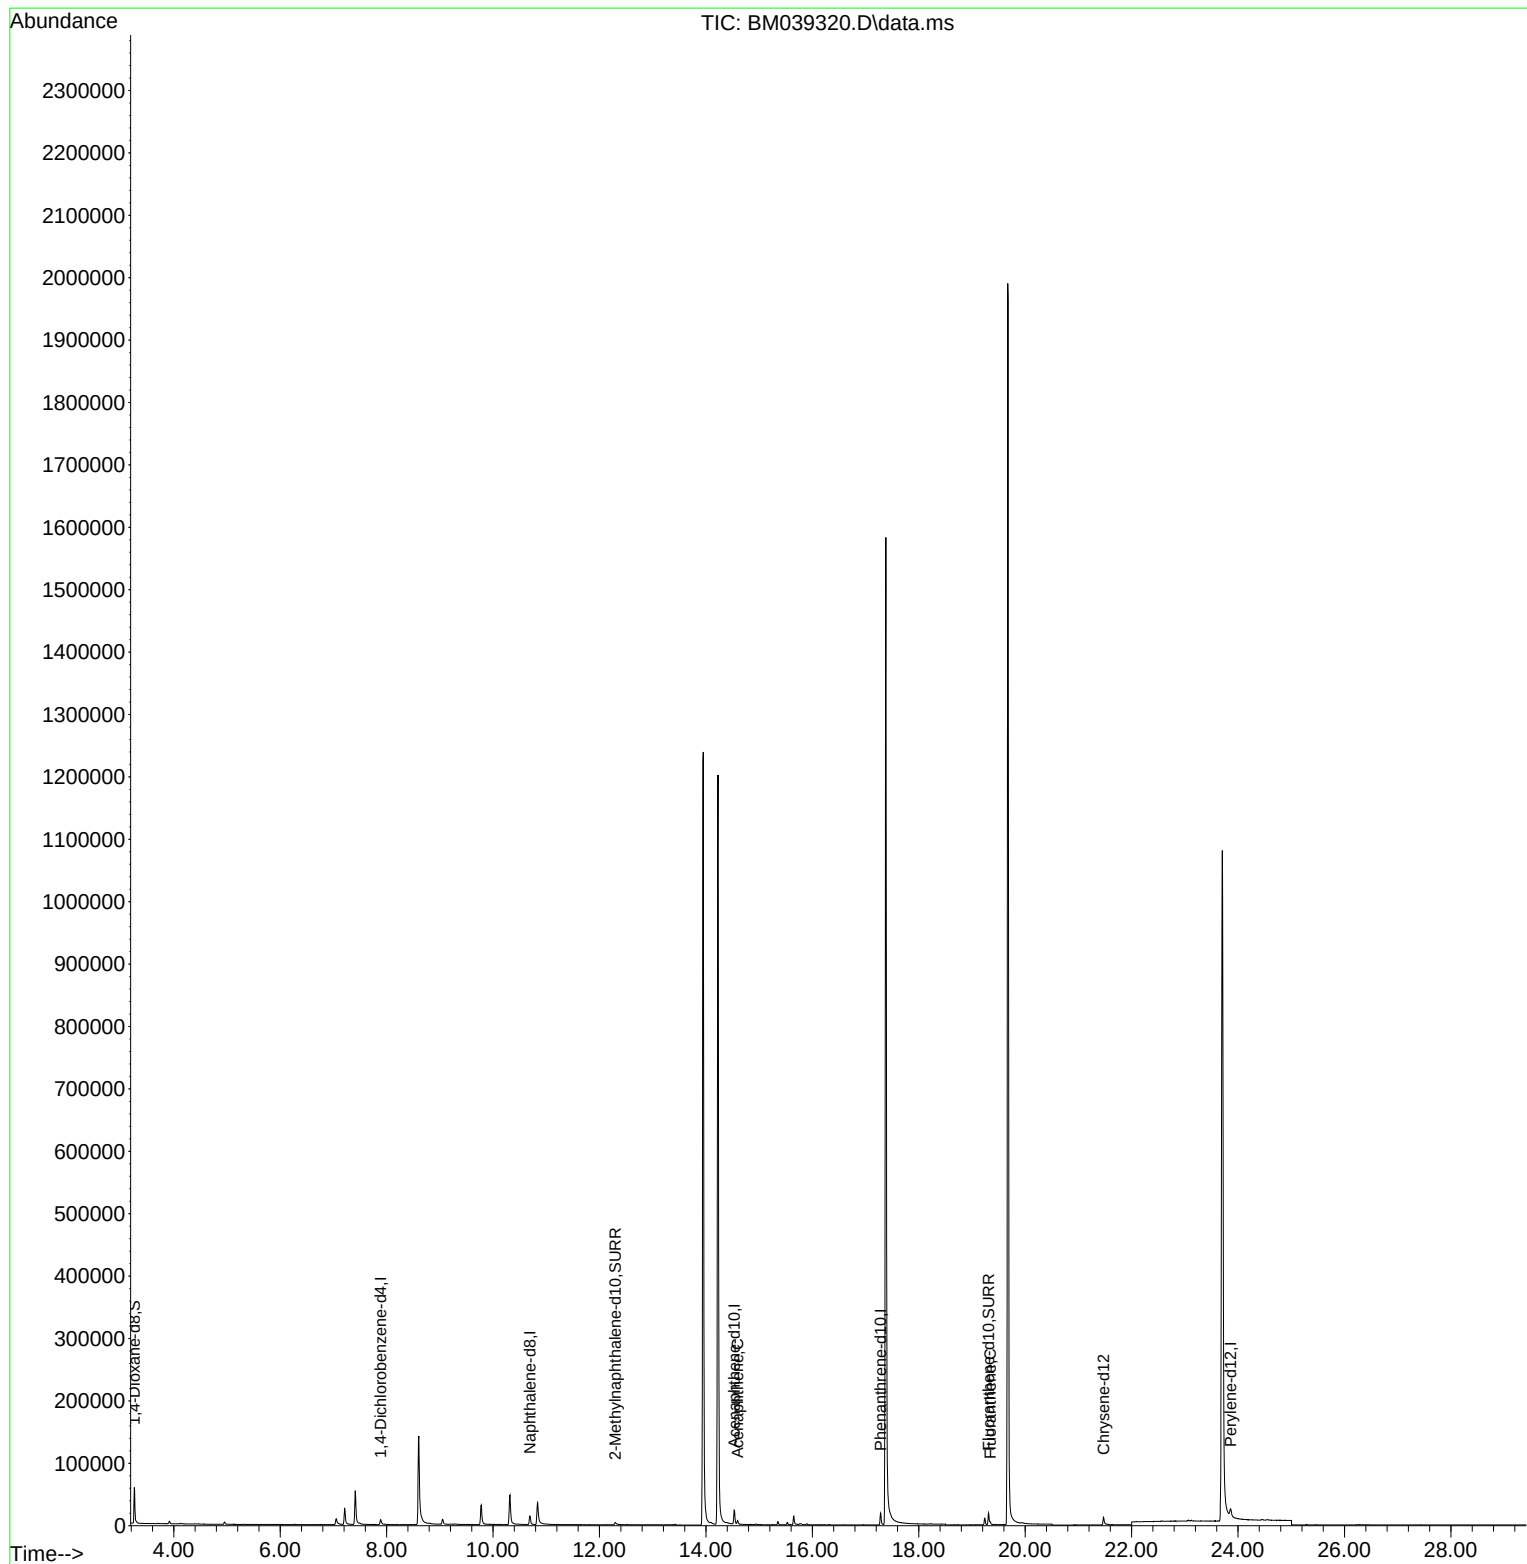


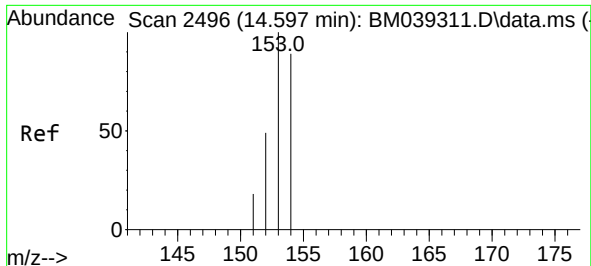

#11
Acenaphthene
Concen: 0.090 ng/ul
RT: 14.597 min Scan# 2496
Delta R.T. -0.000 min
Lab File: BM039320.D
Acq: 06 Apr 2023 16:40

Instrument :
BNA_M
ClientSampleId :
CB9C3

Tgt Ion	Ratio	Lower	Upper
153	100		
152	49.7	40.3	60.5
154	90.1	71.5	107.3

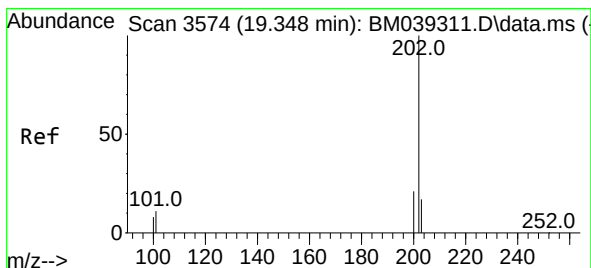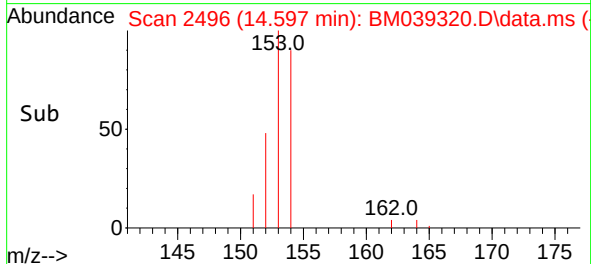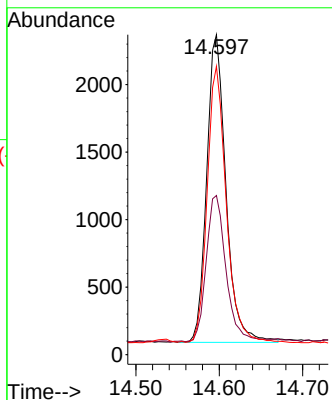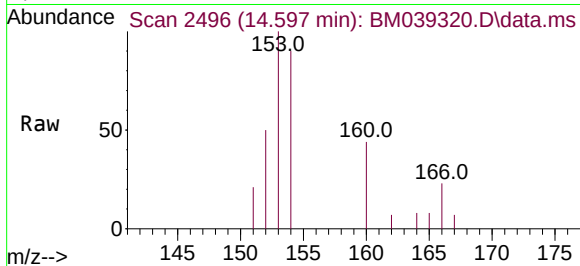

#19
Fluoranthene
Concen: 0.049 ng/ul
RT: 19.343 min Scan# 3573
Delta R.T. -0.005 min
Lab File: BM039320.D
Acq: 06 Apr 2023 16:40

Tgt Ion	Ratio	Lower	Upper
202	100		
101	16.8	9.7	14.5#
100	13.0	7.4	11.0#

