

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039321.D
 Acq On : 06 Apr 2023 17:18
 Operator : CG/JU
 Sample : 02122-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB9C5

Quant Time: Apr 07 02:16:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 23:58:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	5541	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.691	136	21237	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.532	164	13511	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.282	188	25428	0.400	ng/ul	0.00
17) Chrysene-d12	21.471	240	17363	0.400	ng/ul	# 0.00
23) Perylene-d12	23.860	264	22962	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	33473	3.263	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	8666	0.353	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	22715	0.420	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.343	202	1742	0.024	ng/ul#	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039321.D
Acq On : 06 Apr 2023 17:18
Operator : CG/JU
Sample : 02122-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB9C5

Quant Time: Apr 07 02:16:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 23:58:10 2023
Response via : Initial Calibration

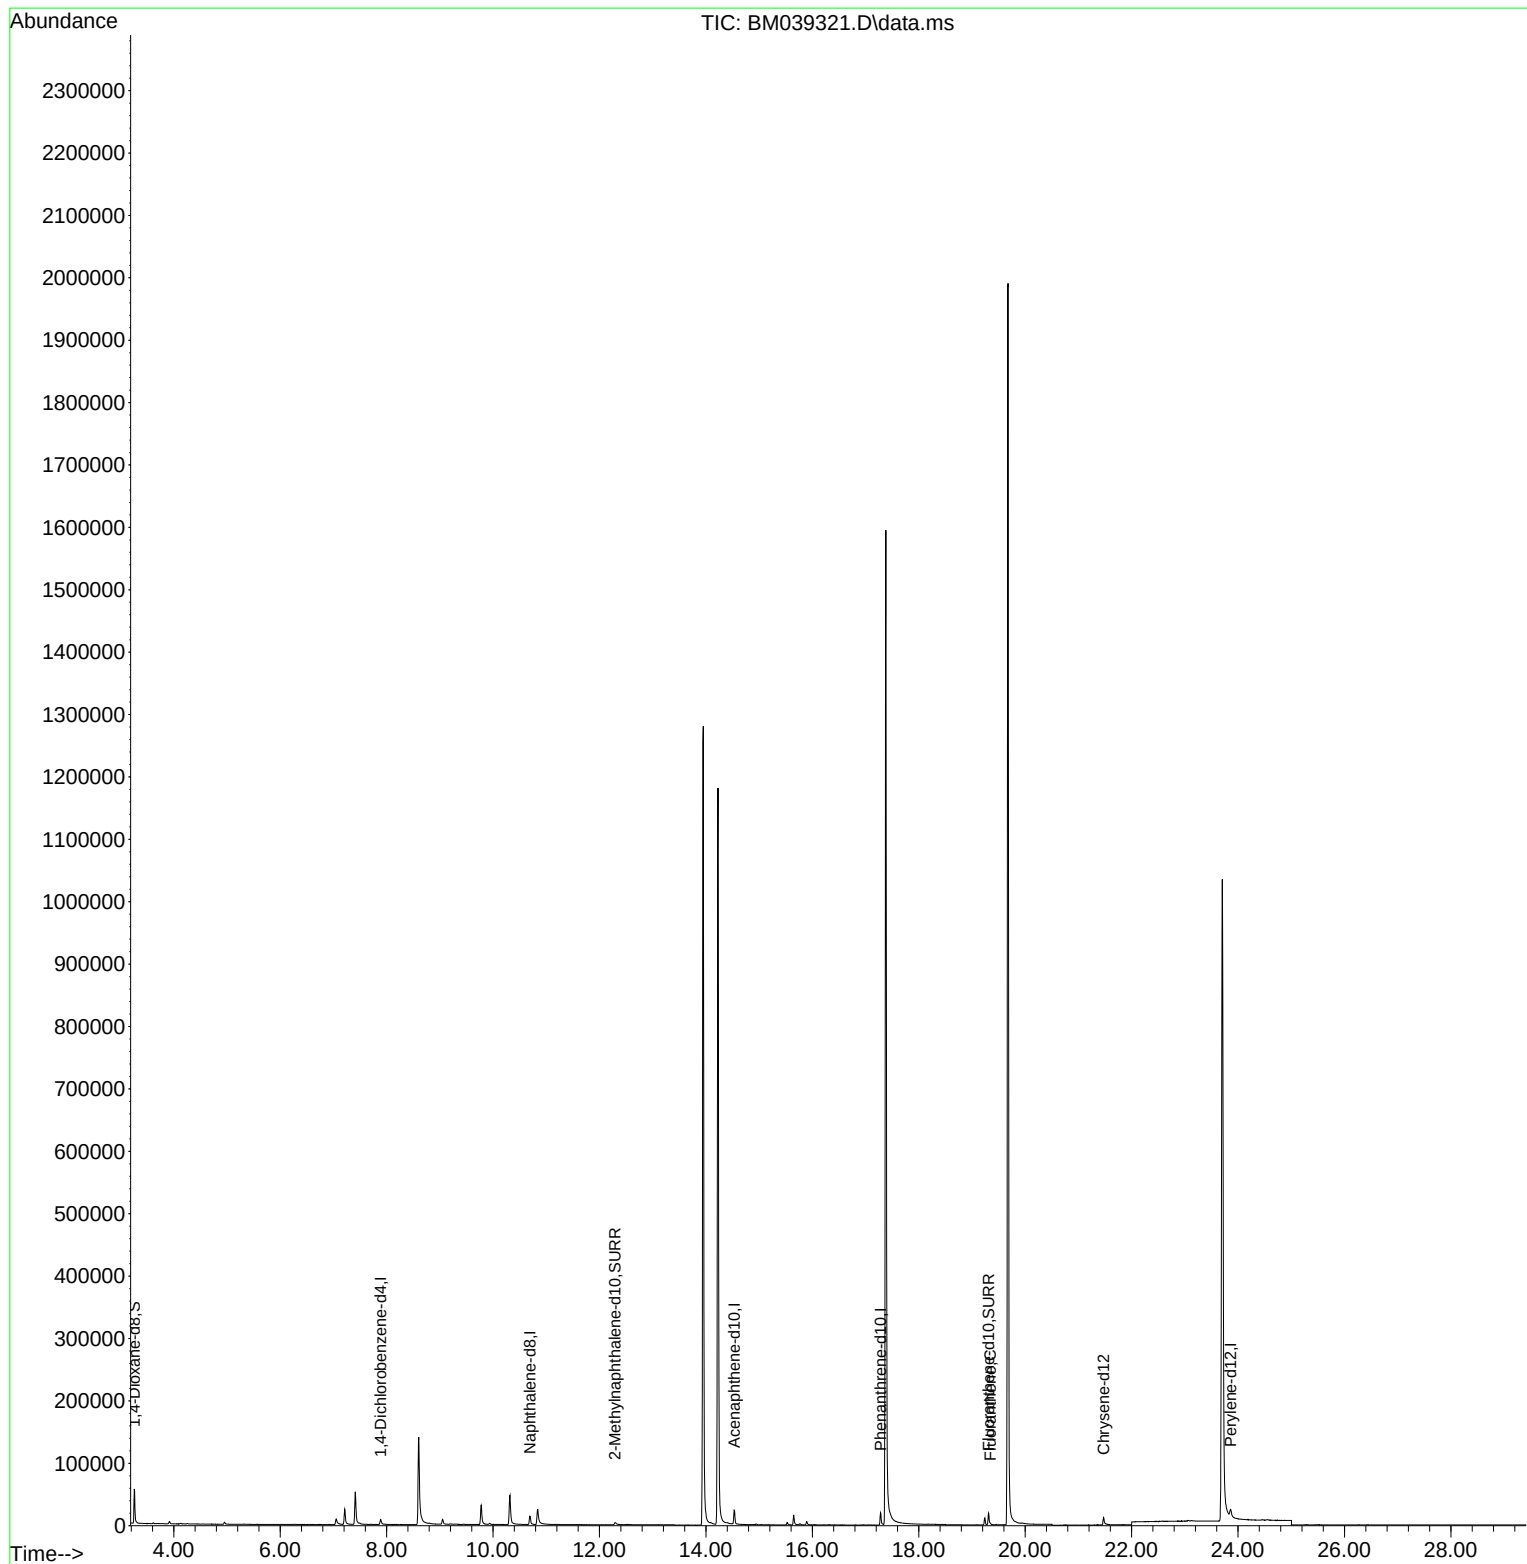

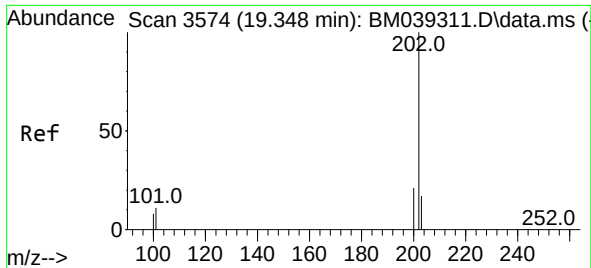

#19

Fluoranthene

Concen: 0.024 ng/ul

RT: 19.343 min Scan# 31

Delta R.T. -0.005 min

Lab File: BM039321.D


Acq: 06 Apr 2023 17:18

Instrument :

BNA_M

ClientSampleId :

CB9C5

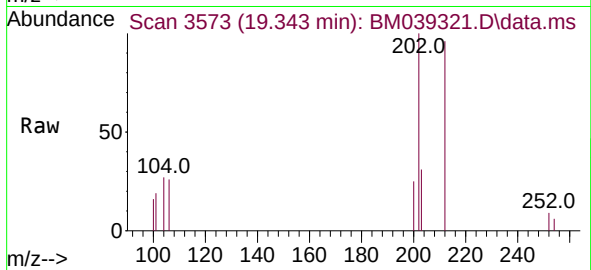

Tgt Ion:202 Resp: 1742

Ion Ratio Lower Upper

202 100

101 19.4 9.7 14.5#

100 15.6 7.4 11.0#

