

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039330.D
 Acq On : 06 Apr 2023 23:40
 Operator : CG/JU
 Sample : 02092-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB978

Quant Time: Apr 07 02:18:10 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 23:58:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	7200	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.691	136	27552	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.532	164	17684	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.282	188	28721	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.469	240	15960	0.400	ng/ul	0.00
23) Perylene-d12	23.857	264	13939	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	35221	2.642	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	7924	0.249	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	14396	0.289	ng/ul	0.00
Target Compounds						
16) Anthracene	17.417	178	5150	0.085	ng/ul#	Qvalue 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039330.D
Acq On : 06 Apr 2023 23:40
Operator : CG/JU
Sample : 02092-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB978

Quant Time: Apr 07 02:18:10 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 23:58:10 2023
Response via : Initial Calibration

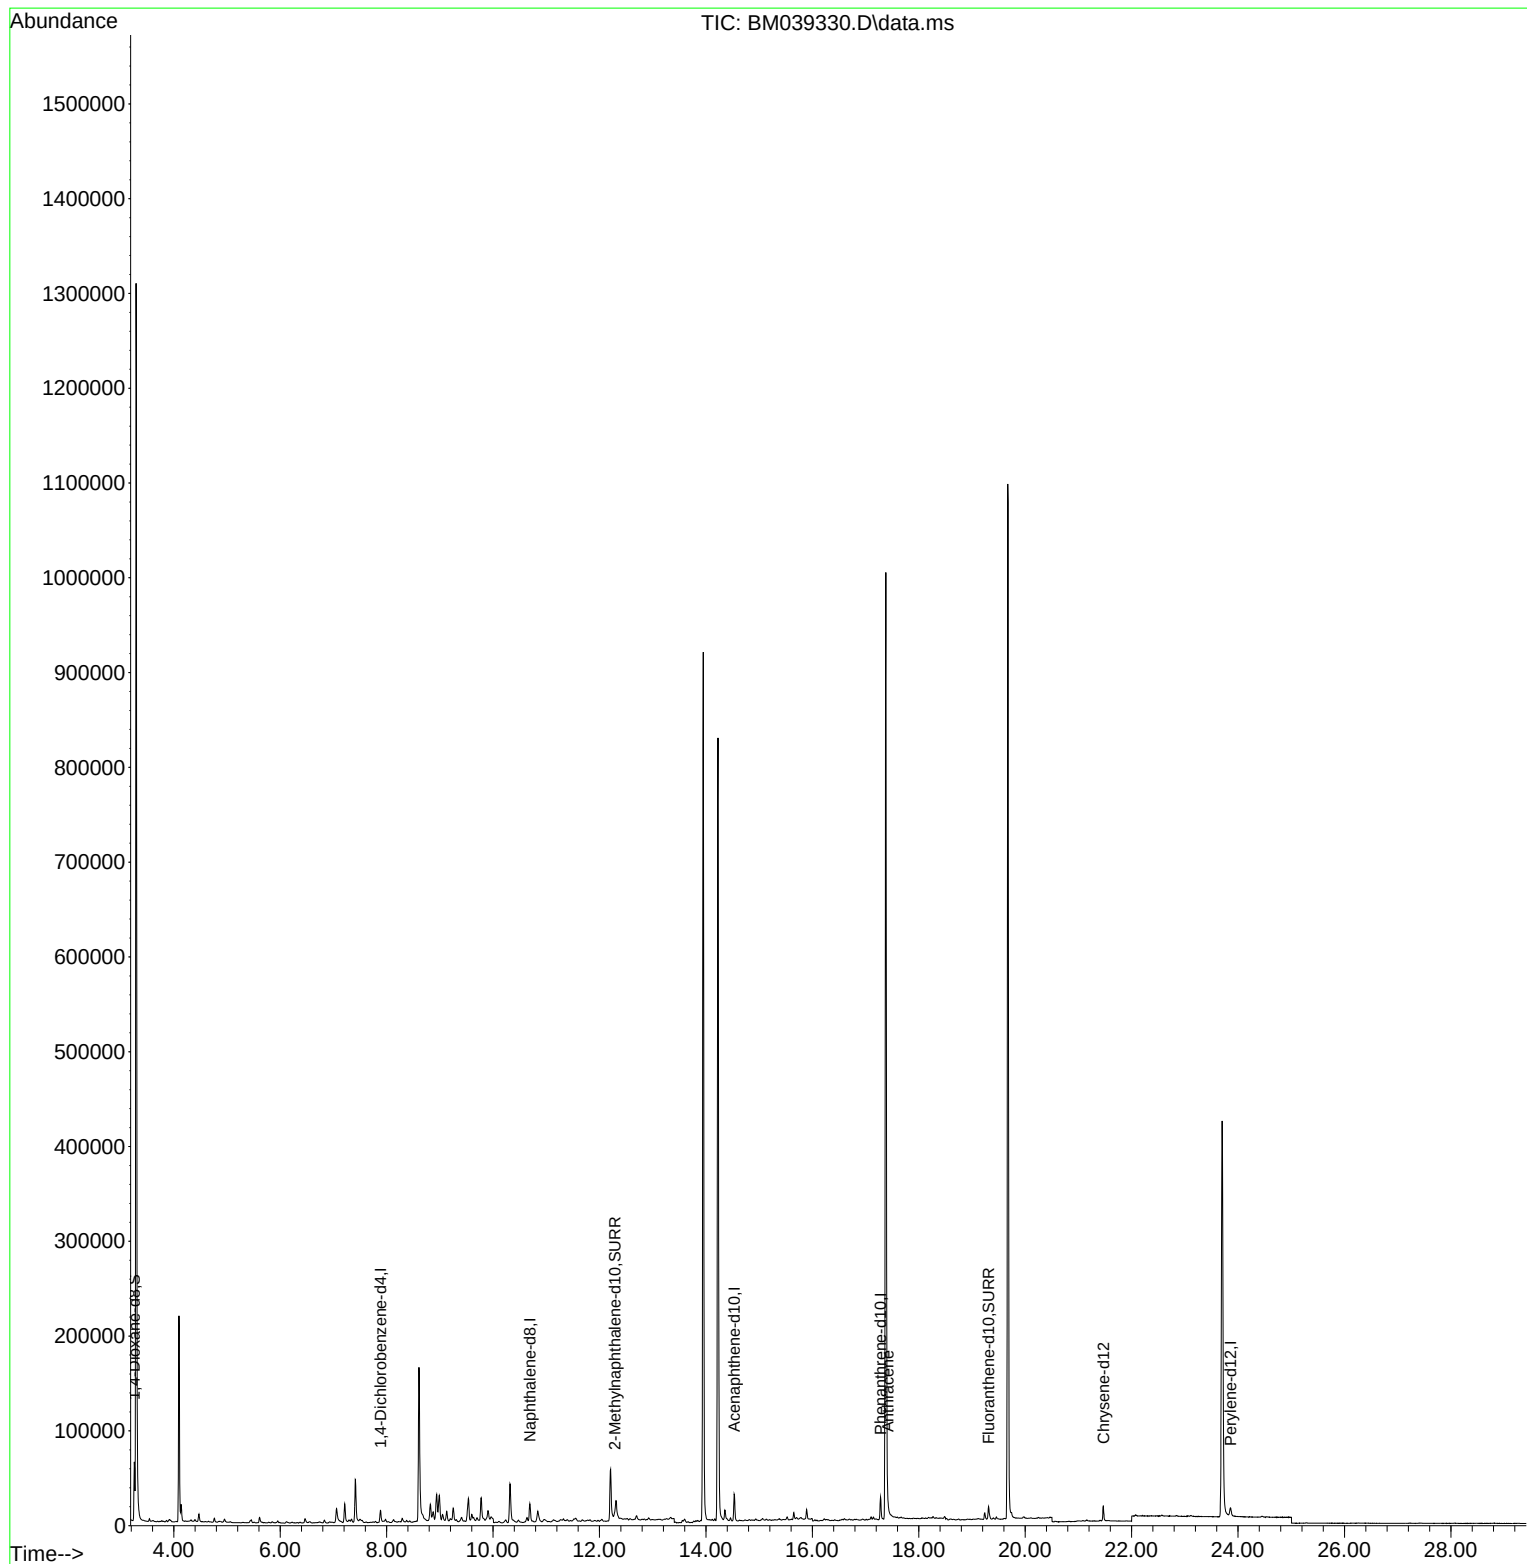

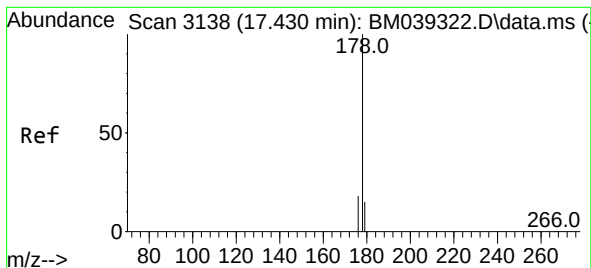

#16

Anthracene

Concen: 0.085 ng/ul

RT: 17.417 min Scan# 31

Delta R.T. -0.009 min

Lab File: BM039330.D


Acq: 06 Apr 2023 23:40

Instrument :

BNA_M

ClientSampleId :

CB978

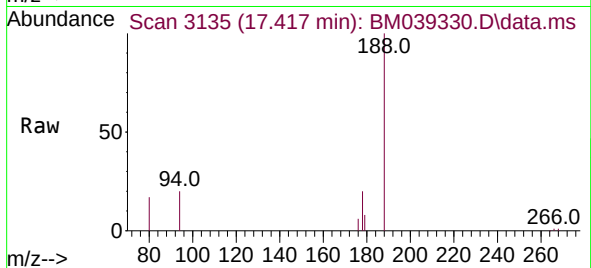

Tgt Ion:178 Resp: 5150

Ion Ratio Lower Upper

178 100

179 37.6 14.6 21.8#

176 31.9 16.6 24.8#

