

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039331.D
 Acq On : 07 Apr 2023 00:17
 Operator : CG/JU
 Sample : 02092-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB982

Quant Time: Apr 07 02:42:08 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 23:58:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	6101	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.691	136	21324	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.532	164	17600	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.282	188	20525	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.466	240	12931	0.400	ng/ul	# 0.00
23) Perylene-d12	23.860	264	14064	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	33484	2.965	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	9621	0.390	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	16690	0.414	ng/ul	0.00
Target Compounds						
						Qvalue
16) Anthracene	17.417	178	16471	0.380	ng/ul#	85
21) Benzo(a)anthracene	21.451	228	2479	0.083	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039331.D
Acq On : 07 Apr 2023 00:17
Operator : CG/JU
Sample : 02092-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB982

Quant Time: Apr 07 02:42:08 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 23:58:10 2023
Response via : Initial Calibration




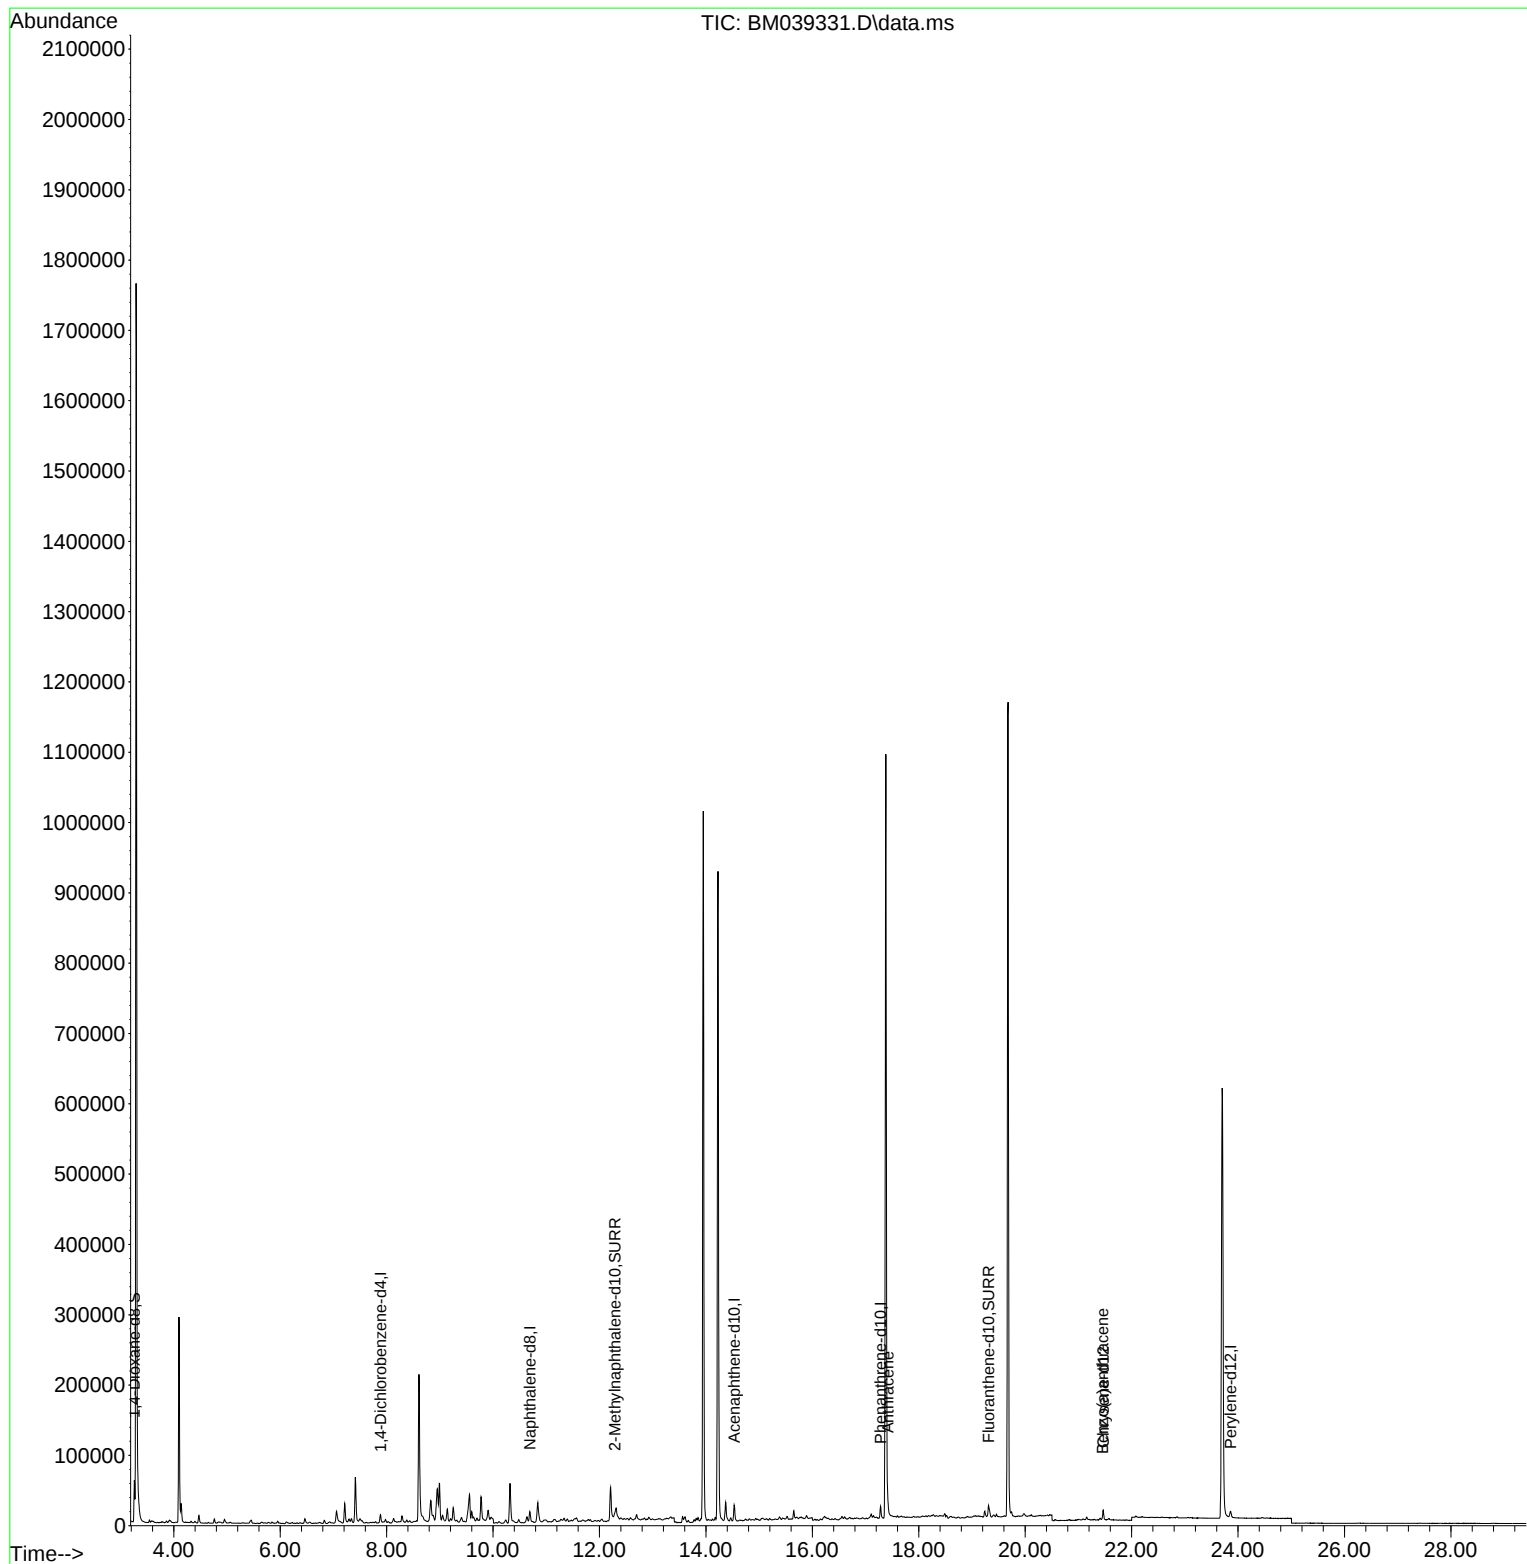


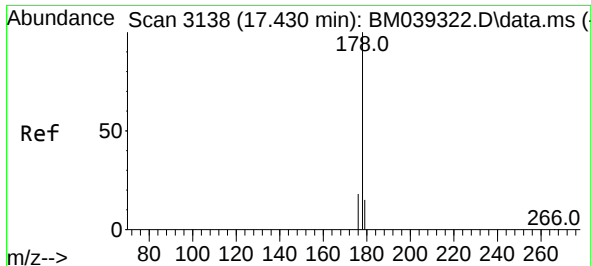

#16
 Anthracene
 Concen: 0.380 ng/ul
 RT: 17.417 min Scan# 3135
 Delta R.T. -0.009 min
 Lab File: BM039331.D
 Acq: 07 Apr 2023 00:17

Instrument :
 BNA_M
 ClientSampleId :
 CB982

Tgt Ion:178 Resp: 16471
 Ion Ratio Lower Upper
 178 100
 179 26.1 14.6 21.8#
 176 26.3 16.6 24.8#

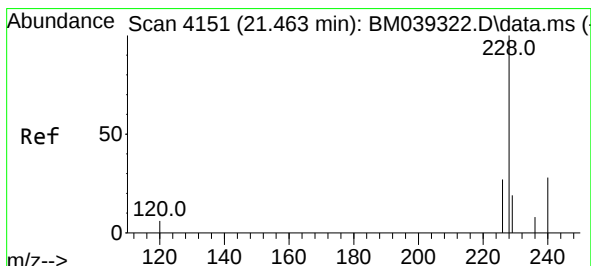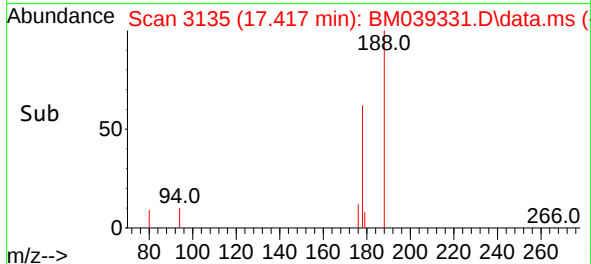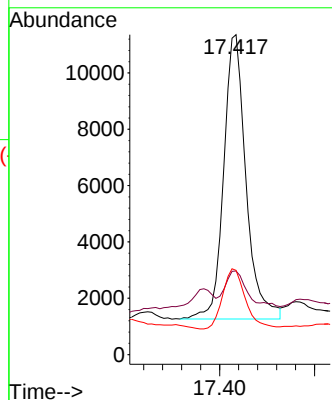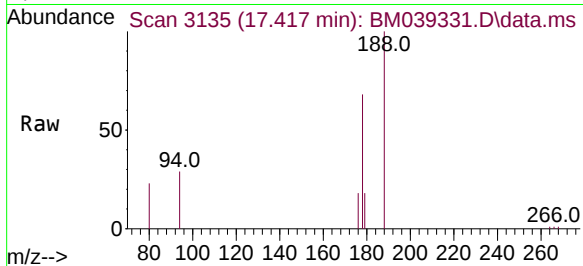

#21
 Benzo(a)anthracene
 Concen: 0.083 ng/ul
 RT: 21.451 min Scan# 4147
 Delta R.T. -0.009 min
 Lab File: BM039331.D
 Acq: 07 Apr 2023 00:17

Tgt Ion:228 Resp: 2479
 Ion Ratio Lower Upper
 228 100
 229 66.7 16.6 24.8#
 226 52.4 22.6 34.0#

