

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039335.D
 Acq On : 07 Apr 2023 02:46
 Operator : CG/JU
 Sample : 02092-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB984

Quant Time: Apr 07 03:21:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 23:58:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	5800	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.691	136	22397	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.532	164	14085	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	27404	0.400	ng/ul	0.00
17) Chrysene-d12	21.469	240	19379	0.400	ng/ul	# 0.00
23) Perylene-d12	23.857	264	23478	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	36898	3.436	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	10609	0.410	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	25009	0.414	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.944	266	262	0.040	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039335.D
Acq On : 07 Apr 2023 02:46
Operator : CG/JU
Sample : 02092-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB984

Quant Time: Apr 07 03:21:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 23:58:10 2023
Response via : Initial Calibration

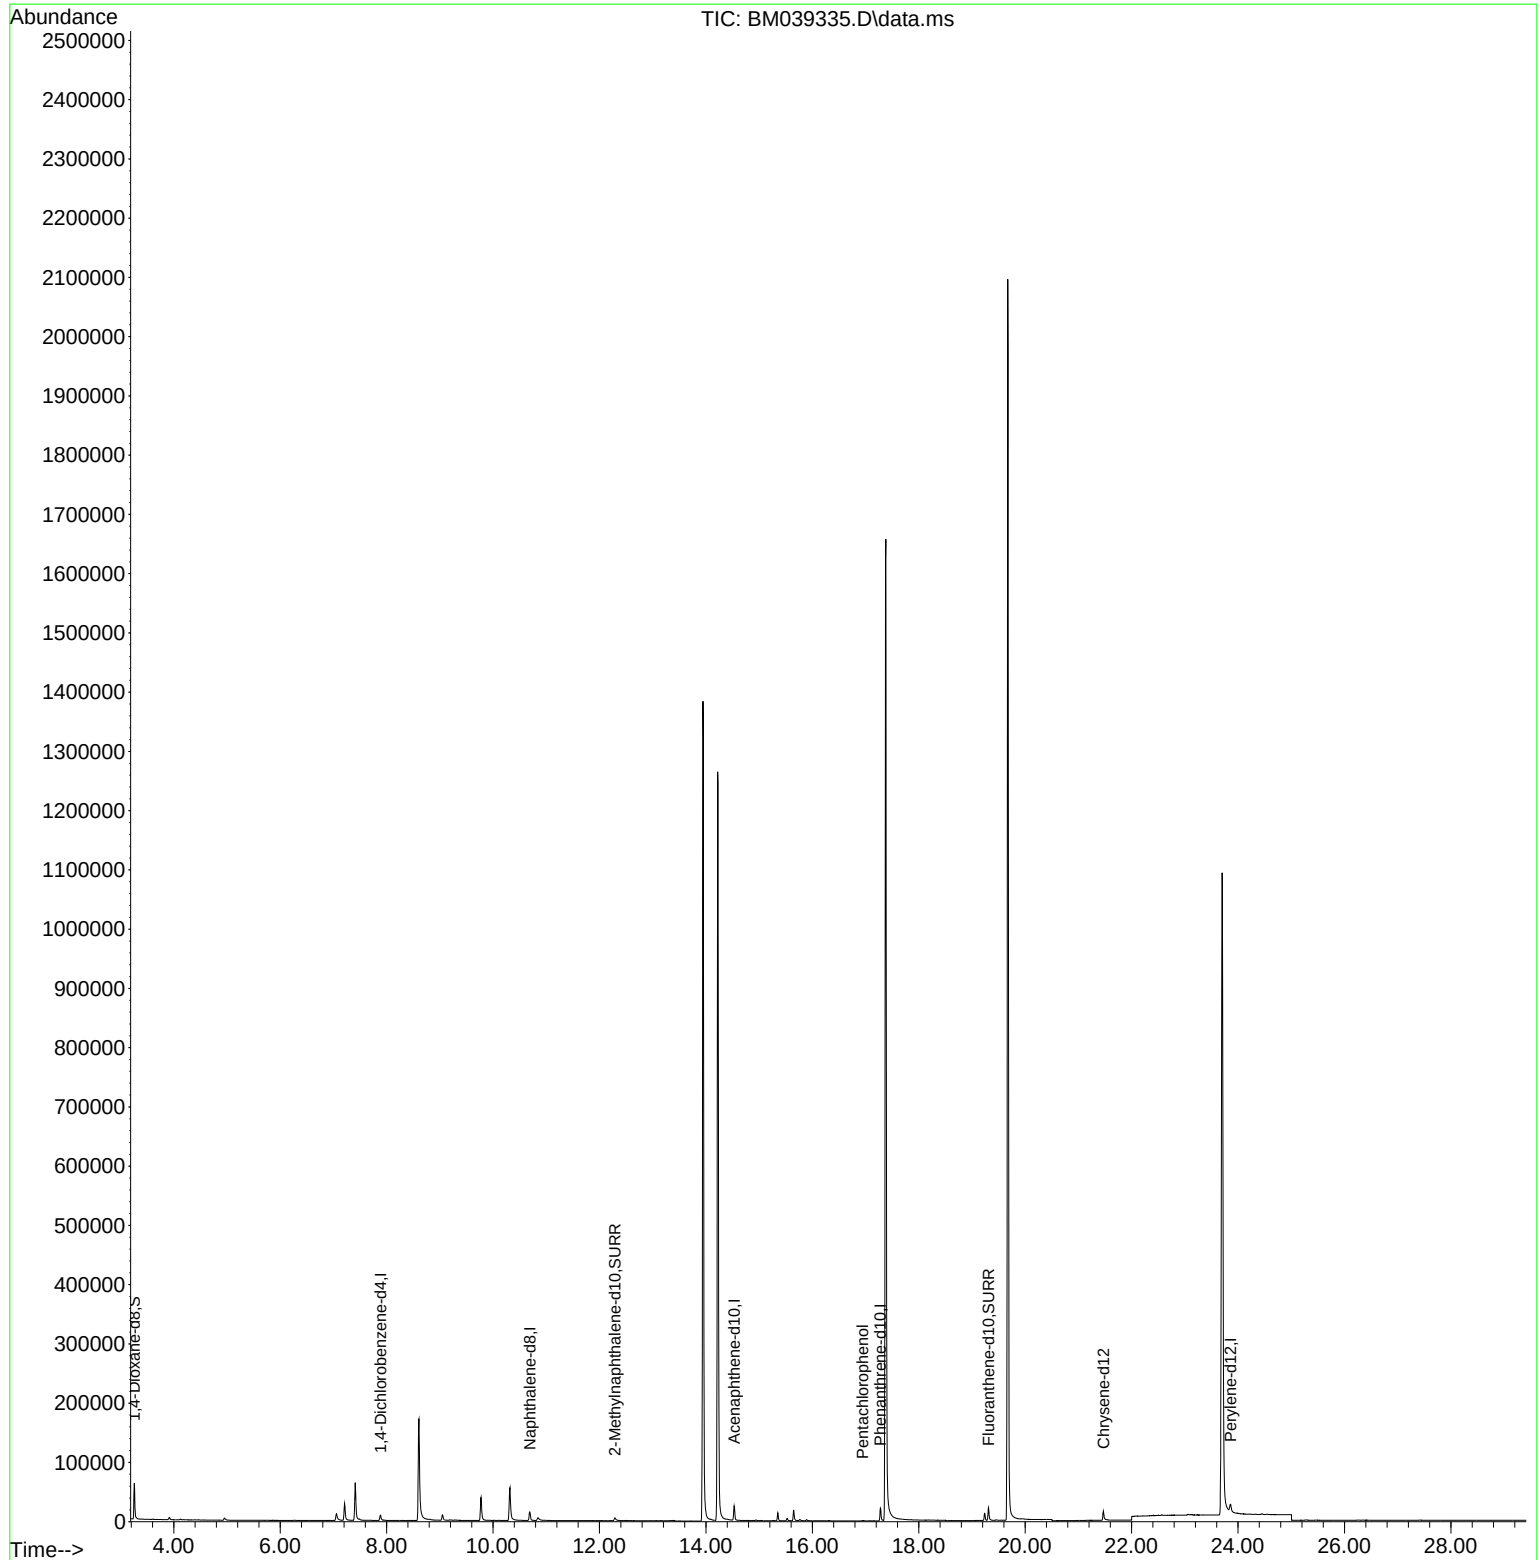

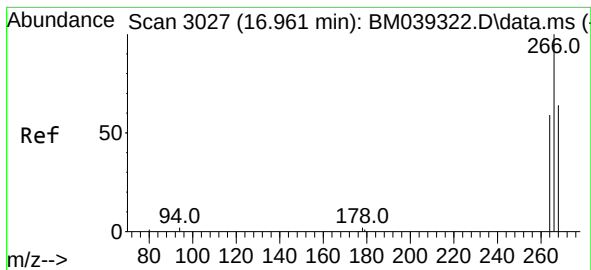

#14

Pentachlorophenol

Concen: 0.040 ng/ul

RT: 16.944 min Scan# 30

Delta R.T. -0.009 min

Lab File: BM039335.D


Acq: 07 Apr 2023 02:46

Instrument :

BNA_M

ClientSampleId :

CB984

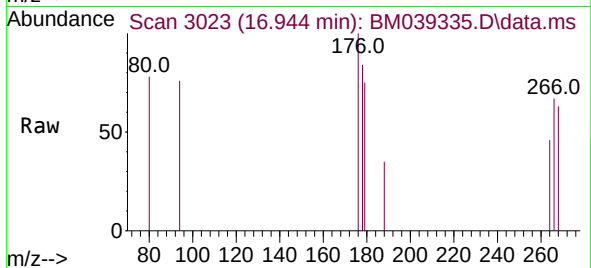

Tgt Ion:266 Resp: 262

Ion Ratio Lower Upper

266 100

264 63.4 39.6 59.4#

268 75.6 42.4 63.6#

