

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
 Data File : BM039365.D
 Acq On : 07 Apr 2023 22:23
 Operator : CG/JU
 Sample : 02122-13
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB9C5

Quant Time: Apr 08 00:20:08 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 07 23:05:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	6276	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.680	136	24132	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.527	164	14593	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.274	188	27914	0.400	ng/ul	0.00
17) Chrysene-d12	21.466	240	16375	0.400	ng/ul	# 0.00
23) Perylene-d12	23.851	264	17784	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	33452	2.879	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	9238	0.331	ng/ul	0.00
18) Fluoranthene-d10	19.306	212	21969	0.431	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.334	202	1640	0.024	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040623\
Data File : BM039365.D
Acq On : 07 Apr 2023 22:23
Operator : CG/JU
Sample : 02122-13
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB9C5

Quant Time: Apr 08 00:20:08 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 07 23:05:01 2023
Response via : Initial Calibration

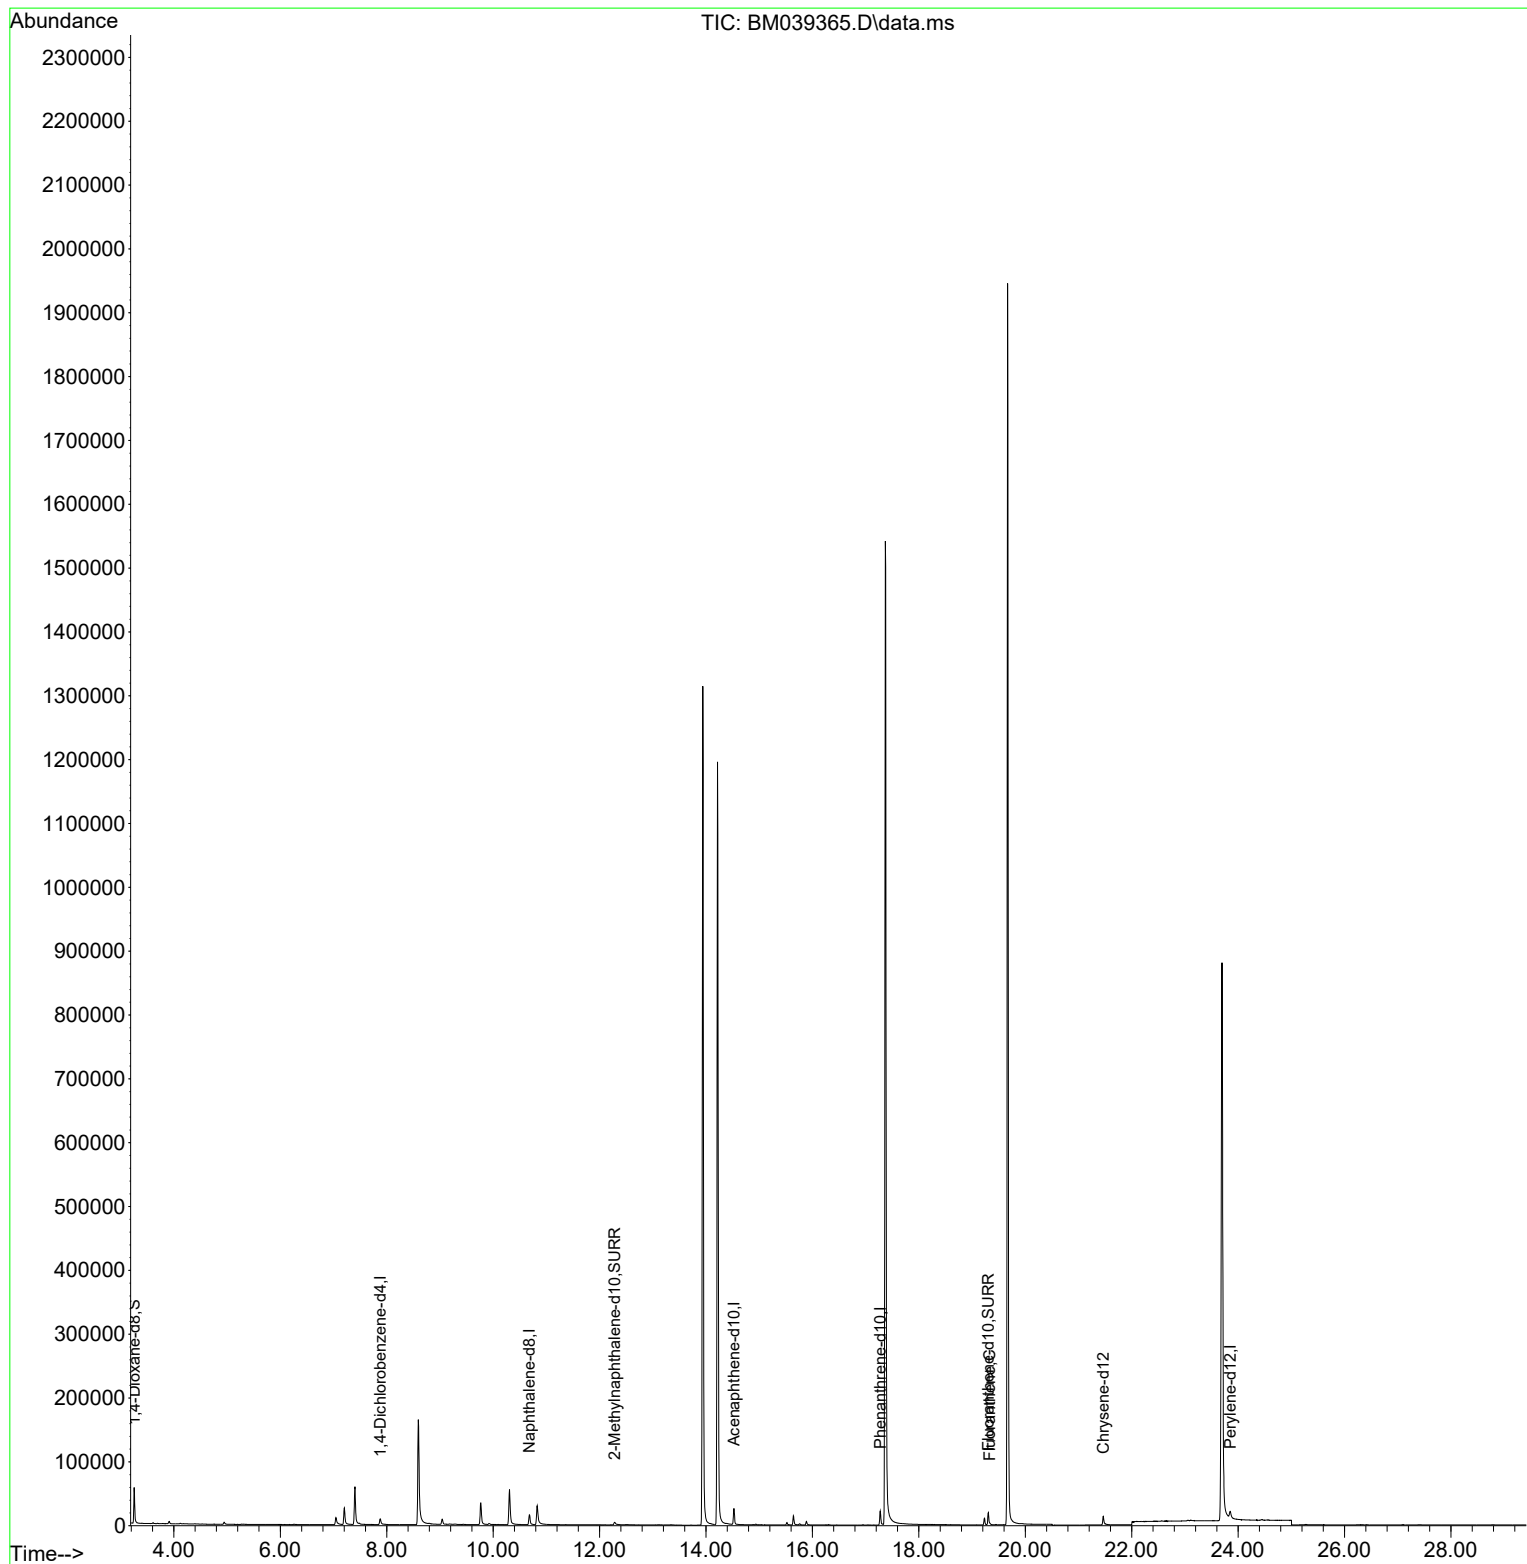

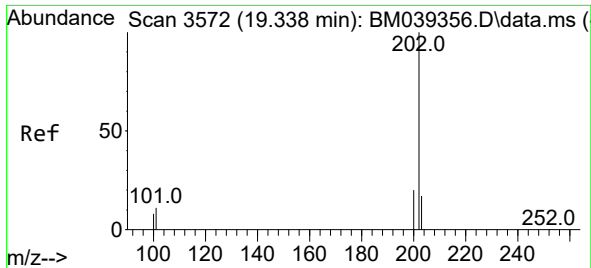

#19

Fluoranthene

Concen: 0.024 ng/ul

RT: 19.334 min Scan# 31

Delta R.T. -0.005 min

Lab File: BM039365.D


Acq: 07 Apr 2023 22:23

Instrument :

BNA_M

ClientSampleId :

CB9C5

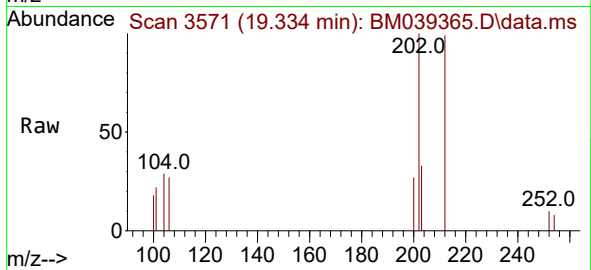

Tgt Ion:202 Resp: 1640

Ion Ratio Lower Upper

202 100

101 22.3 9.7 14.5#

100 18.2 7.4 11.0#

