

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040716\
 Data File : BM004917.D
 Acq On : 07 Apr 2016 15:43
 Operator : UM/SJ
 Sample : PB89605BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Quant Time: Apr 08 00:59:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 00:57:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	34594	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	163388	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	105050	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.20	188	259314	20.00	ng/ul	0.00
78) Chrysene-d12	21.39	240	337231	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	345556	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	5316	6.22	ng/uL	0.00
5) Phenol-d5	6.98	99	104863	34.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	64250	38.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	86022	36.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	88605	34.32	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	43881	37.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	49632	38.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	86392	35.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	133956	46.70	ng/ul	0.00
44) Dimethylphthalate-d6	13.86	166	328916	39.69	ng/ul	0.00
47) Acenaphthylene-d8	14.15	160	381259	38.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.65	143	55457	33.84	ng/ul	0.00
58) Fluorene-d10	15.45	176	285104	39.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	47557	30.61	ng/ul	0.00
71) Anthracene-d10	17.30	188	466015	40.16	ng/ul	0.00
79) Pyrene-d10	19.60	212	561995	38.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	623107	40.70	ng/ul	0.00


Target Compounds					Qvalue
46) 2,6-Dinitrotoluene	13.86	165	2344	1.43 ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040716\
Data File : BM004917.D
Acq On : 07 Apr 2016 15:43
Operator : UM/SJ
Sample : PB89605BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Time: Apr 08 00:59:41 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 00:57:37 2016
Response via : Initial Calibration

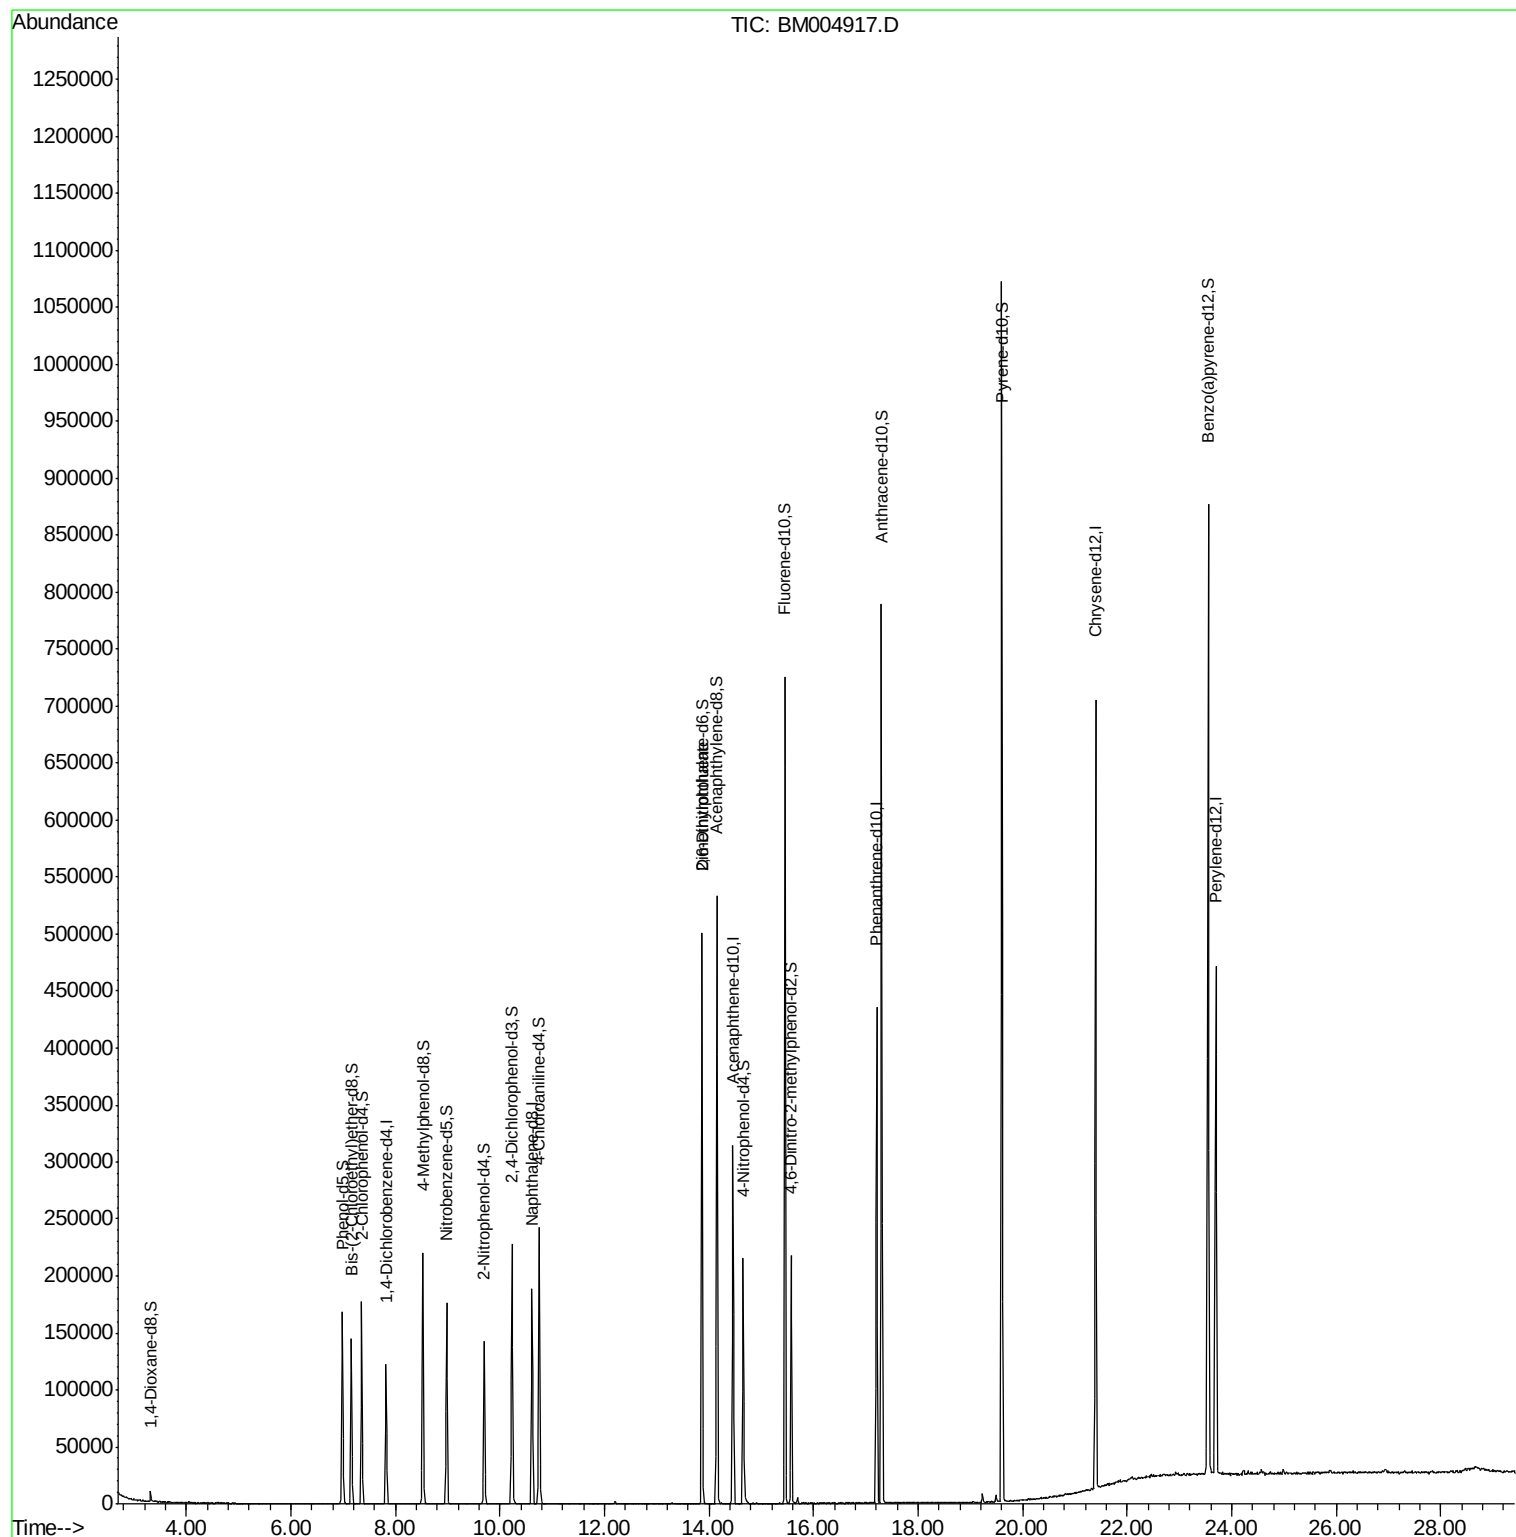


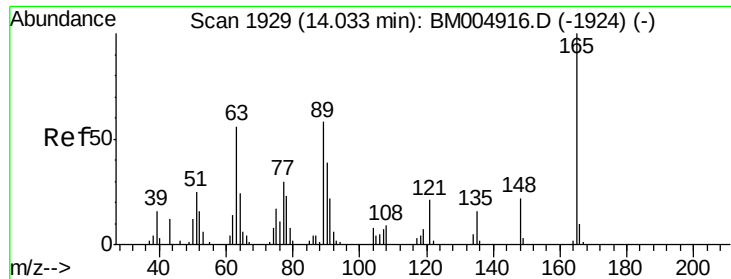

#46
 2,6-Dinitrotoluene
 Concen: 1.43 ng/ul
 RT: 13.86 min Scan# 1900
 Delta R.T. -0.17 min
 Lab File: BM004917.D
 Acq: 07 Apr 2016 15:43

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	42.4	63.6#
121	33.4	16.6	24.8#

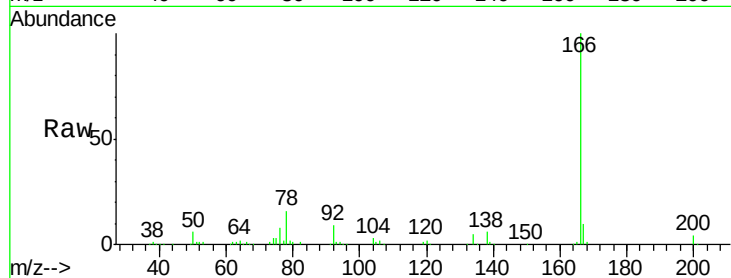

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 89.00 (88.70 to 89.70): BM0
 Ion 121.00 (120.70 to 121.70): E

