

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040716\
 Data File : BM004918.D
 Acq On : 07 Apr 2016 16:19
 Operator : UM/SJ
 Sample : H2275-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T74

Quant Time: Apr 08 00:59:50 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 00:57:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	39947	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	180774	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.46	164	111393	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.20	188	275221	20.00	ng/ul	0.00
78) Chrysene-d12	21.39	240	360127	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	355780	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	22913	23.21	ng/uL	-0.02
5) Phenol-d5	6.98	99	20501	5.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	57842	30.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	63154	23.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	41823	14.03	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	39056	30.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	43920	30.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	77542	29.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	5091	1.60	ng/ul	0.00
44) Dimethylphthalate-d6	13.86	166	317873	36.17	ng/ul	0.00
47) Acenaphthylene-d8	14.15	160	361894	34.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.65	143	9067	5.22	ng/ul	0.00
58) Fluorene-d10	15.45	176	274742	36.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	49438	29.98	ng/ul	0.00
71) Anthracene-d10	17.30	188	476754	38.71	ng/ul	0.00
79) Pyrene-d10	19.60	212	576286	36.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	601192	38.14	ng/ul	0.00


Target Compounds					Qvalue
46) 2,6-Dinitrotoluene	13.87	165	2100	1.21 ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040716\
Data File : BM004918.D
Acq On : 07 Apr 2016 16:19
Operator : UM/SJ
Sample : H2275-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T74

Quant Time: Apr 08 00:59:50 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 00:57:37 2016
Response via : Initial Calibration

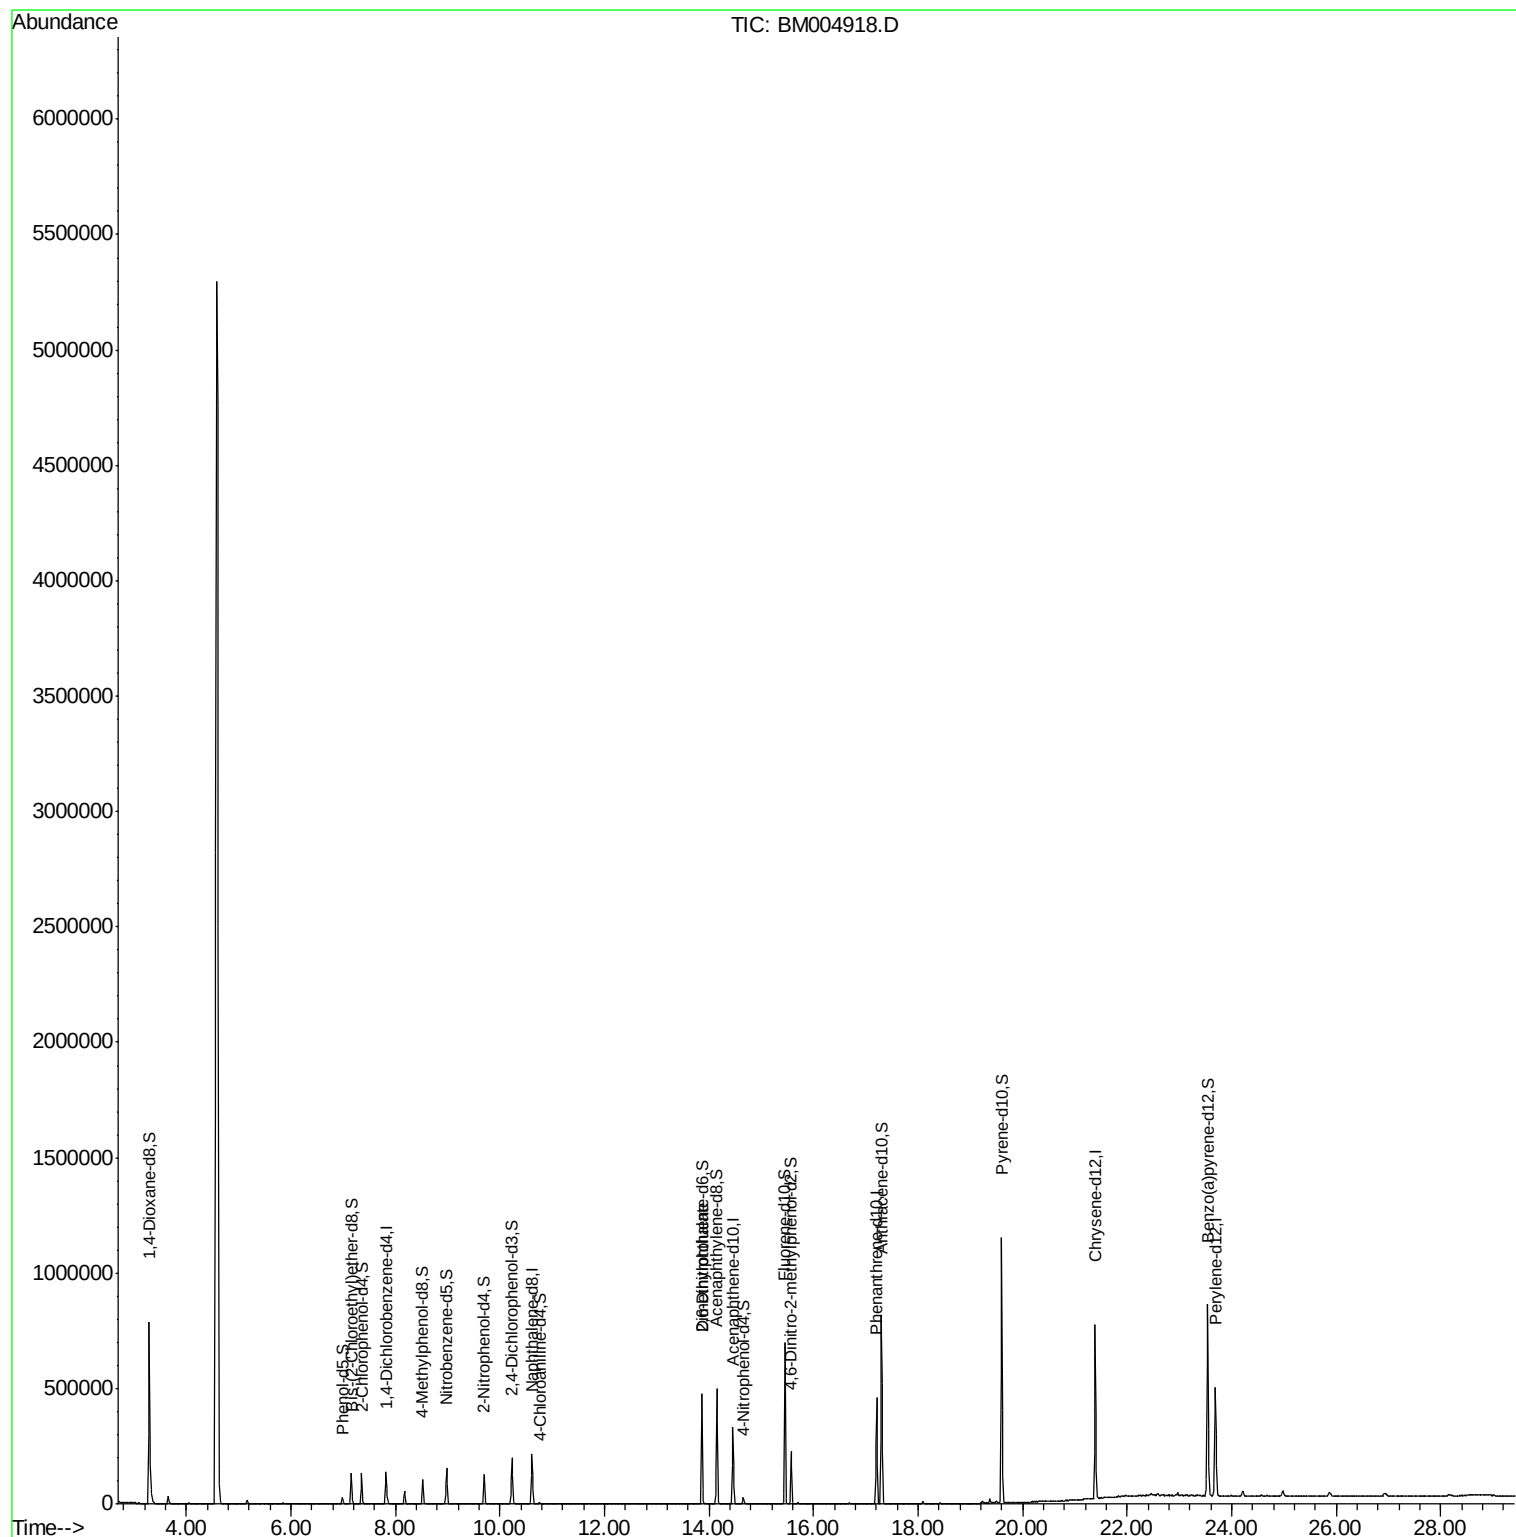

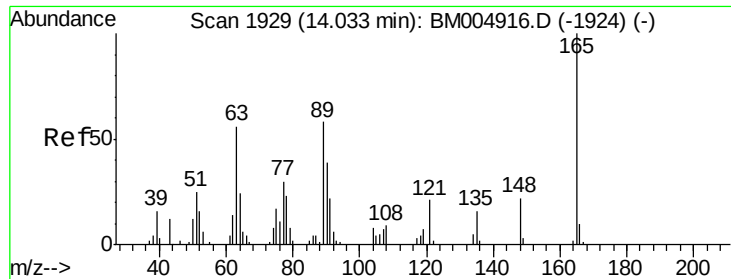

#46

2,6-Dinitrotoluene

Concen: 1.21 ng/ul

RT: 13.87 min Scan# 1901

Delta R.T. -0.16 min

Lab File: BM004918.D


Acq: 07 Apr 2016 16:19

Instrument :

BNA_M

ClientSampleId :

D9T74

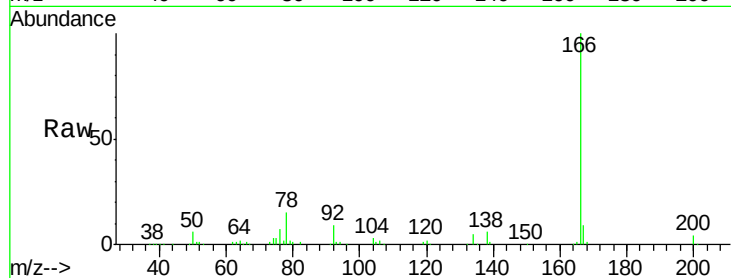

Tgt Ion:	165	Resp:	2100
Ion Ratio	Lower	Upper	
165	100		
89	0.0	42.4	63.6#
121	30.1	16.6	24.8#

