

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040716\
 Data File : BM004919.D
 Acq On : 07 Apr 2016 16:56
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.563	314	319	328	rBV	66704	104438	6.39%	0.888%
2	6.987	725	731	739	rBB	22989	36536	2.24%	0.311%
3	7.151	754	759	769	rBB	110918	172667	10.57%	1.468%
4	7.351	788	793	801	rBV	109718	170187	10.42%	1.447%
5	7.822	867	873	881	rBB	136754	211016	12.92%	1.794%
6	8.516	986	991	1001	rBB	82541	128255	7.85%	1.090%
7	8.975	1063	1069	1079	rBB	134785	221105	13.53%	1.879%
8	9.692	1185	1191	1200	rVB	107555	176939	10.83%	1.504%
9	10.228	1276	1282	1298	rBB	156382	262917	16.09%	2.235%
10	10.610	1340	1347	1359	rVB	210561	343384	21.02%	2.919%
11	13.863	1894	1900	1909	rVB	415323	560098	34.28%	4.761%
12	14.151	1942	1949	1962	rBV	421692	636013	38.93%	5.406%
13	14.457	1995	2001	2009	rVB2	335608	504419	30.87%	4.287%
14	14.651	2030	2034	2045	rVB	19423	32489	1.99%	0.276%
15	15.451	2164	2170	2177	rVB	642160	912369	55.84%	7.755%
16	15.568	2184	2190	2196	rBV	212283	279190	17.09%	2.373%
17	17.204	2462	2468	2474	rBV	468779	669544	40.98%	5.691%
18	17.298	2478	2484	2502	rVB2	761296	1142974	69.96%	9.715%
19	19.598	2869	2875	2887	rBV	1053155	1471601	90.07%	12.508%
20	21.392	3174	3180	3190	rBV	769006	1000946	61.26%	8.508%
21	22.968	3444	3448	3455	rVB3	12371	23829	1.46%	0.203%
22	23.538	3537	3545	3555	rBV2	852219	1633849	100.00%	13.887%
23	23.686	3562	3570	3579	rVB	498708	987005	60.41%	8.389%
24	24.209	3655	3659	3668	rVB3	20137	38167	2.34%	0.324%
25	24.980	3785	3790	3800	rVB2	20724	45285	2.77%	0.385%


Sum of corrected areas: 11765222

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040716\
Data File : BM004919.D
Acq On : 07 Apr 2016 16:56
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

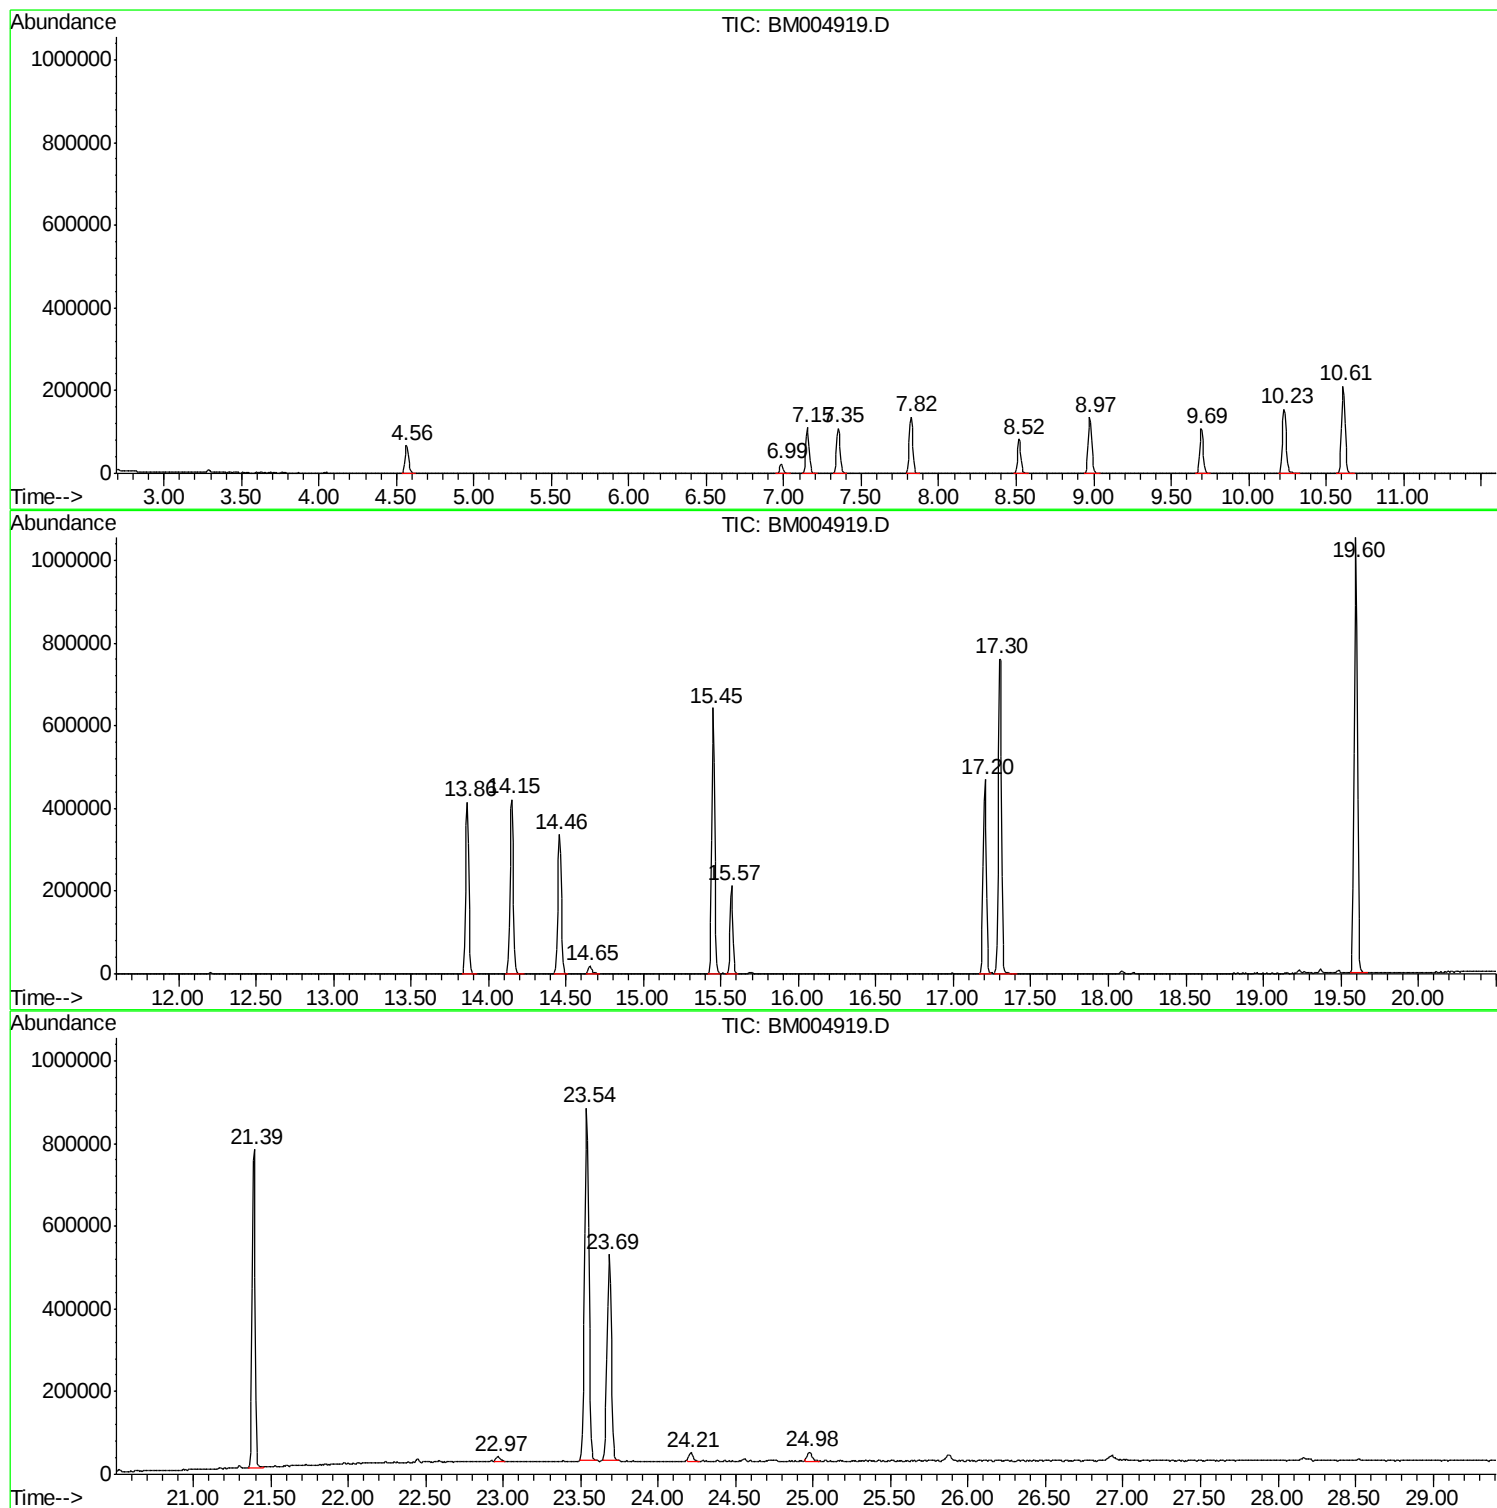

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040716\
Data File : BM004919.D
Acq On : 07 Apr 2016 16:56
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040716\
Data File : BM004919.D
Acq On : 07 Apr 2016 16:56
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc