


Data Path : Z:\HPCHEM1\BNA_M\Data\BM040717\
Data File : BM009594.D
Acq On : 06 Apr 2017 15:23
Operator : SJ/MA
Sample : I2526-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 06 17:51:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040417-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 06 10:55:00 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampled :
CB396

Manual Integrations
APPROVED

mohammad
4/7/2017 2:10:07 PM

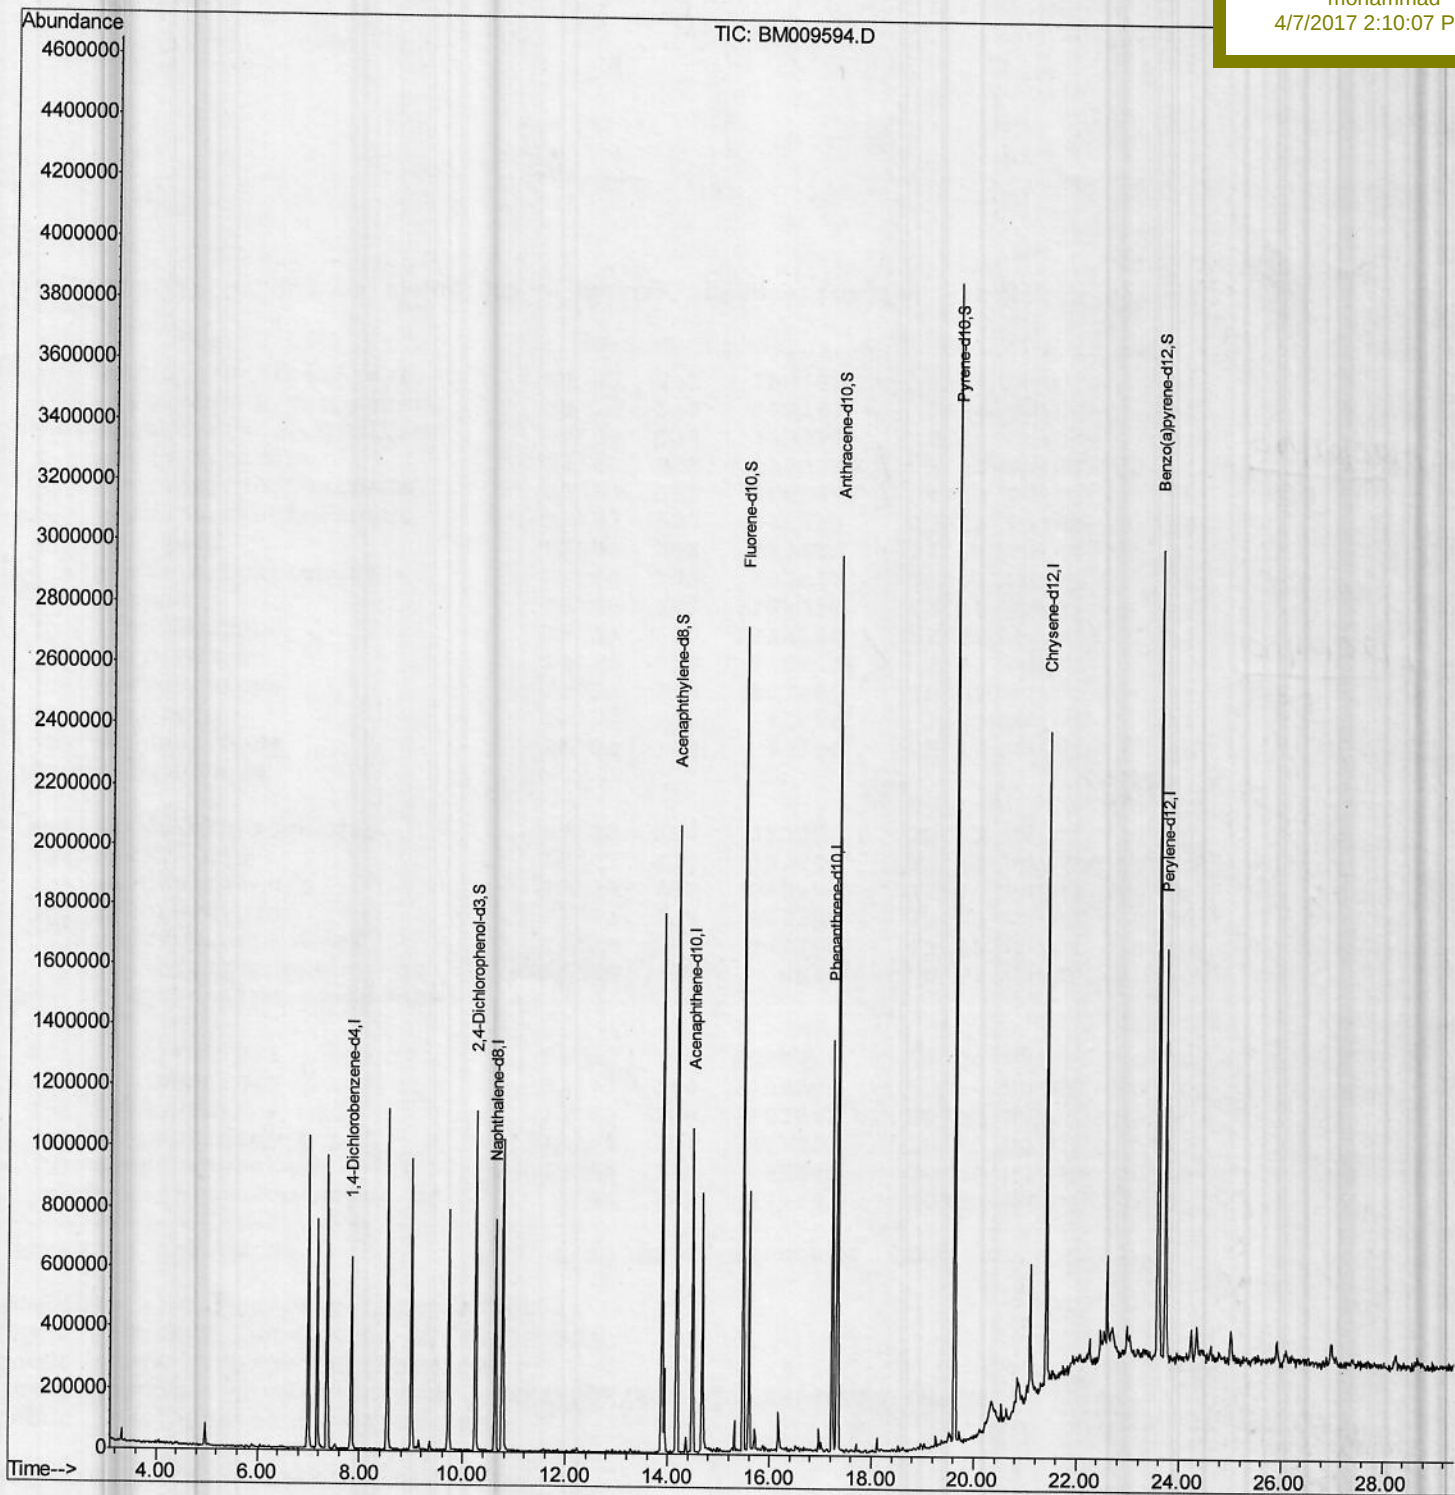

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM040717\
 Data File : BM009594.D
 Acq On : 06 Apr 2017 15:23
 Operator : SJ/MA
 Sample : I2526-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 06 17:34:56 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 10:55:00 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 CB396

Manual Integrations
 APPROVED

mohammad
 4/7/2017 2:10:07 PM

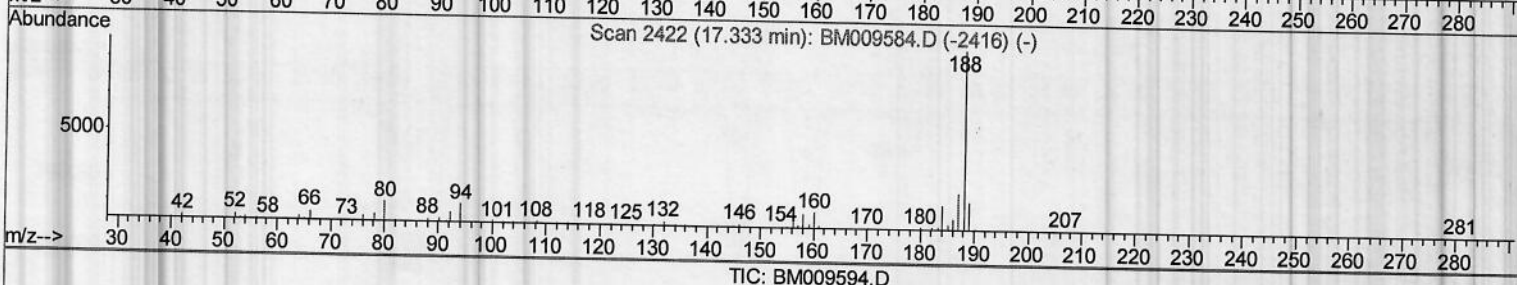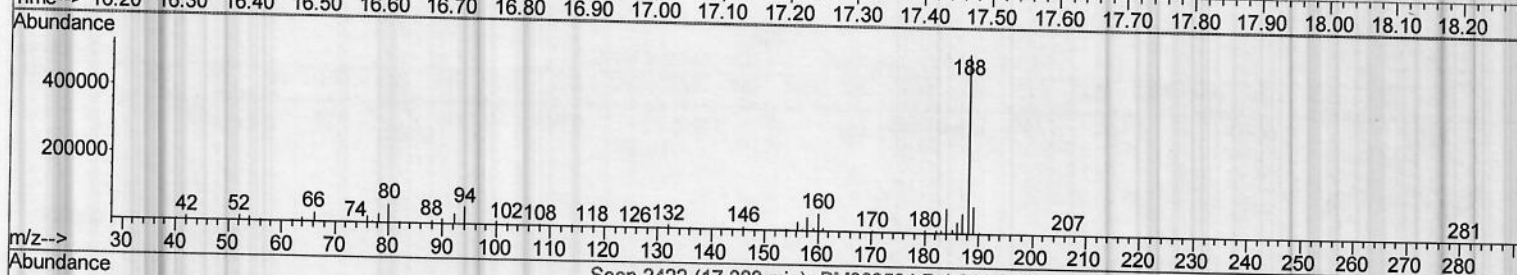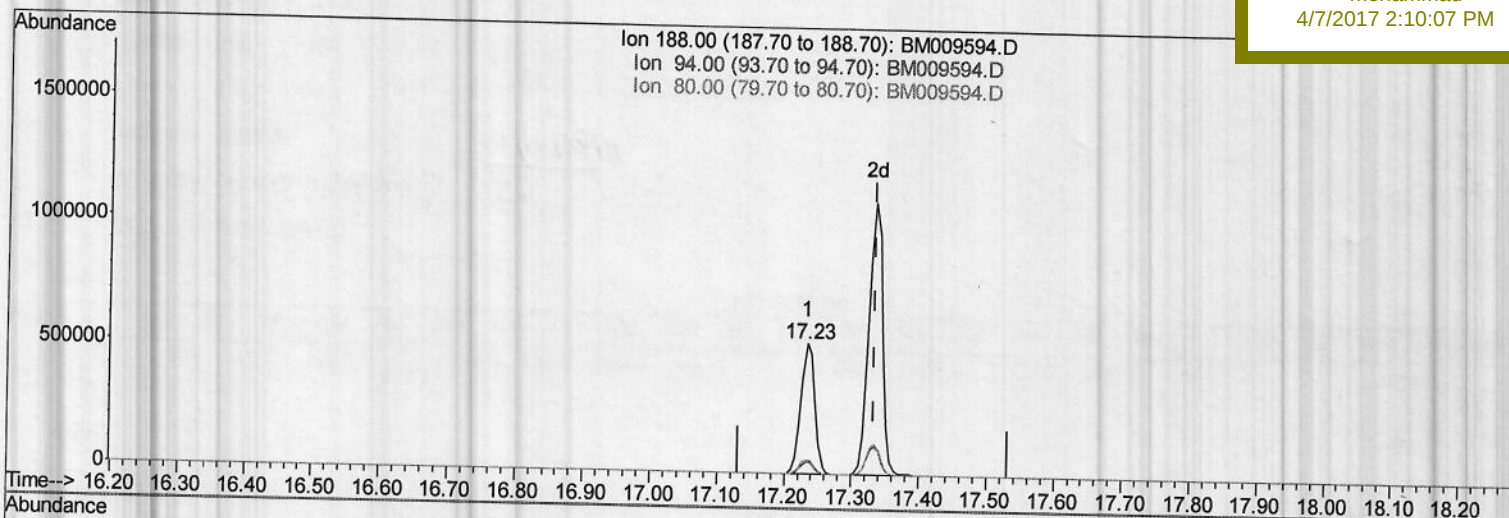

(15) Anthracene-d10 (S)
 17.233min (-0.100) 20.90ng/ul
 response 753184

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.55
80.00	9.10	10.55
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM040717\
Data File : BM009594.D
Acq On : 06 Apr 2017 15:23
Operator : SJ/MA
Sample : I2526-16
Misc :
ALS Vial : 12 Sample Multiplier: 1




Quant Time: Apr 06 17:34:56 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040417-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 06 10:55:00 2017
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB396

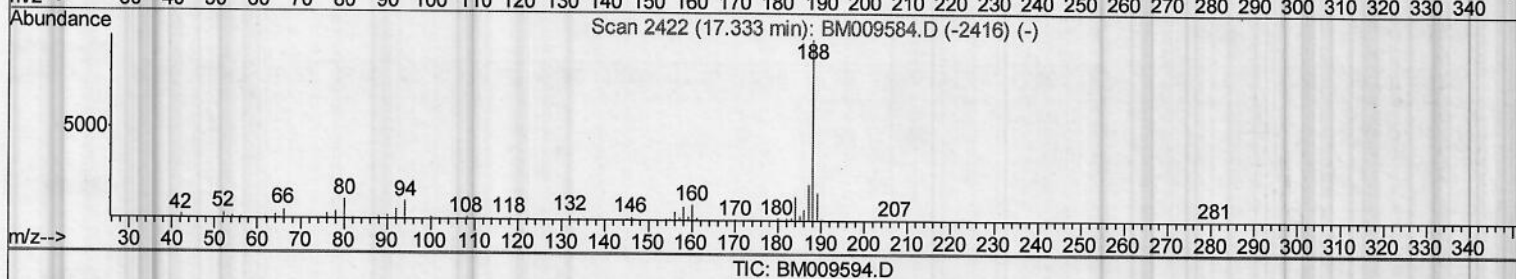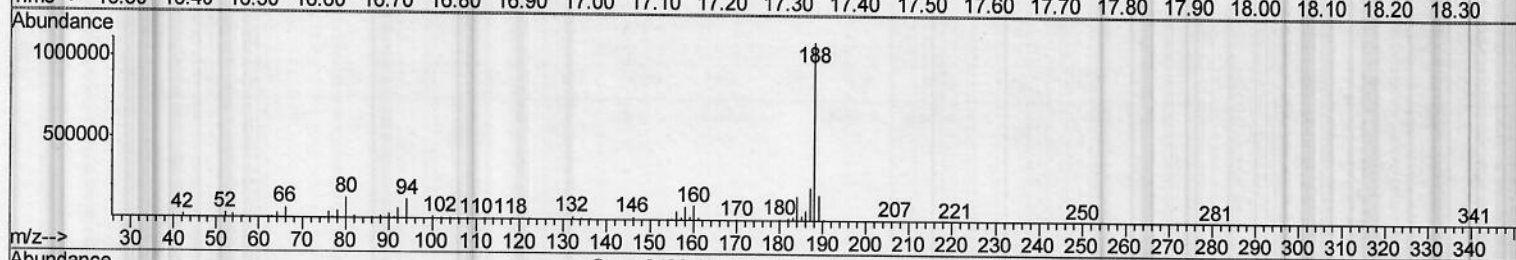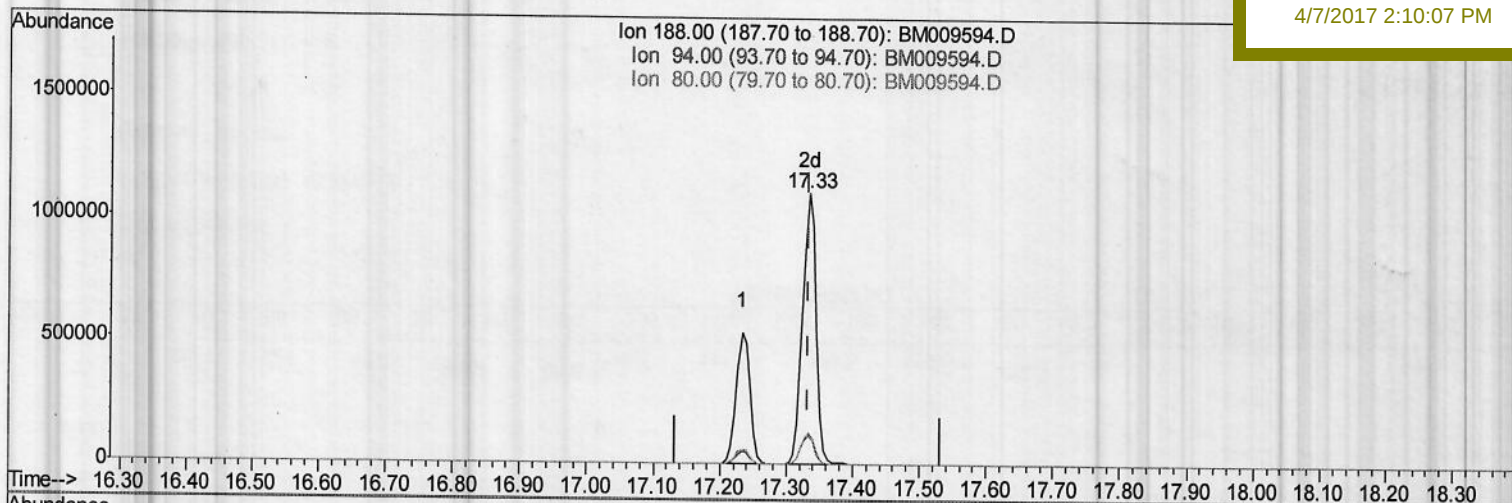Manual Integrations
APPROVEDmohammad
4/7/2017 2:10:07 PM

(15) Anthracene-d10 (S)

17.333min (+0.000) 43.16ng/ul m

response 1555185

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.67
80.00	9.10	11.47#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM040717\
 Data File : BM009594.D
 Acq On : 06 Apr 2017 15:23
 Operator : SJ/MA
 Sample : I2526-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 06 17:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 10:55:00 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 CB396

Manual Integrations
 APPROVED

mohammad
 4/7/2017 2:10:07 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	143524	20.00	ng/ul	0.00
2) Naphthalene-d8	10.64	136	564678	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.49	164	319016	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.23	188	753184	20.00	ng/ul	0.00
18) Chrysene-d12	21.42	240	990200	20.00	ng/ul	0.00
23) Perylene-d12	23.74	264	961001	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.25	165	343225	39.53	ng/uL	0.00
7) Acenaphthylene-d8	14.18	160	1357441	43.42	ng/ul	0.00
10) Fluorene-d10	15.48	176	951007	42.29	ng/ul	0.00
15) Anthracene-d10	17.33	188	1555185m	43.16	ng/ul	0.00
19) Pyrene-d10	19.63	212	1817950	44.68	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.59	264	1896629	44.70	ng/ul	0.00

ST
 04/10/2017

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed