

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040717\
 Data File : BM009605.D
 Acq On : 06 Apr 2017 21:59
 Operator : SJ/MA
 Sample : I2525-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB344

Manual Integrations
 APPROVED

mohammad
 4/7/2017 2:10:20 PM

Quant Time: Apr 07 03:38:18 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 03:19:28 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	149025	20.00	ng/ul	0.00
2) Naphthalene-d8	10.63	136	582503	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.49	164	327013	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.23	188	771021	20.00	ng/ul	0.00
18) Chrysene-d12	21.42	240	1032745	20.00	ng/ul	0.00
23) Perylene-d12	23.74	264	1009592	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.26	165	152662	17.04	ng/uL	0.00
7) Acenaphthylene-d8	14.18	160	1062337	33.15	ng/ul	0.00
10) Fluorene-d10	15.48	176	761391	33.03	ng/ul	0.00
15) Anthracene-d10	17.33	188	1198065m	32.48	ng/ul	0.00
19) Pyrene-d10	19.63	212	1471615	34.67	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.59	264	1510884	33.90	ng/ul	0.00
Target Compounds				Qvalue		
8) Acenaphthylene	14.20	152	80115	2.49	ng/ul#	90
14) Phenanthrene	17.27	178	375886	8.67	ng/ul	97
16) Anthracene	17.37	178	98451	2.20	ng/ul	99
17) Fluoranthene	19.29	202	882403	16.35	ng/ul	97
20) Pyrene	19.66	202	862036	15.33	ng/ul	95
21) Benzo(a)anthracene	21.40	228	576320	9.87	ng/ul	99
22) Chrysene	21.45	228	571862	10.68	ng/ul	96
24) Benzo(b)fluoranthene	23.04	252	965928	15.47	ng/ul#	93
25) Benzo(k)fluoranthene	23.07	252	281275m	4.73	ng/ul	
27) Benzo(a)pyrene	23.64	252	660285	11.12	ng/ul	98
28) Indeno(1,2,3-cd)pyrene	26.10	276	548243	8.24	ng/ul	95
29) Dibenzo(a,h)anthracene	26.10	278	141416	2.50	ng/ul	95
30) Benzo(a,h,i)perylene	26.83	276	507904	9.26	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM040717\
Data File : BM009605.D
Acq On : 06 Apr 2017 21:59
Operator : SJ/MA
Sample : I2525-01
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
CB344

Manual Integrations
APPROVED

mohammad
4/7/2017 2:10:20 PM

Quant Time: Apr 07 03:38:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 03:19:28 2017
Response via : Initial Calibration

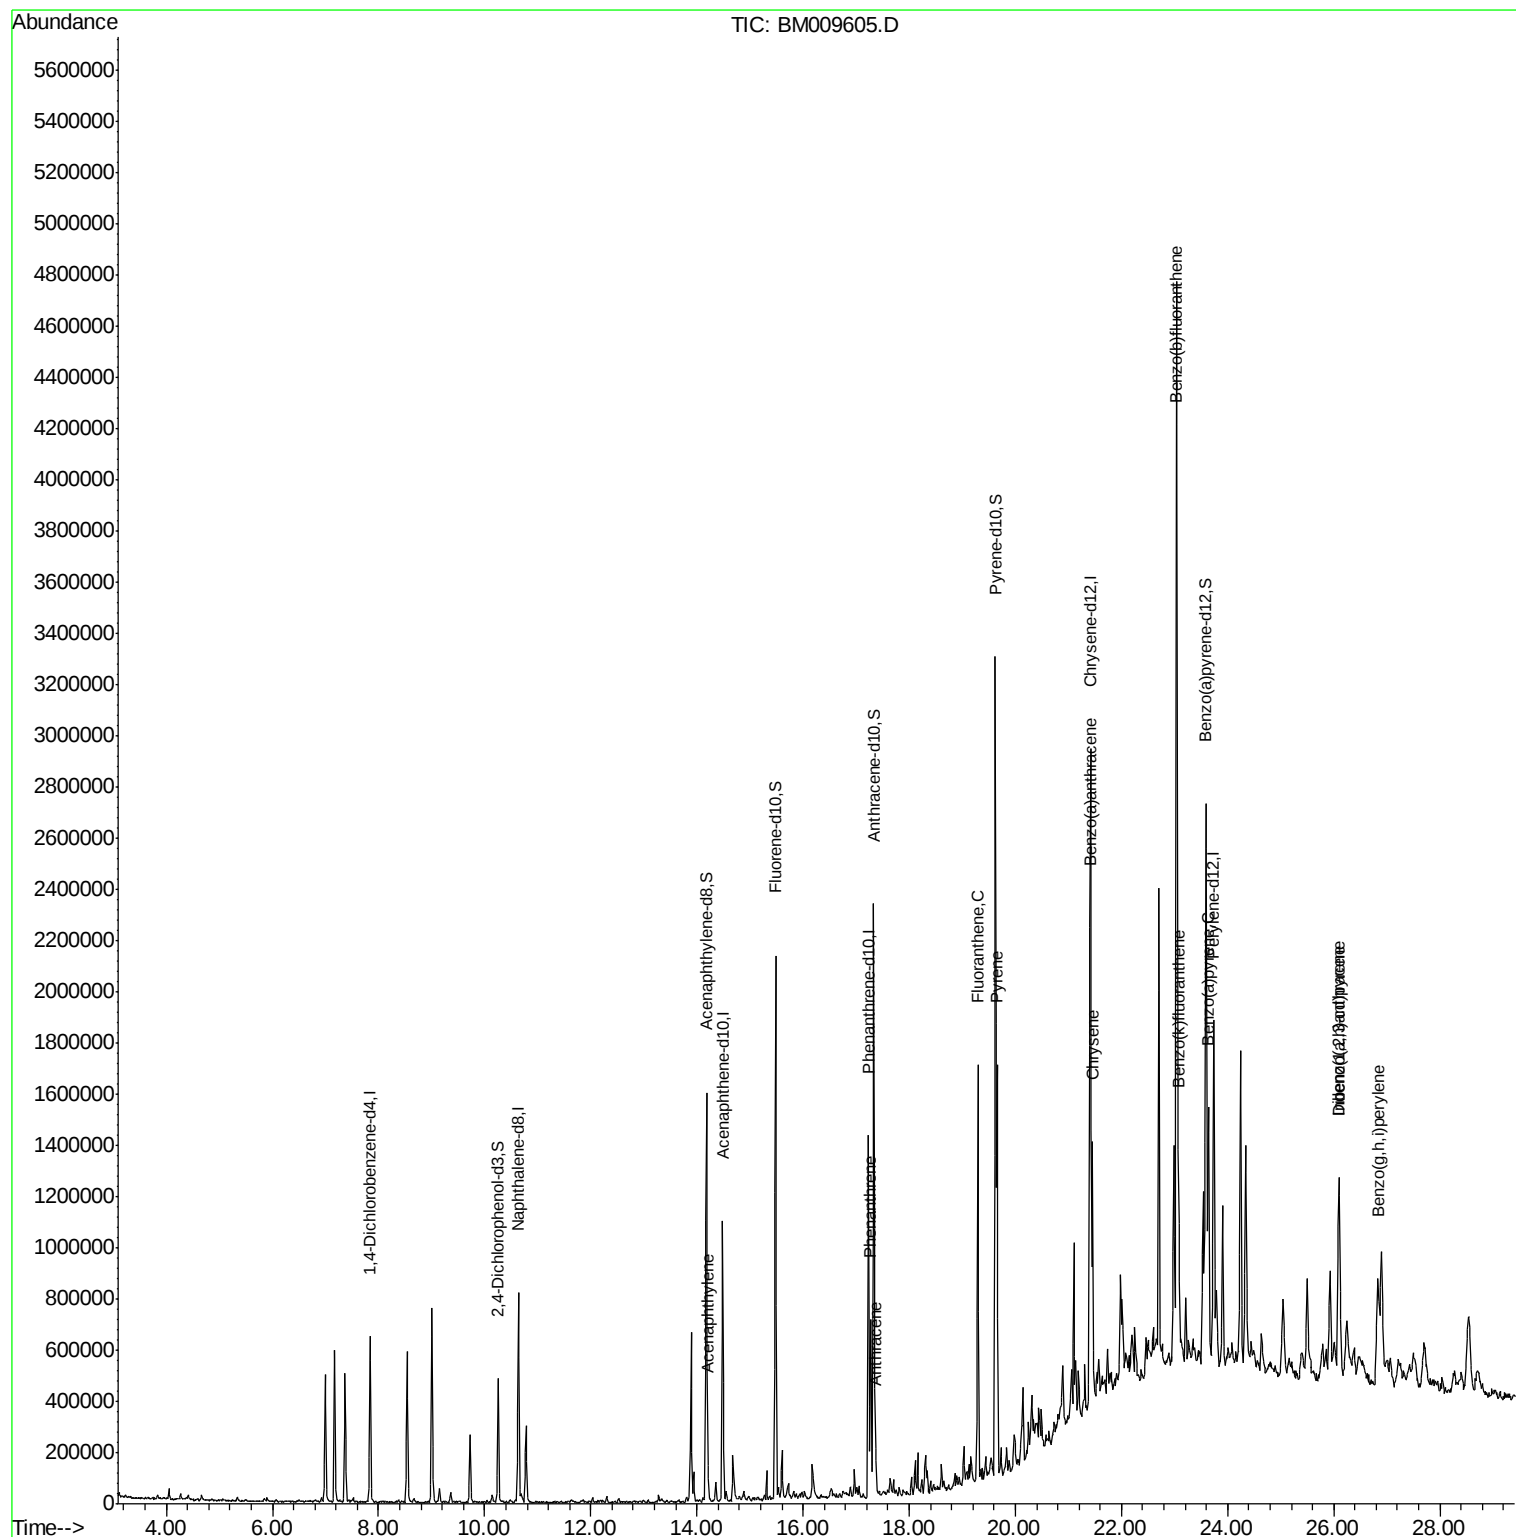

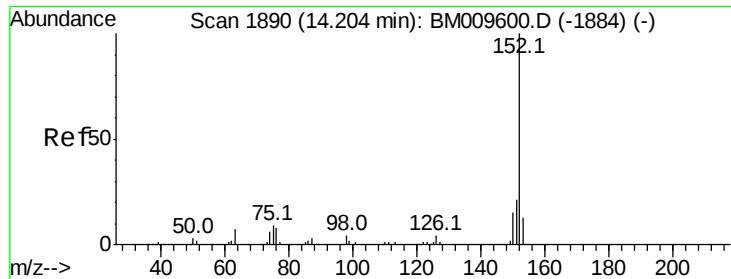

#8

Acenaphthylene

Concen: 2.49 ng/ul

RT: 14.20 min Scan# 1890

Delta R.T. 0.00 min

Lab File: BM009605.D

Acq: 06 Apr 2017 21:59

Instrument :

BNA_M


ClientSampleId :

CB344




Tot Ion:	152	Resp:	80115
Ion Ratio	Lower	Upper	
152	100		
151	14.5	17.5	26.3#
153	14.1	10.6	16.0

Manual Integrations
APPROVED

mohammad
4/7/2017 2:10:20 PM

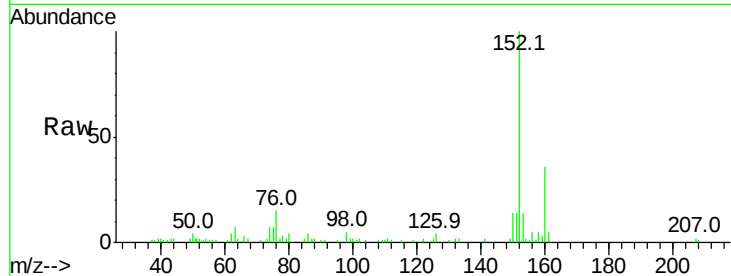

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

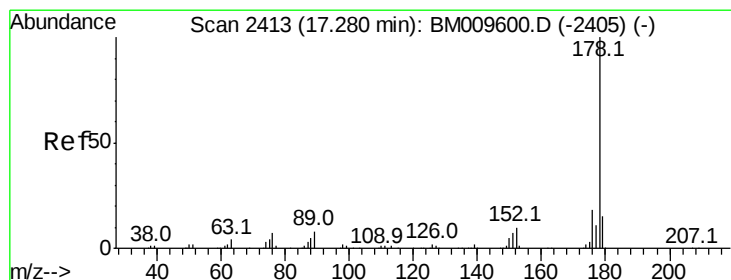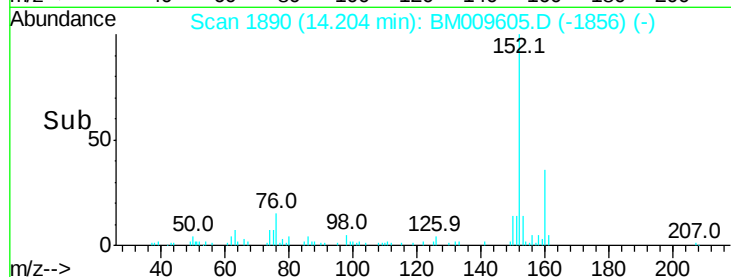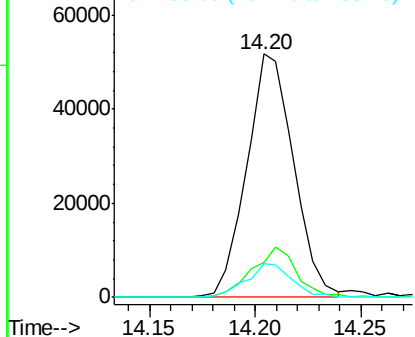

#14

Phenanthrene

Concen: 8.67 ng/ul


RT: 17.27 min Scan# 2412

Delta R.T. -0.01 min



Lab File: BM009605.D


Acq: 06 Apr 2017 21:59

Tgt Ion:	178	Resp:	375886
Ion Ratio	Lower	Upper	
178	100		
179	14.9	12.2	18.4
176	18.6	16.4	24.6

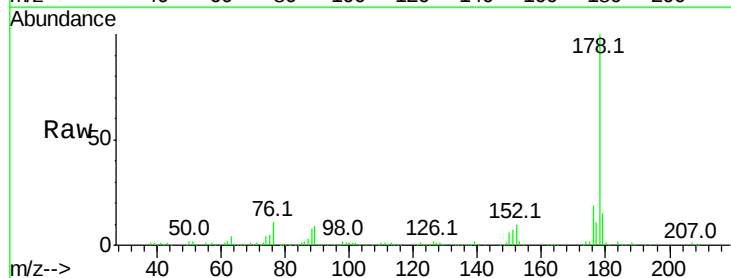

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

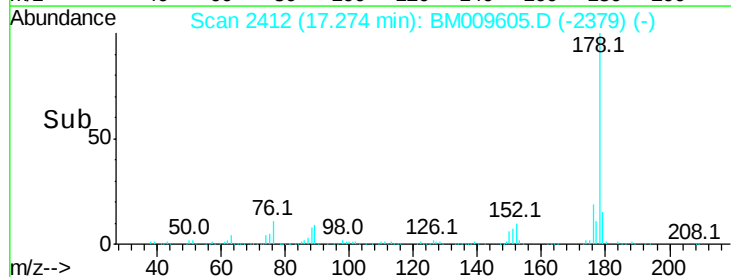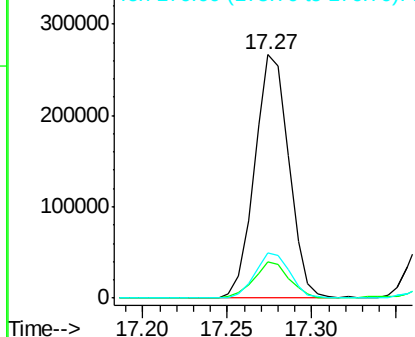

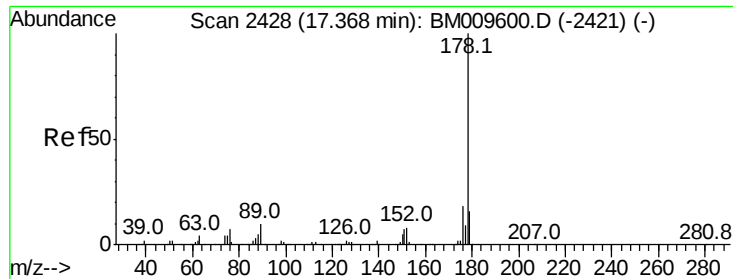





#16
 Anthracene
 Concen: 2.20 ng/ul
 RT: 17.37 min Scan# 2428
 Delta R.T. 0.00 min
 Lab File: BM009605.D
 Acq: 06 Apr 2017 21:59

Instrument :
 BNA_M
 ClientSampleId :
 CB344

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.8	12.7	19.1
176	19.9	15.8	23.8




Manual Integrations
 APPROVED


mohammad
 4/7/2017 2:10:20 PM

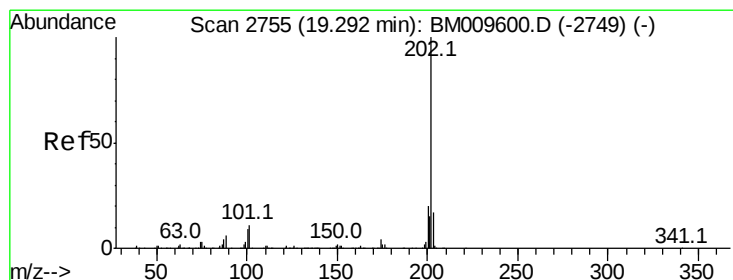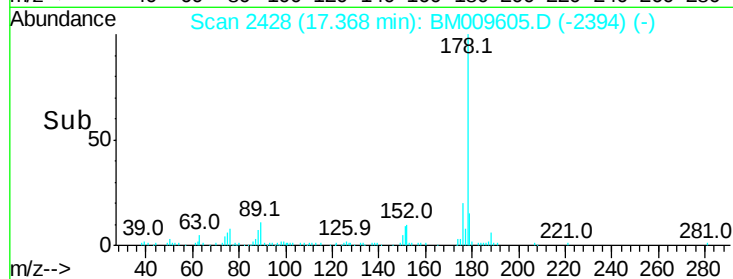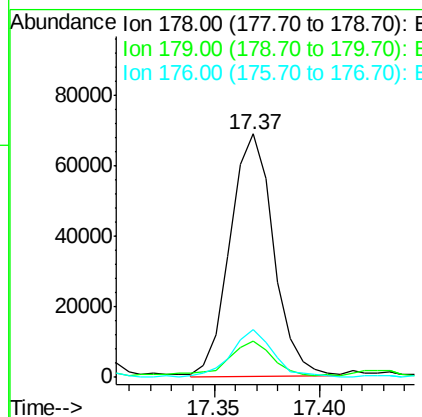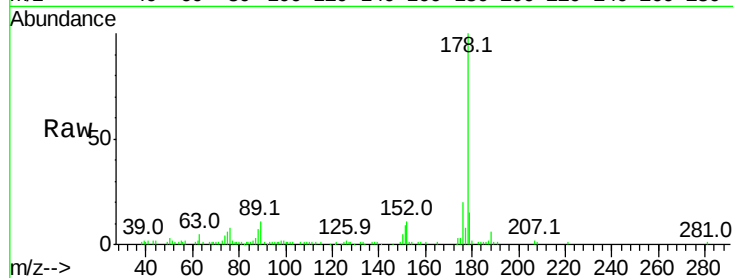

#17
 Fluoranthene
 Concen: 16.35 ng/ul
 RT: 19.29 min Scan# 2755
 Delta R.T. 0.00 min
 Lab File: BM009605.D
 Acq: 06 Apr 2017 21:59

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.4	9.8	14.8
100	9.4	7.5	11.3

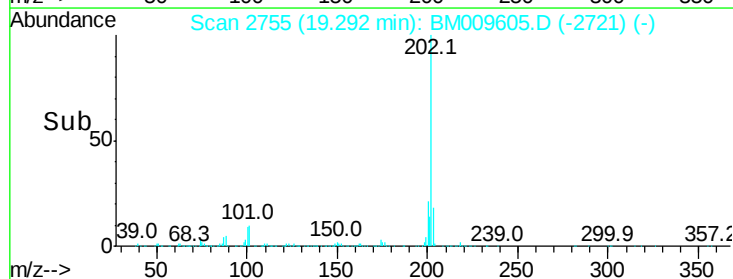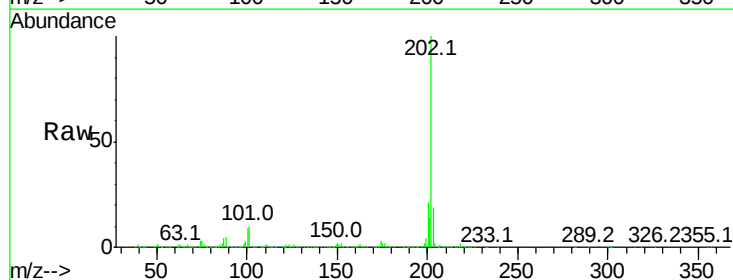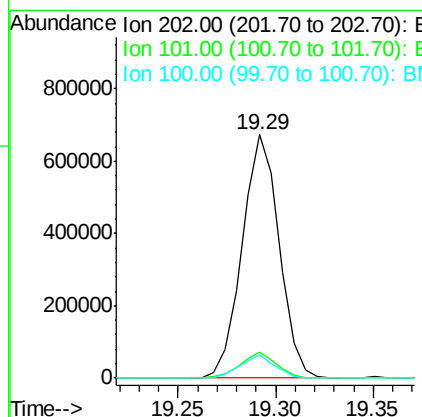

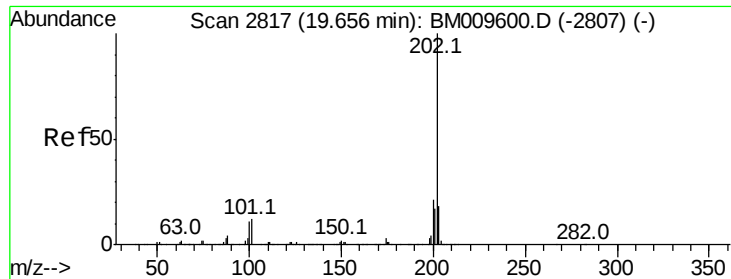





#20
Pvrene
Concen: 15.33 ng/ul
RT: 19.66 min Scan# 2817
Delta R.T. 0.00 min
Lab File: BM009605.D
Acq: 06 Apr 2017 21:59

Instrument :
BNA_M
ClientSampleId :
CB344

Tot Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	12.3	11.2	16.8
100	10.1	9.8	14.6




Manual Integrations
APPROVED


mohammad
4/7/2017 2:10:20 PM

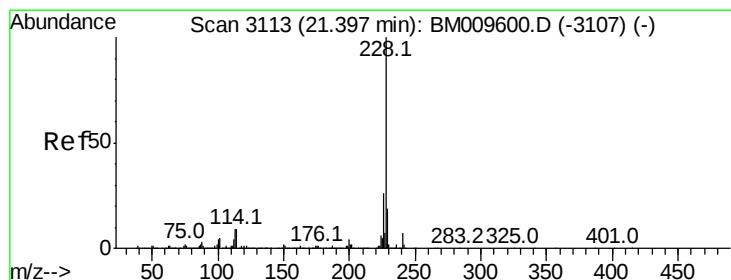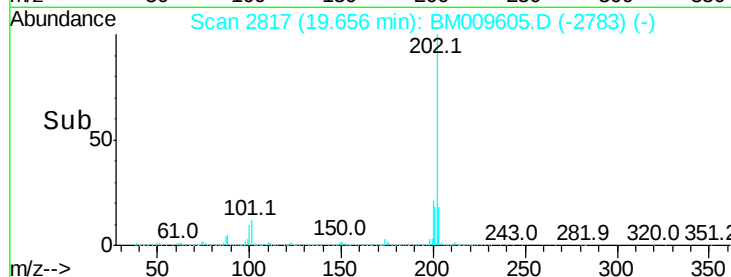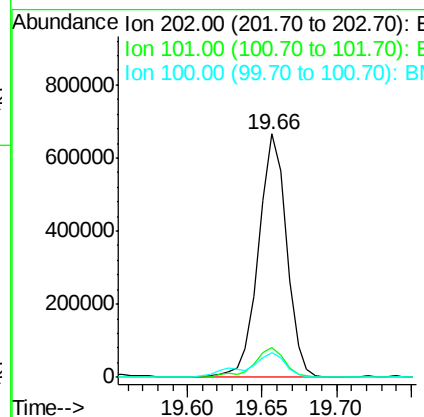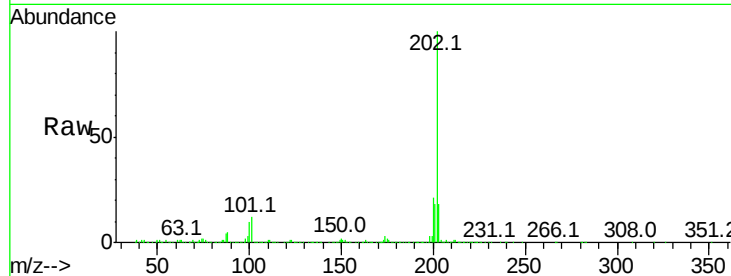

#21
Benzo(a)anthracene
Concen: 9.87 ng/ul
RT: 21.40 min Scan# 3113
Delta R.T. 0.00 min
Lab File: BM009605.D
Acq: 06 Apr 2017 21:59

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
229	20.6	15.9	23.9
226	27.0	22.1	33.1

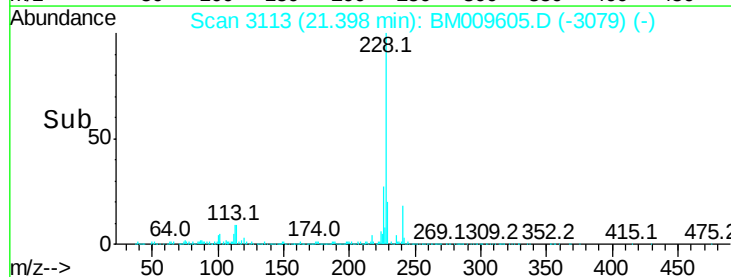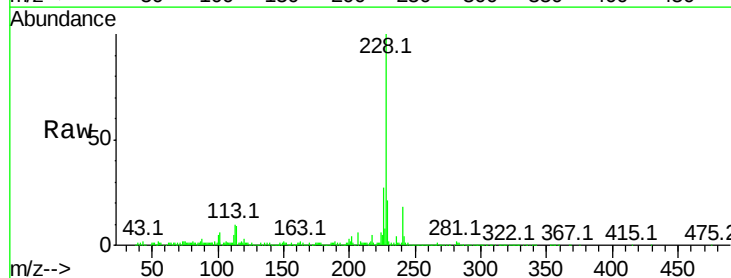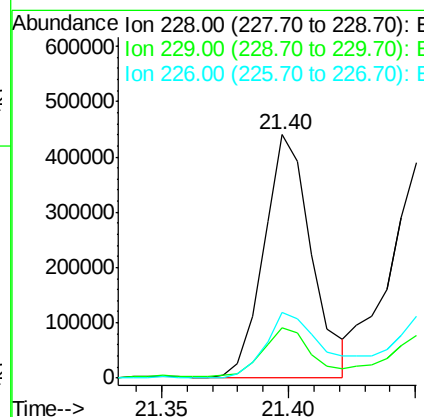

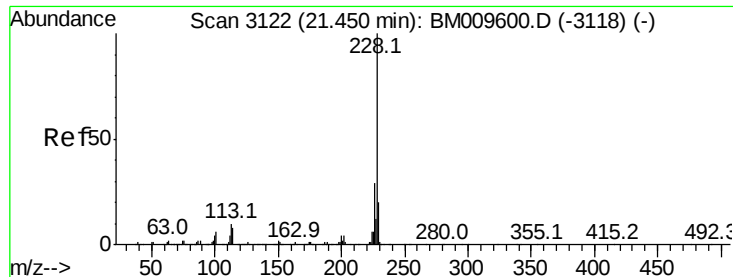

#22

Chrysene

Concen: 10.68 ng/ul

RT: 21.45 min Scan# 3122

Delta R.T. 0.00 min

Lab File: BM009605.D

Acq: 06 Apr 2017 21:59

Instrument :

BNA_M





ClientSampleID :

CB344

Tot Ion:	228	Resp:	571862
Ion Ratio	Lower	Upper	
228	100		
226	28.4	25.0	37.6
229	20.0	16.6	25.0

Manual Integrations
APPROVED

mohammad
4/7/2017 2:10:20 PM

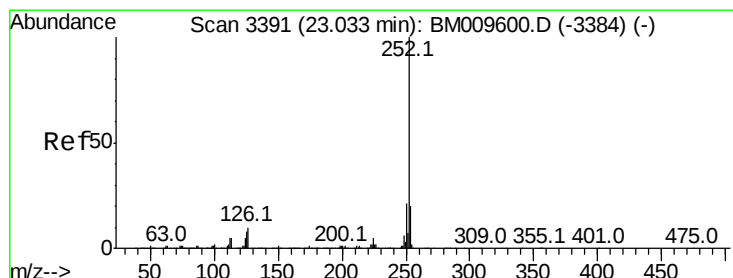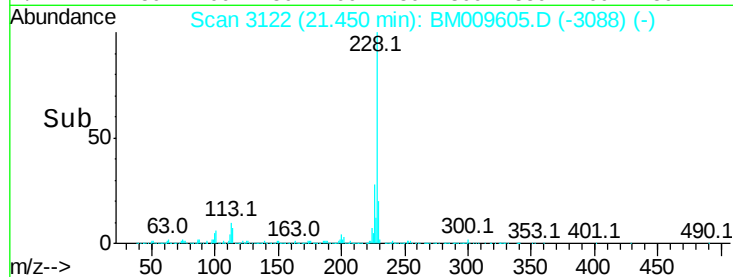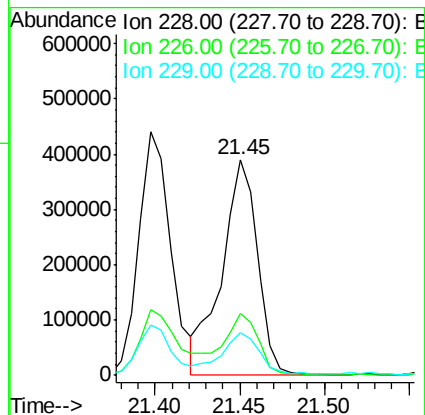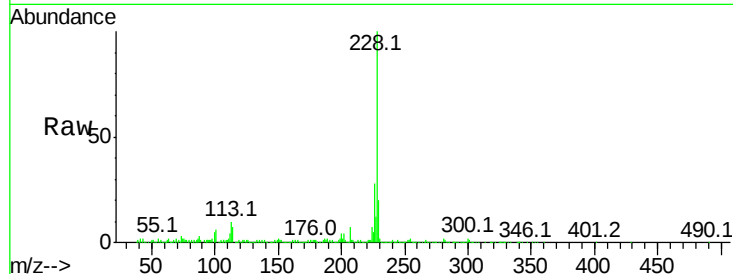

#24

Benzo(b)fluoranthene

Concen: 15.47 ng/ul




RT: 23.04 min Scan# 3392


Delta R.T. 0.01 min

Lab File: BM009605.D

Acq: 06 Apr 2017 21:59

Tgt Ion:	252	Resp:	965928
Ion Ratio	Lower	Upper	
252	100		
253	21.3	17.8	26.6
125	18.6	9.4	14.0#

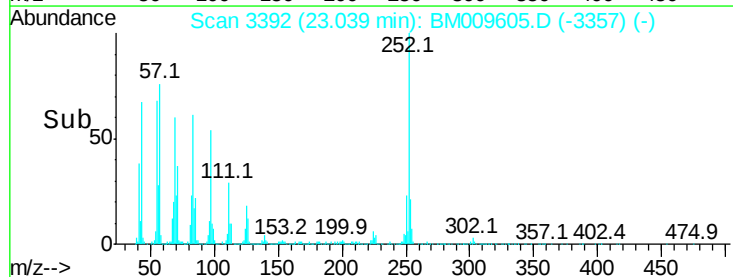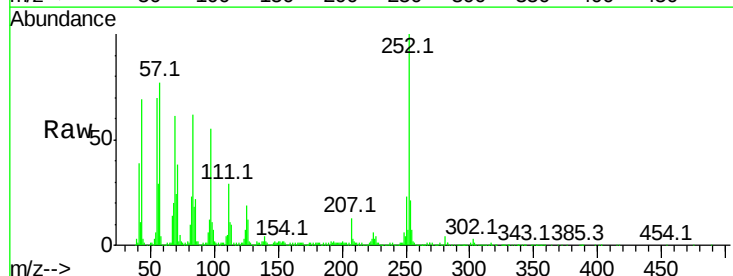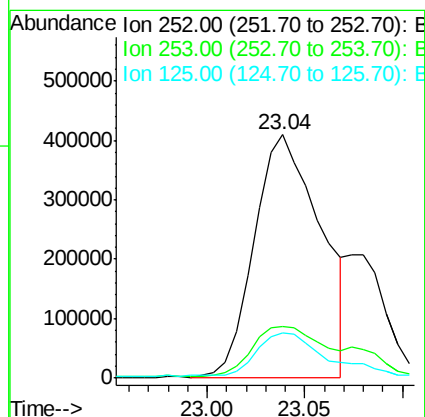

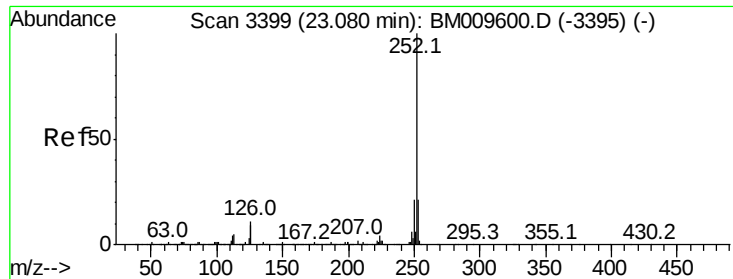





#25
Benzo(k)fluoranthene
Concen: 4.73 ng/ul m
RT: 23.07 min Scan# 3398
Delta R.T. -0.01 min
Lab File: BM009605.D
Acq: 06 Apr 2017 21:59

Instrument :
BNA_M
ClientSampleId :
CB344

Tot Ion	Ratio	Resp	Lower	Upper
252	100	281275		
253	24.8		17.4	26.2
125	12.0		8.8	13.2




Manual Integrations
APPROVED


mohammad
4/7/2017 2:10:20 PM

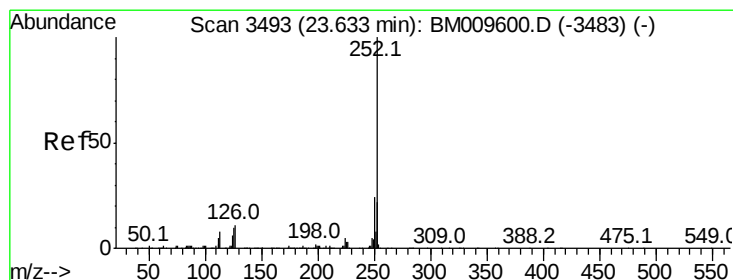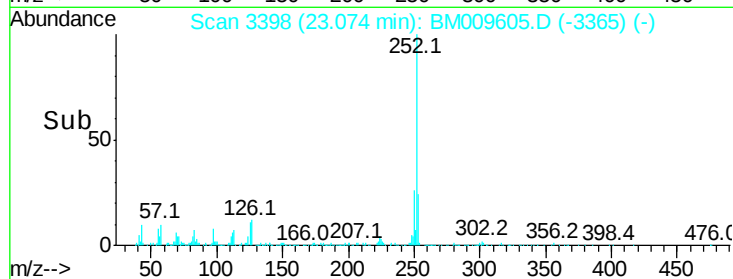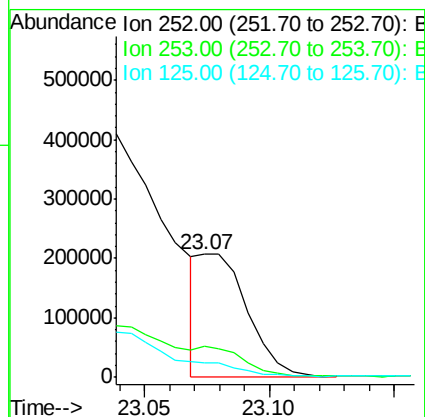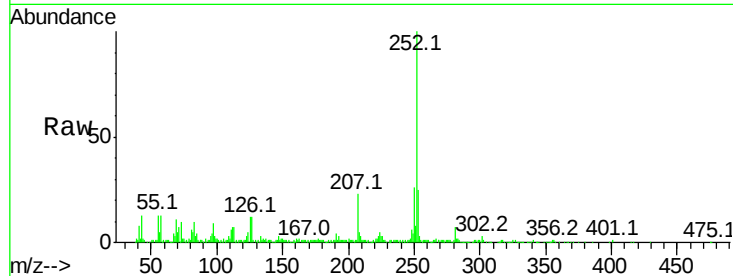

#27
Benzo(a)pyrene
Concen: 11.12 ng/ul
RT: 23.64 min Scan# 3494
Delta R.T. 0.01 min
Lab File: BM009605.D
Acq: 06 Apr 2017 21:59

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	660285		
253	21.6		17.1	25.7
125	10.0		9.4	14.2

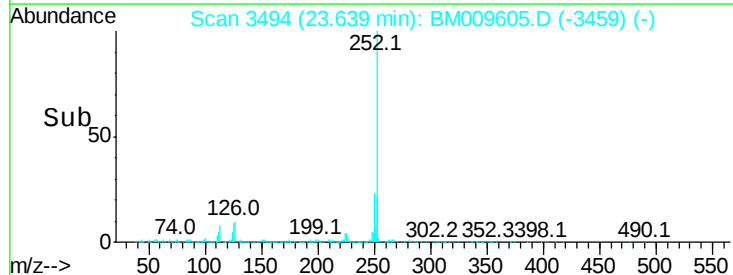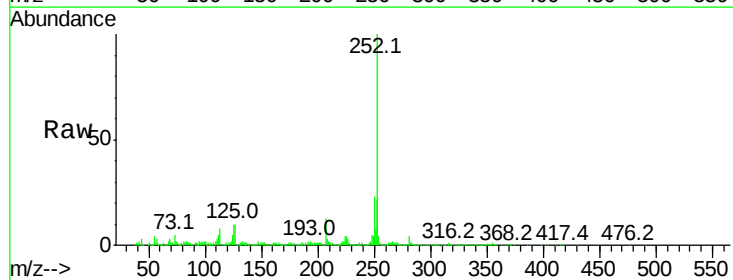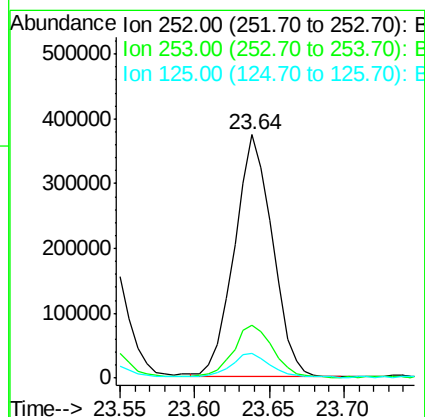

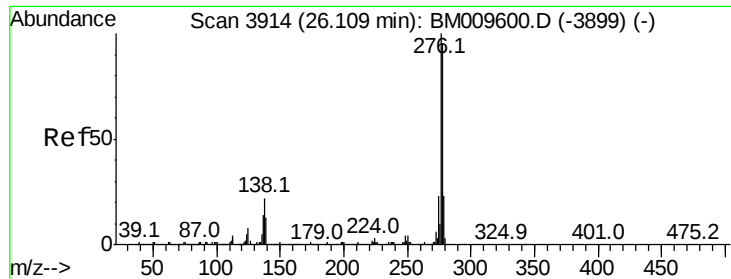





#28
 Indeno(1,2,3-cd)pyrene
 Concen: 8.24 ng/ul
 RT: 26.10 min Scan# 3913
 Delta R.T. -0.01 min
 Lab File: BM009605.D
 Acq: 06 Apr 2017 21:59

Instrument :
 BNA_M
 ClientSampleId :
 CB344

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.0	17.8	26.6
277	22.1	19.4	29.0




Manual Integrations
 APPROVED


mohammad
 4/7/2017 2:10:20 PM

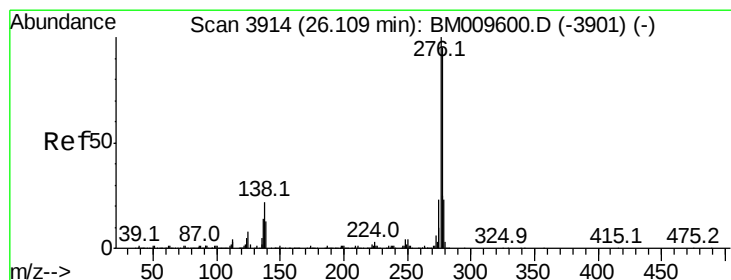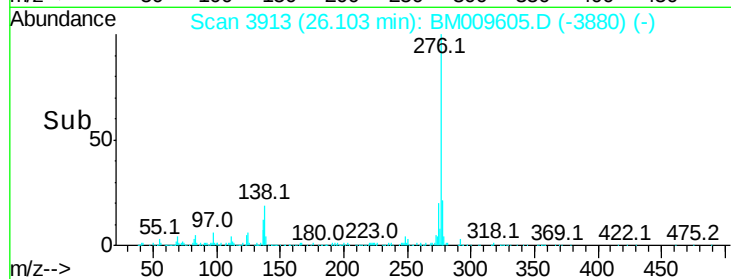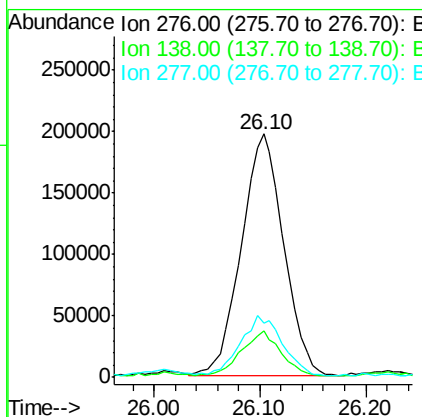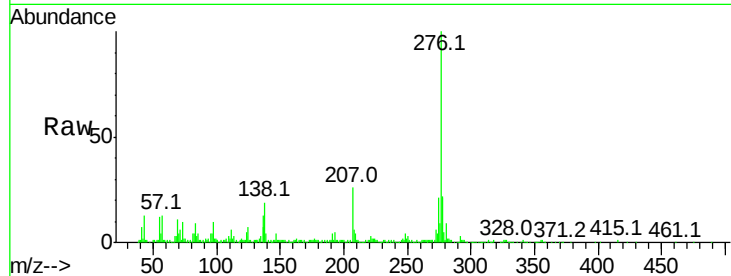

#29
 Dibenzo(a,h)anthracene
 Concen: 2.50 ng/ul
 RT: 26.10 min Scan# 3913
 Delta R.T. -0.01 min
 Lab File: BM009605.D
 Acq: 06 Apr 2017 21:59

Tgt Ion	Ratio	Lower	Upper
278	100		
139	20.5	14.0	21.0
279	24.1	20.6	31.0

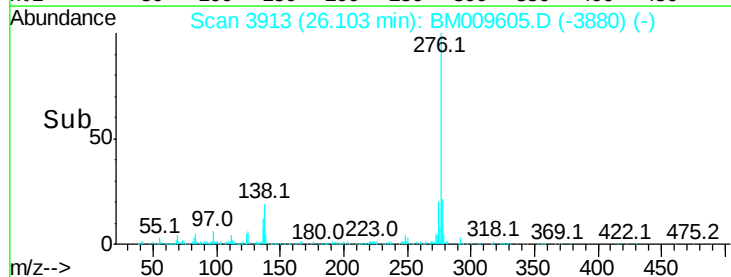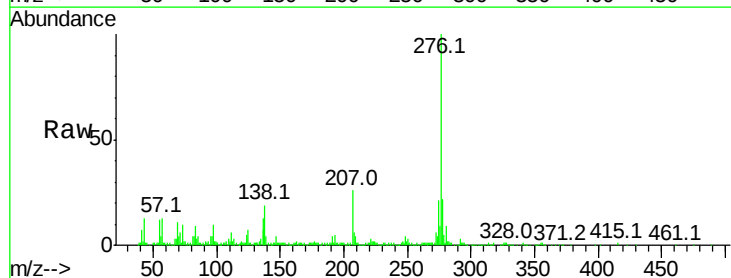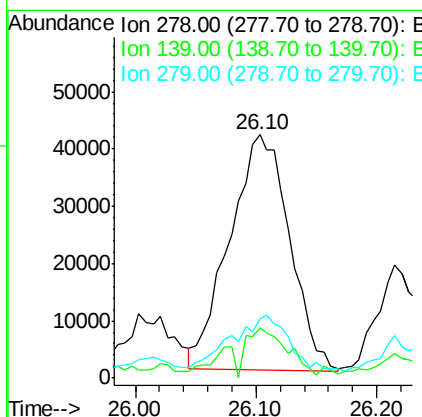

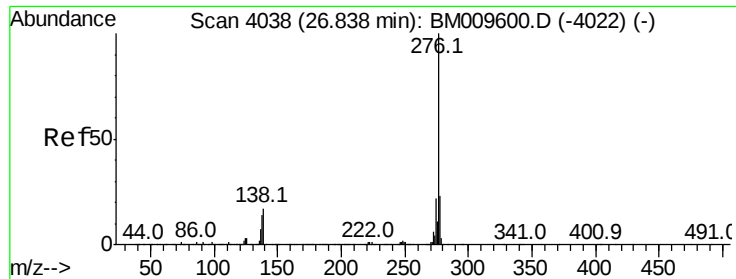

#30

Benzo(a,h,i)perylene

Concen: 9.26 ng/ul

RT: 26.83 min Scan# 4037

Delta R.T. -0.01 min

Lab File: BM009605.D

Acq: 06 Apr 2017 21:59

Instrument :

BNA_M

ClientSampleId :

CB344

Tot Ion:	276	Resp:	507904
Ion Ratio	Lower	Upper	
276	100		
138	17.5	19.0	28.4#
277	23.4	19.7	29.5

Manual Integrations
APPROVED

mohammad
4/7/2017 2:10:20 PM

