

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040721\
 Data File : BM029416.D
 Acq On : 08 Apr 2021 20:38
 Operator : CG/JU
 Sample : M1959-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B55

Quant Time: Apr 09 01:52:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 09 01:33:50 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	136835	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	546026	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	332391	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.06	188	636191	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	452275	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	386470	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
70) Phenanthrene	17.10	178	50423	1.377	ng/ul	96
77) Fluoranthene	19.12	202	73378	1.770	ng/ul	96
85) Chrysene	21.27	228	29110	1.044	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040721\
Data File : BM029416.D
Acq On : 08 Apr 2021 20:38
Operator : CG/JU
Sample : M1959-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B55

Quant Time: Apr 09 01:52:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 09 01:33:50 2021
Response via : Initial Calibration

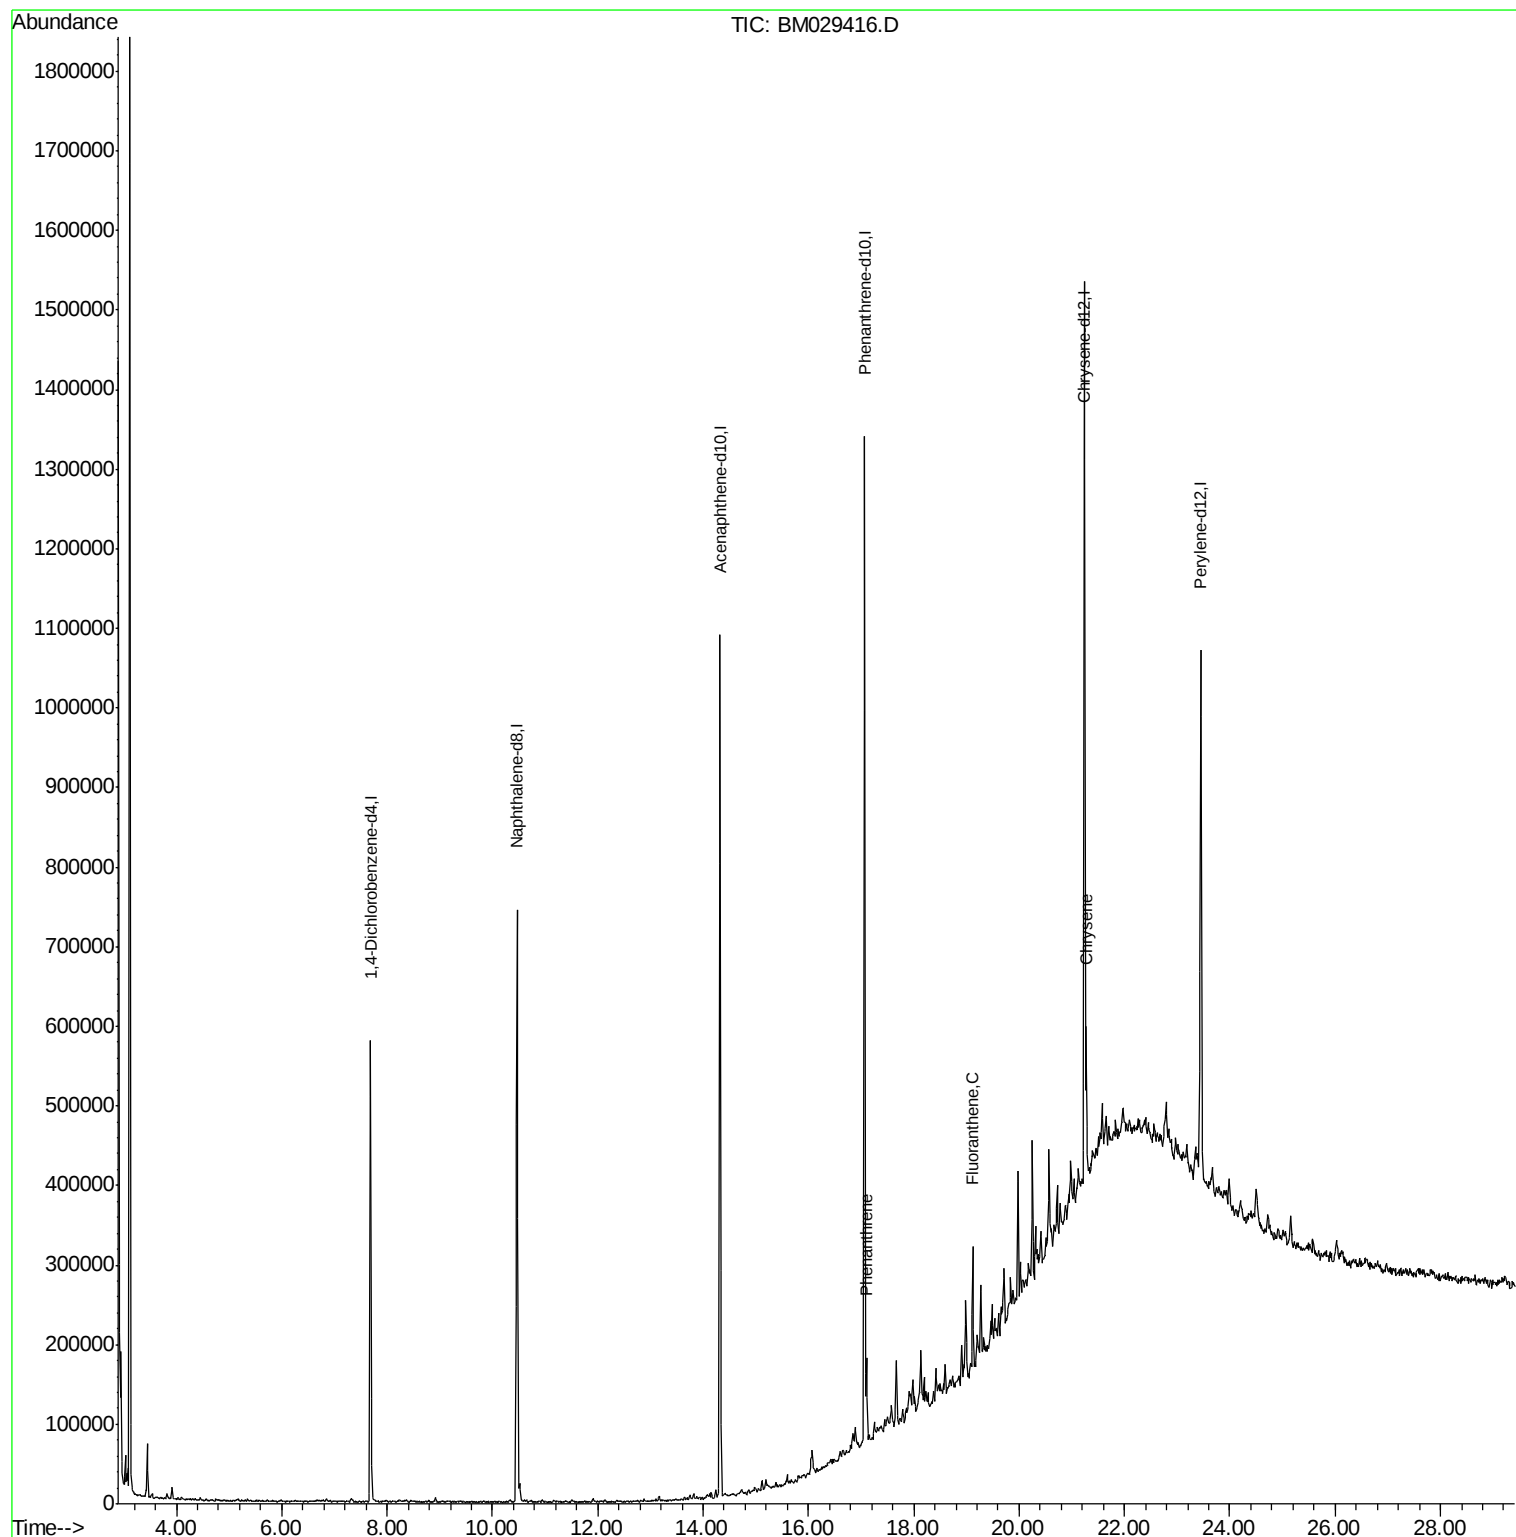


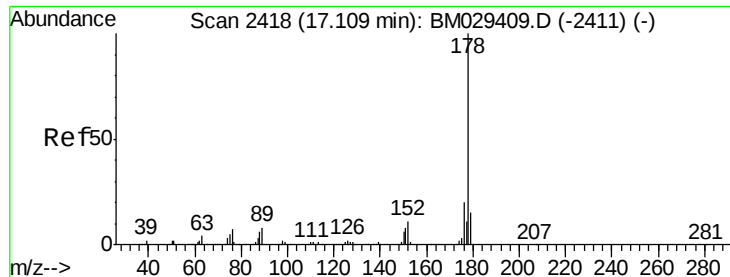




#70
Phenanthrene
Concen: 1.377 ng/ul
RT: 17.10 min Scan# 2417
Delta R.T. -0.01 min
Lab File: BM029416.D
Acq: 08 Apr 2021 20:38

Instrument :
BNA_M
ClientSampleId :
C0B55

Tot Ion:178 Resp: 50423
Ion Ratio Lower Upper
178 100
179 16.4 12.2 18.2
176 21.8 15.4 23.2

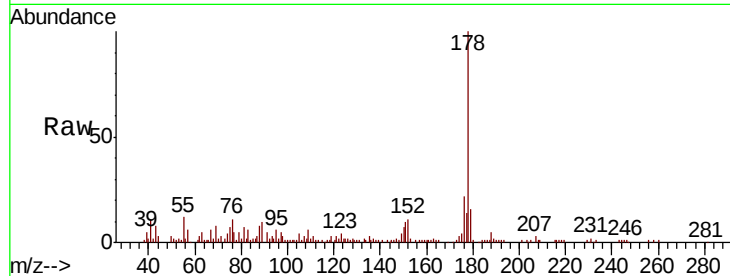


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

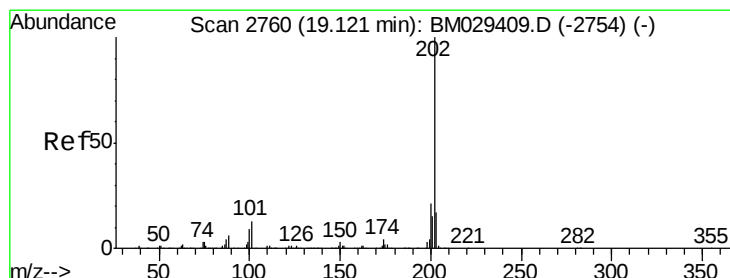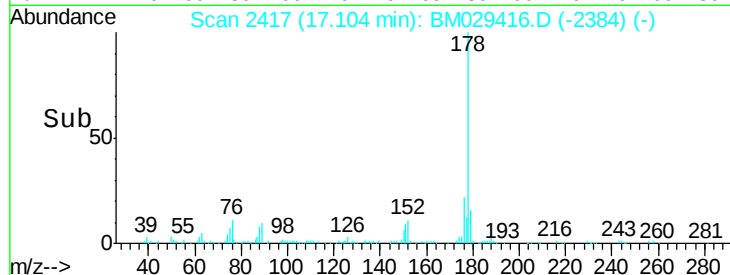
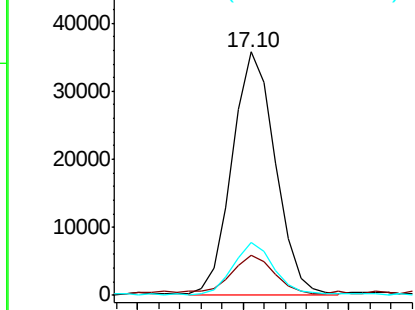



#77
Fluoranthene
Concen: 1.770 ng/ul
RT: 19.12 min Scan# 2760
Delta R.T. -0.00 min
Lab File: BM029416.D
Acq: 08 Apr 2021 20:38

Tgt Ion:202 Resp: 73378
Ion Ratio Lower Upper
202 100
101 10.5 9.8 14.6
100 10.3 7.4 11.0

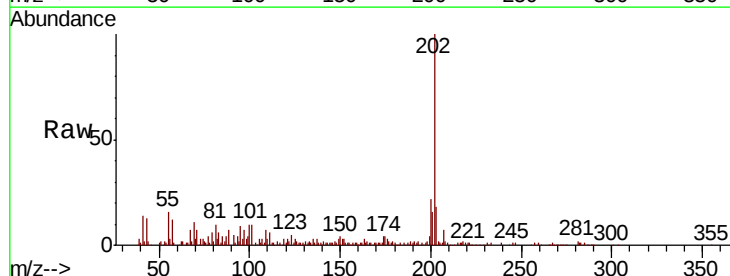

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

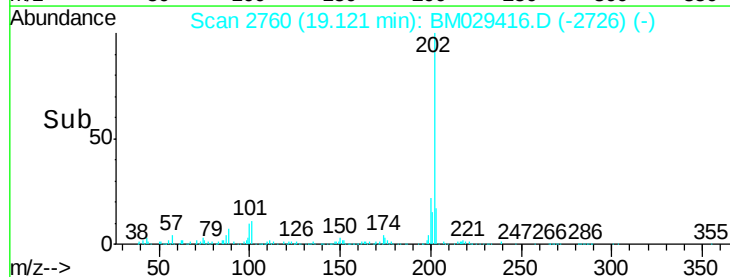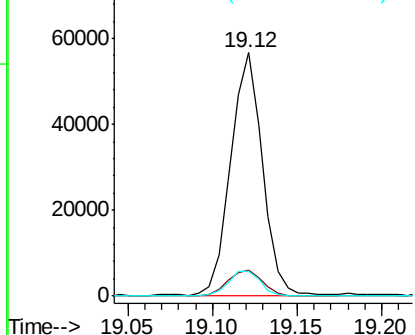

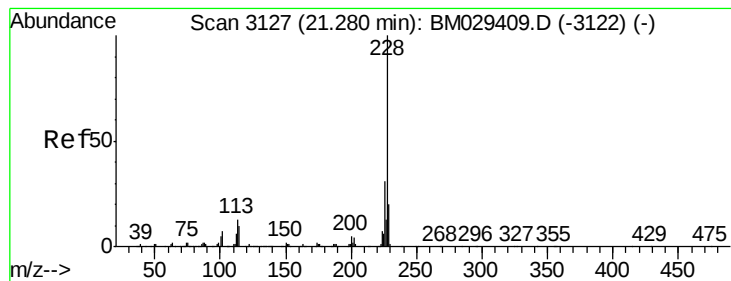

#85

Chrysene

Concen: 1.044 ng/ul

RT: 21.27 min Scan# 3126

Delta R.T. -0.01 min

Lab File: BM029416.D

Acq: 08 Apr 2021 20:38

Instrument :

BNA_M

ClientSampleId :

C0B55


Tot Ion: 228 Resp: 29110

Ion Ratio Lower Upper

228 100

226 27.6 24.0 36.0

229 21.2 15.4 23.0

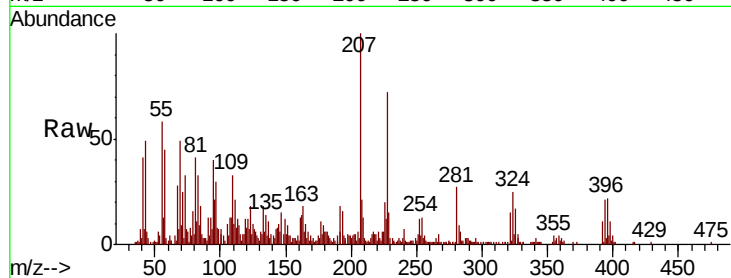

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

