
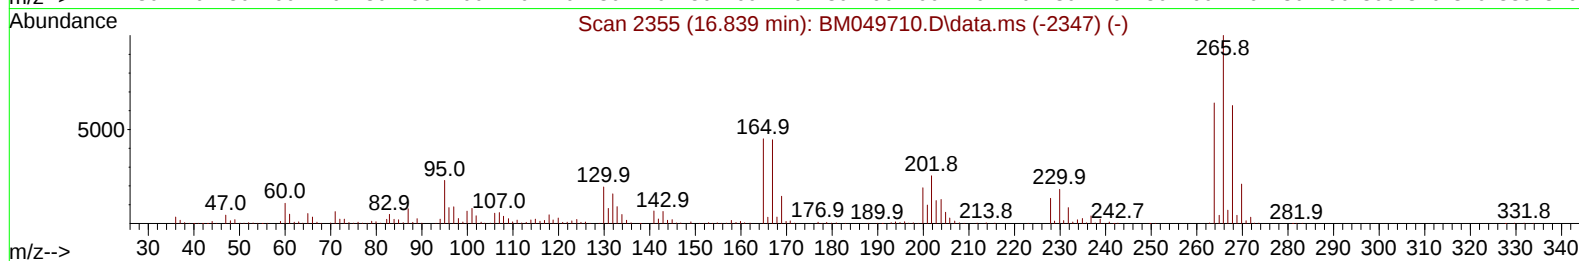
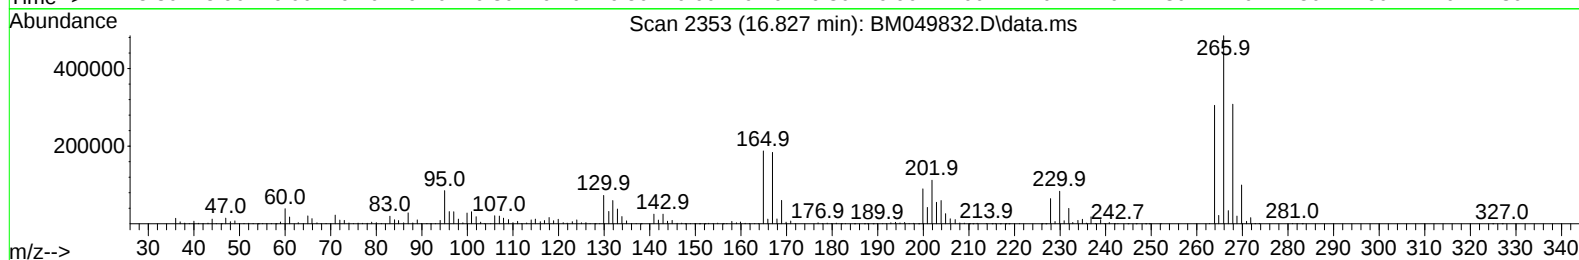


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040725\
Data File : BM049832.D
Acq On : 07 Apr 2025 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 11:52:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

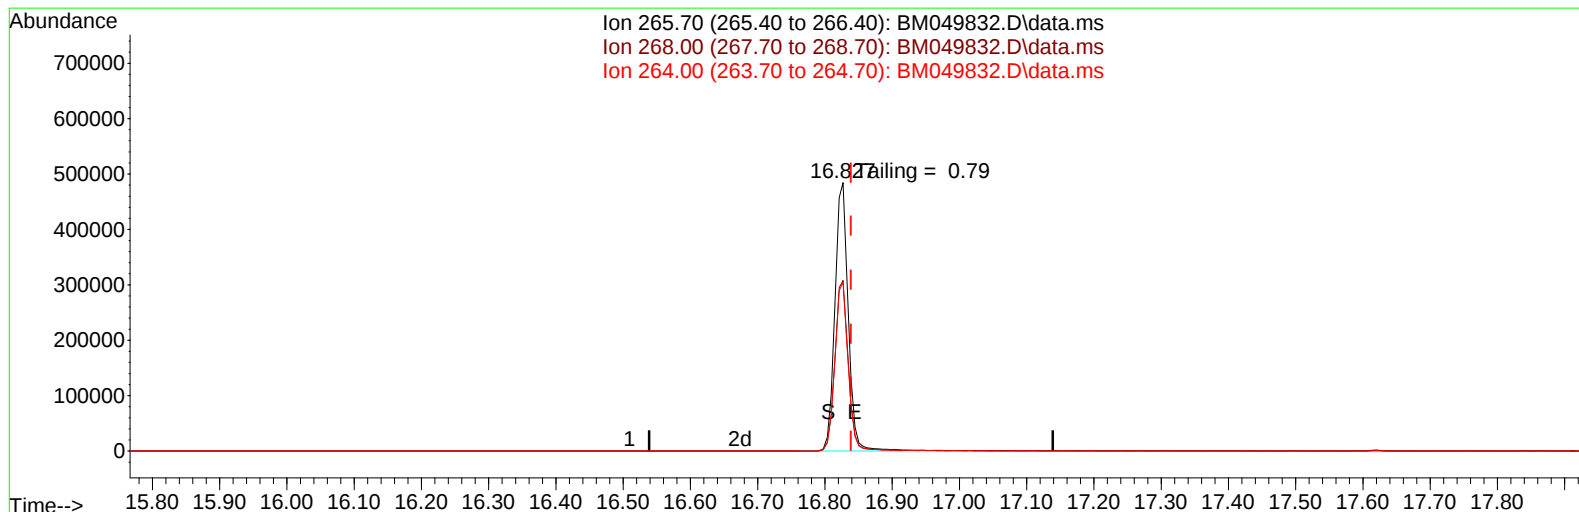

TIC: BM049832.D\data.ms

(70) Pentachlorophenol (C)




16.827min (-0.012) 198903.16 ng m

response 666998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.57
264.00	64.10	62.98
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040725\  
Data File : BM049832.D  
Acq On    : 07 Apr 2025  10:04  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 07 11:52:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

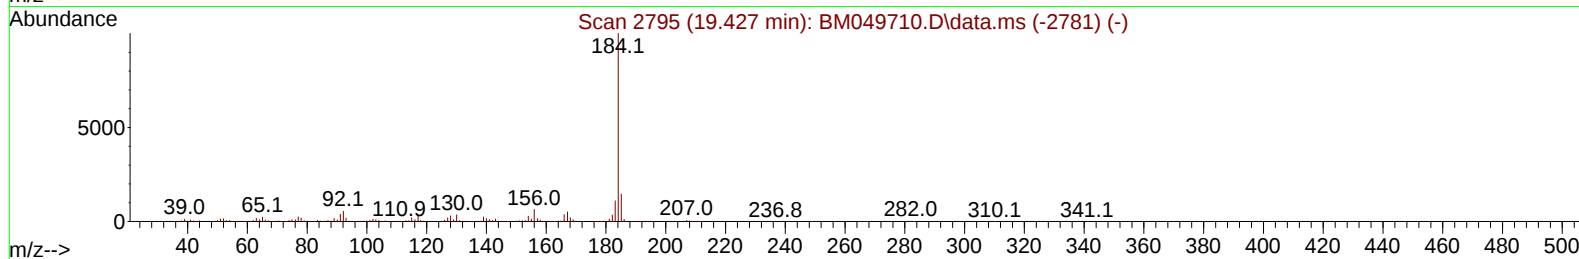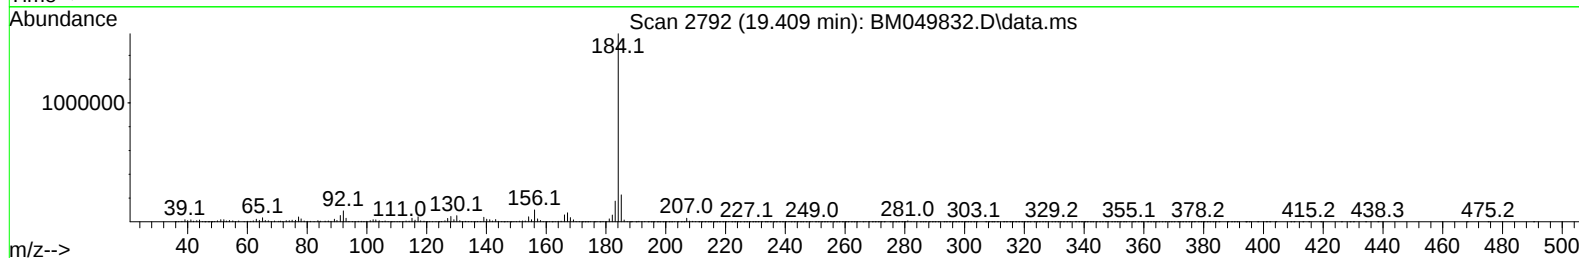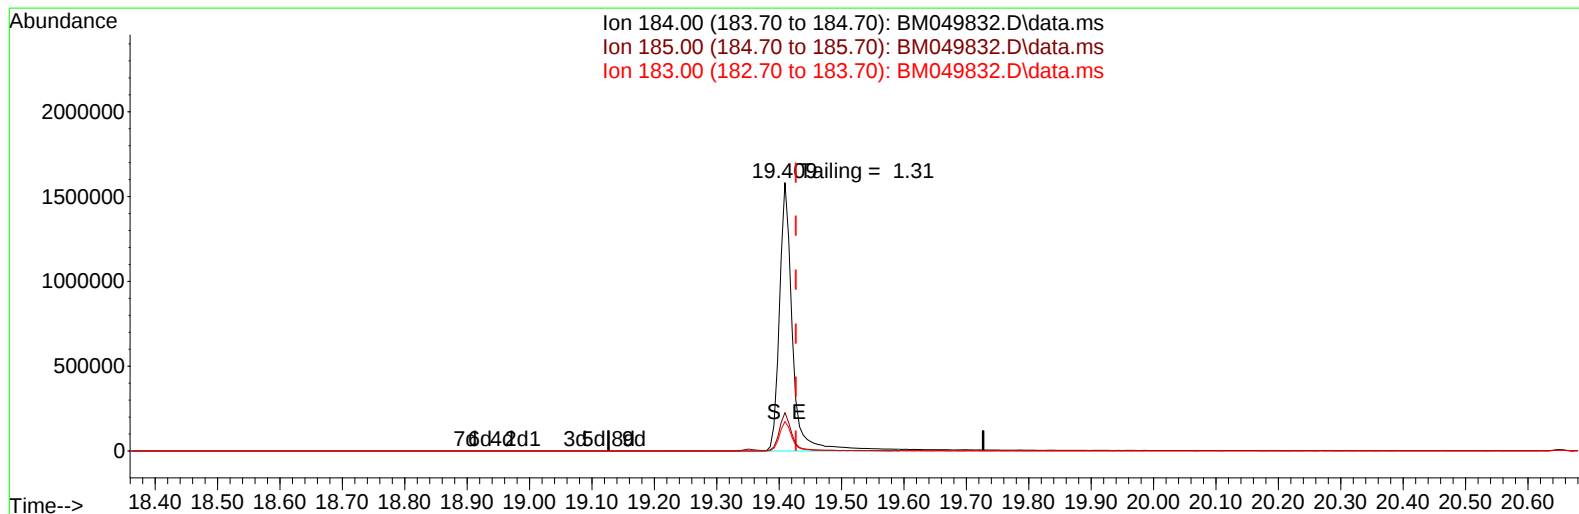

TIC: BM049832.D\data.ms

(77) Benzidine

19.409min (-0.018) 1046979.26 ng m

response **2352162**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.60	14.32
--------	-------	-------

183.00	11.00	10.99
--------	-------	-------

0.00 0.00 0.00