


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040815\
 Data File : BM000901.D
 Acq On : 08 Apr 2015 09:23
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 07 15:59:39 2015

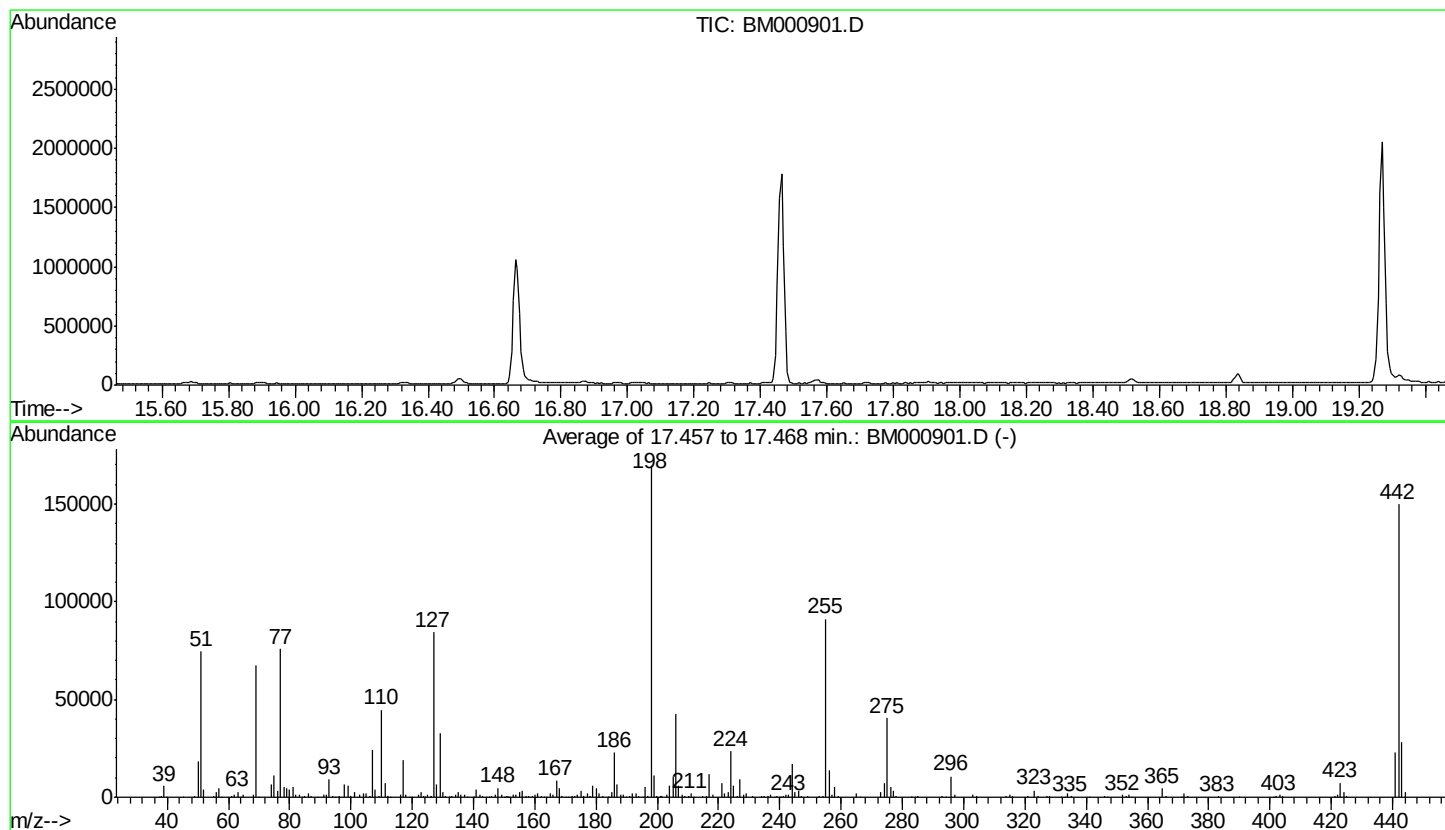

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	74474	PASS
68	69	0.00	2	1.7	1171	PASS
69	198	0.00	100	39.8	67552	PASS
70	69	0.00	2	0.4	247	PASS
127	198	10	80	49.7	84301	PASS
197	198	0.00	2	0.2	383	PASS
198	198	100	100	100.0	169640	PASS
199	198	5	9	6.7	11387	PASS
275	198	10	60	23.9	40474	PASS
365	198	1	100	2.7	4564	PASS
441	442	0.01	24	15.2	22730	PASS
442	198	50	100	88.2	149701	PASS
443	442	15	24	19.0	28405	PASS