


Data Path : Z:\HPCHEM1\BNA_M\Data\BM040815\
 Data File : BM000919.D
 Acq On : 09 Apr 2015 08:44
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

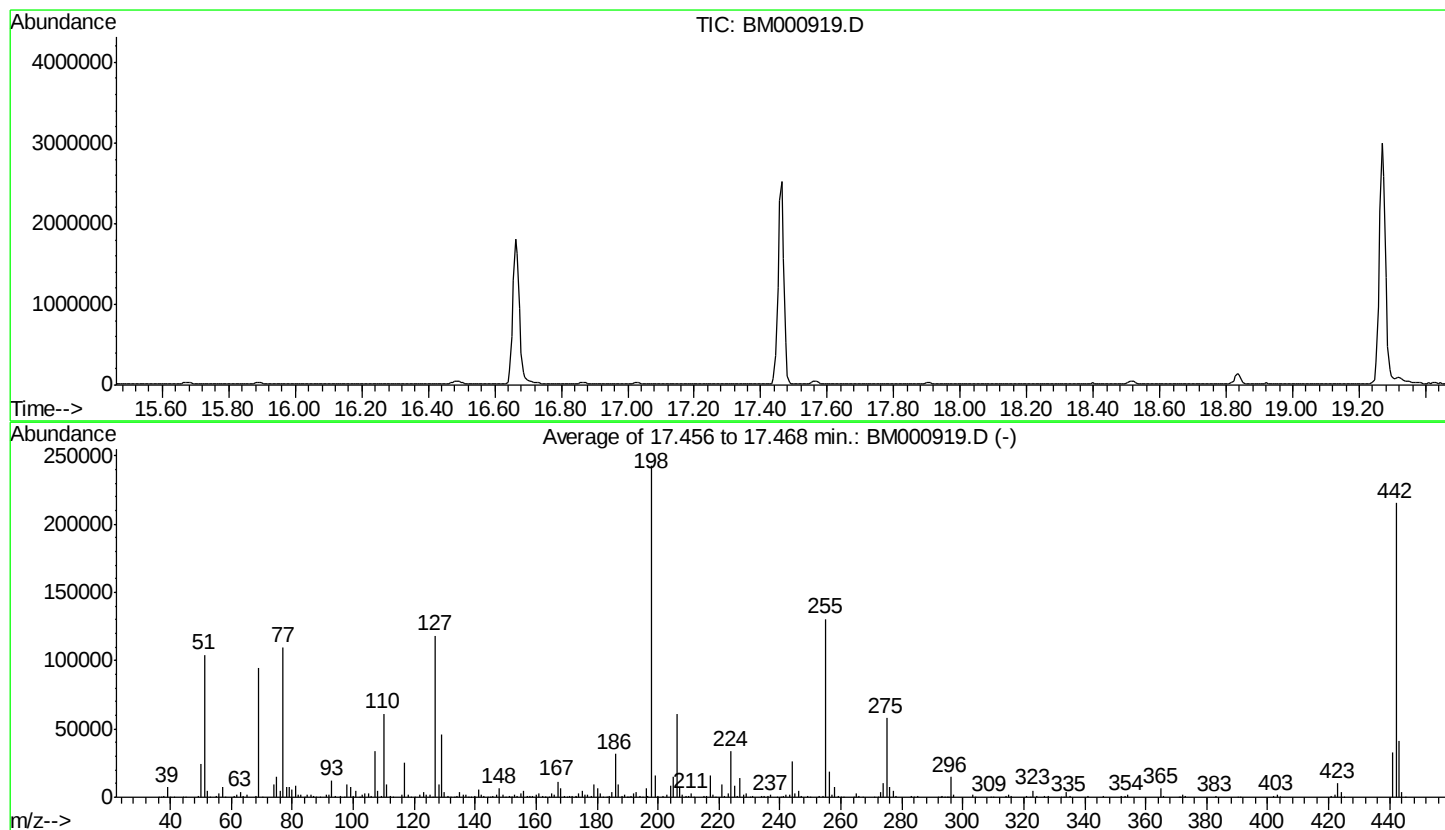

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	104133	PASS
68	69	0.00	2	1.5	1390	PASS
69	198	0.00	100	38.9	94541	PASS
70	69	0.00	2	0.5	429	PASS
127	198	10	80	48.8	118562	PASS
197	198	0.00	2	0.4	949	PASS
198	198	100	100	100.0	242773	PASS
199	198	5	9	6.5	15822	PASS
275	198	10	60	23.8	57800	PASS
365	198	1	100	2.6	6408	PASS
441	442	0.01	24	15.1	32637	PASS
442	198	50	100	88.8	215488	PASS
443	442	15	24	19.0	40909	PASS