

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040816\
 Data File : BM004925.D
 Acq On : 08 Apr 2016 11:29
 Operator : UM/SJ
 Sample : PB89604BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK04

Manual Integrations
 APPROVED

Sohil
 4/11/2016 5:47:47 PM

Quant Time: Apr 09 01:20:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 09 01:17:35 2016
 Response via : Initial Calibration

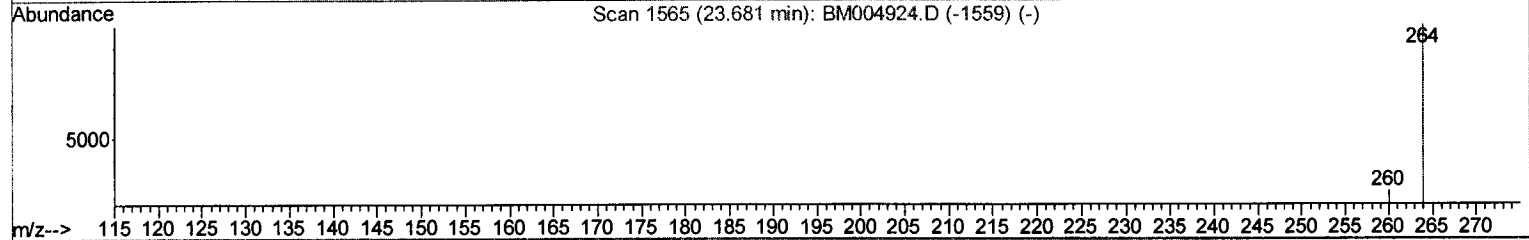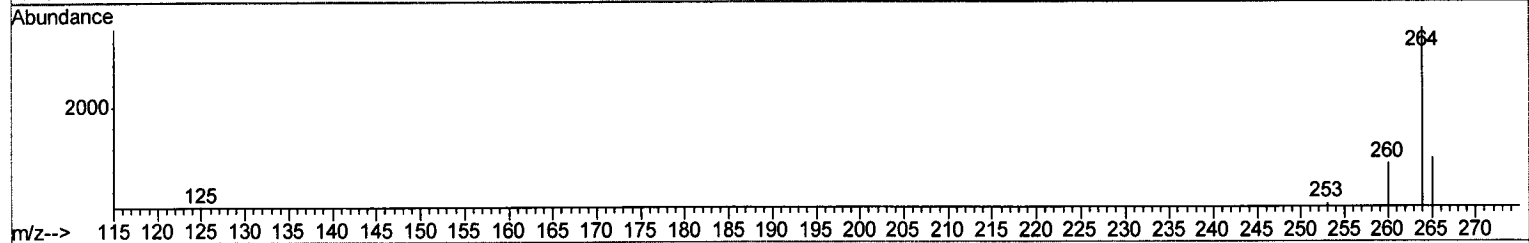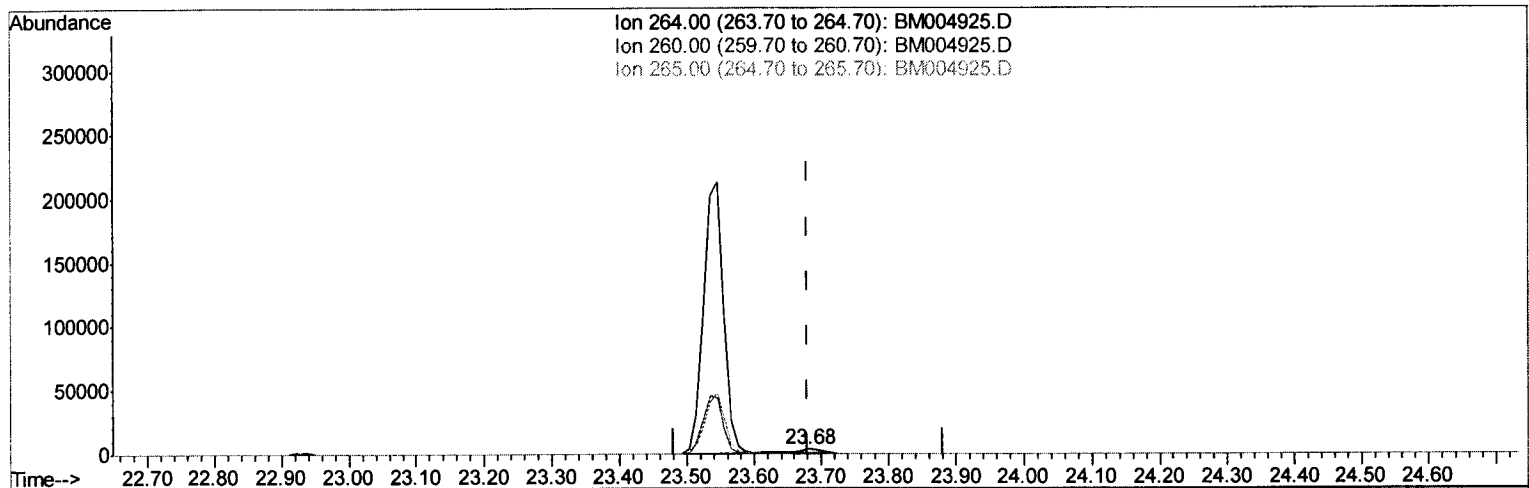

TIC: BM004925.D

(22) Perylene-d12 (I)

23.681min (+0.000) 0.40ng/ul m > V.M.

response 5962

04/22/16

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.99
265.00	38.20	29.48#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040816\
Data File : BM004925.D
Acq On : 08 Apr 2016 11:29
Operator : UM/SJ
Sample : PB89604BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
4/11/2016 5:47:47 PM

Quant Time: Apr 09 01:20:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 09 01:17:35 2016
Response via : Initial Calibration

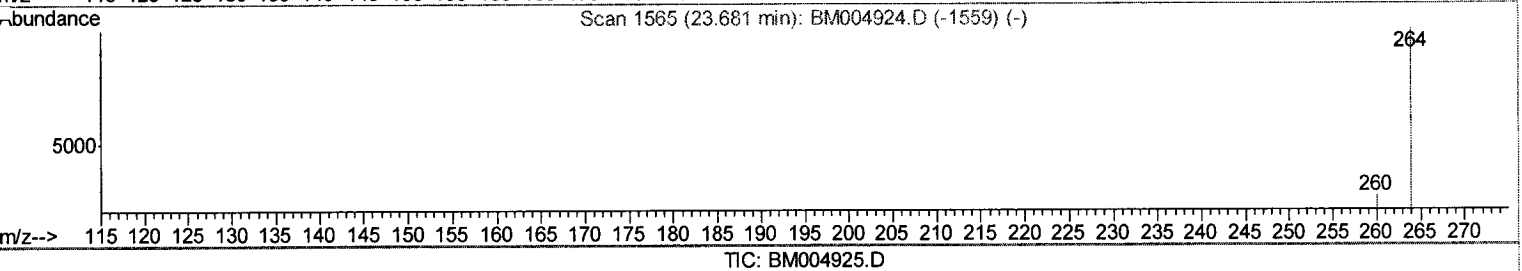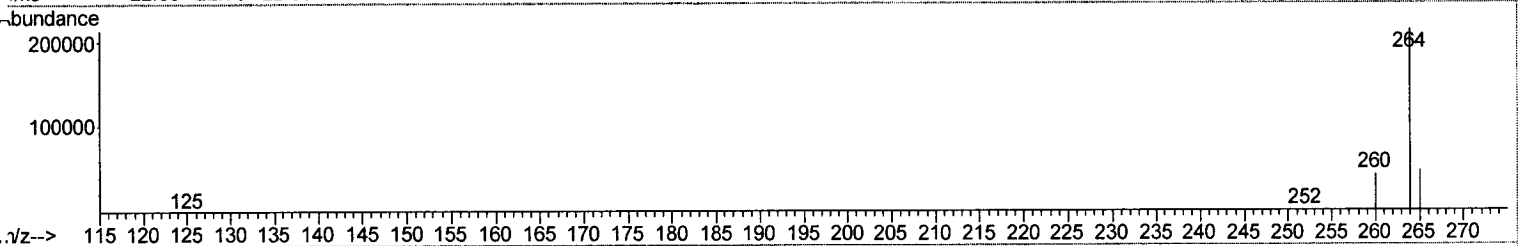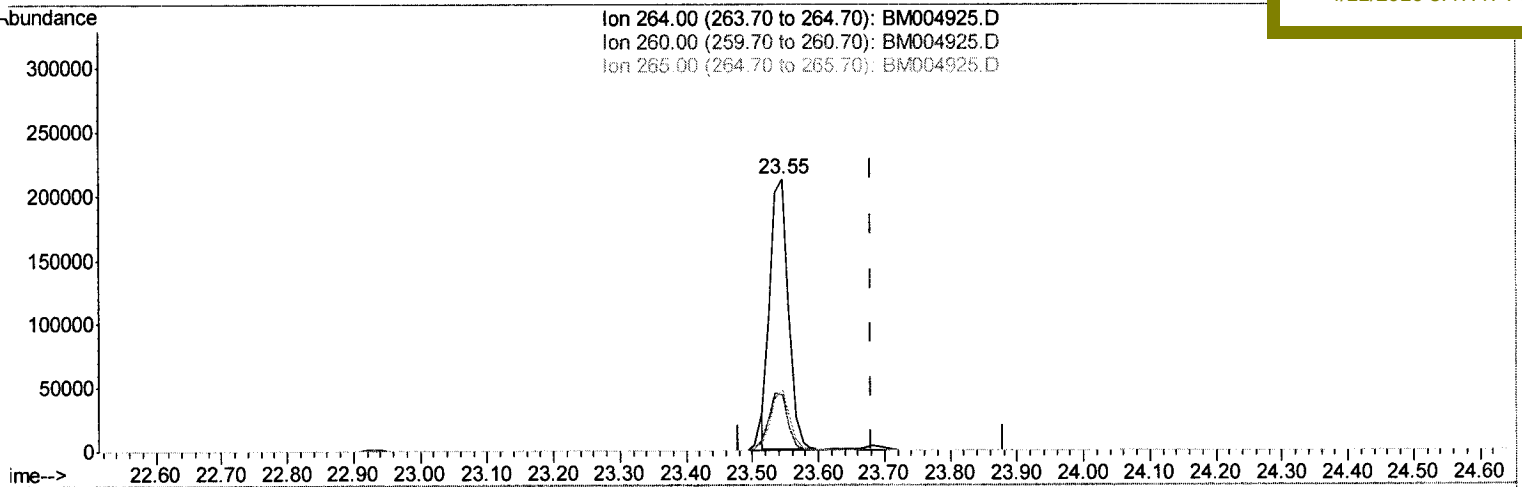

(22) Perylene-d12 (I)

23.545min (-0.135) 0.40ng/ul

response 415316

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	20.28#
265.00	38.20	22.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040816\
 Data File : BM004925.D
 Acq On : 08 Apr 2016 11:29
 Operator : UM/SJ
 Sample : PB89604BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK04

Manual Integrations
 APPROVED

Sohil
 4/11/2016 5:47:47 PM

Quant Time: Apr 09 01:20:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 09 01:17:35 2016
 Response via : Initial Calibration

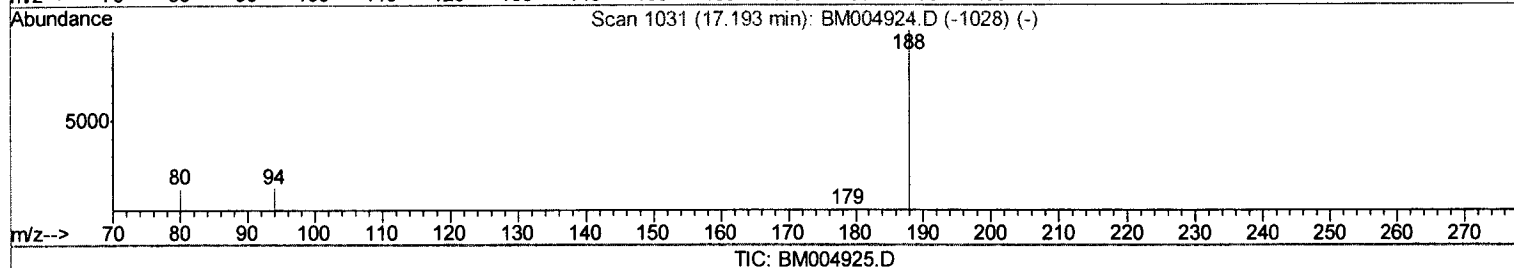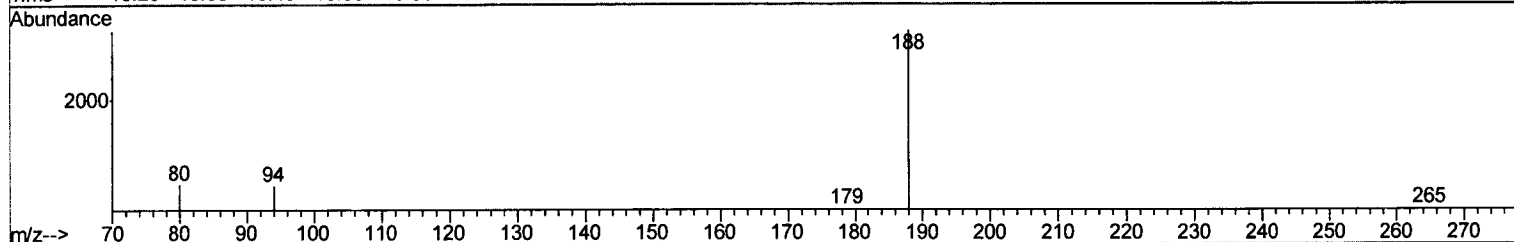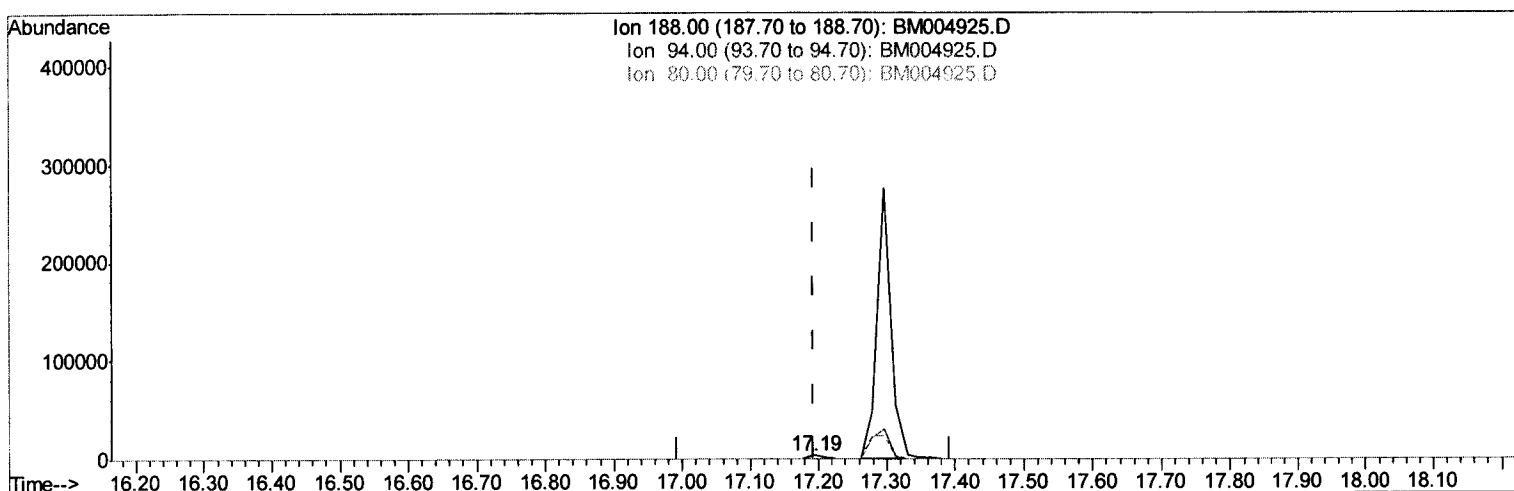

(12) Phenanthrene-d10 (I)

17.193min (+0.000) 0.40ng/ul m U.M.
04/22/16

response 5311

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	14.92#
80.00	11.90	15.35#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040816\
Data File : BM004925.D
Acq On : 08 Apr 2016 11:29
Operator : UM/SJ
Sample : PB89604BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
4/11/2016 5:47:47 PM

Quant Time: Apr 09 01:20:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 09 01:17:35 2016
Response via : Initial Calibration

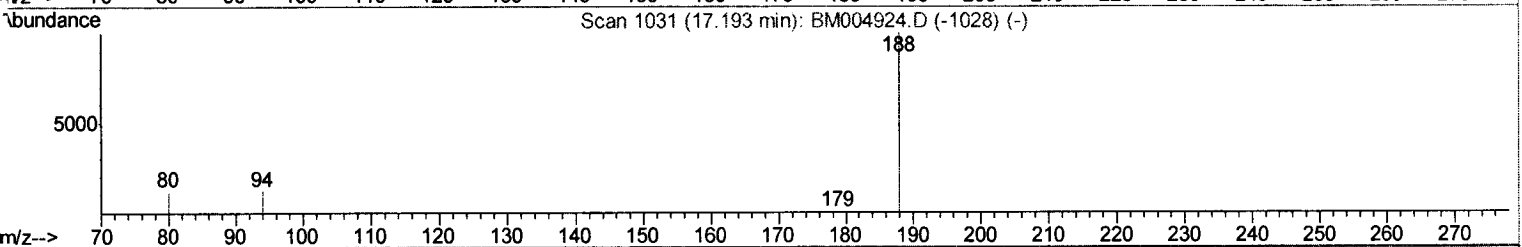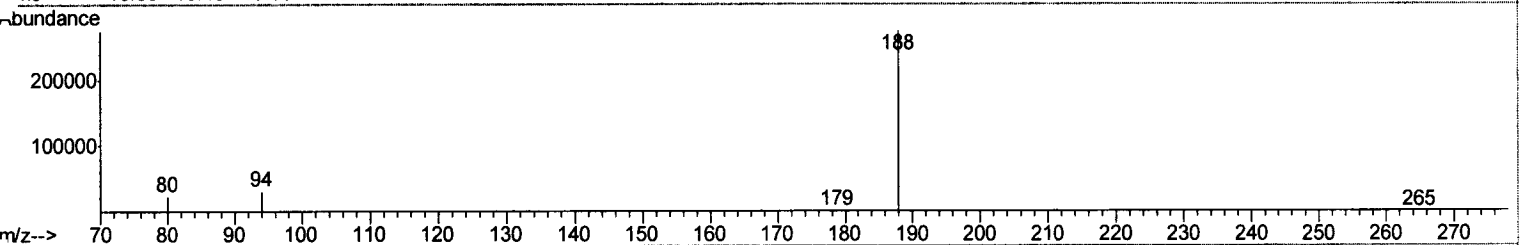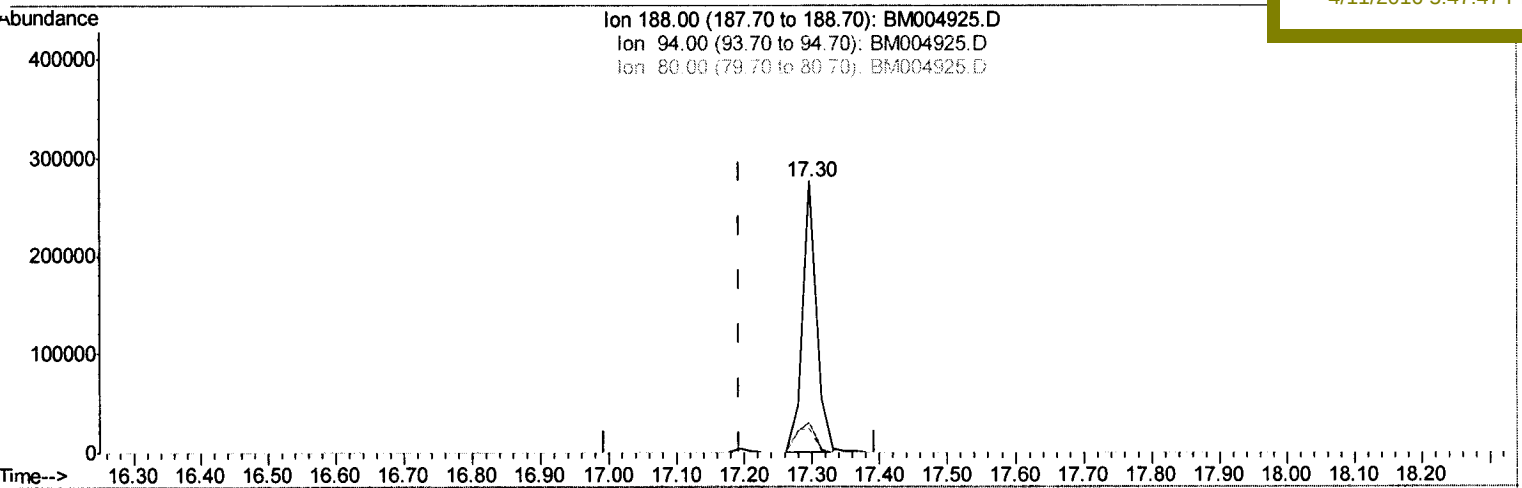

TIC: BM004925.D

(12) Phenanthrene-d10 (I)

17.296min (+0.103) 0.40ng/ul

response 391010

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	11.14
80.00	11.90	8.55#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040816\
Data File : BM004925.D
Acq On : 08 Apr 2016 11:29
Operator : UM/SJ
Sample : PB89604BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
4/11/2016 5:47:47 PM

Quant Time: Apr 09 01:25:40 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 09 01:17:35 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	889	0.40	ng/ul	0.00
4) Naphthalene-d8	10.61	136	3828	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.45	164	2347	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.19	188	5311m	0.40	ng/ul	0.00
18) Chrysene-d12	21.40	240	5830	0.40	ng/ul	0.01
22) Perylene-d12	23.68	264	5962m	0.40	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.31	96	5993	14.96	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.21	152	1863	0.35	ng/ul	0.00
16) Fluoranthene-d10	19.23	212	4939	0.39	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M.
04/22/16

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040816\
 Data File : BM004925.D
 Acq On : 08 Apr 2016 11:29
 Operator : UM/SJ
 Sample : PB89604BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK04

Manual Integrations
 APPROVED

Sohil
 4/11/2016 5:47:47 PM

Quant Time: Apr 09 01:25:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 09 01:17:35 2016
 Response via : Initial Calibration

