

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040824\
 Data File : BM045056.D
 Acq On : 09 Apr 2024 00:40
 Operator : MA/JU
 Sample : P2013-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

Quant Time: Apr 09 03:17:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 09 02:13:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.627	152	1866	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.396	136	6155	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.275	164	3543	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.031	188	8118m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.254	240	6369m	0.400	ng/ul	0.00
23) Perylene-d12	23.460	264	5738m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	11013	4.493	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.019	152	3415	0.409	ng/ul	-0.02
18) Fluoranthene-d10	19.072	212	8643	0.537	ng/ul	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.239	88	133	0.057	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040824\
Data File : BM045056.D
Acq On : 09 Apr 2024 00:40
Operator : MA/JU
Sample : P2013-04
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EOMB0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024


Quant Time: Apr 09 03:17:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 09 02:13:29 2024
Response via : Initial Calibration

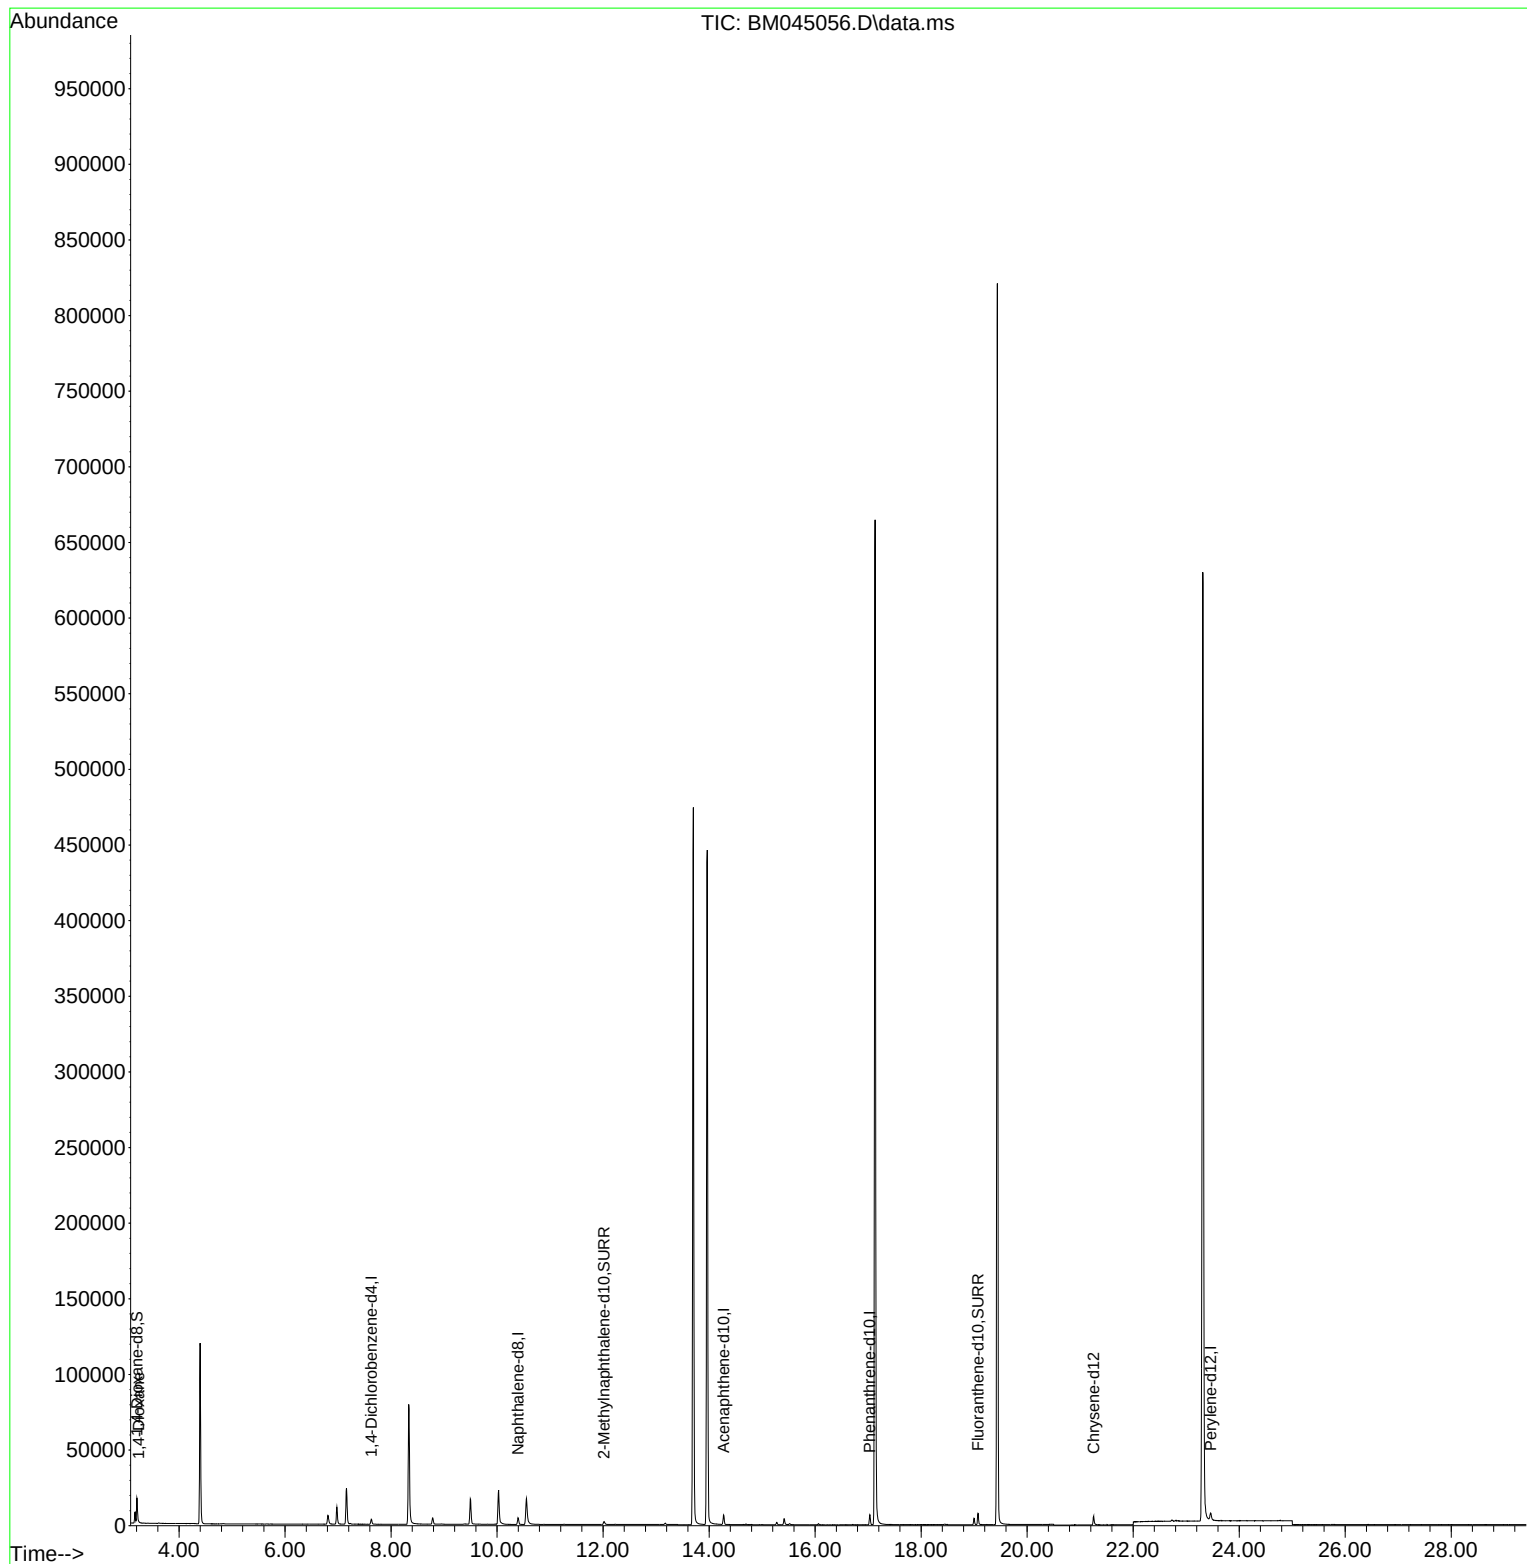

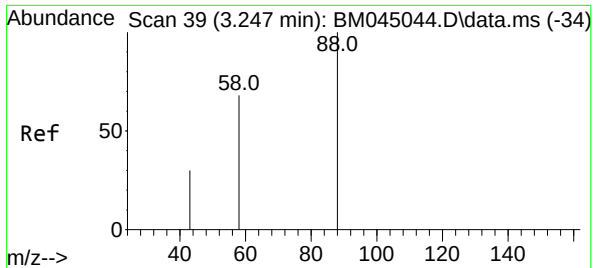

#2
 1,4-Dioxane
 Concen: 0.057 ng/ul
 RT: 3.239 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: BM045056.D
 Acq: 09 Apr 2024 00:40

Instrument :
 BNA_M
 ClientSampleId :
 E0MB0

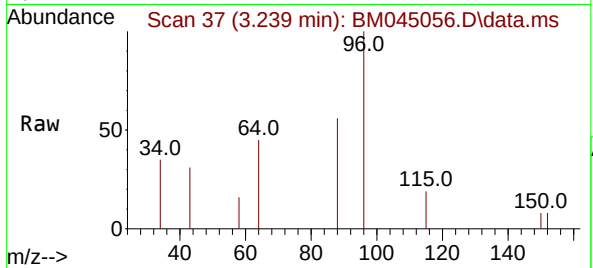

Tgt Ion: 88 Resp: 133
 Ion Ratio Lower Upper
 88 100
 43 55.4 30.6 46.0
 58 29.1 32.6 48.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

