
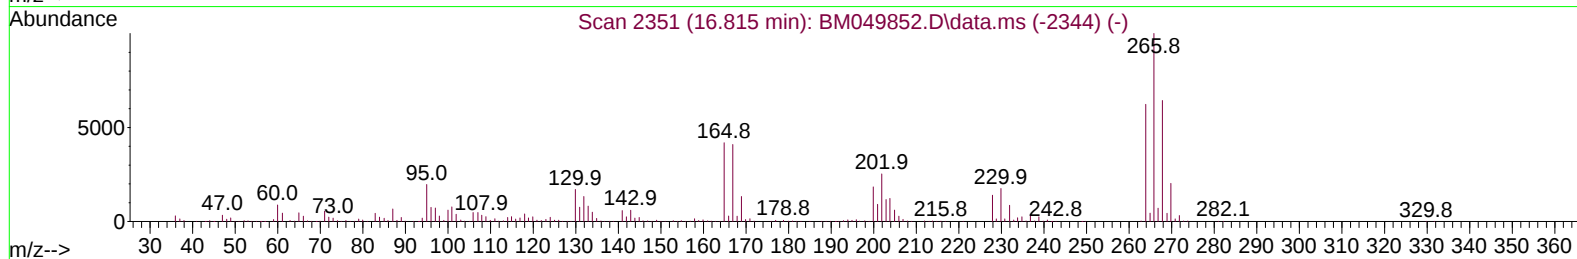
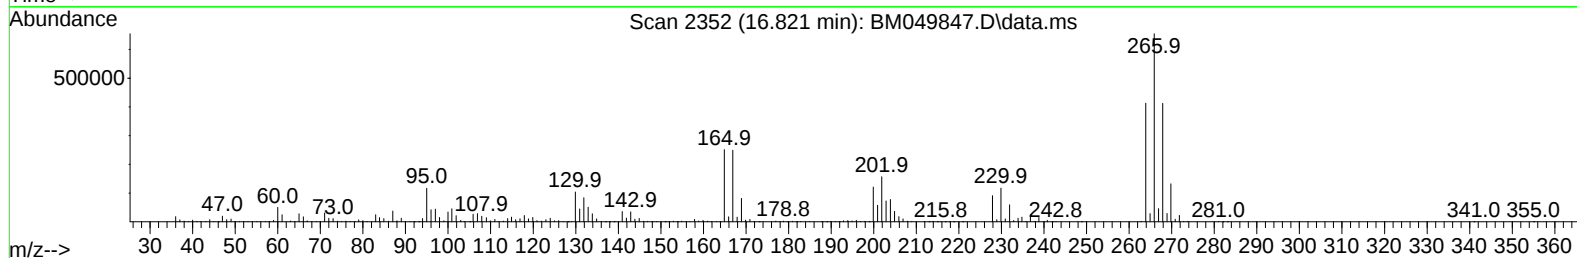


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040825\
Data File : BM049847.D
Acq On : 08 Apr 2025 12:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:09:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

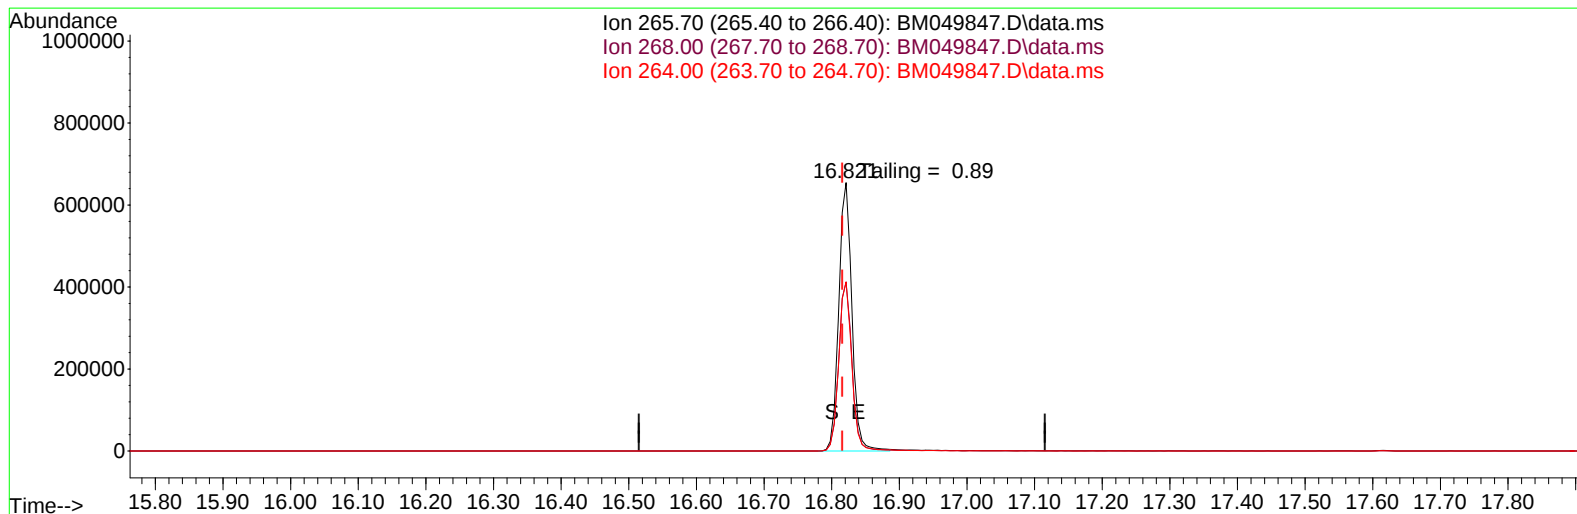

TIC: BM049847.D\data.ms

(70) Pentachlorophenol (C)




16.821min (+ 0.006) 230006.58 ng m

response 888392

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	62.99
264.00	62.30	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040825\
Data File : BM049847.D
Acq On : 08 Apr 2025 12:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:09:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

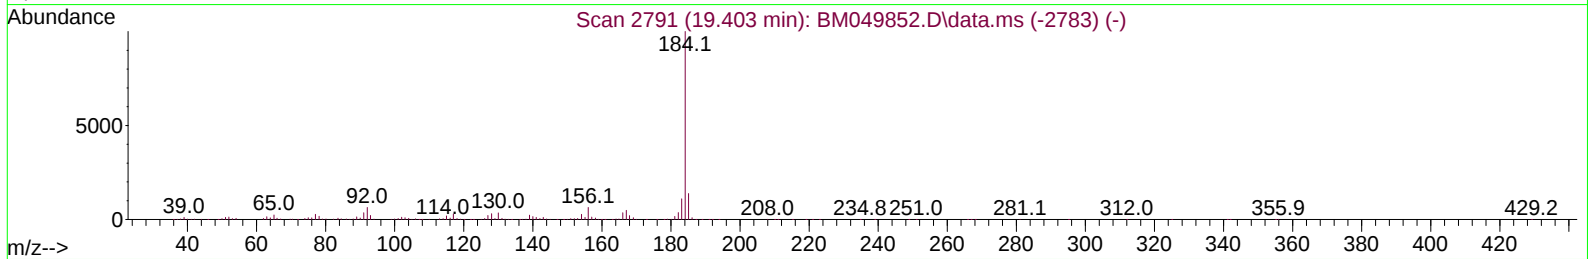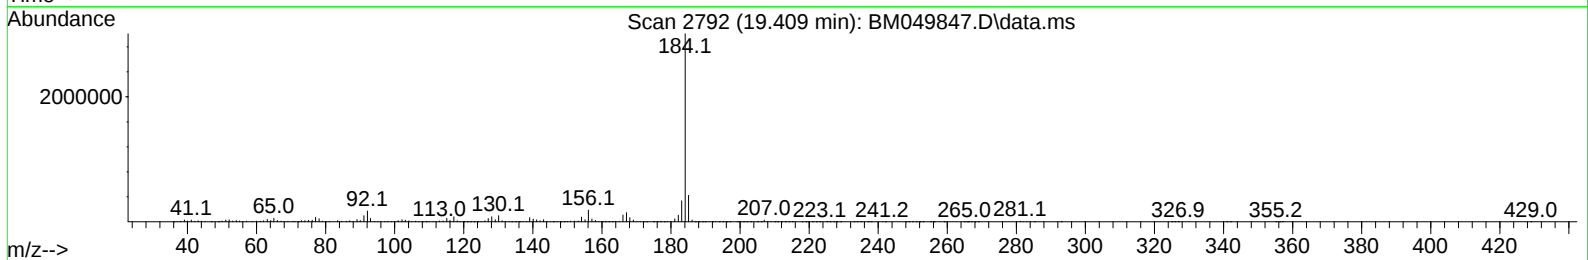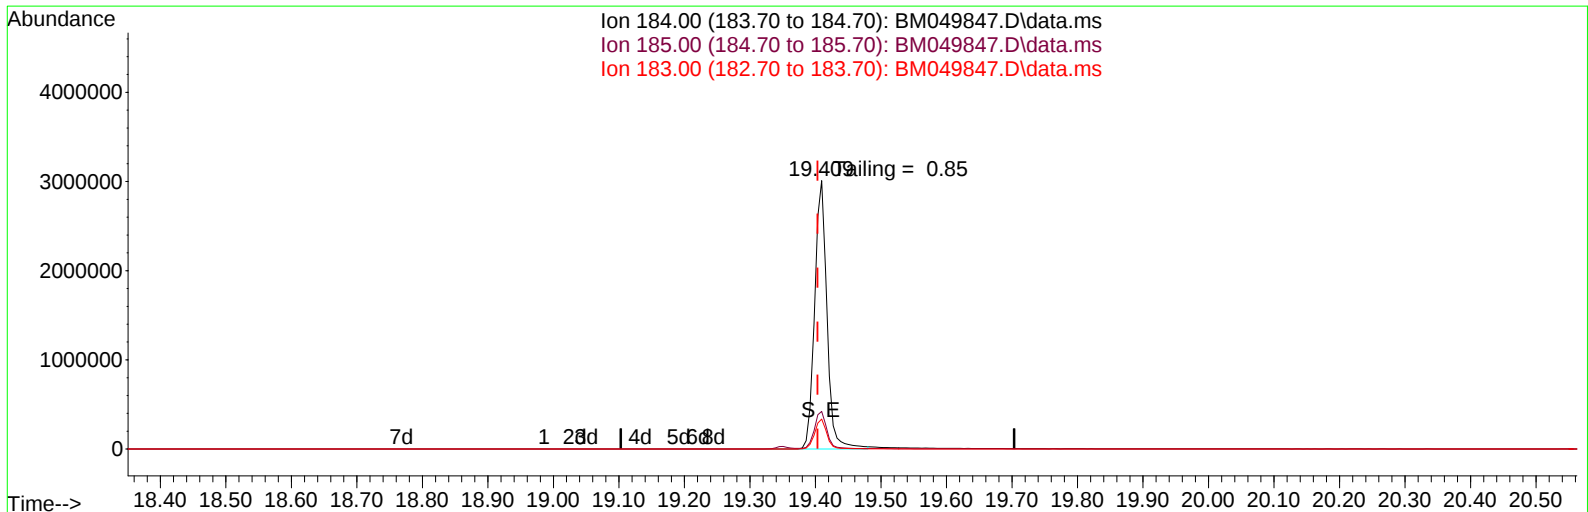

TIC: BM049847.D\data.ms

(77) Benzidine**19.409min (+ 0.006) 842986.98 ng m****response 4014847**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.02
183.00	11.00	11.14
0.00	0.00	0.00