


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040915\
 Data File : BM000926.D
 Acq On : 09 Apr 2015 17:14
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 10 06:37:57 2015

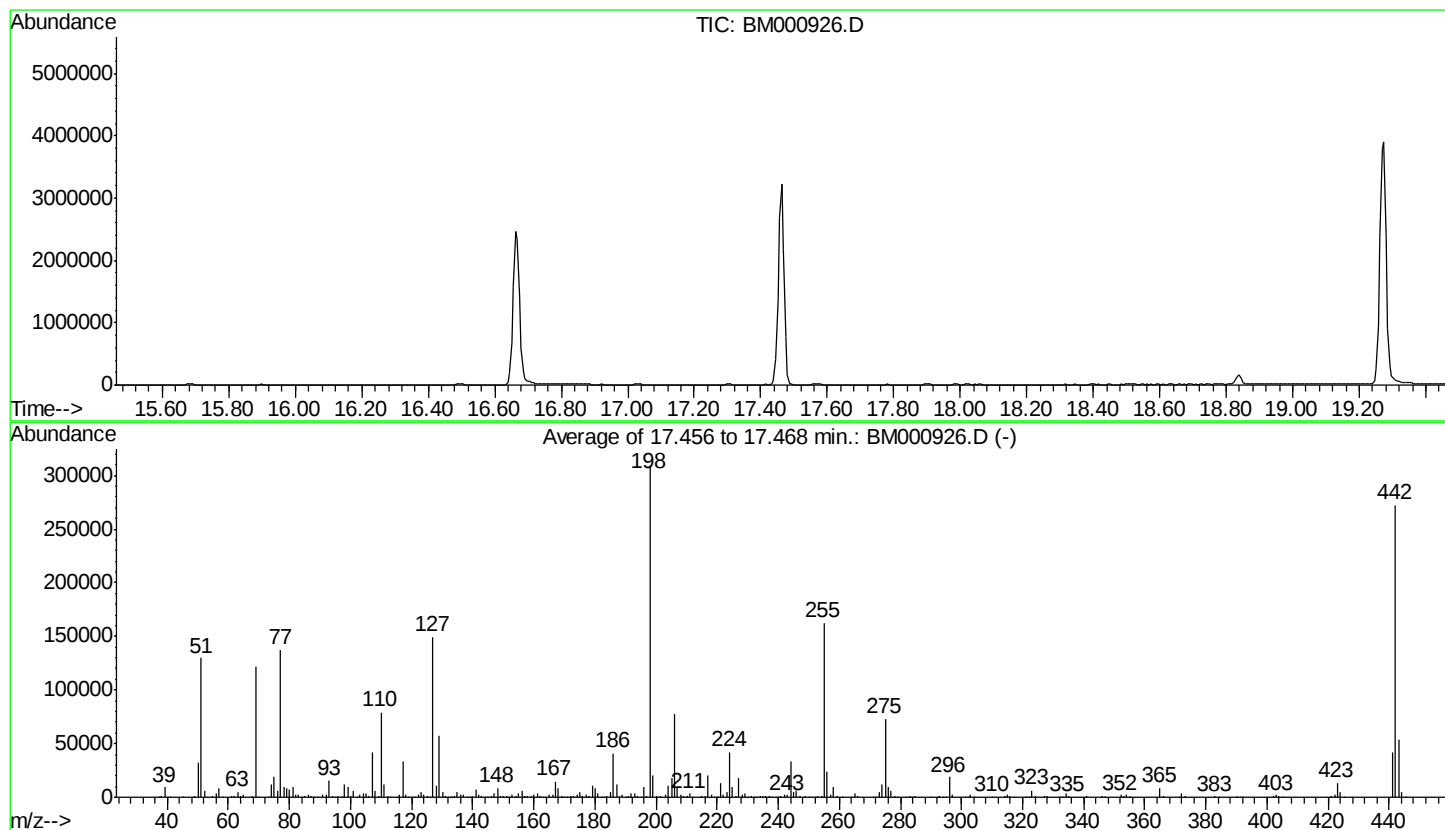

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	129898	PASS
68	69	0.00	2	1.5	1821	PASS
69	198	0.00	100	39.5	122218	PASS
70	69	0.00	2	0.5	571	PASS
127	198	10	80	48.4	149682	PASS
197	198	0.00	2	0.6	1725	PASS
198	198	100	100	100.0	309184	PASS
199	198	5	9	6.7	20765	PASS
275	198	10	60	23.6	72970	PASS
365	198	1	100	2.7	8491	PASS
441	442	0.01	24	15.2	41504	PASS
442	198	50	100	88.2	272661	PASS
443	442	15	24	19.7	53640	PASS