




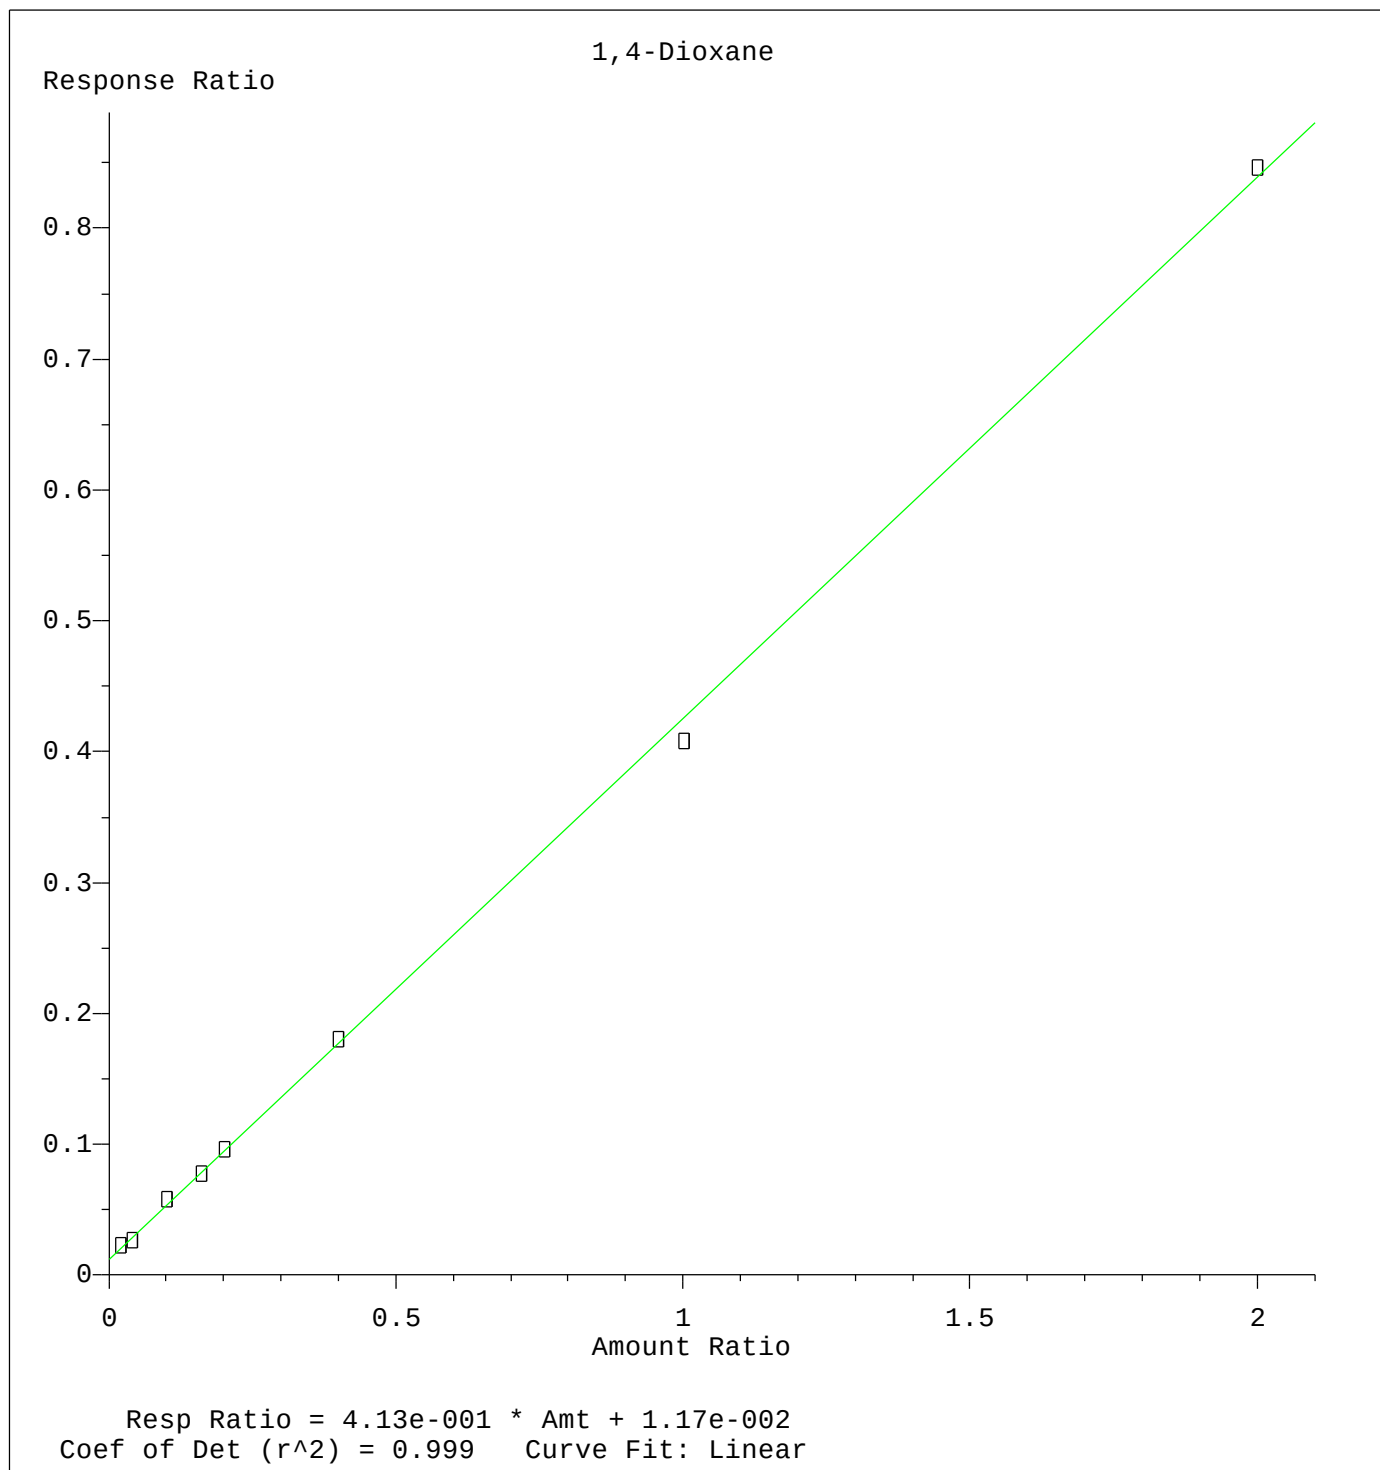


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:31:57 2015

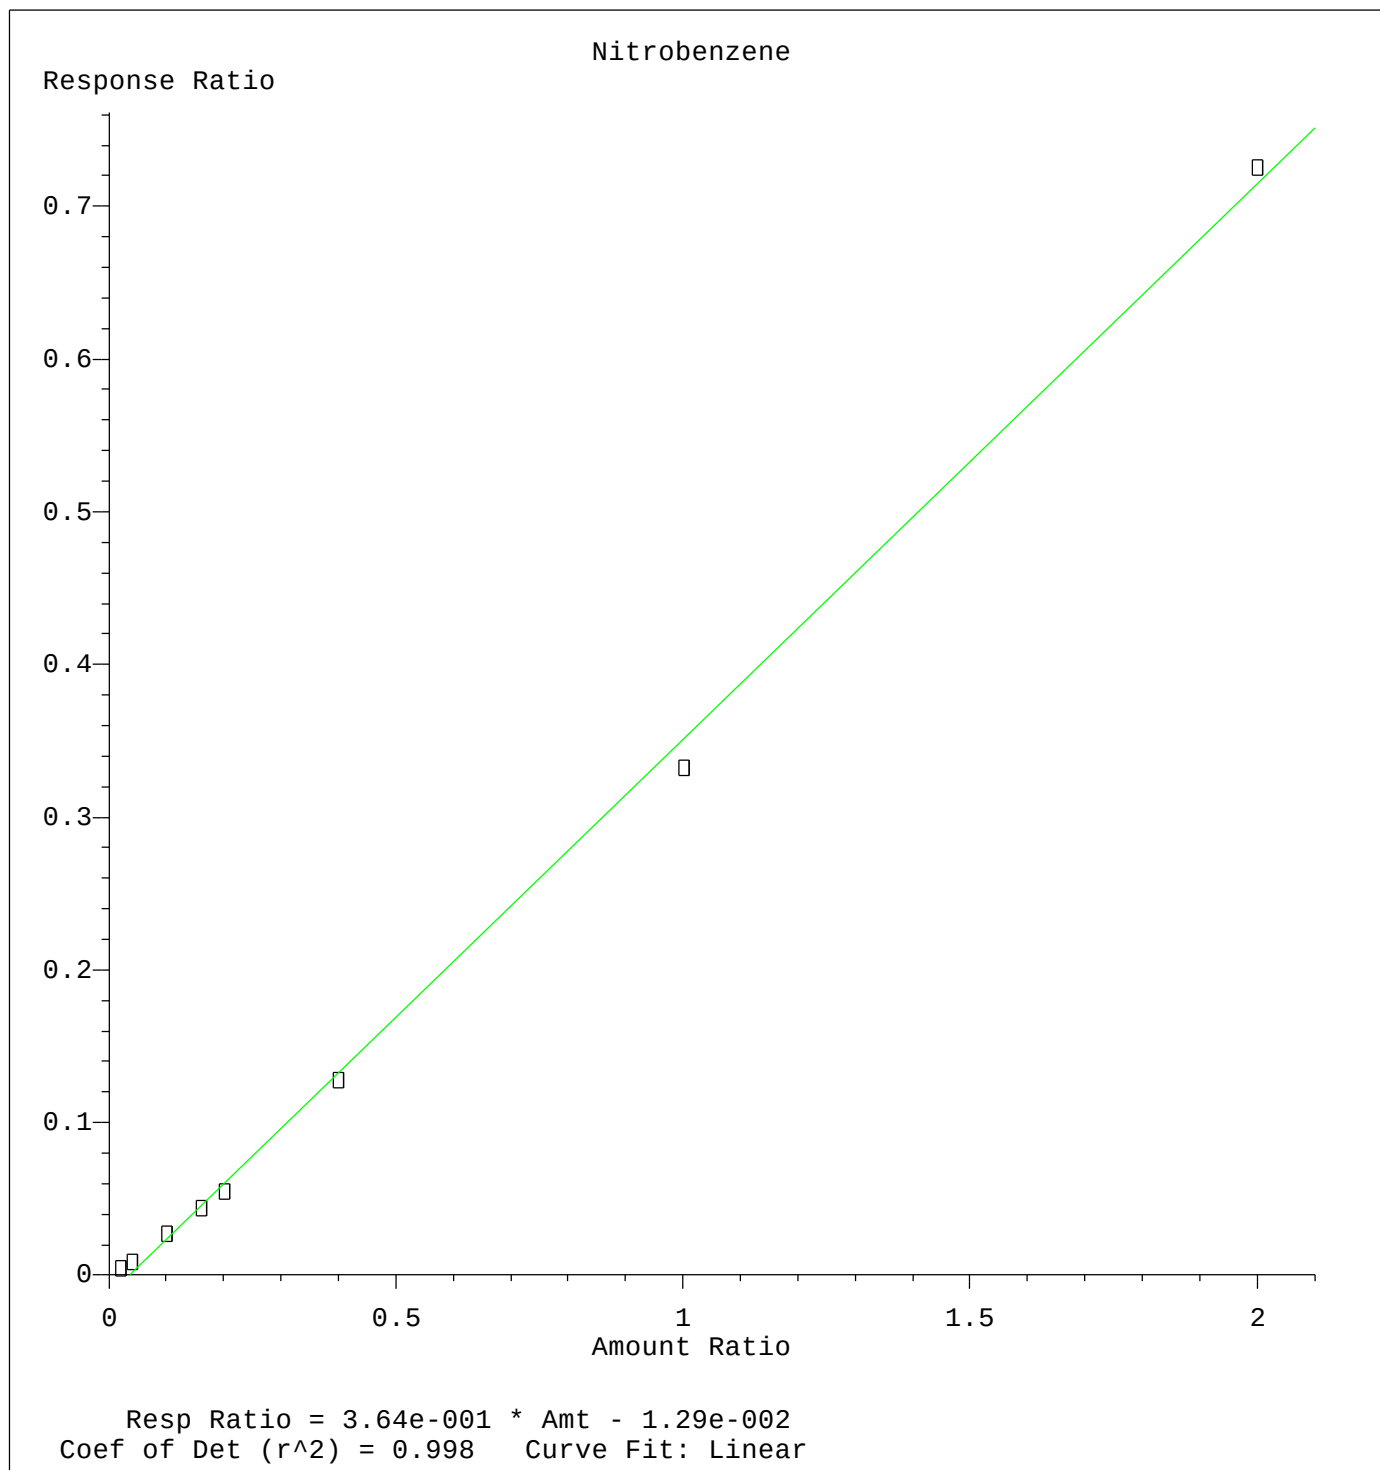


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:35:36 2015

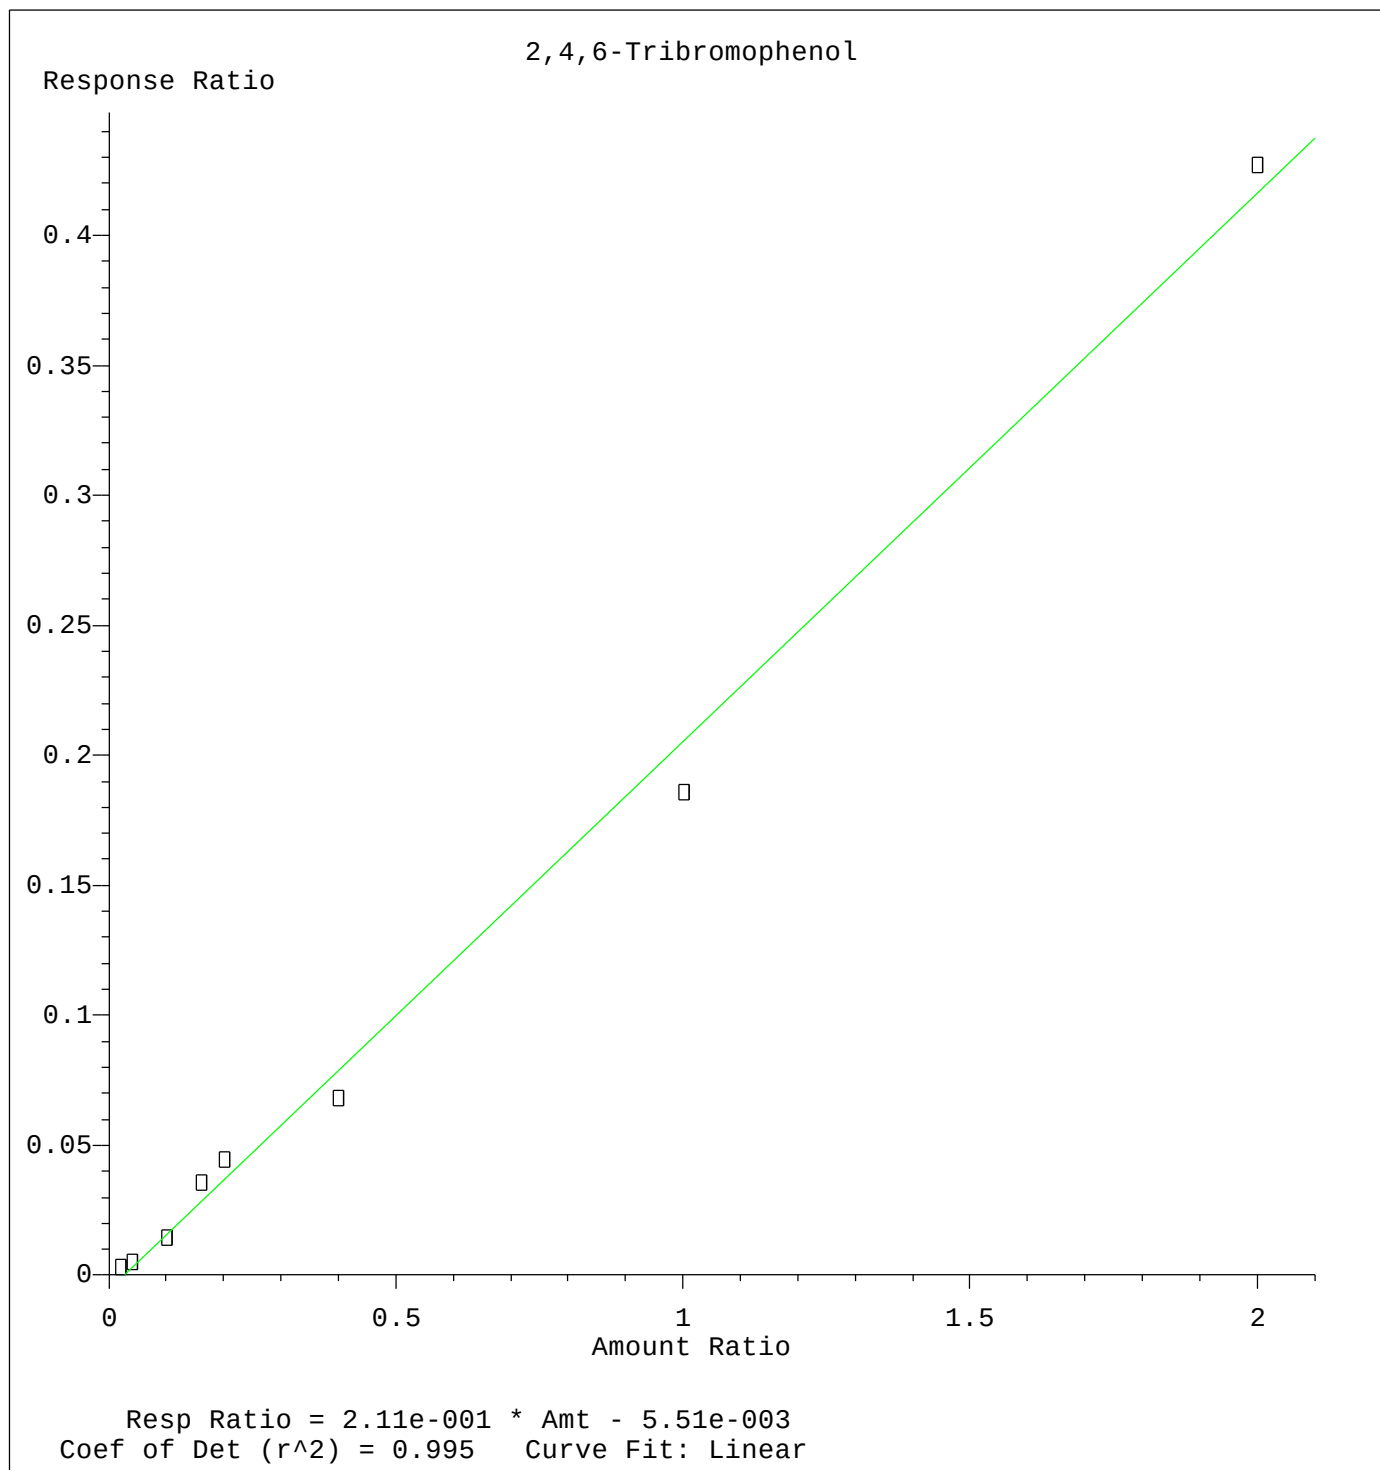


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:35:56 2015

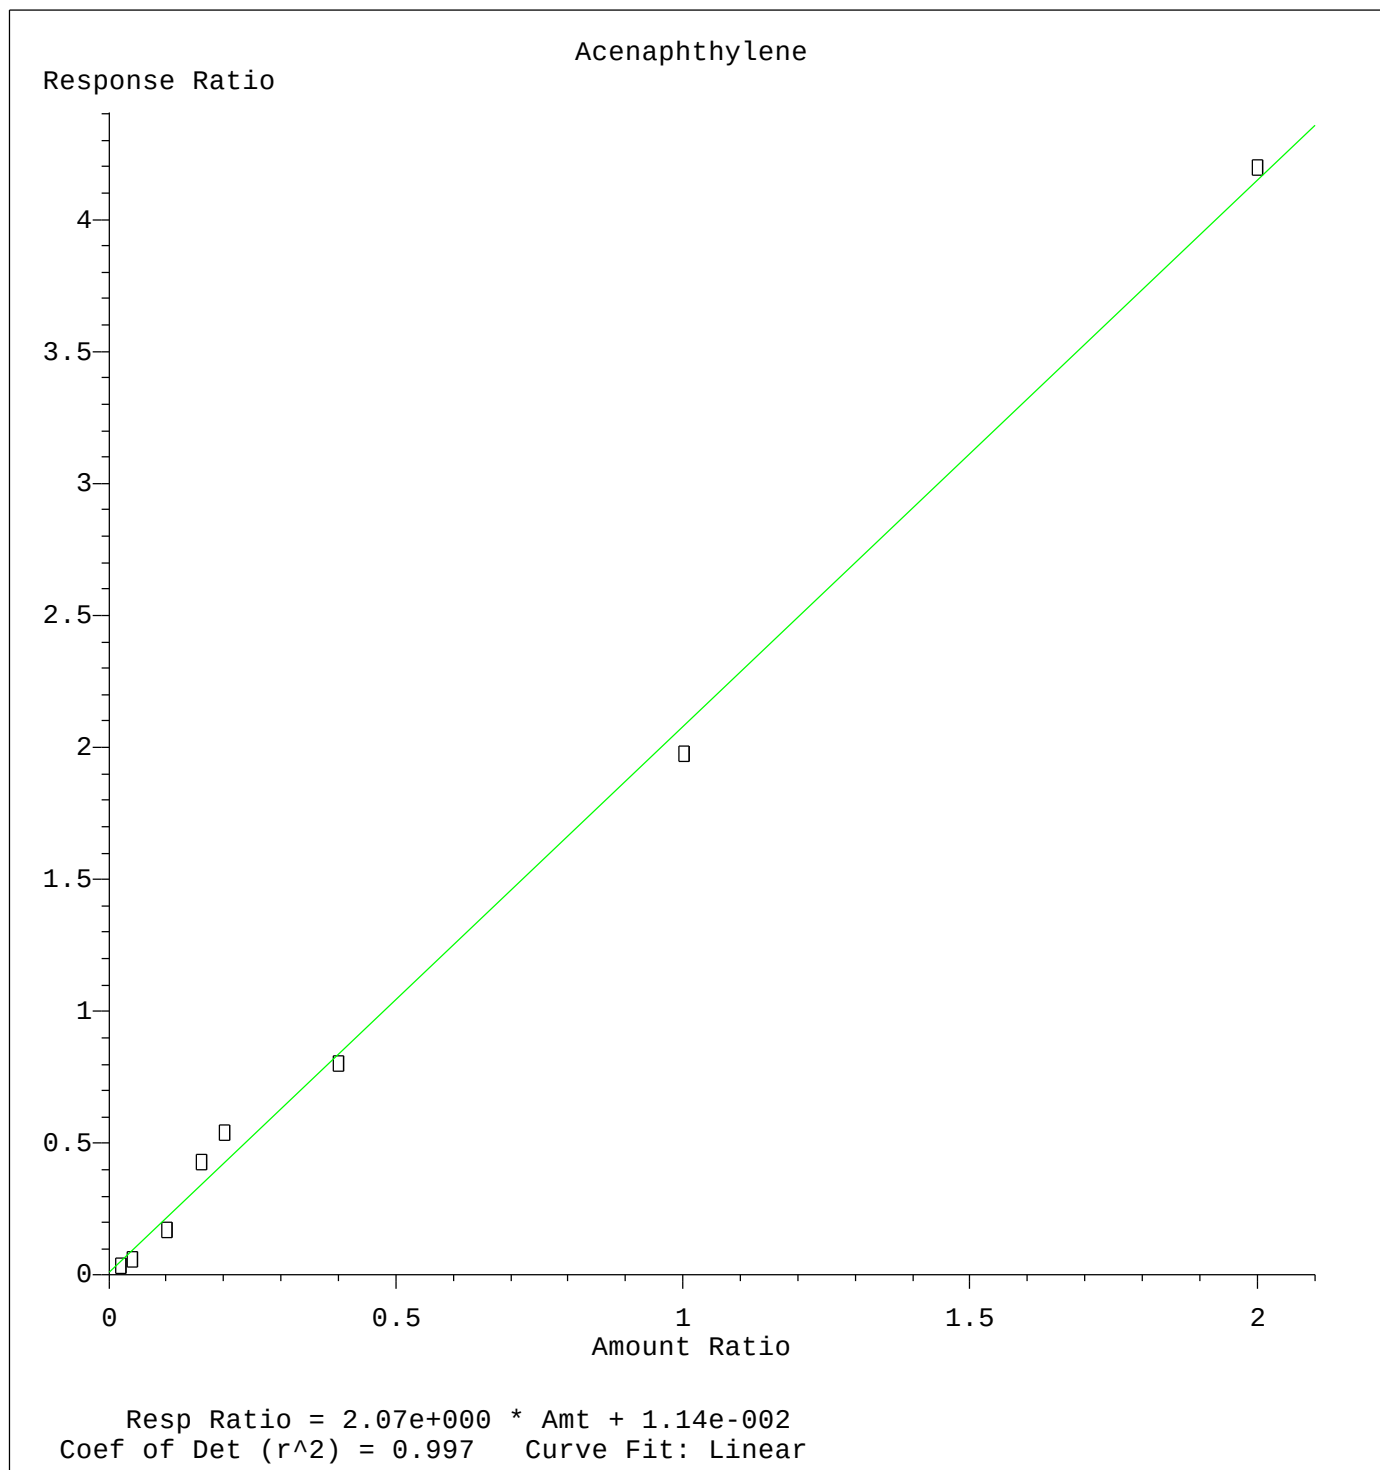


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:36:19 2015

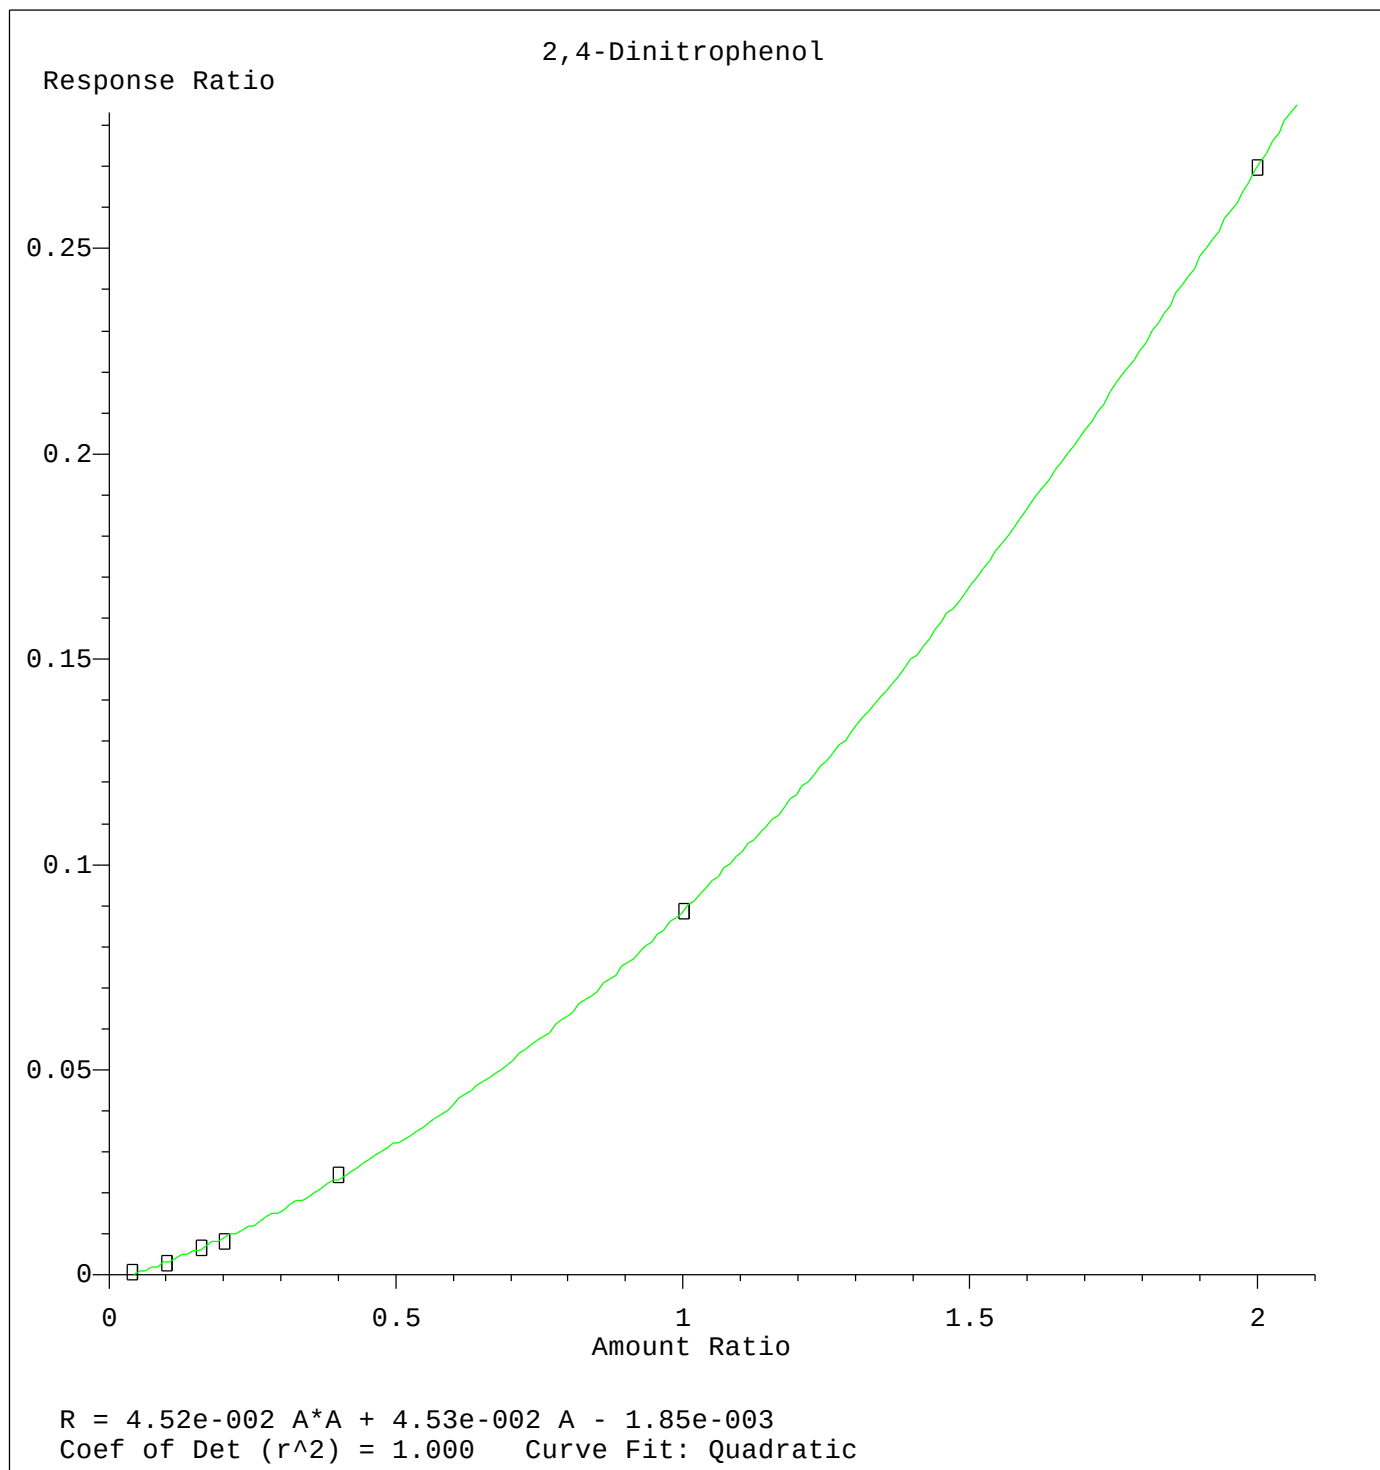

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:36:34 2015

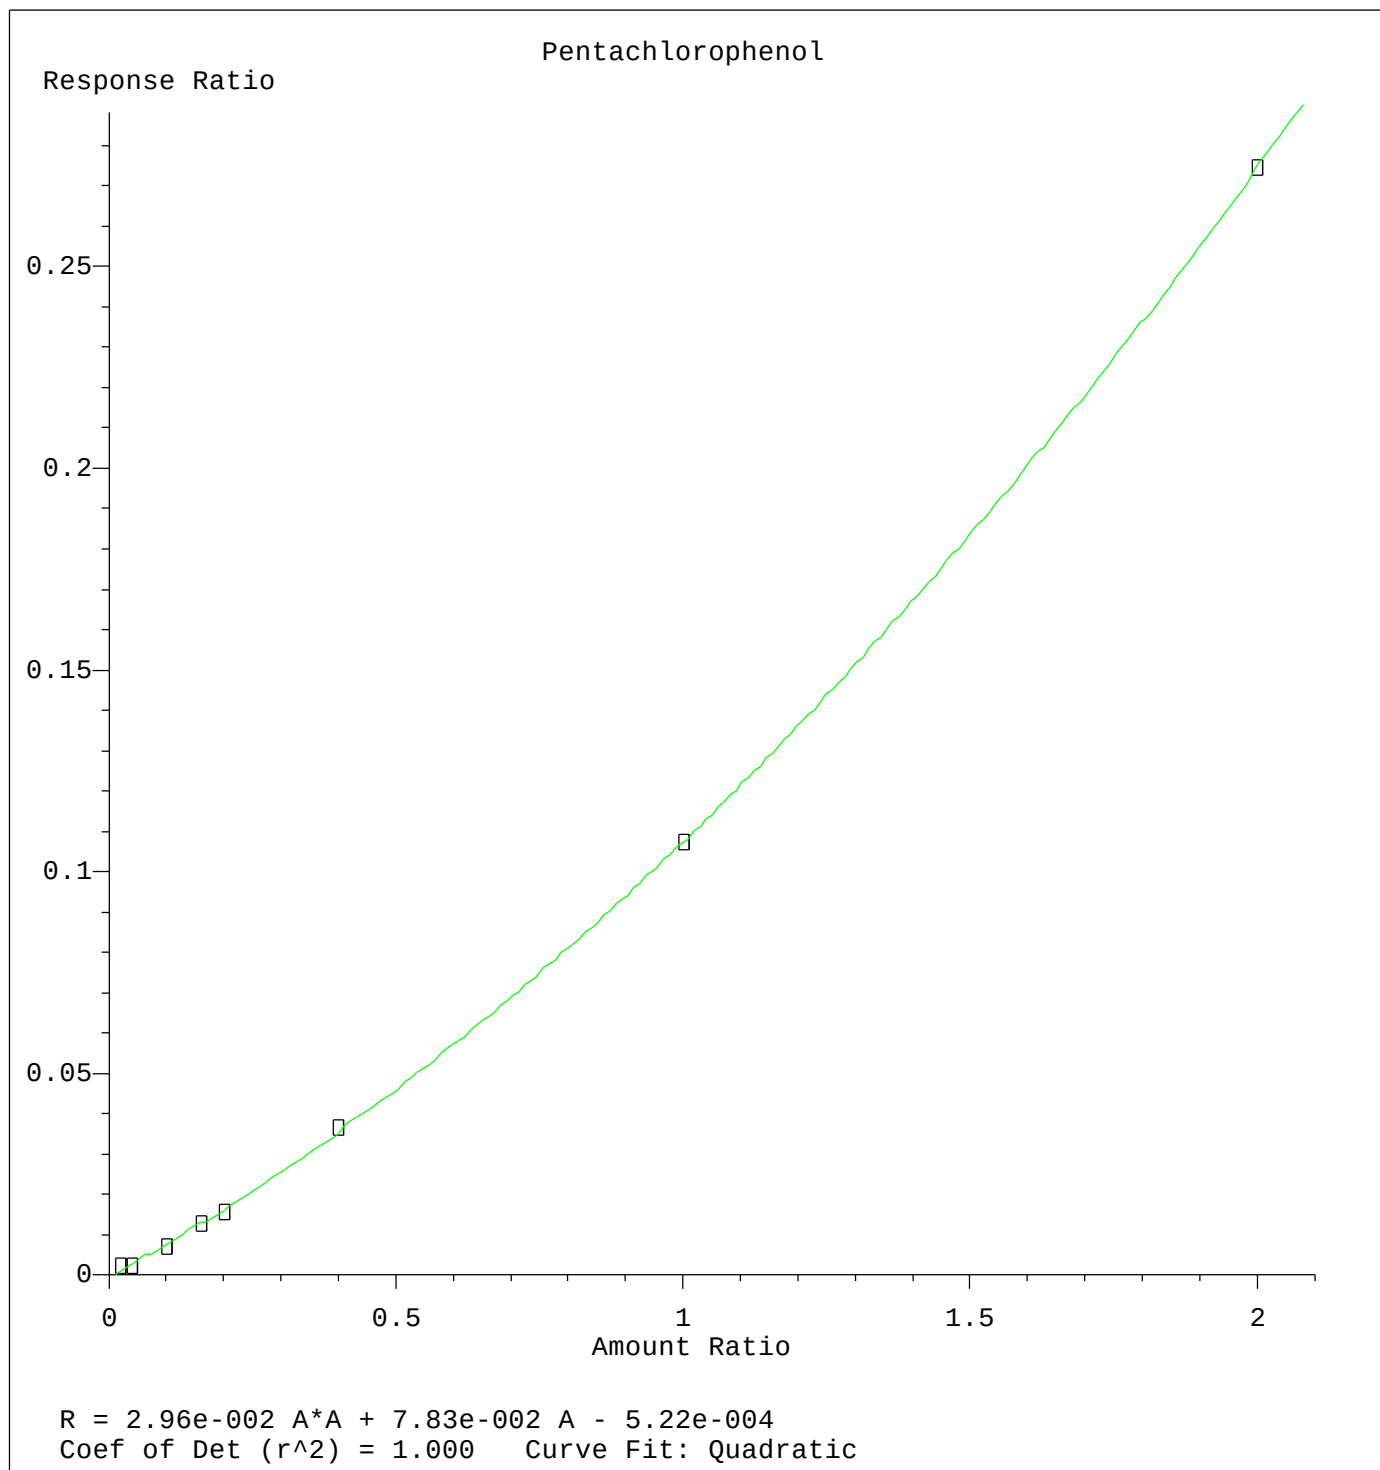


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:36:52 2015

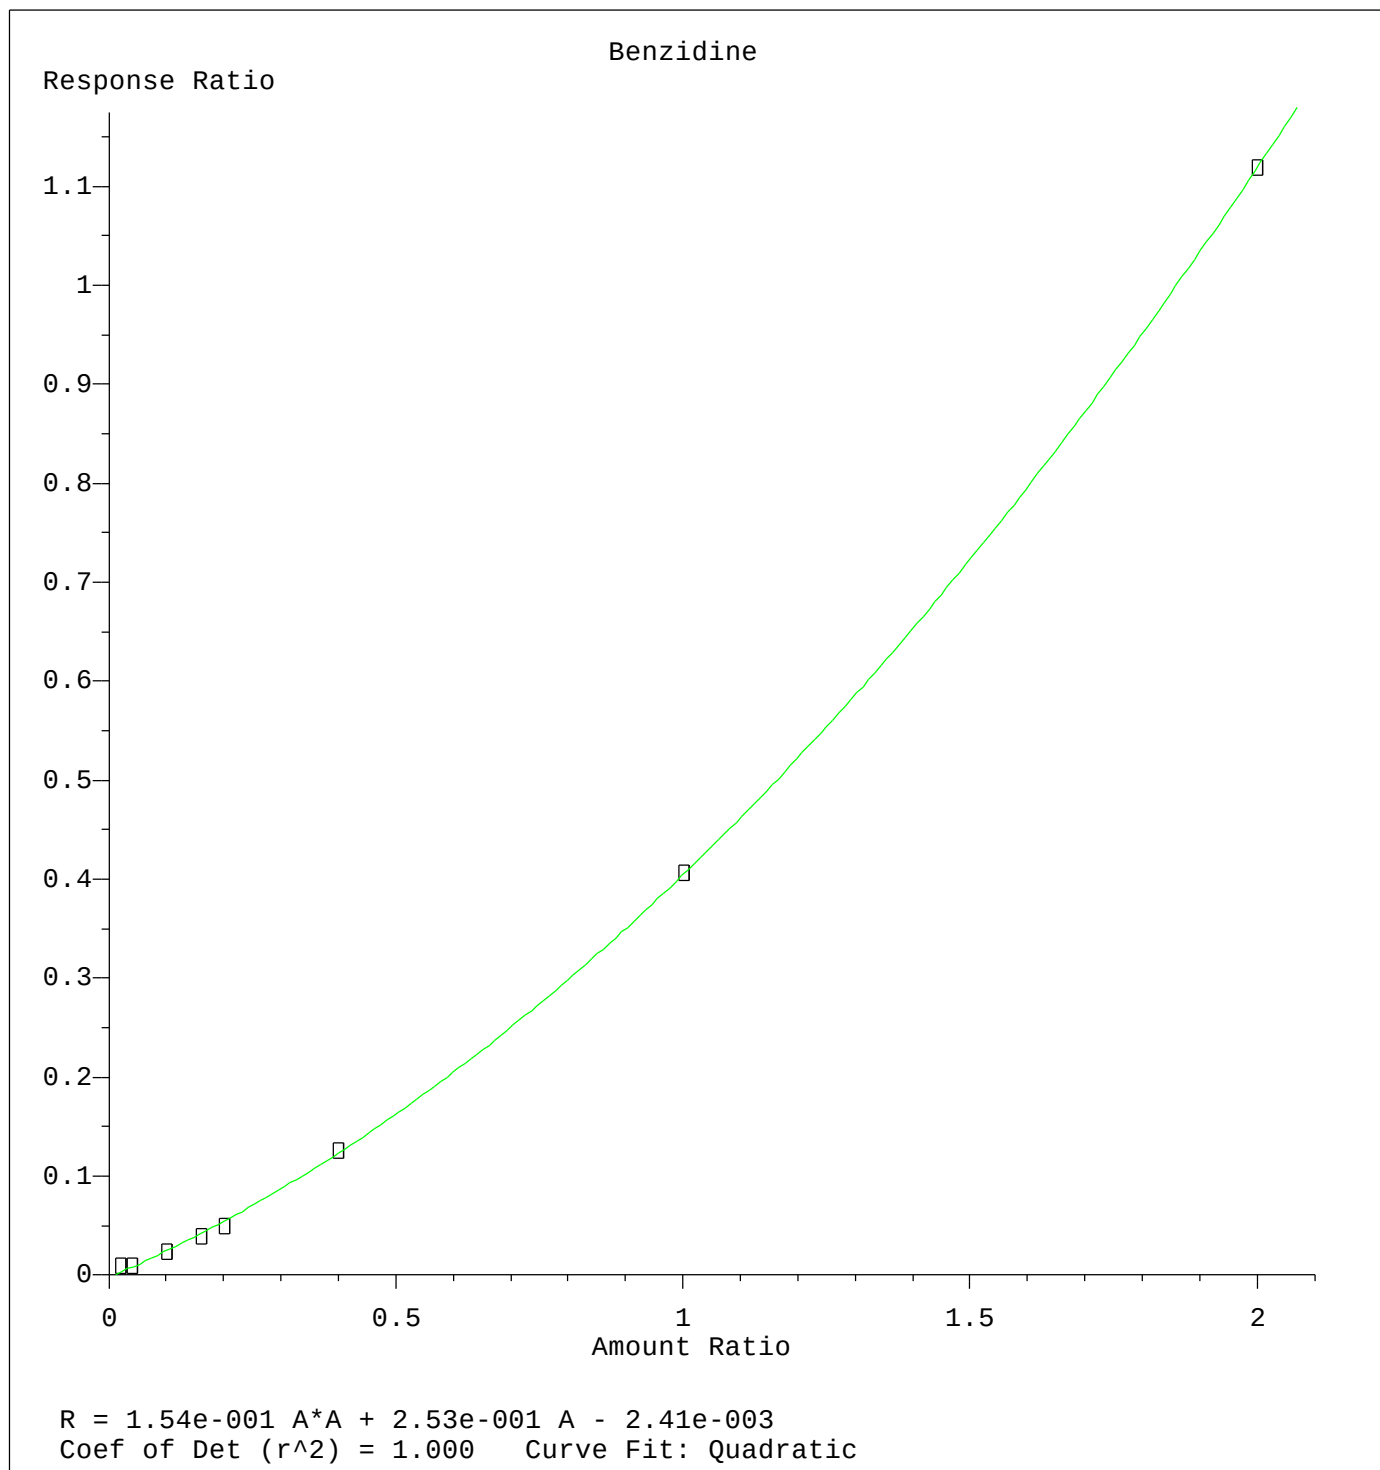

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:37:15 2015

3,3'-Dichlorobenzidine

Response Ratio

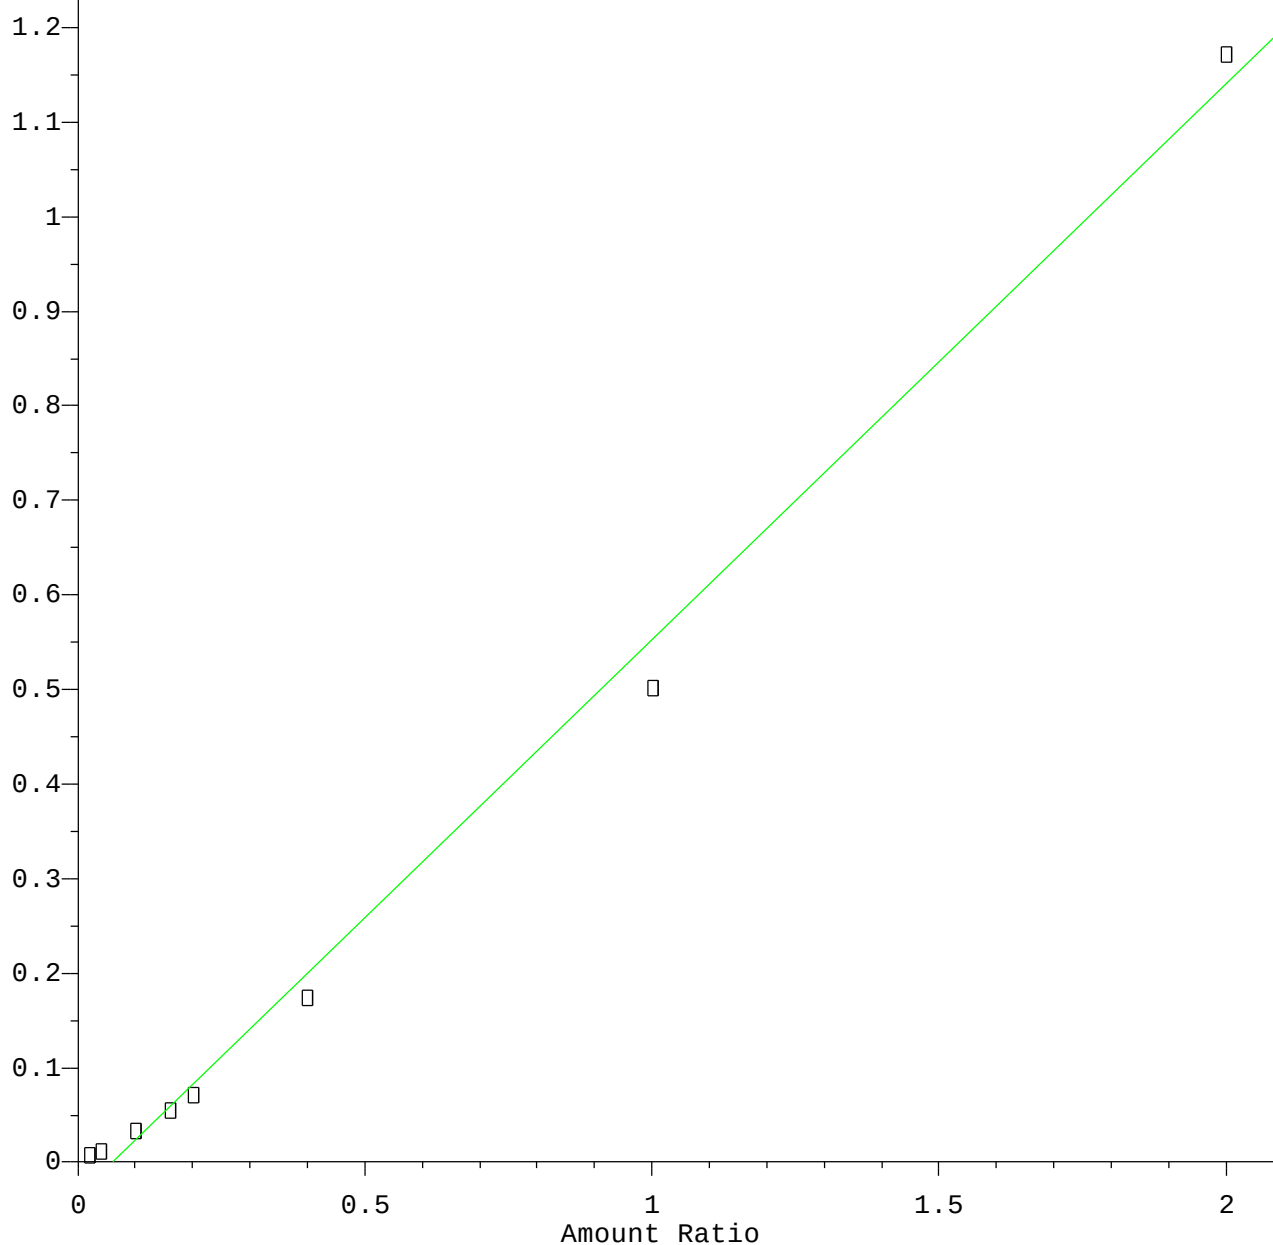

Resp Ratio = $5.88 \times 10^{-1} \times \text{Amt} - 3.56 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
Calibration Table Last Updated: Fri Apr 10 06:37:40 2015