

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
 Data File : BM019832.D
 Acq On : 09 Apr 2019 17:25
 Operator : JU/SJ
 Sample : PB118672BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK72

Quant Time: Apr 10 03:42:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	96668	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	392998	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	218229	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	476043	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	452449	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	460749	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.12	96	14512	5.88	ng/uL	0.00
5) Phenol-d5	6.75	99	233208	27.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	142678	24.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	186935	28.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	183577	28.41	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	86361	30.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	103169	33.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	168965	28.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	233132	32.97	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	558701	31.73	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	668656	30.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	66680	24.16	ng/ul	0.02
58) Fluorene-d10	15.22	176	457194	30.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	57912	18.40	ng/ul	0.00
71) Anthracene-d10	17.09	188	713763	31.24	ng/ul	0.00
79) Pyrene-d10	19.40	212	698201	33.41	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	700709	28.69	ng/ul	0.00


Target Compounds					Qvalue	
85) Chrysene	21.24	228	34195	1.309	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
Data File : BM019832.D
Acq On : 09 Apr 2019 17:25
Operator : JU/SJ
Sample : PB118672BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK72

Quant Time: Apr 10 03:42:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

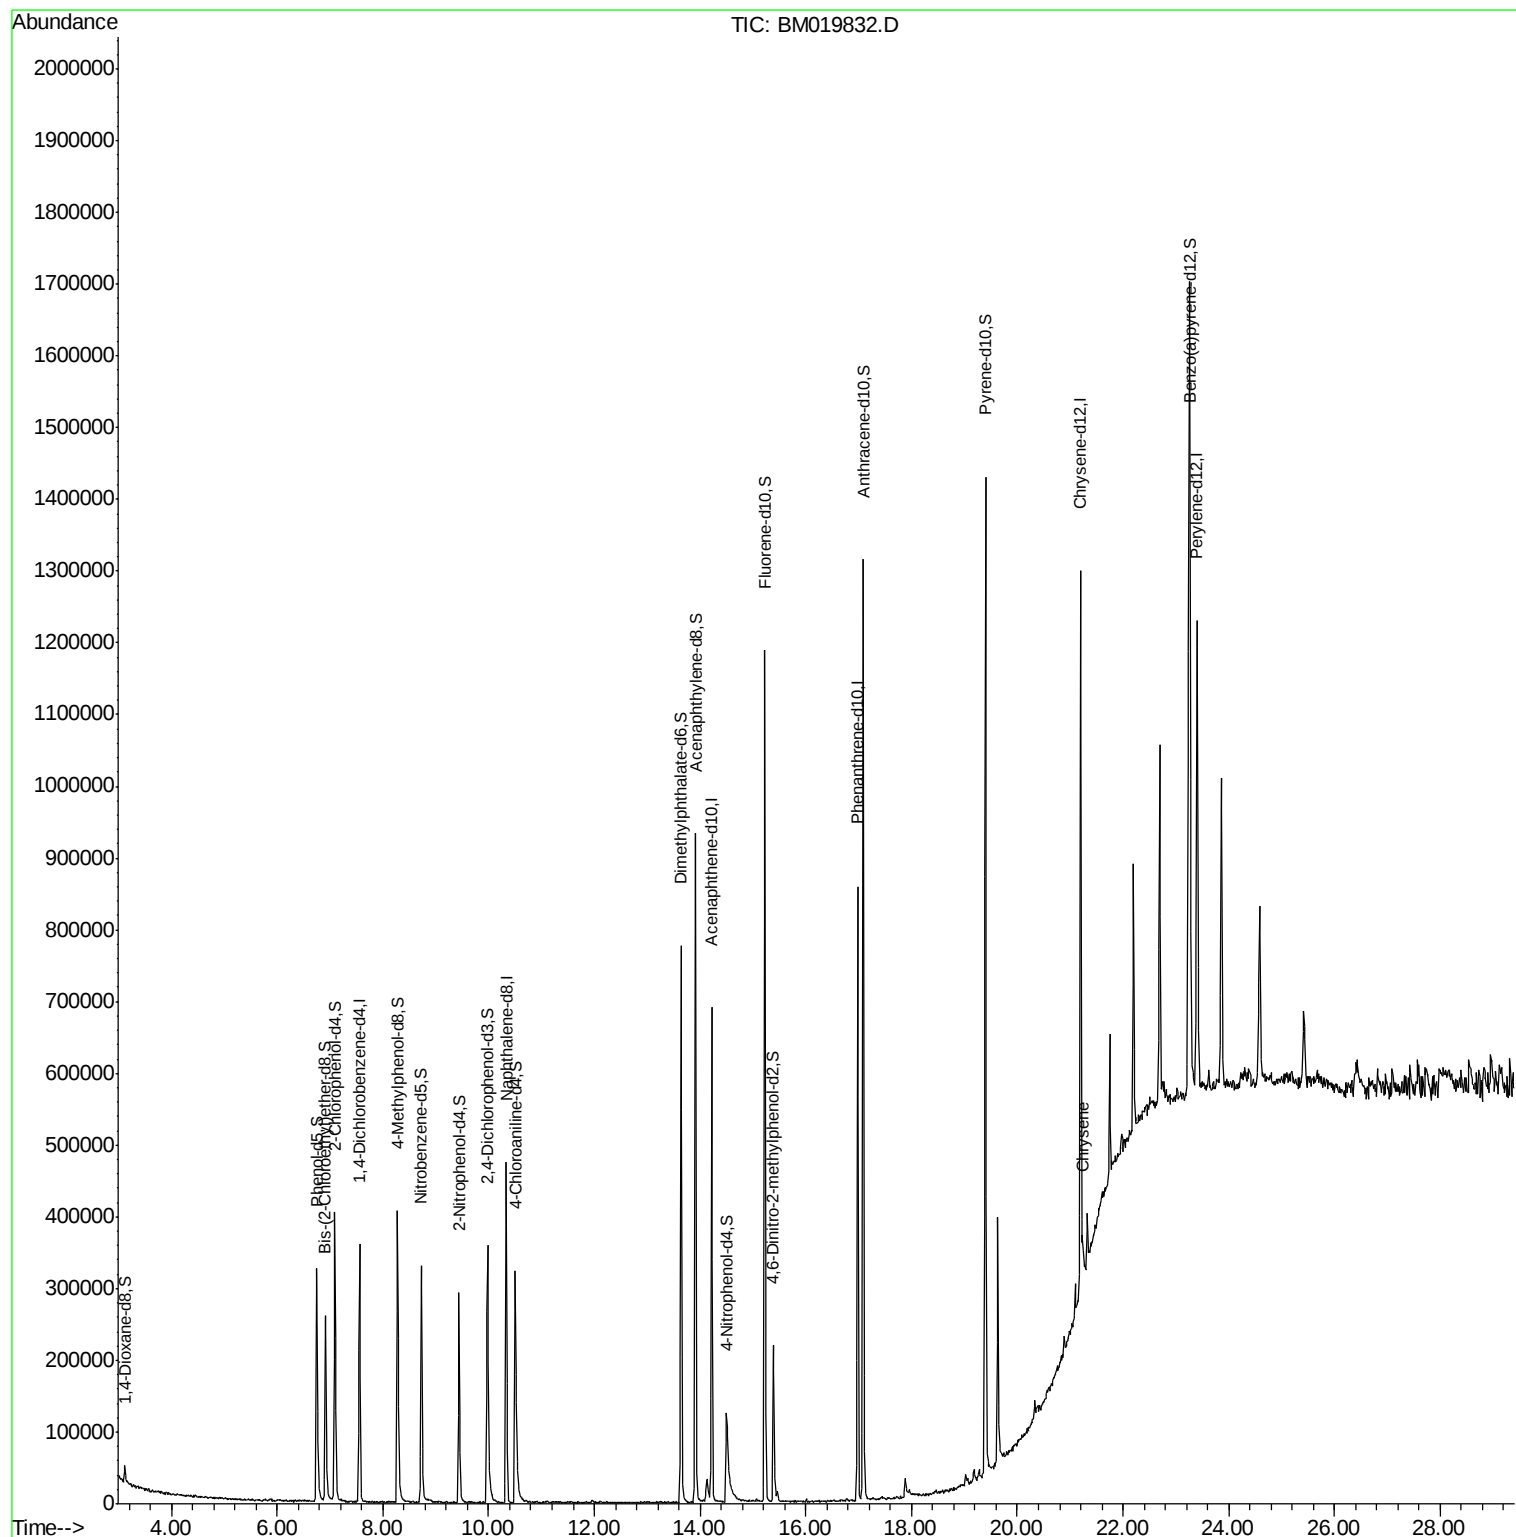

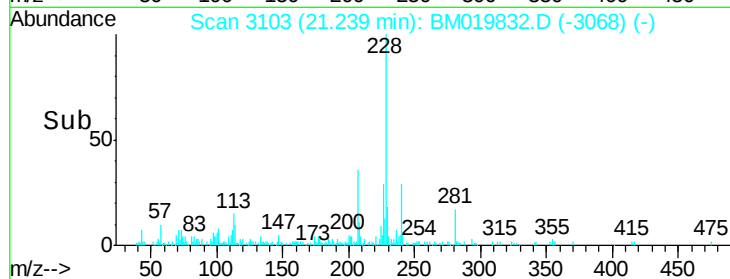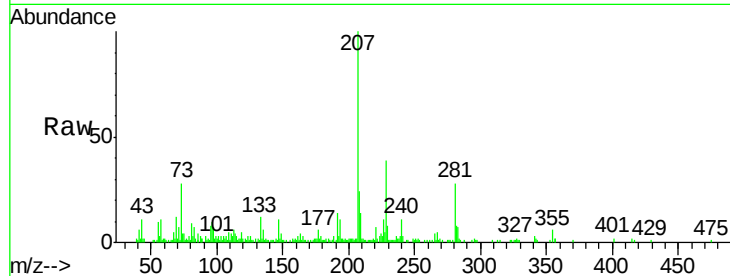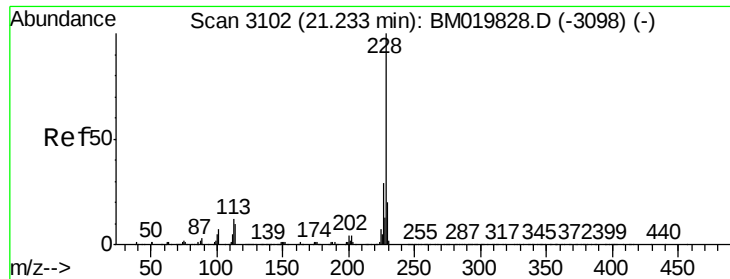

#85

Chrysene

Concen: 1.309 ng/ul

RT: 21.24 min Scan# 3103

Delta R.T. 0.01 min

Lab File: BM019832.D

Acq: 09 Apr 2019 17:25

Instrument :

BNA_M

ClientSampleId :

SBLK72

Tgt Ion:228 Resp: 34195

Ion Ratio Lower Upper

228 100

226 29.0 24.1 36.1

229 20.1 16.0 24.0

