

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
 Data File : BM019836.D
 Acq On : 09 Apr 2019 19:52
 Operator : JU/SJ
 Sample : K2255-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC54

Quant Time: Apr 10 03:42:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	111693	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	423763	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	211858	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	441989	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	463712	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	517730	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	17926	6.28	ng/uL	0.00
5) Phenol-d5	6.75	99	134943	13.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	92310	13.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	114521	15.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	85295	11.42	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	50561	16.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	57583	17.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	85161	13.42	ng/ul	0.01
29) 4-Chloroaniline-d4	10.52	131	111588	14.64	ng/ul	0.01
44) Dimethylphthalate-d6	13.65	166	286572	16.76	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	335273	15.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	15601	5.82	ng/ul	0.04
58) Fluorene-d10	15.22	176	226135	15.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	26381	9.03	ng/ul	0.00
71) Anthracene-d10	17.08	188	323382	15.25	ng/ul	0.00
79) Pyrene-d10	19.39	212	338957	15.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	391736	14.27	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	13.69	163	73476	4.284 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
Data File : BM019836.D
Acq On : 09 Apr 2019 19:52
Operator : JU/SJ
Sample : K2255-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC54

Quant Time: Apr 10 03:42:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

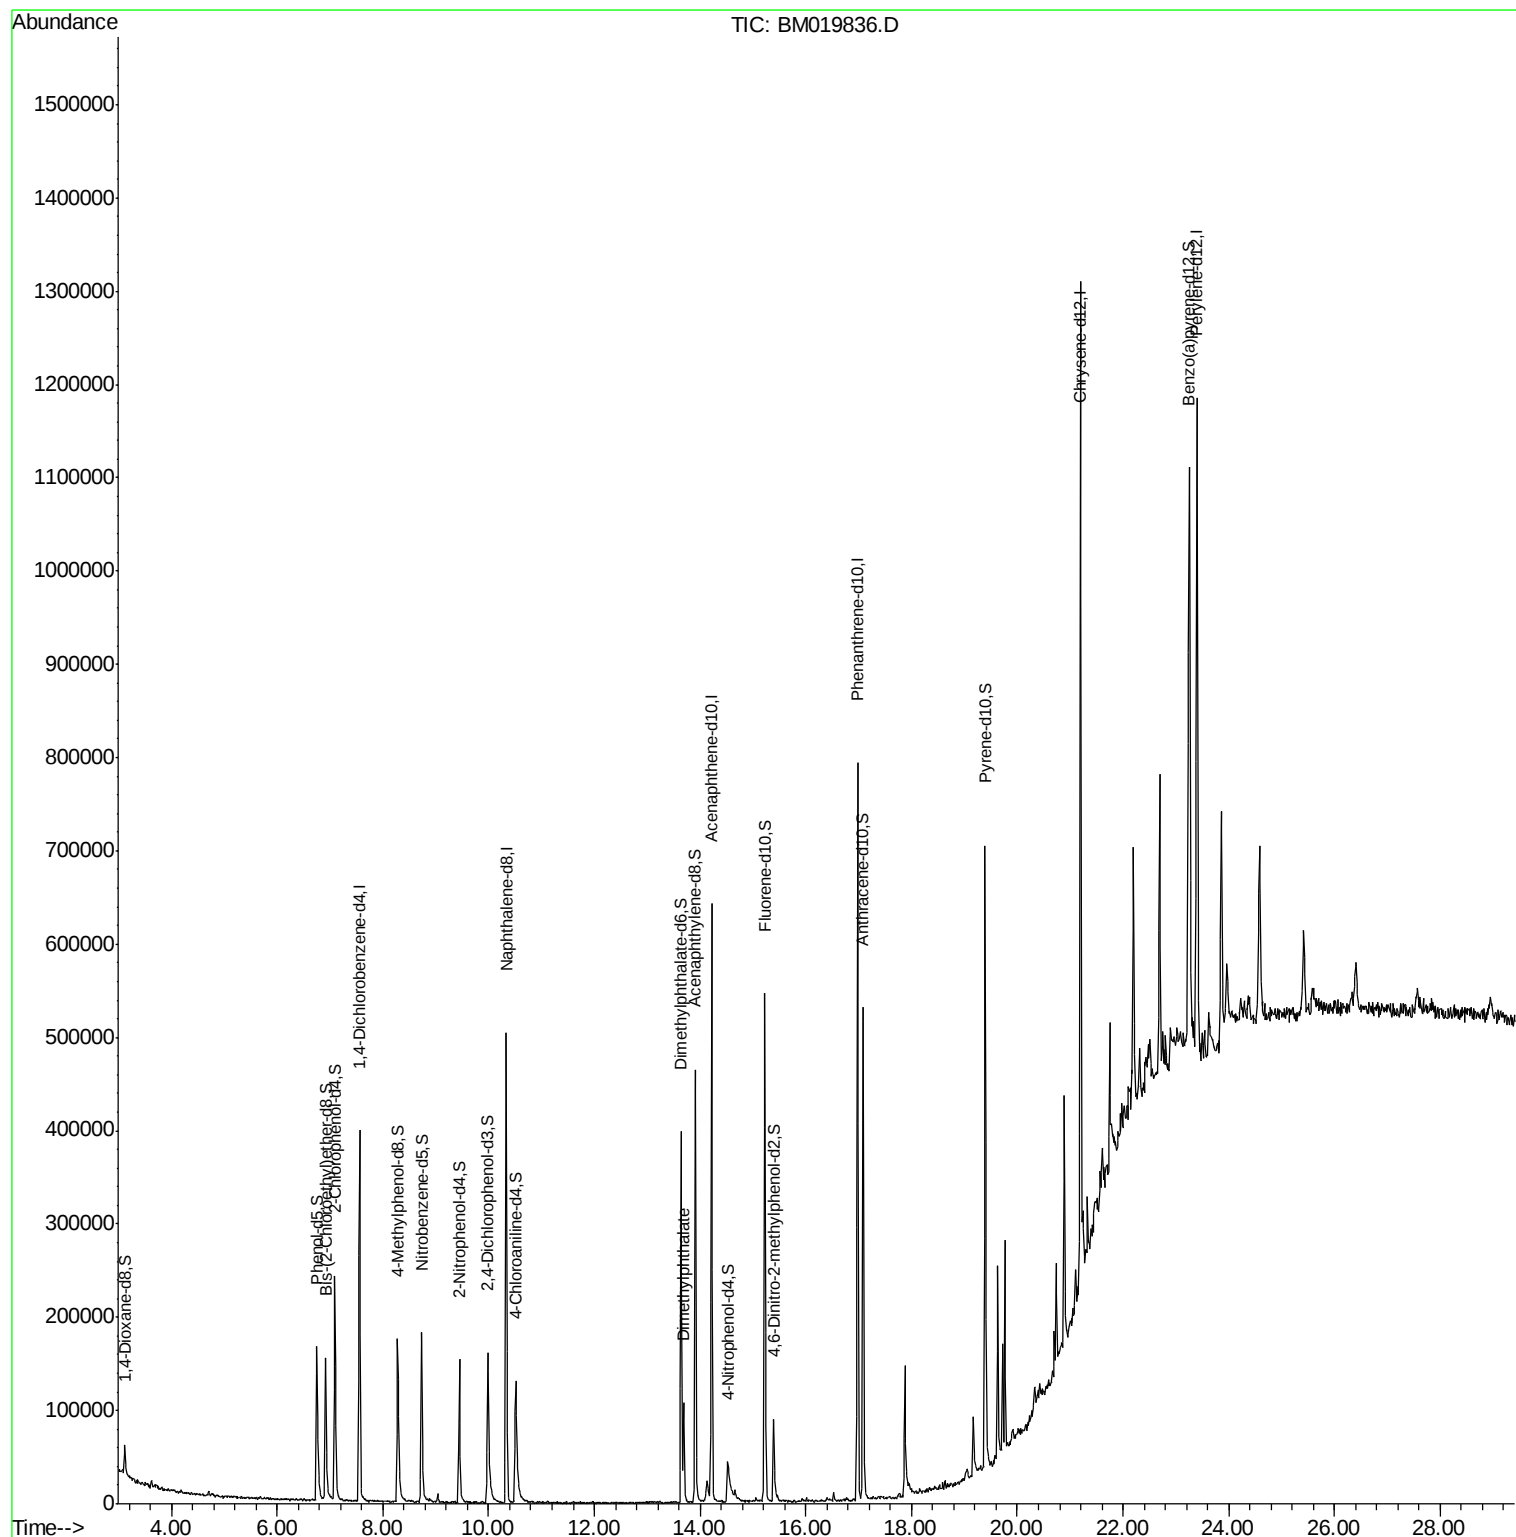

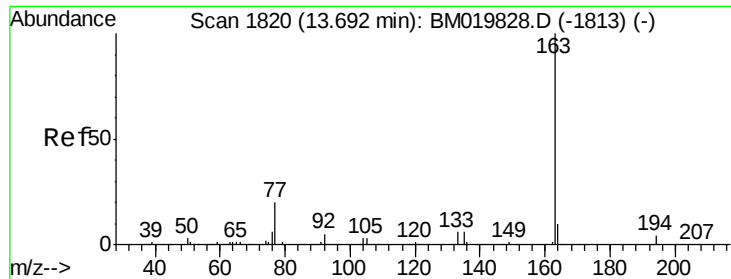

#45

Dimethylphthalate

Concen: 4.284 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. 0.00 min

Lab File: BM019836.D

Acq: 09 Apr 2019 19:52

Instrument :

BNA_M

ClientSampleId :

BFC54

Tgt Ion:163 Resp: 73476

Ion Ratio Lower Upper

163 100

194 4.2 4.0 6.0

164 10.0 8.4 12.6

