

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
 Data File : BM019838.D
 Acq On : 09 Apr 2019 21:05
 Operator : JU/SJ
 Sample : K2255-23
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC50

Quant Time: Apr 10 03:43:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	122244	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	480216	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	239983	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	494011	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	535362	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	604141	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	19983	6.40	ng/uL	0.00
5) Phenol-d5	6.75	99	136192	12.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	95807	13.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	119471	14.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	107207	13.12	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	49989	14.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	58394	15.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	88693	12.33	ng/ul	0.01
29) 4-Chloroaniline-d4	10.52	131	124633	14.43	ng/ul	0.01
44) Dimethylphthalate-d6	13.64	166	302827	15.64	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	358000	14.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	14221	4.69	ng/ul	0.05
58) Fluorene-d10	15.22	176	246920	14.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	16131	4.94	ng/ul	0.01
71) Anthracene-d10	17.08	188	369661	15.59	ng/ul	0.00
79) Pyrene-d10	19.39	212	377739	15.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	435647	13.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	86027	4.428	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
Data File : BM019838.D
Acq On : 09 Apr 2019 21:05
Operator : JU/SJ
Sample : K2255-23
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC50

Quant Time: Apr 10 03:43:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

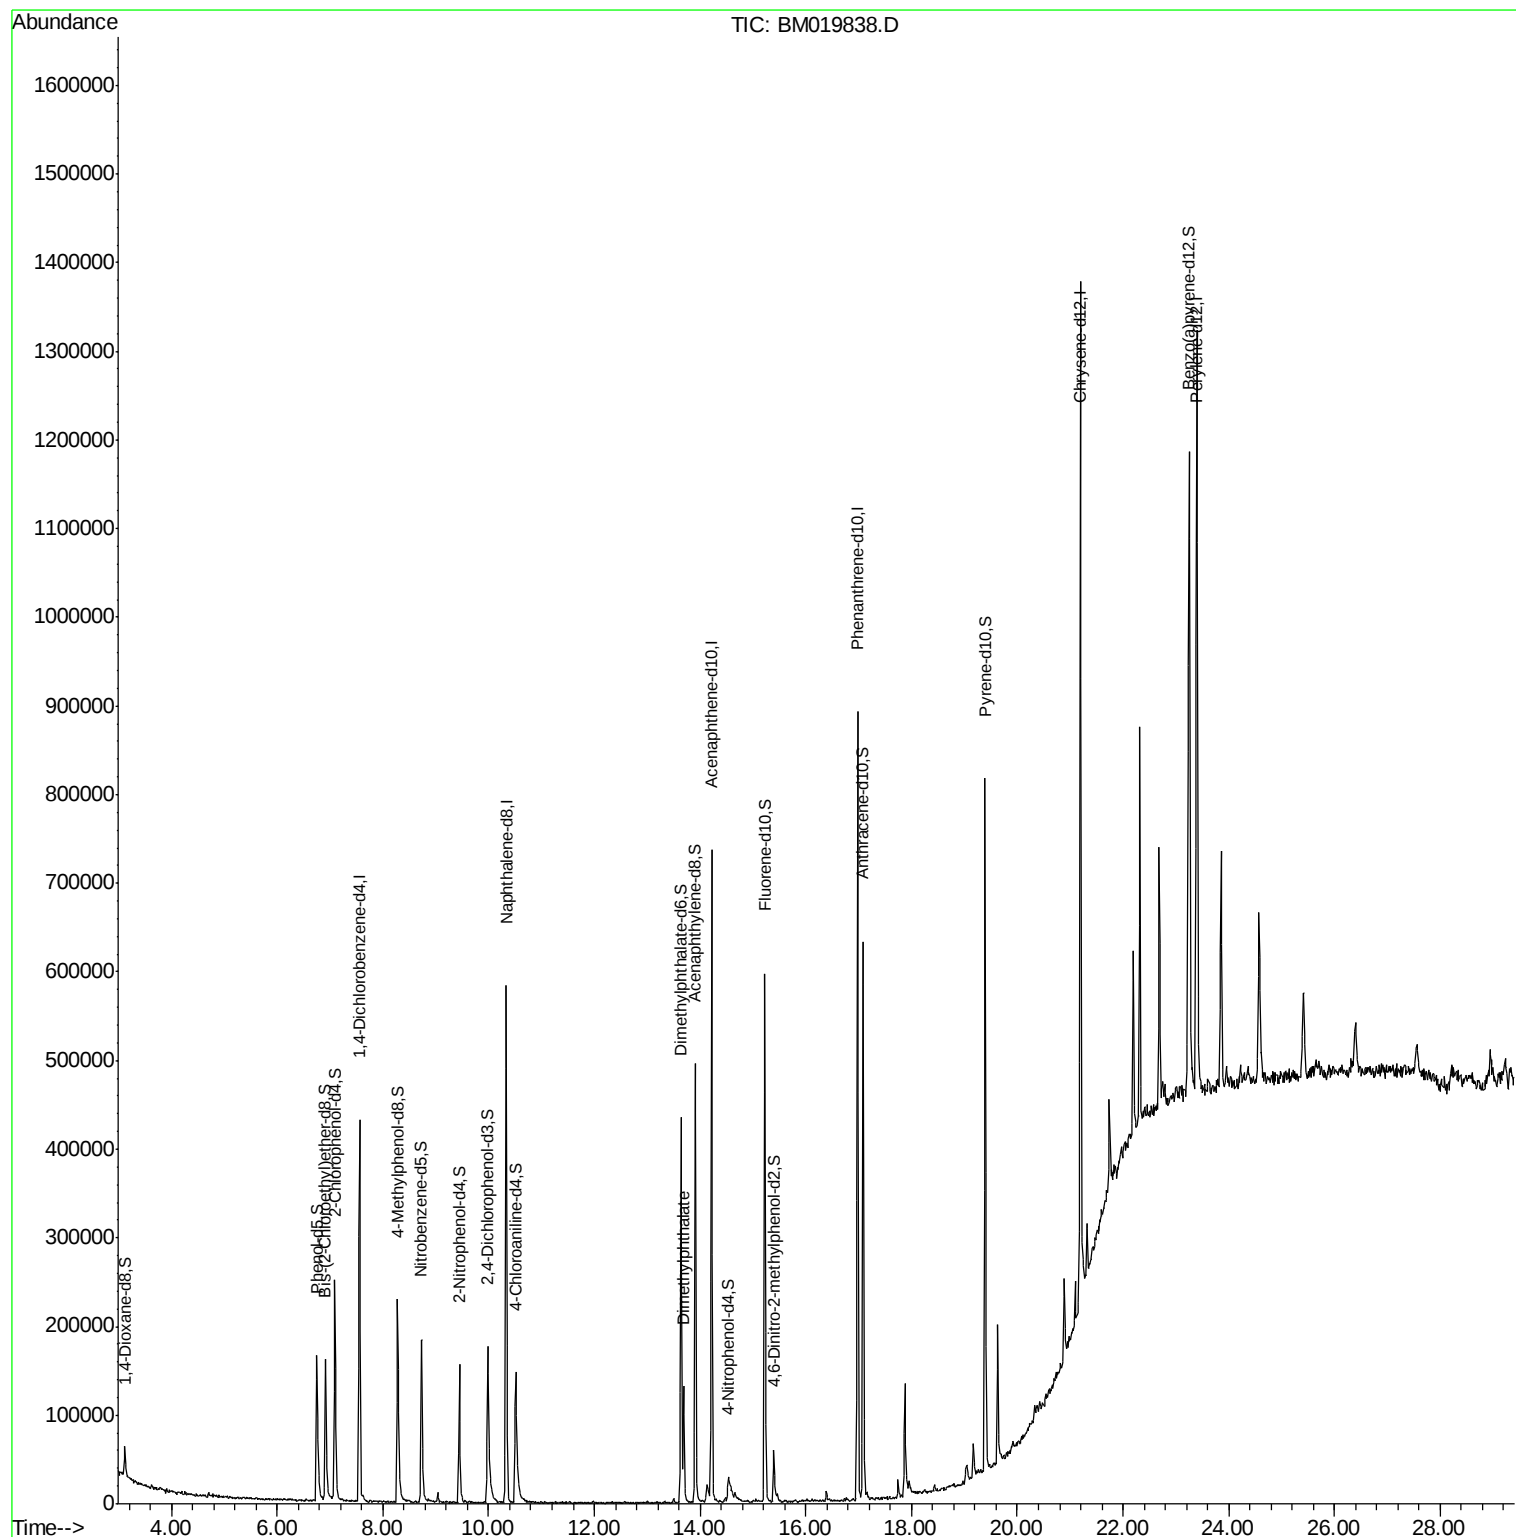

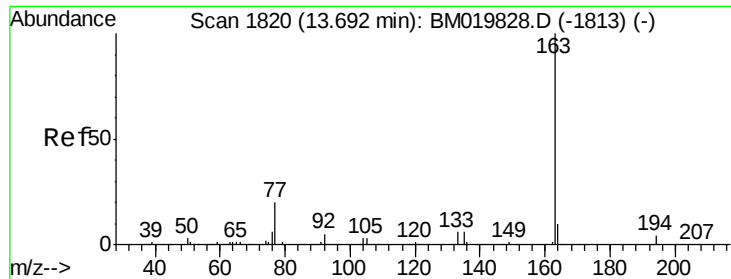

#45

Dimethylphthalate

Concen: 4.428 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BM019838.D

Acq: 09 Apr 2019 21:05

Instrument :

BNA_M

ClientSampleId :

BFC50


Tgt Ion:163 Resp: 86027

Ion Ratio Lower Upper

163 100

194 3.9 4.0 6.0#

164 9.5 8.4 12.6

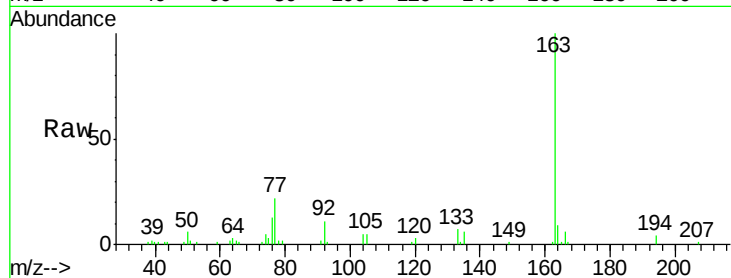

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

