


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
Data File : BM019852.D
Acq On : 10 Apr 2019 05:46
Operator : JU/SJ
Sample : K2255-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC35

Manual Integrations
APPROVED

Sohil
4/10/2019 6:19:11 PM

Quant Time: Apr 10 06:40:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

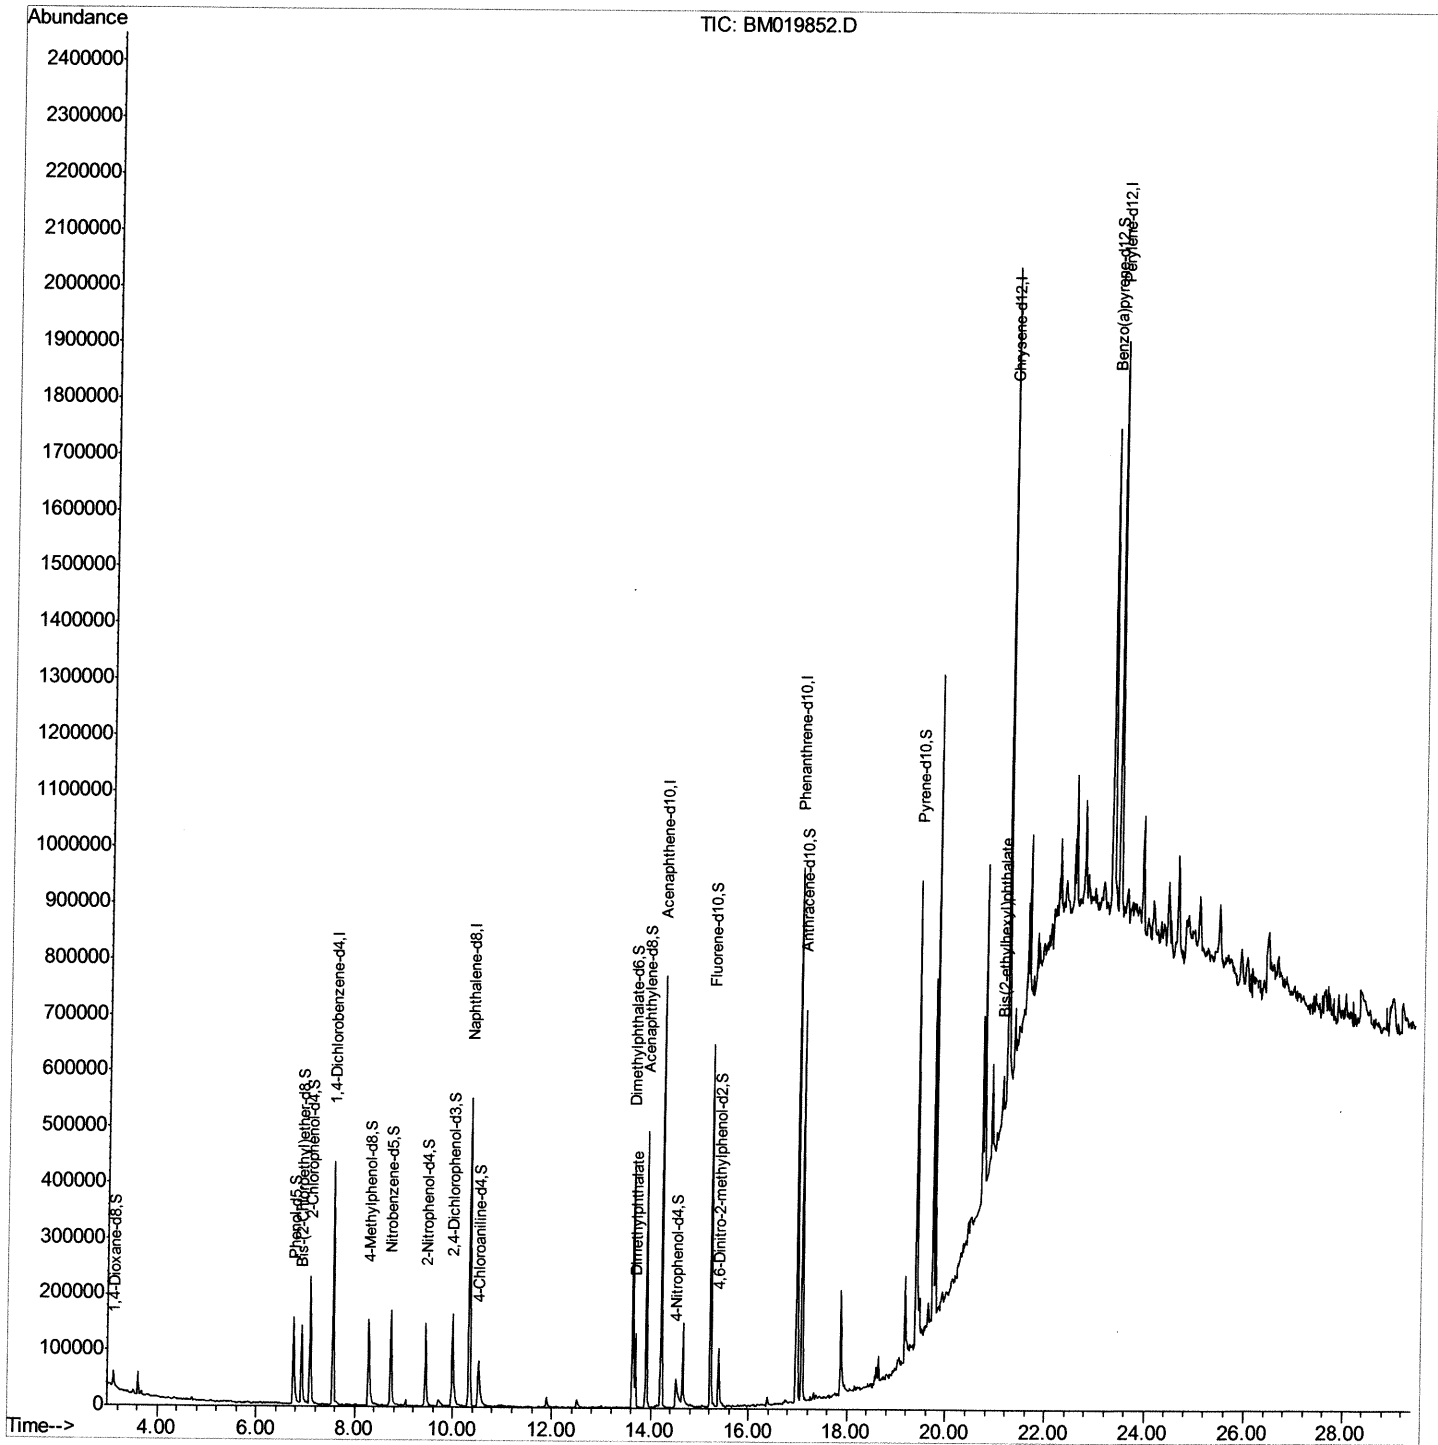

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
Data File : BM019852.D
Acq On : 10 Apr 2019 05:46
Operator : JU/SJ
Sample : K2255-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC35

Manual Integrations
APPROVED

Sohil
4/10/2019 6:19:11 PM

Quant Time: Apr 10 06:38:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

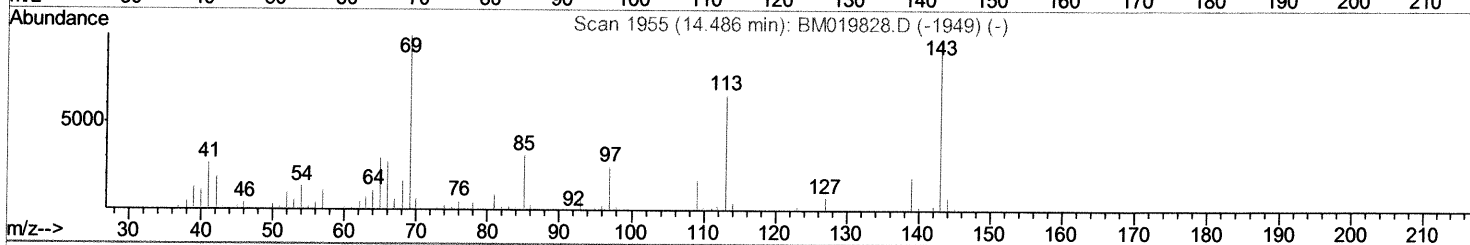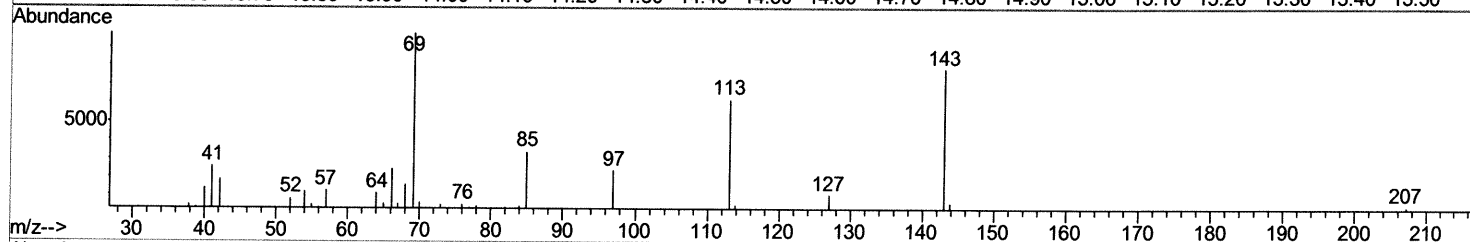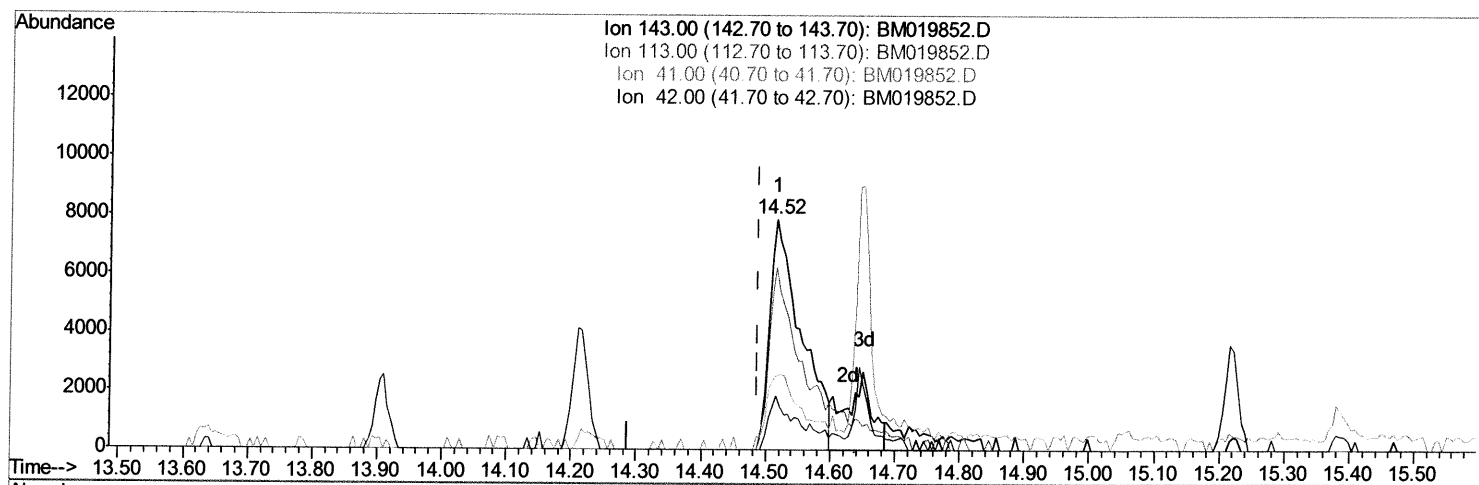

TIC: BM019852.D

(52) 4-Nitrophenol-d4 (S)

14.516min (+0.029) 8.80ng/ul

response 26836

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	79.01
41.00	32.60	32.45
42.00	22.30	23.49

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
 Data File : BM019852.D
 Acq On : 10 Apr 2019 05:46
 Operator : JU/SJ
 Sample : K2255-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC35

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:19:11 PM

Quant Time: Apr 10 06:38:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

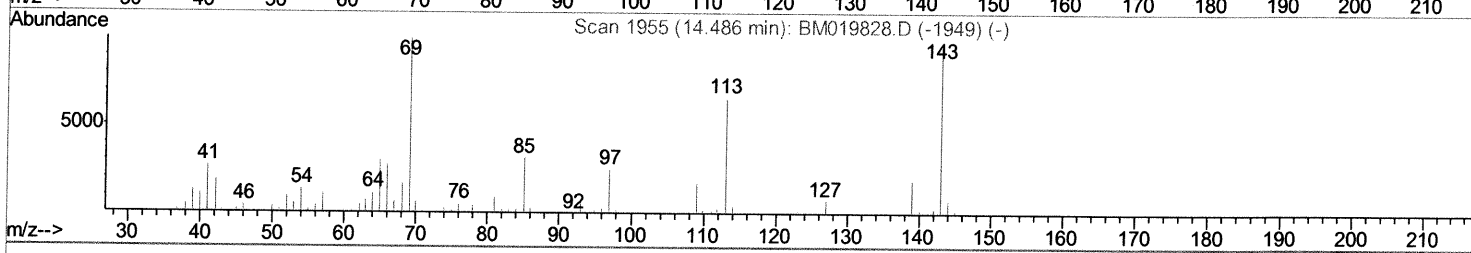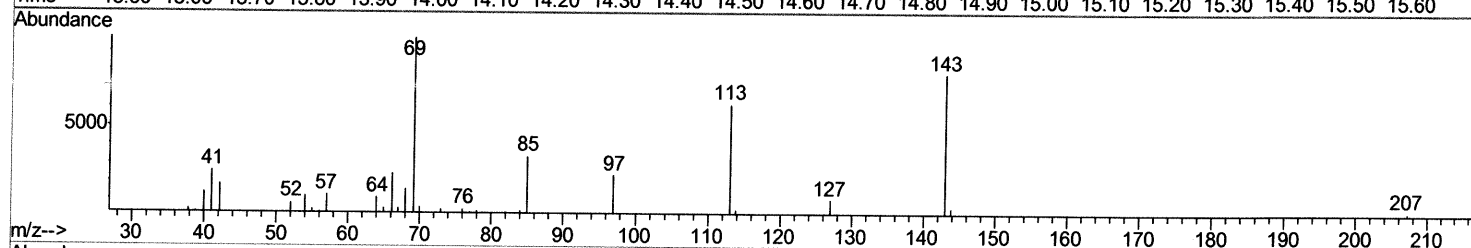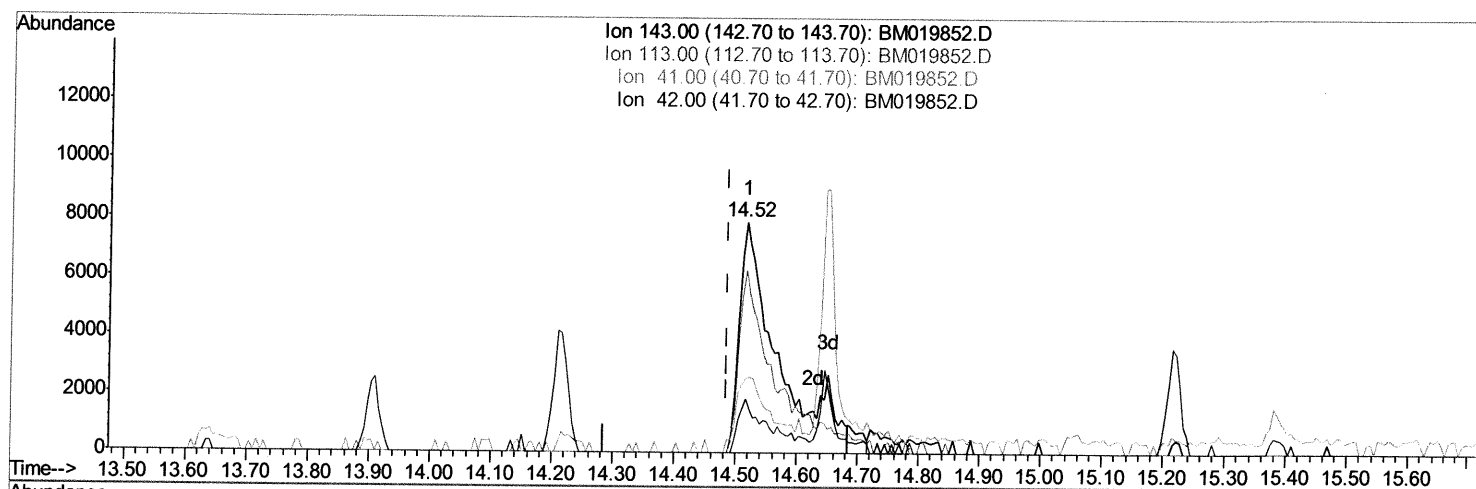

TIC: BM019852.D

(52) 4-Nitrophenol-d4 (S)

14.516min (+0.029) 11.72ng/ul m > SJ 4/16/19

response 35728

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	79.01
41.00	32.60	32.45
42.00	22.30	23.49

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040919\
 Data File : BM019852.D
 Acq On : 10 Apr 2019 05:46
 Operator : JU/SJ
 Sample : K2255-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BFC35

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:19:11 PM

Quant Time: Apr 10 06:40:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	116682	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	466385	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	241060	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	515713	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	585519	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	695815	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.12	96	18865	6.33	ng/uL	0.00
5) Phenol-d5	6.75	99	123545	11.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	81558	11.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	106528	13.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	79454	10.19	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	47018	14.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	56775	15.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	91713	13.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	71260	8.49	ng/ul	0.01
44) Dimethylphthalate-d6	13.64	166	306537	15.76	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	355958	14.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	35728m	11.72	ng/ul	0.03
58) Fluorene-d10	15.22	176	259641	15.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	28220	8.27	ng/ul	0.00
71) Anthracene-d10	17.08	188	380984	15.39	ng/ul	0.00
79) Pyrene-d10	19.39	212	410723	15.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	497134	13.48	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.69	163	84247	4.317	ng/ul#	97
84) Bis(2-ethylhexyl)phthalate	21.09	149	24943	1.234	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

52 4116119