

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040919\
 Data File : BM019841.D
 Acq On : 09 Apr 2019 22:56
 Operator : JU/SJ
 Sample : K2273-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC53

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:19:01 PM

Quant Time: Apr 10 04:29:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	113876	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	423230	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	219960	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	425874	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	444900	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	519252	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	24742	8.51	ng/uL	0.00
5) Phenol-d5	6.75	99	219663	21.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	141219	20.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	182864	23.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	169270	22.24	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	80464	26.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	91250	27.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	155734	24.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	203163	26.68	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	450984	25.41	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	561316	25.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	41310m	14.85	ng/ul	0.03
58) Fluorene-d10	15.22	176	384070	25.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	36419	12.93	ng/ul	0.00
71) Anthracene-d10	17.08	188	558891	27.35	ng/ul	0.00
79) Pyrene-d10	19.39	212	574437	27.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	698792	25.39	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.69	163	97381	5.469	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040919\
Data File : BM019841.D
Acq On : 09 Apr 2019 22:56
Operator : JU/SJ
Sample : K2273-05
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BFC53

Manual Integrations
APPROVED

Sohil
4/10/2019 6:19:01 PM

Quant Time: Apr 10 04:29:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

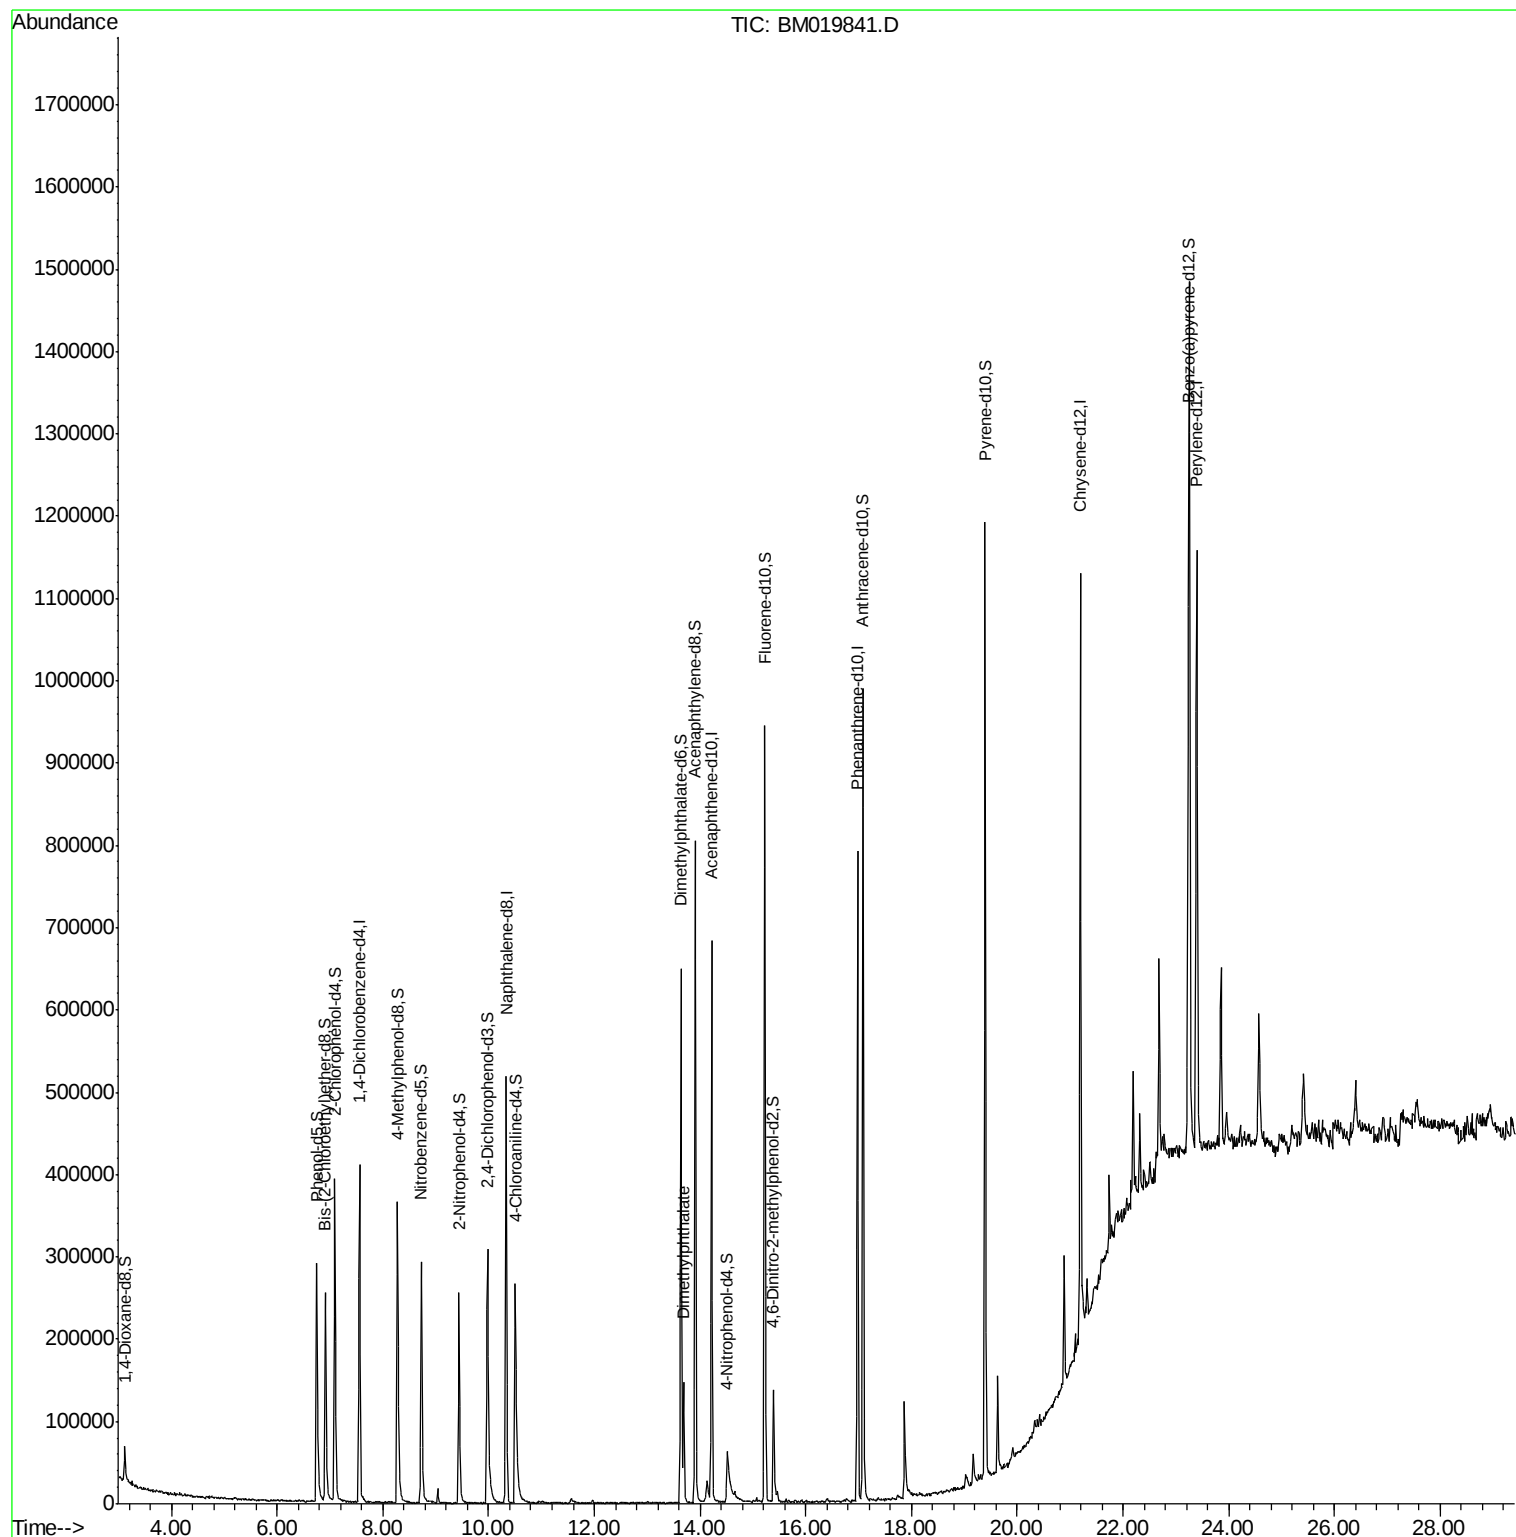

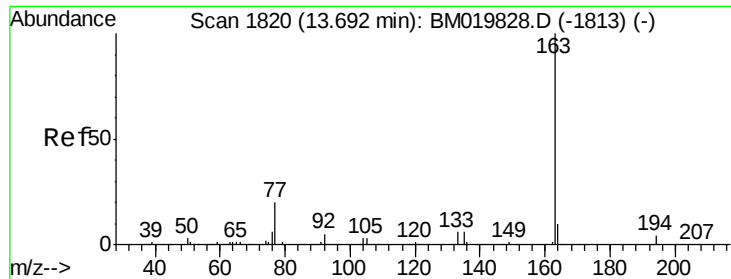

#45
 Dimethylphthalate
 Concen: 5.469 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BM019841.D
 Acq: 09 Apr 2019 22:56

Instrument :
 BNA_M
 ClientSampleId :
 BFC53

Tot Ion	Ratio	Resp	Lower	Upper
163	100	97381		
194	4.0		4.0	6.0#
164	9.6		8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:19:01 PM

