

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040919\
 Data File : BM019843.D
 Acq On : 10 Apr 2019 00:12
 Operator : JU/SJ
 Sample : K2304-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF891

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:19:03 PM

Quant Time: Apr 10 04:33:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 10 03:34:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	107092	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	414517	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	207631	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	423489	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	459691	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	522632	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	25495	9.32	ng/uL	0.00
5) Phenol-d5	6.75	99	182318	19.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	120965	18.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	155161	21.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	141991	19.84	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	70994	24.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	77777	23.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	127155	20.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	159516	21.39	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	390688	23.32	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	450557	21.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	45146m	17.19	ng/ul	0.03
58) Fluorene-d10	15.22	176	318581	22.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	41934	14.97	ng/ul	0.00
71) Anthracene-d10	17.08	188	446221	21.96	ng/ul	0.00
79) Pyrene-d10	19.39	212	471436	22.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	548853	19.81	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.69	163	80628	4.797	ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040919\
Data File : BM019843.D
Acq On : 10 Apr 2019 00:12
Operator : JU/SJ
Sample : K2304-06
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BF891

Manual Integrations
APPROVED

Sohil
4/10/2019 6:19:03 PM

Quant Time: Apr 10 04:33:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 10 03:34:56 2019
Response via : Initial Calibration

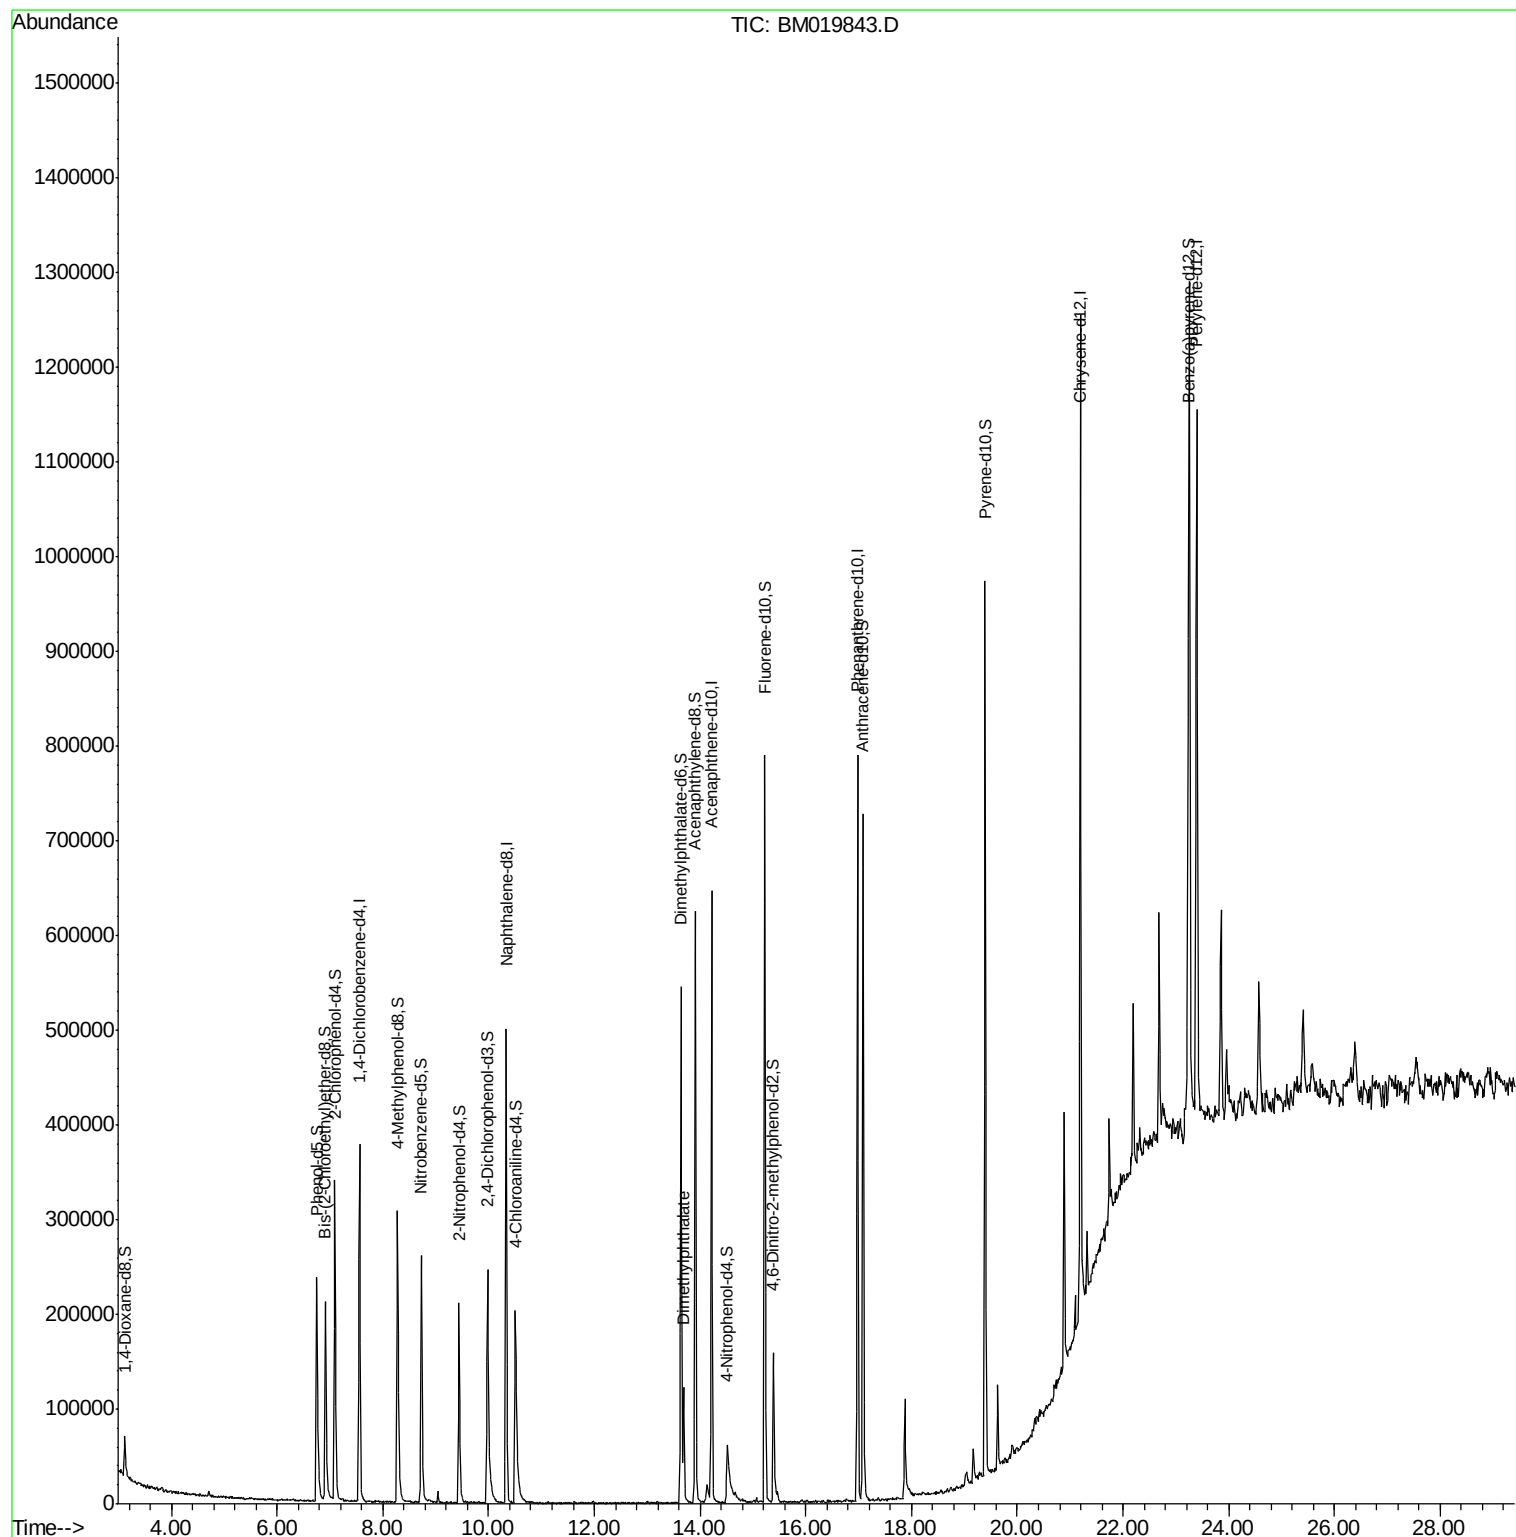

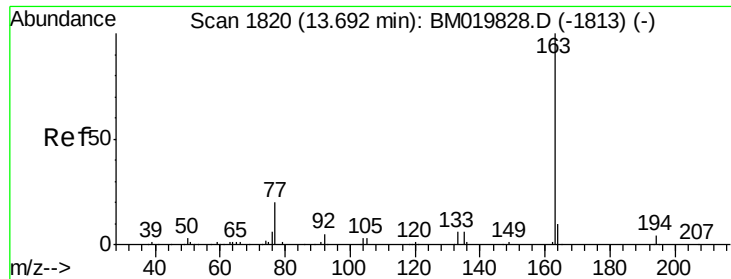

#45
 Dimethylphthalate
 Concen: 4.797 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BM019843.D
 Acq: 10 Apr 2019 00:12

Instrument :
 BNA_M
 ClientSampleId :
 BF891

Tot Ion	Ratio	Resp	Lower	Upper
163	100	80628		
194	3.7		4.0	6.0#
164	10.0		8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:19:03 PM

