


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041023\
 Data File : BM039370.D
 Acq On : 10 Apr 2023 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 11 16:05:42 2023

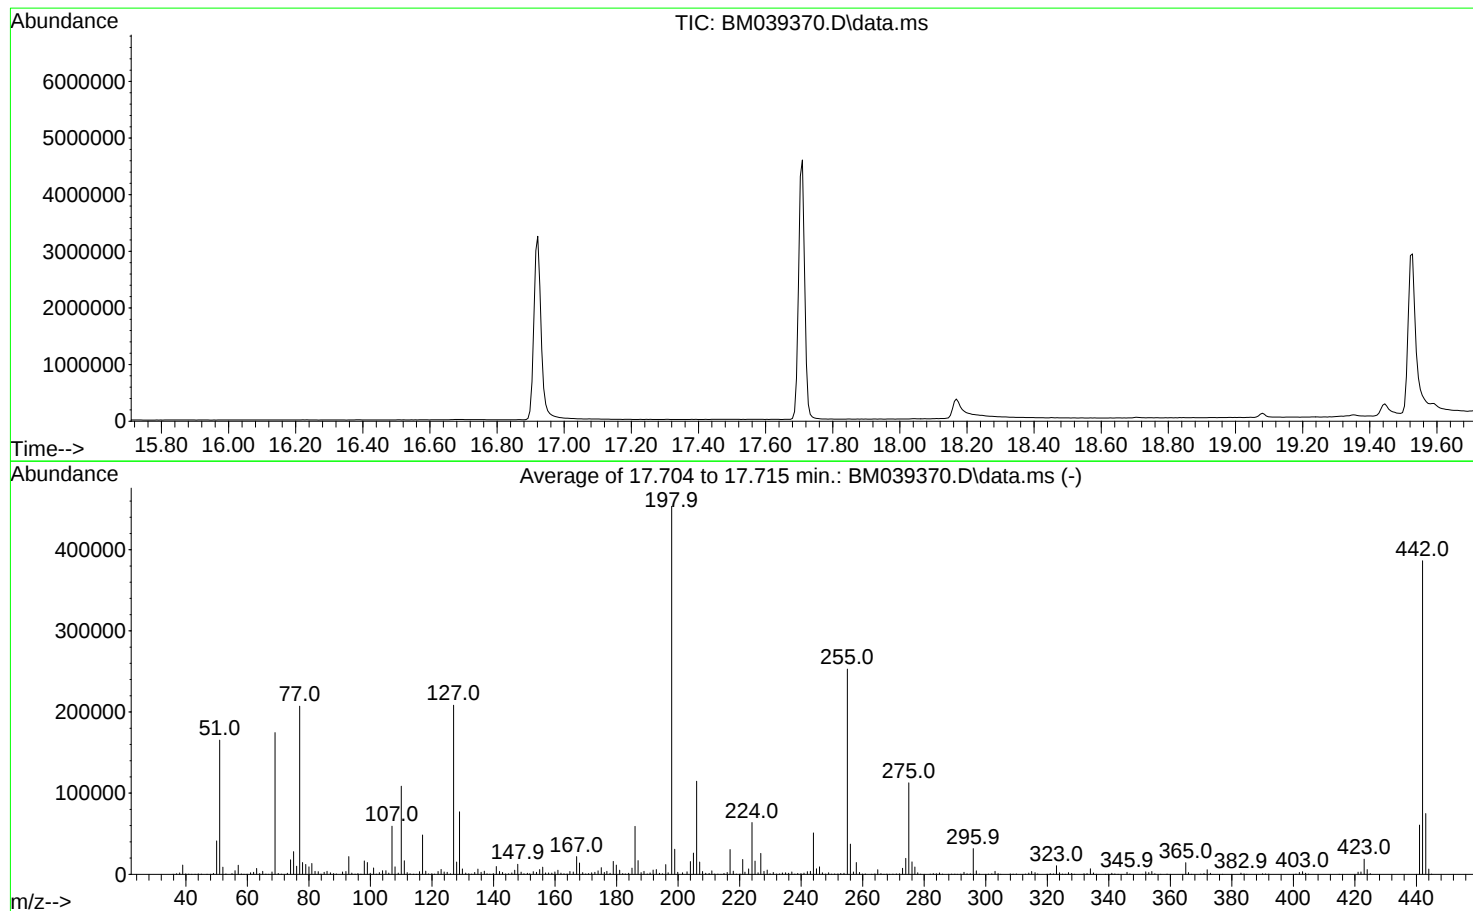




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	165442	PASS
68	69	0.00	2	1.6	2863	PASS
69	198	0.00	100	38.5	174686	PASS
70	69	0.00	2	0.6	1041	PASS
127	198	10	80	45.9	208256	PASS
197	198	0.00	2	0.4	1913	PASS
198	198	100	100	100.0	453376	PASS
199	198	5	9	6.8	30912	PASS
275	198	10	60	24.9	112712	PASS
365	198	1	100	3.2	14325	PASS
441	198	0.01	100	13.4	60565	PASS
442	442	50	100	100.0	386389	PASS
443	442	15	24	19.4	74899	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041023\
 Data File : BM039370.D
 Acq On : 10 Apr 2023 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 11 03:56:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 11 02:05:37 2023
 Response via : Initial Calibration

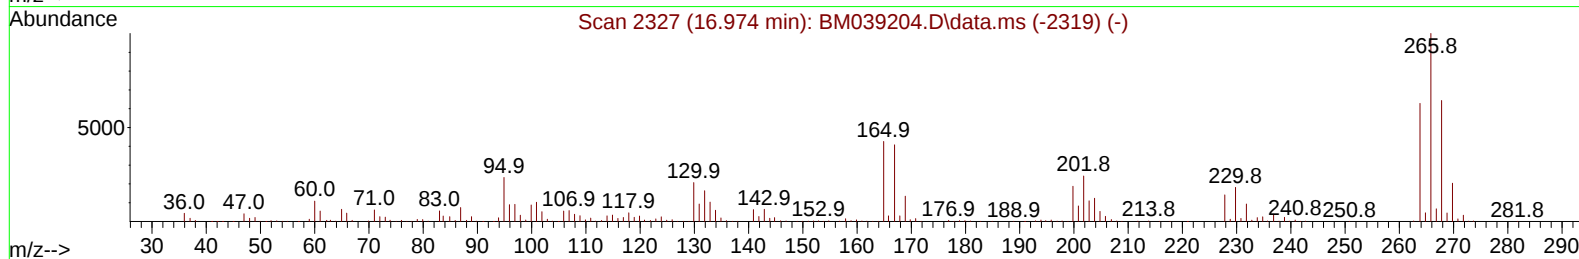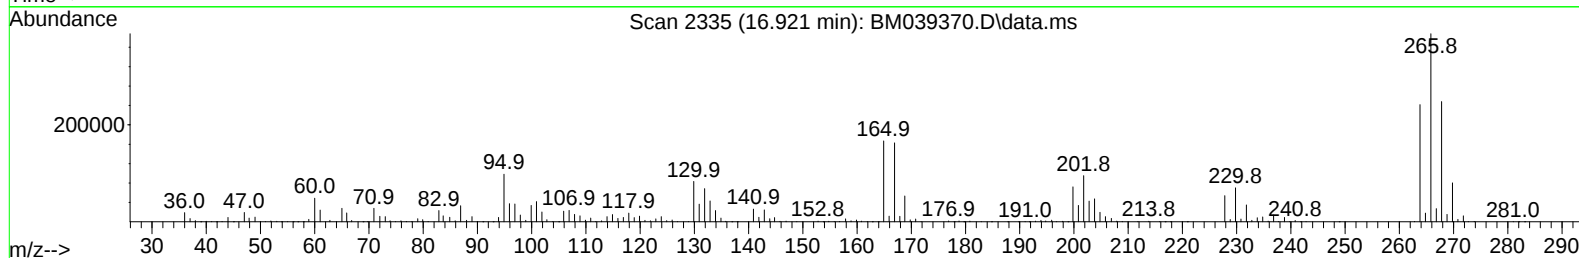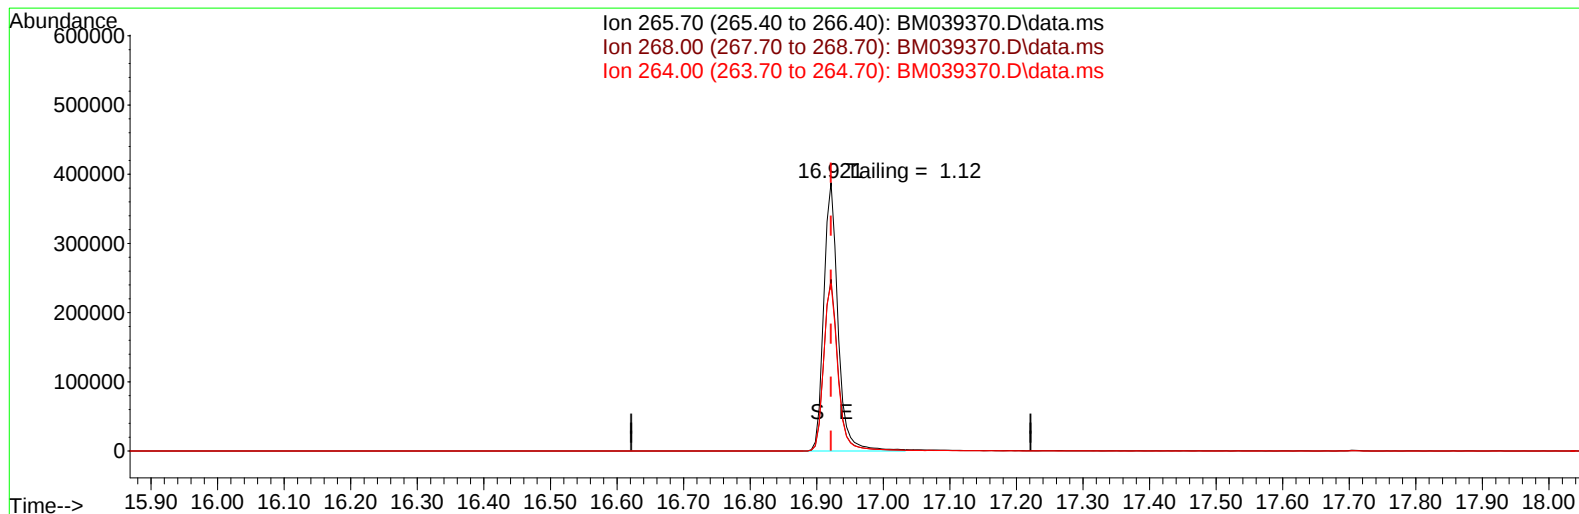

TIC: BM039370.D\data.ms

(70) Pentachlorophenol (C)

16.921min (-0.000) 0.00 ng




response 578679

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.93
264.00	62.80	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041023\
 Data File : BM039370.D
 Acq On : 10 Apr 2023 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 11 03:56:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 11 02:05:37 2023
 Response via : Initial Calibration

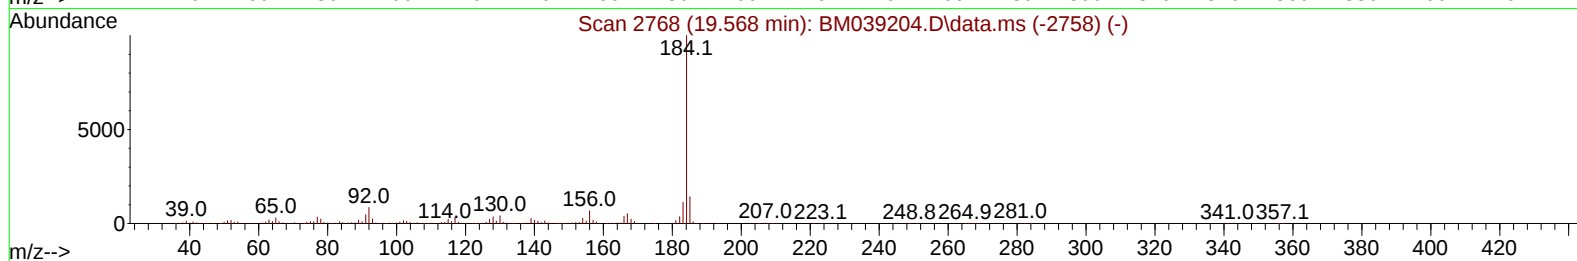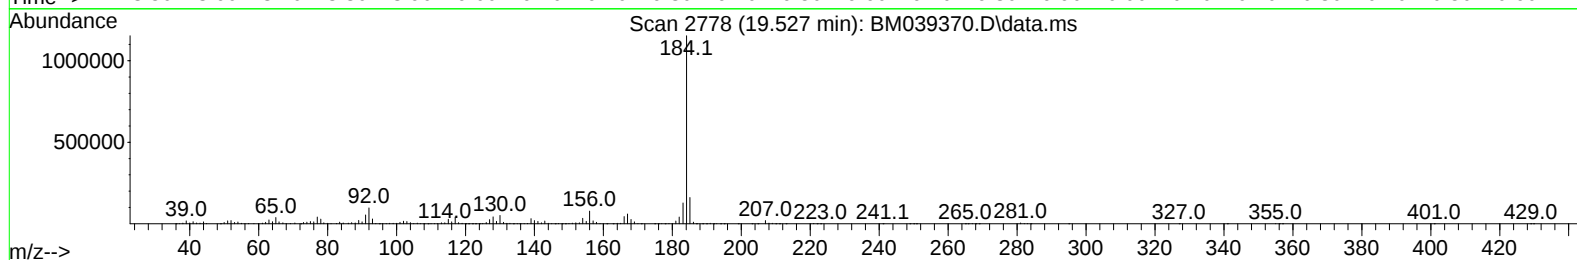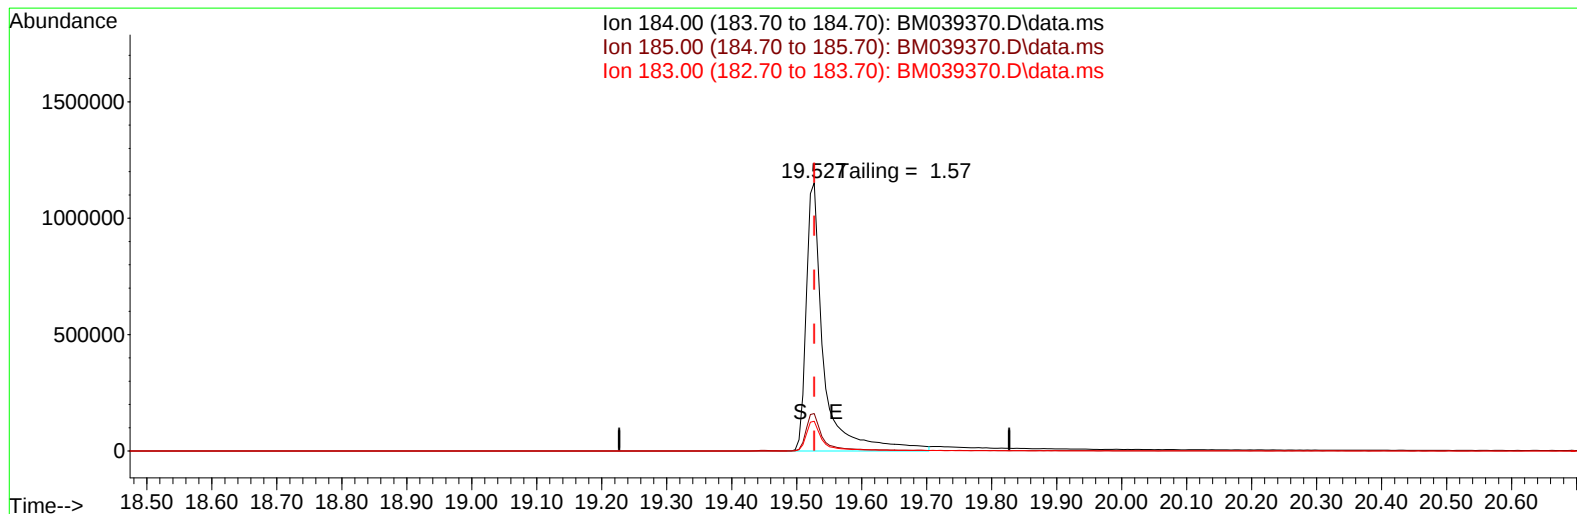

TIC: BM039370.D\data.ms

(77) Benzidine

19.527min (-0.000) 52744.53 ng

response 2168899

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.20	11.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/10/2023	BNA_M	<u>BM039370.D</u>
Compound Name	Response	Retention Time
DDT	1467201	20.75
DDD	23994	20.362
DDE	1486	19.803
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25480	1492681	1.71

Instrument :
BNA_M
ClientSampleId :
DFTPP