

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041024\
 Data File : BM045120.D
 Acq On : 11 Apr 2024 04:14
 Operator : MA/JU
 Sample : P1973-13
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSW4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/12/2024
 Supervised By :mohammad ahmed 04/12/2024

Quant Time: Apr 11 04:44:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 10 11:09:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.623	152	1443	0.400	ng/u1	-0.02
4) Naphthalene-d8	10.391	136	4538	0.400	ng/u1	-0.03
9) Acenaphthene-d10	14.265	164	2354	0.400	ng/u1	#-0.02
13) Phenanthrene-d10	17.026	188	5186m	0.400	ng/u1	-0.03
17) Chrysene-d12	21.258	240	3614m	0.400	ng/u1	0.00
23) Perylene-d12	23.455	264	3185m	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	7326	3.865	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.013	152	2452	0.399	ng/u1	-0.02
18) Fluoranthene-d10	19.066	212	5389	0.590	ng/u1	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.243	88	1156	0.636	ng/u1	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041024\
Data File : BM045120.D
Acq On : 11 Apr 2024 04:14
Operator : MA/JU
Sample : P1973-13
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
YCSW4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/12/2024


Quant Time: Apr 11 04:44:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 10 11:09:26 2024
Response via : Initial Calibration

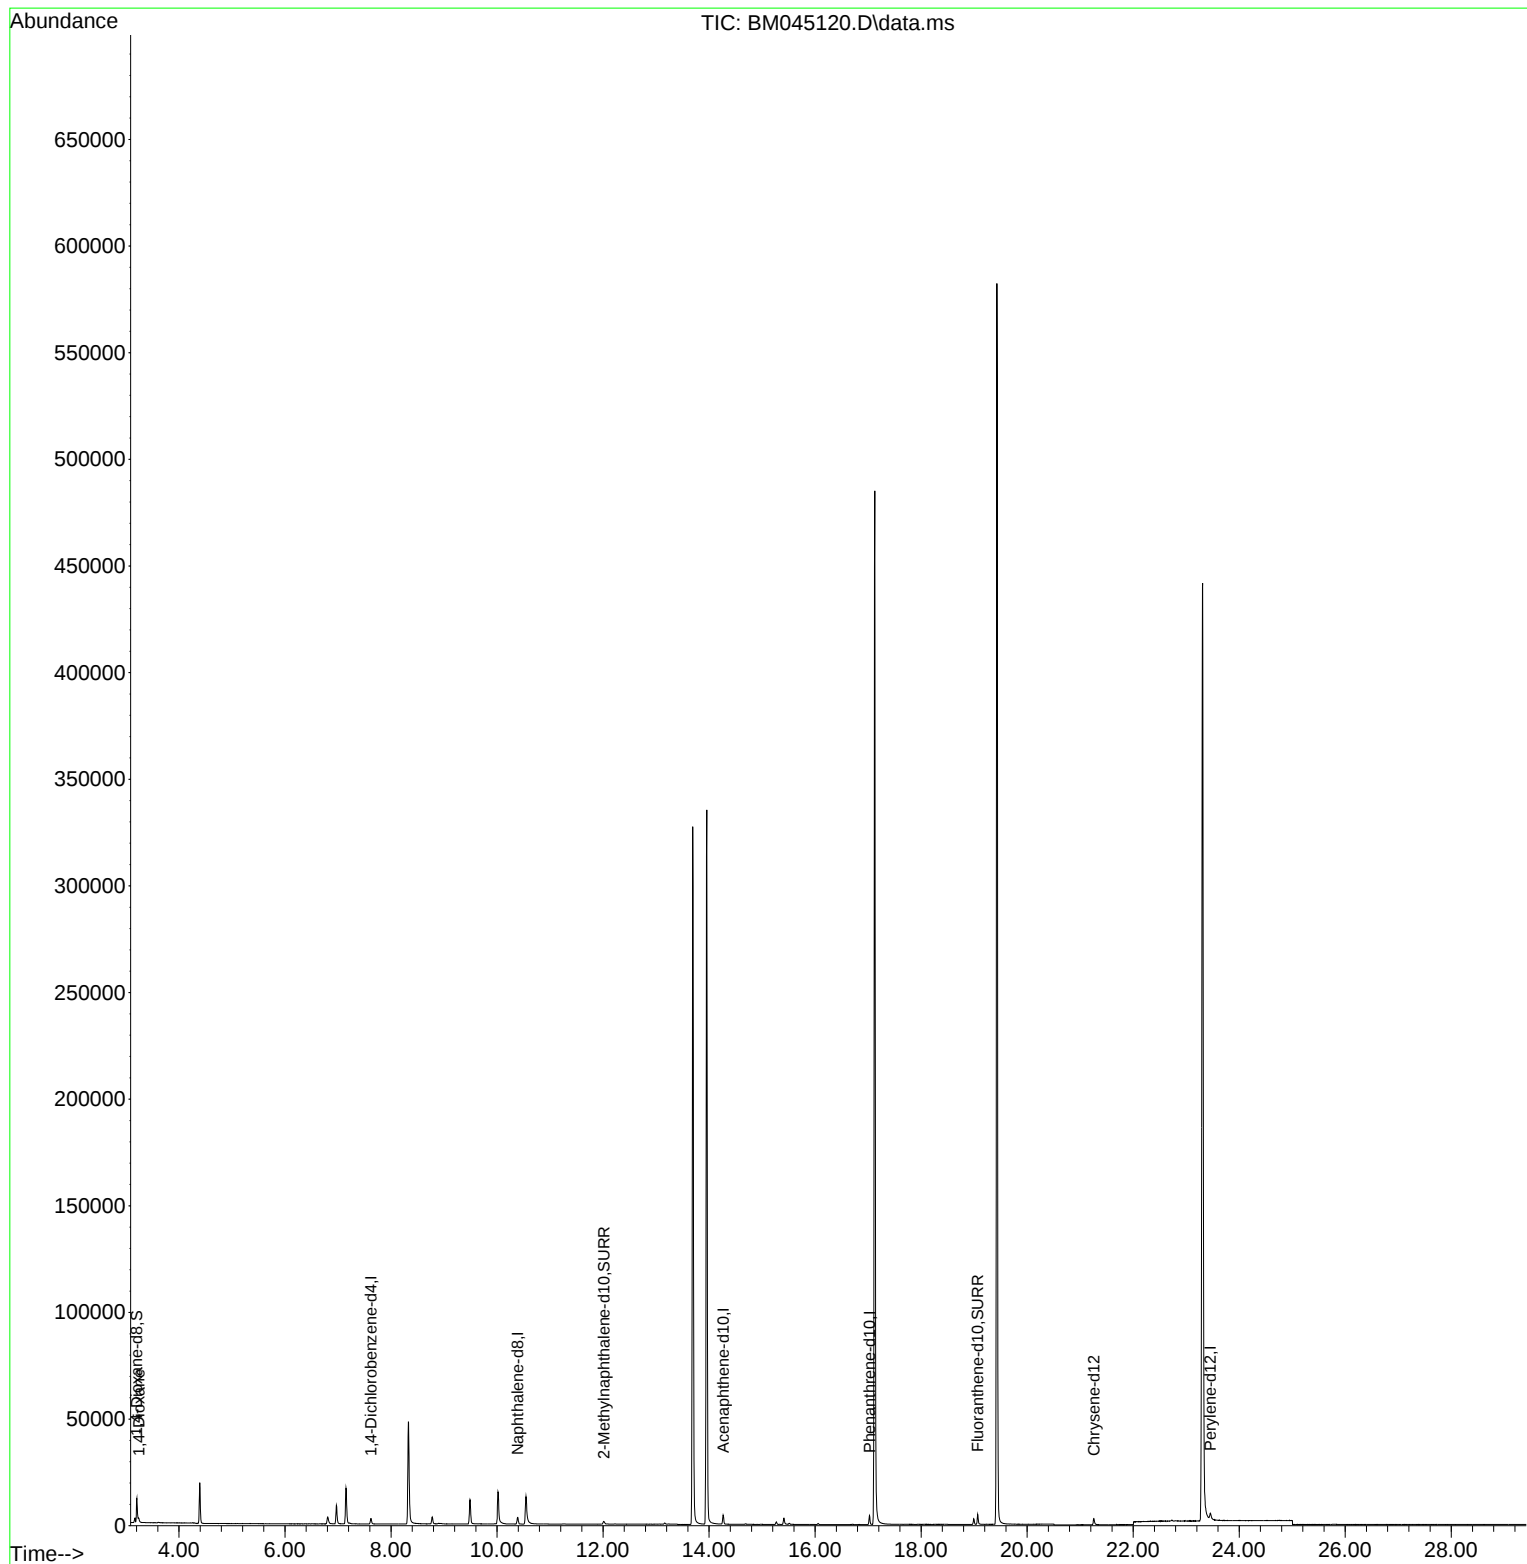

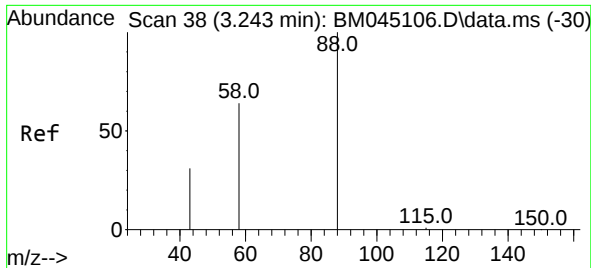

#2
 1,4-Dioxane
 Concen: 0.636 ng/ul
 RT: 3.243 min Scan# 38
 Delta R.T. 0.000 min
 Lab File: BM045120.D
 Acq: 11 Apr 2024 04:14

Instrument :
 BNA_M
 ClientSampleId :
 YCSW4

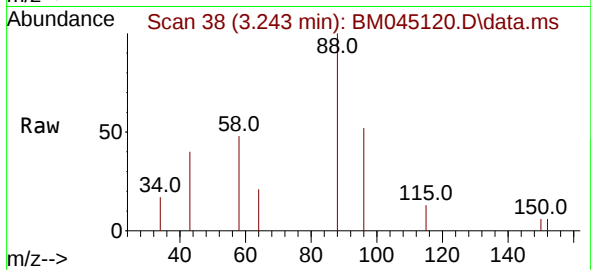

Tgt Ion: 88 Resp: 1150
 Ion Ratio Lower Upper
 88 100
 43 40.3 30.6 46.0
 58 48.3 32.6 48.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/12/2024
 Supervised By :mohammad ahmed 04/12/2024

