

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
Data File : BM004934.D
Acq On : 11 Apr 2016 12:31
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Manual Integrations
APPROVED

Sohil
4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:13:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 01:10:05 2016
Response via : Initial Calibration

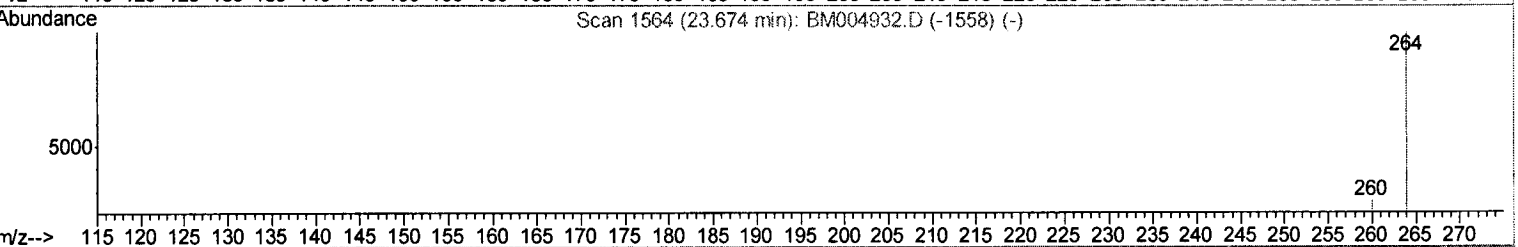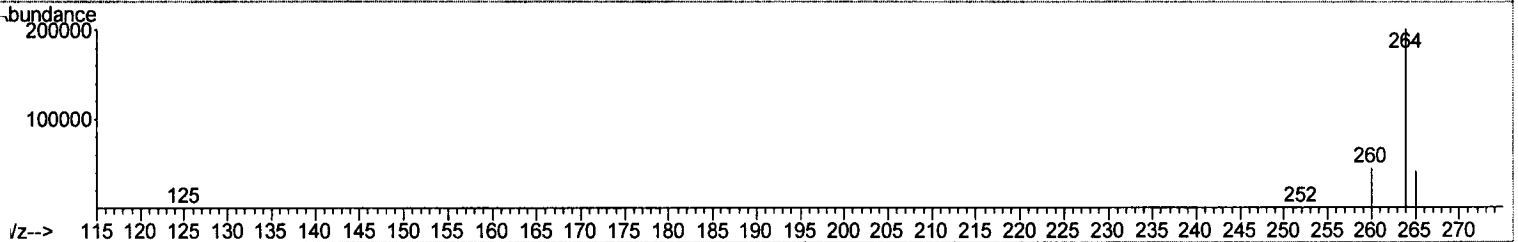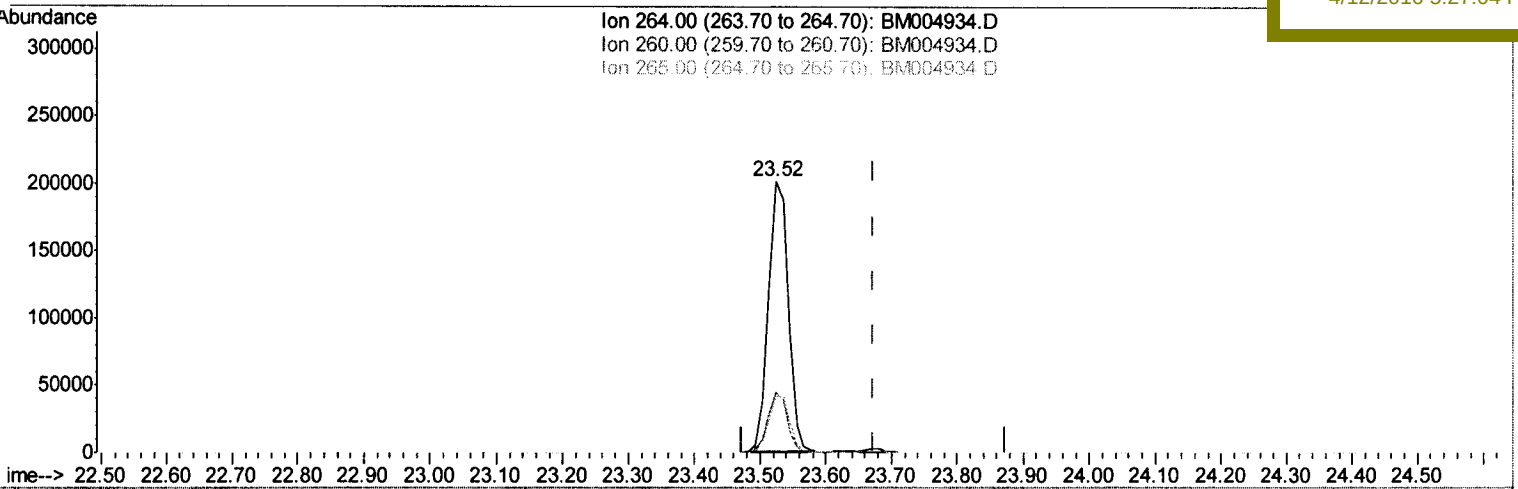

TIC: BM004934.D

(22) Perylene-d12 (I)

23.525min (-0.149) 0.40ng/ul

response 412422

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	22.11
265.00	38.20	20.64#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:13:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

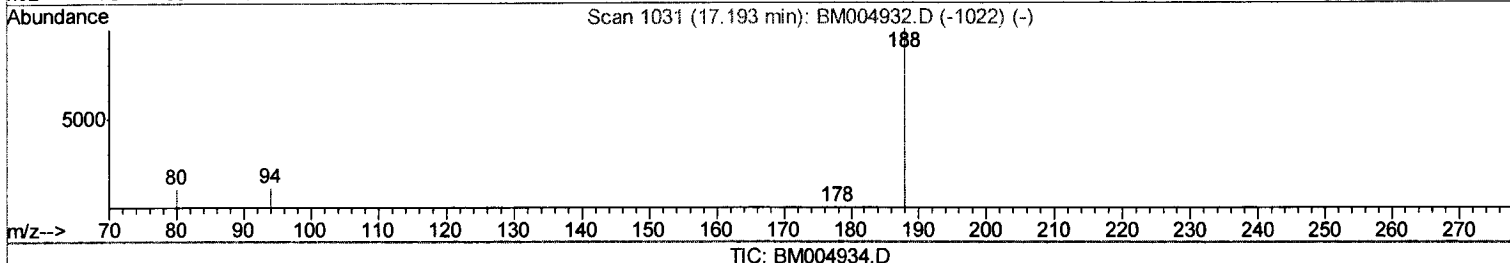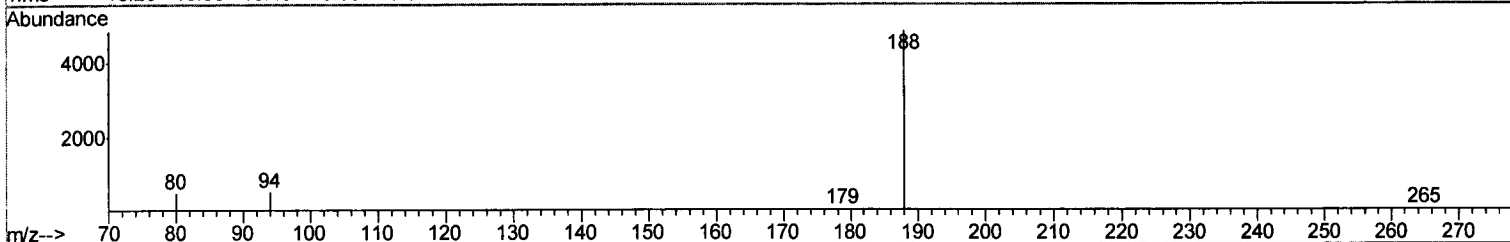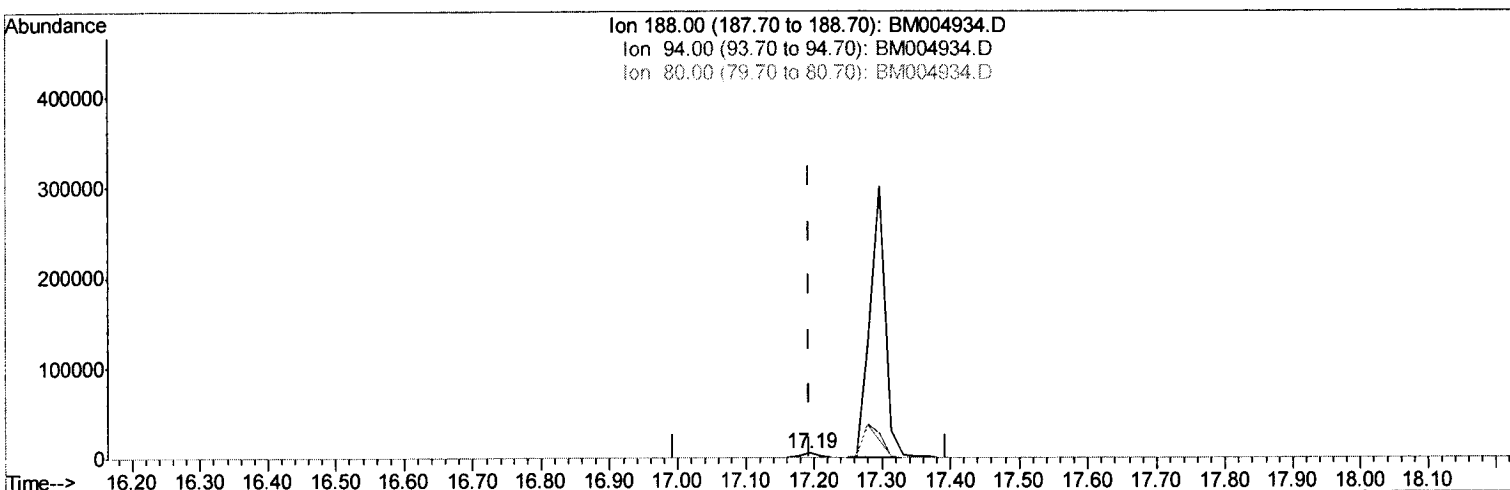

(12) Phenanthrene-d10 (I)

17.194min (+0.000) 0.40ng/ul m

response 6963

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	10.93
80.00	11.90	10.34
0.00	0.00	0.00

U.M
 04/22/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
Data File : BM004934.D
Acq On : 11 Apr 2016 12:31
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Quant Time: Apr 12 01:13:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 01:10:05 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/12/2016 5:27:04 PM

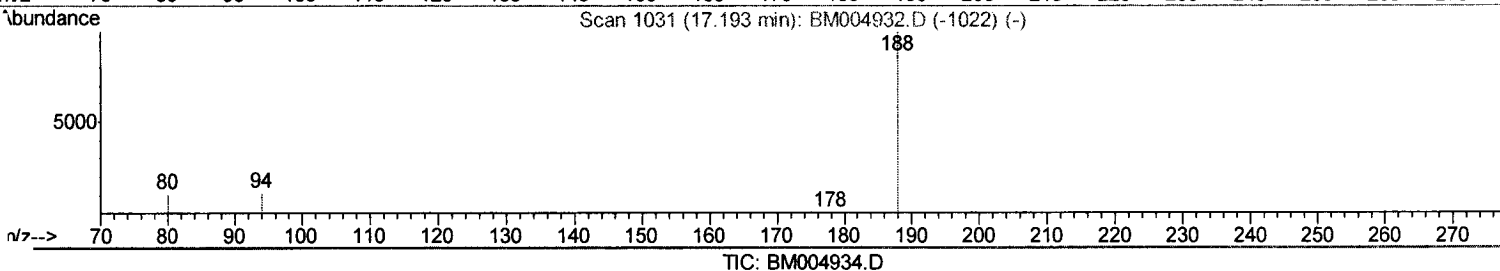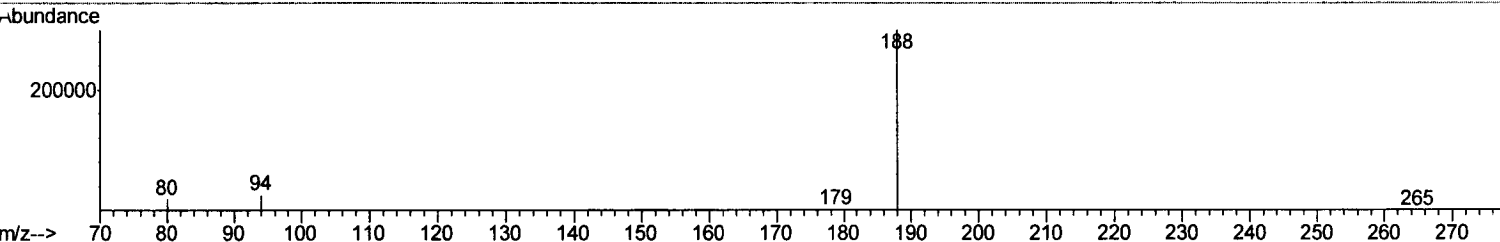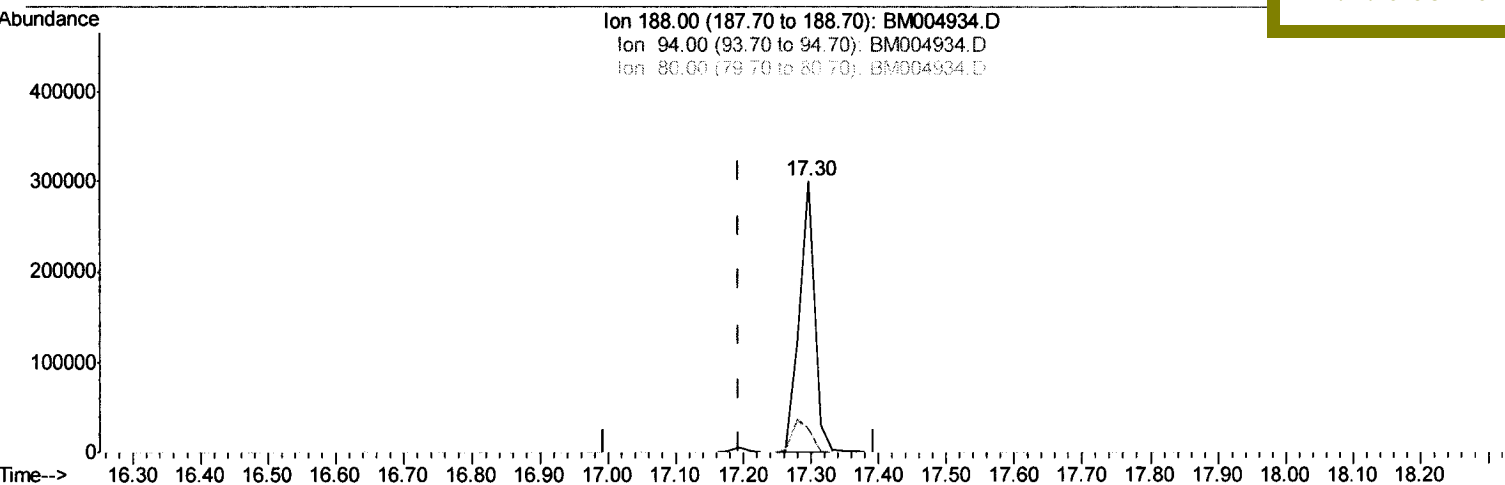

(12) Phenanthrene-d10 (I)

17.297min (+0.103) 0.40ng/ul

response 470515

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	8.52#
80.00	11.90	6.13#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:25:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	1303	0.40	ng/ul	0.00
4) Naphthalene-d8	10.61	136	5698	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.45	164	3345	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.19	188	6963m	0.40	ng/ul	0.00
18) Chrysene-d12	21.39	240	7131	0.40	ng/ul	0.00
22) Perylene-d12	23.67	264	5255m	0.40	ng/ul	0.00

U.M
 04/22/16

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.32	96	1648	2.81	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.21	152	2182	0.27	ng/ul	0.00
16) Fluoranthene-d10	19.23	212	5827	0.35	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) 2-Methylnaphthalene	12.28	142	268	0.03	ng/ul	99
9) Acenaphthylene	14.16	152	451	0.03	ng/ul#	68
10) Acenaphthene	14.50	153	266	0.02	ng/ul#	76
11) Fluorene	15.50	166	1025m	0.08	ng/ul	
13) Pentachlorophenol	16.85	266	186	0.11	ng/ul	91
14) Phenanthrene	17.23	178	2736m	0.14	ng/ul	
15) Anthracene	17.33	178	2425	0.13	ng/ul#	91
17) Fluoranthene	19.25	202	3519	0.16	ng/ul	93
19) Pyrene	19.62	202	4457	0.18	ng/ul#	95
20) Benzo(a)anthracene	21.37	228	2040	0.09	ng/ul#	93
21) Chrysene	21.42	228	1815	0.09	ng/ul	94
23) Benzo(b)fluoranthene	22.98	252	2025m	0.11	ng/ul	
24) Benzo(k)fluoranthene	23.02	252	1444m	0.09	ng/ul	
26) Indeno(1,2,3-cd)pyrene	26.00	276	1222m	0.08	ng/ul	
27) Dibenzo(a,h)anthracene	26.01	278	883m	0.07	ng/ul	
28) Benzo(g,h,i)perylene	26.70	276	923m	0.07	ng/ul	

U.M
 04/22/16

U.M
 04/22/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:25:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

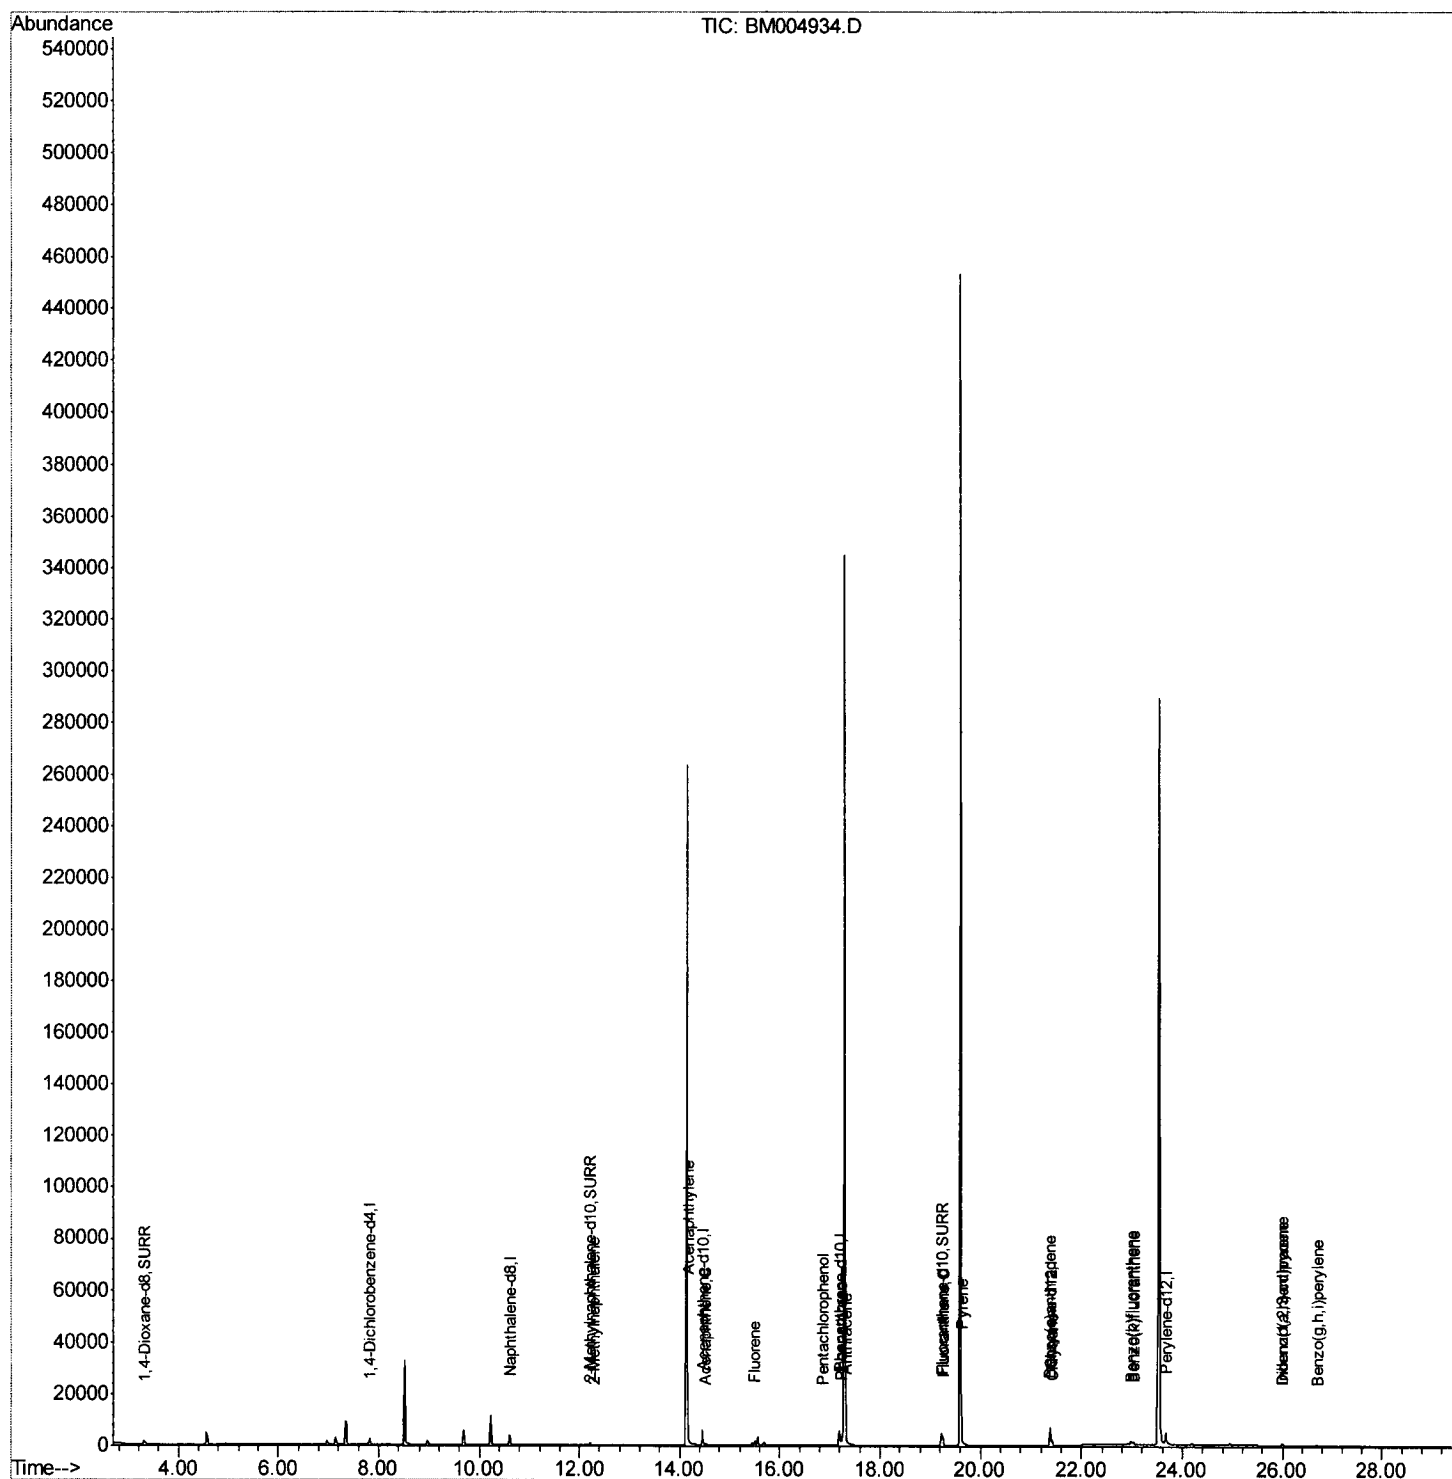

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:13:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

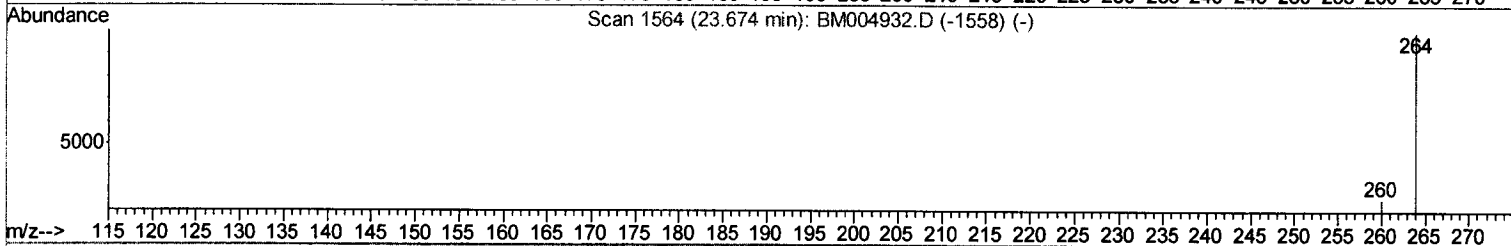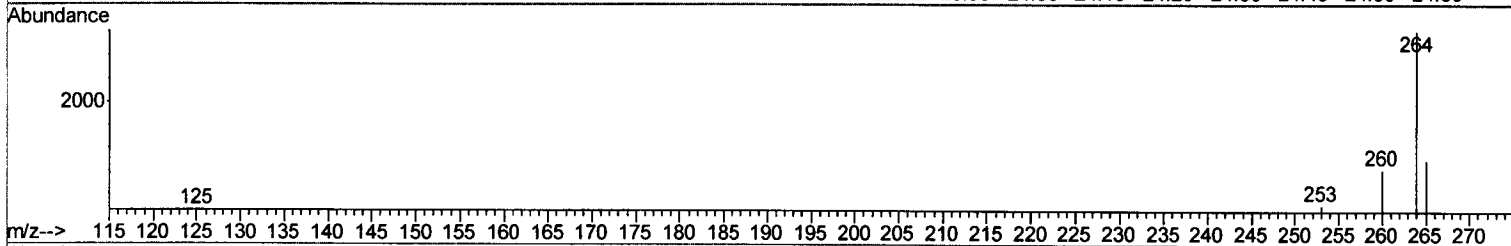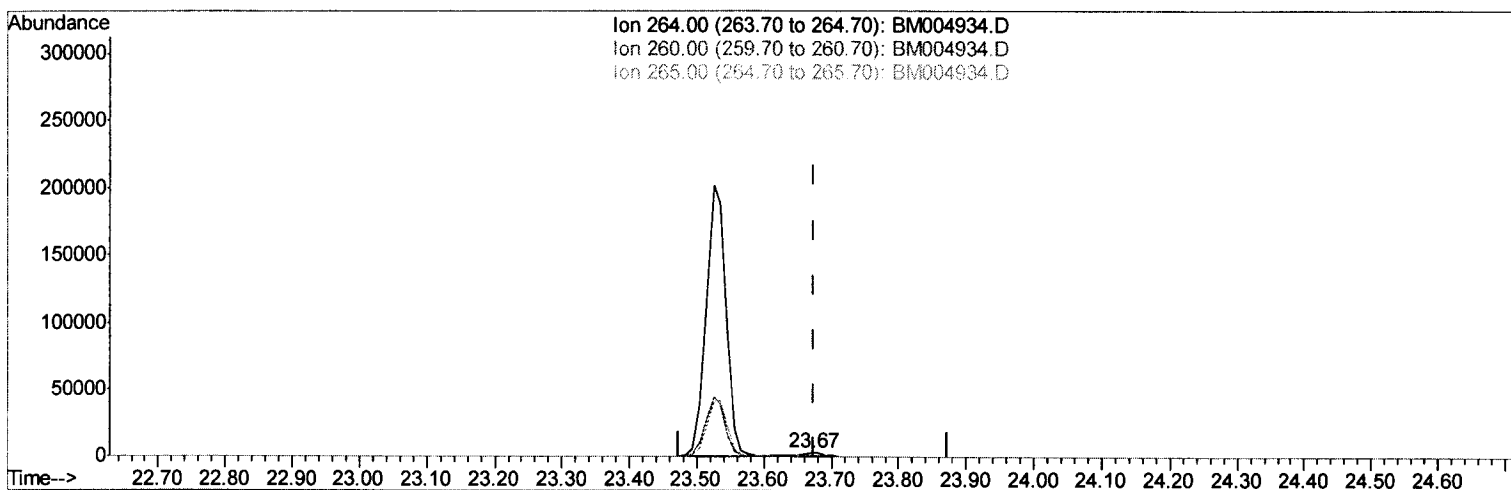

TIC: BM004934.D

(22) Perylene-d12 (I)

23.671min (-0.003) 0.40ng/ul m

response 5255

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.63
265.00	38.20	31.50
0.00	0.00	0.00

U.M
 04/22/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Quant Time: Apr 12 01:21:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

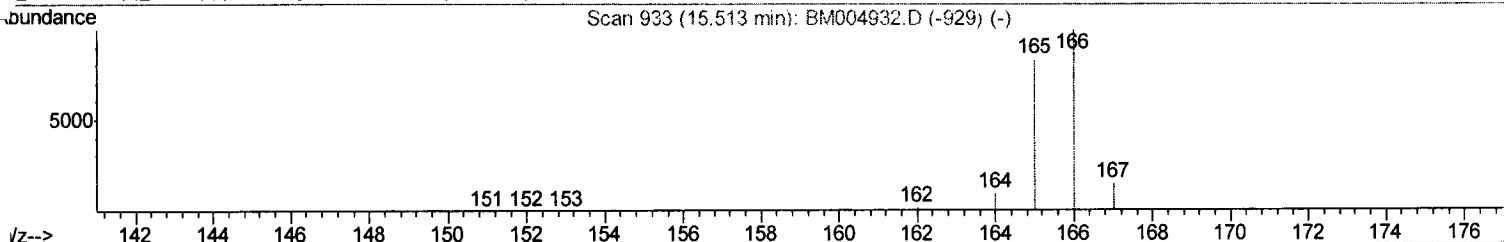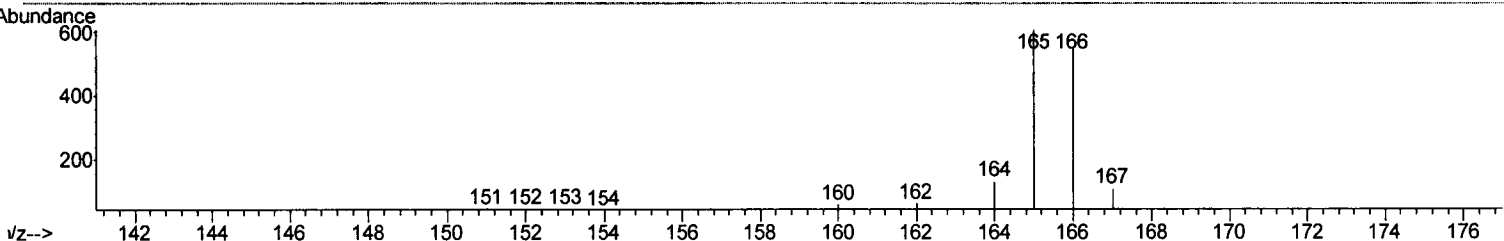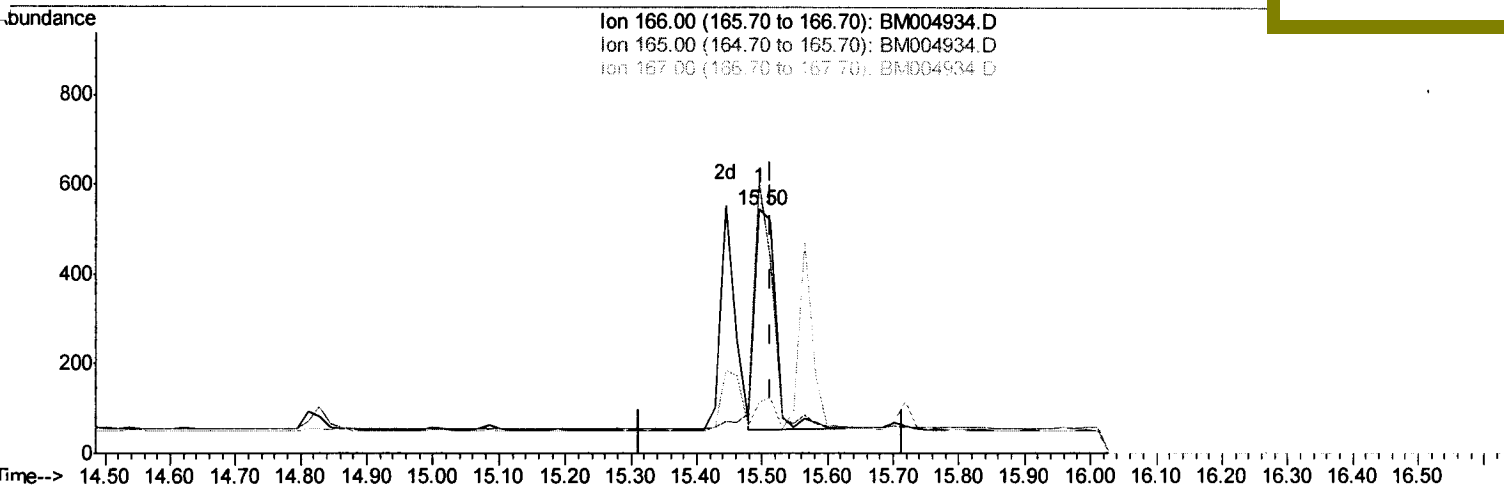

TIC: BM004934.D

(11) Fluorene

15.496min (-0.017) 0.08ng/ul

response 1069

Ion	Exp%	Act%
166.00	100	100
165.00	87.00	111.19#
167.00	14.90	20.55#
0.00	0.00	0.00

```

Data Path   : Z:\HPCHEM1\BNA_M\DATA\BM041116\
Data File   : BM004934.D
Acq On      : 11 Apr 2016   12:31
Operator    : UM/SJ
Sample      : H2275-02
Misc        :
ALS Vial    : 5      Sample Multiplier: 1




```

Instrument :
BNA_M
ClientSampleId :
D9T75

Manual Integrations

Sohil
4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 01:10:05 2016
Response via : Initial Calibration

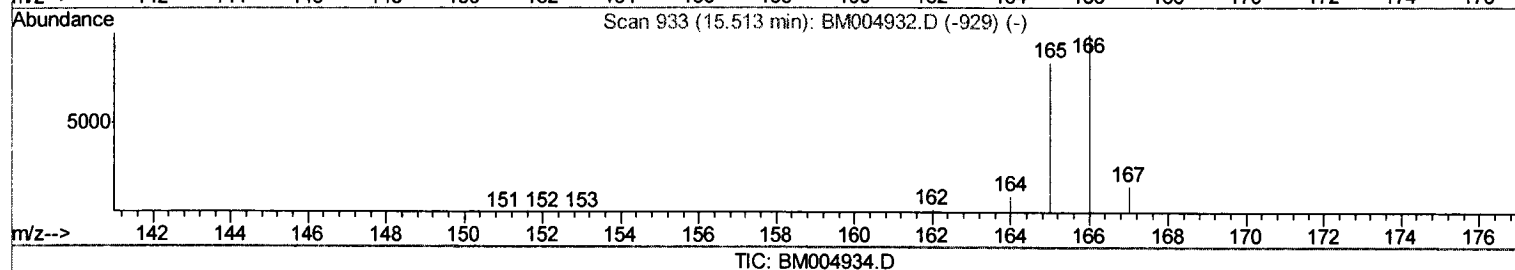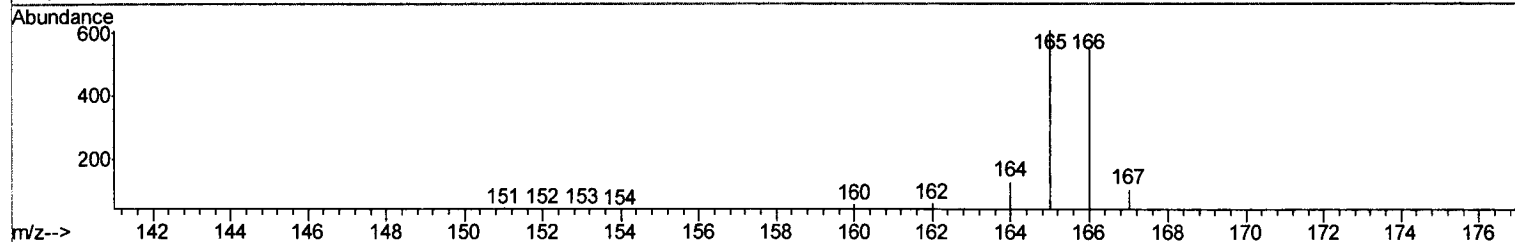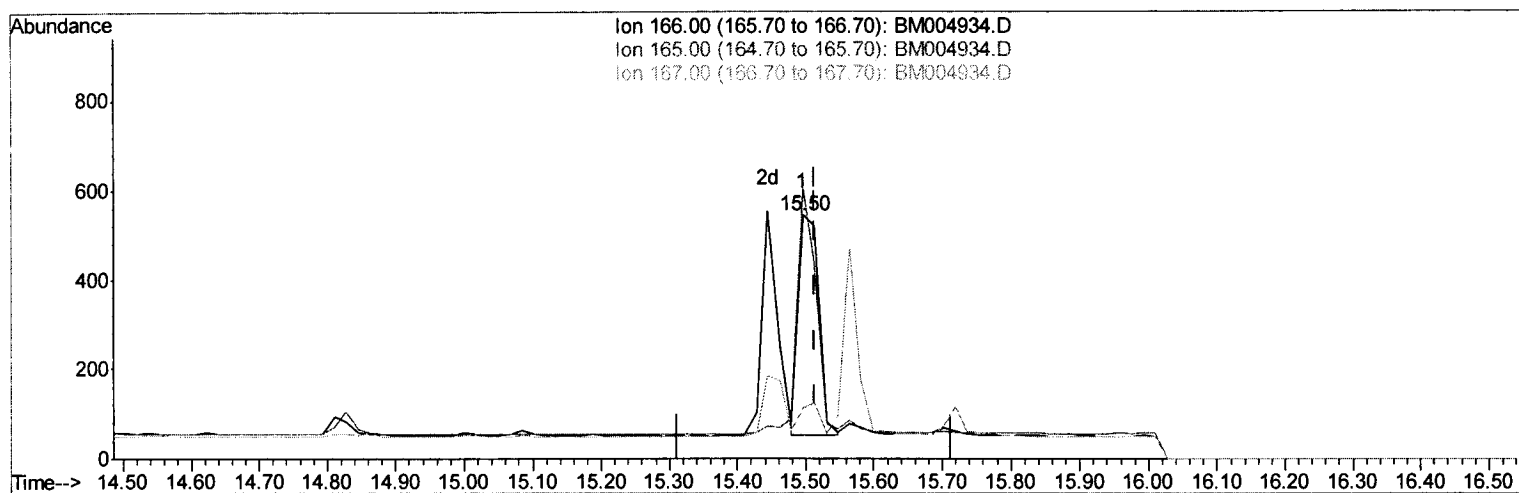

(11) Fluorene

15.496min (-0.017) 0.08ng/ul m

response 1025

Ion	Exp%	Act%
-----	------	------

166.00	100	100
--------	-----	-----

165.00	87.00	111.19#
--------	-------	---------

167.00 14.90 20.55#

0.00 0.00 0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

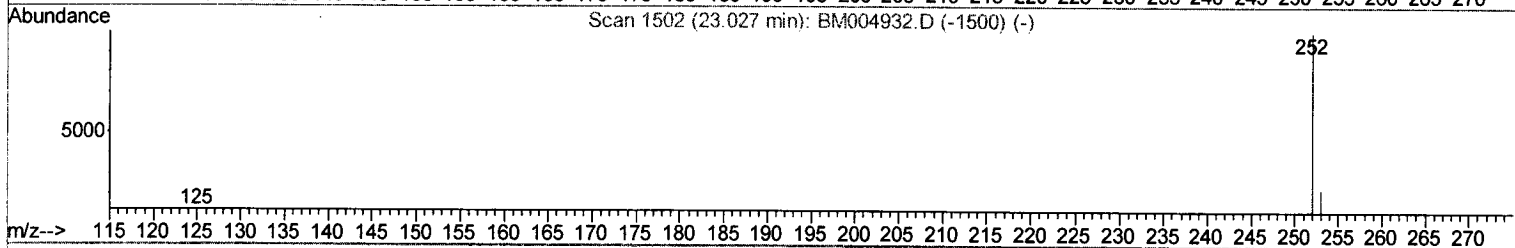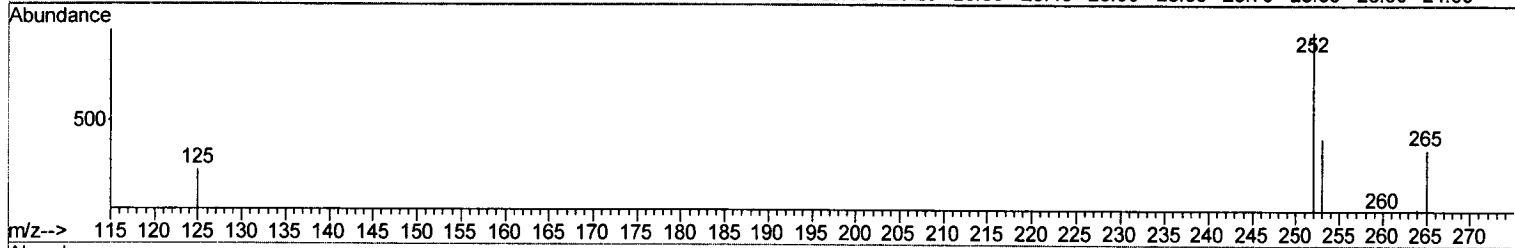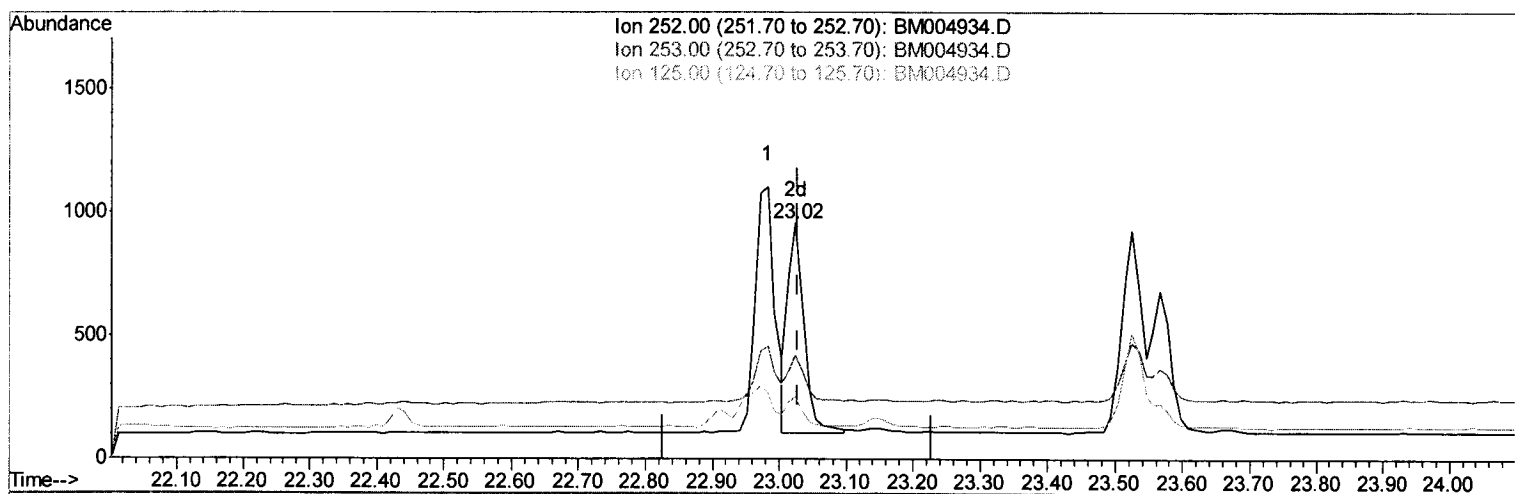

TIC: BM004934.D

(24) Benzo(k)fluoranthene

23.024min (-0.003) 0.09ng/ul m

response 1444

Ion Exp% Act%

252.00 100 100

253.00 24.80 43.87#

125.00 13.00 26.28#

0.00 0.00 0.00

> U.M
 04/22/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

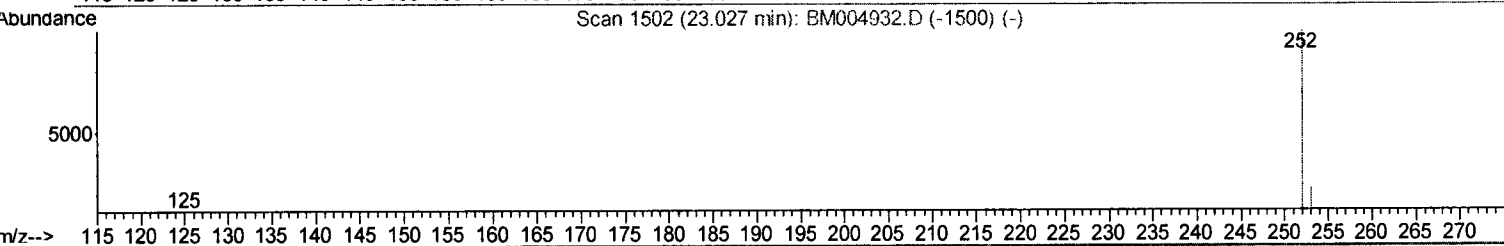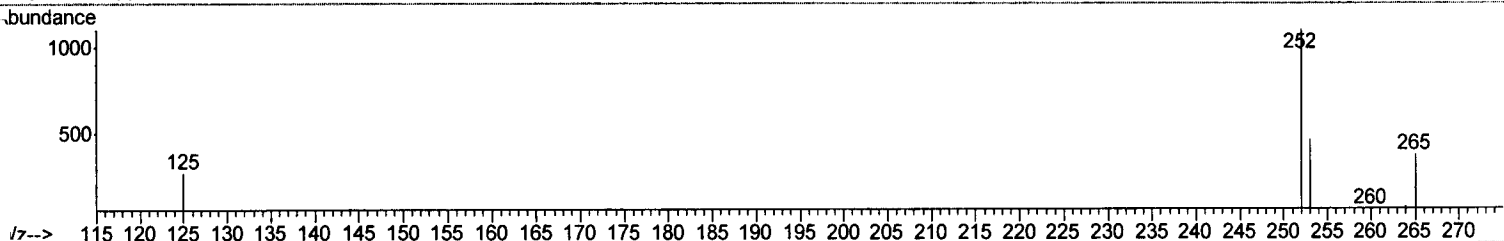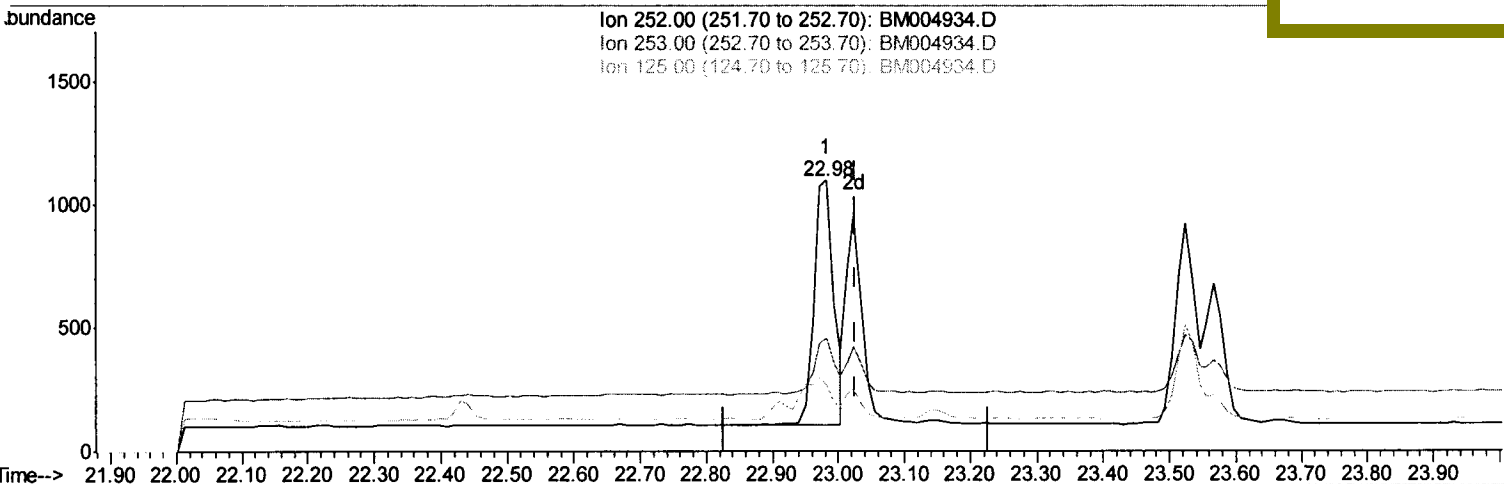

TIC: BM004934.D

(24) Benzo(k)fluoranthene

22.983min (-0.045) 0.13ng/ul

response 2052

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	41.60#
125.00	13.00	24.16#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

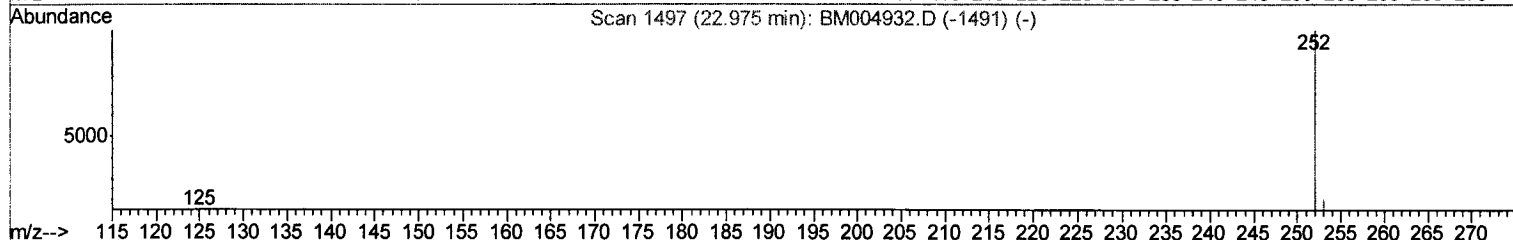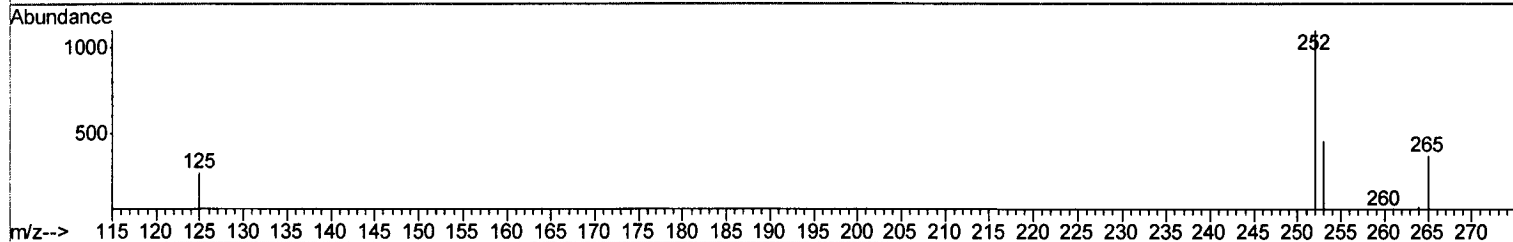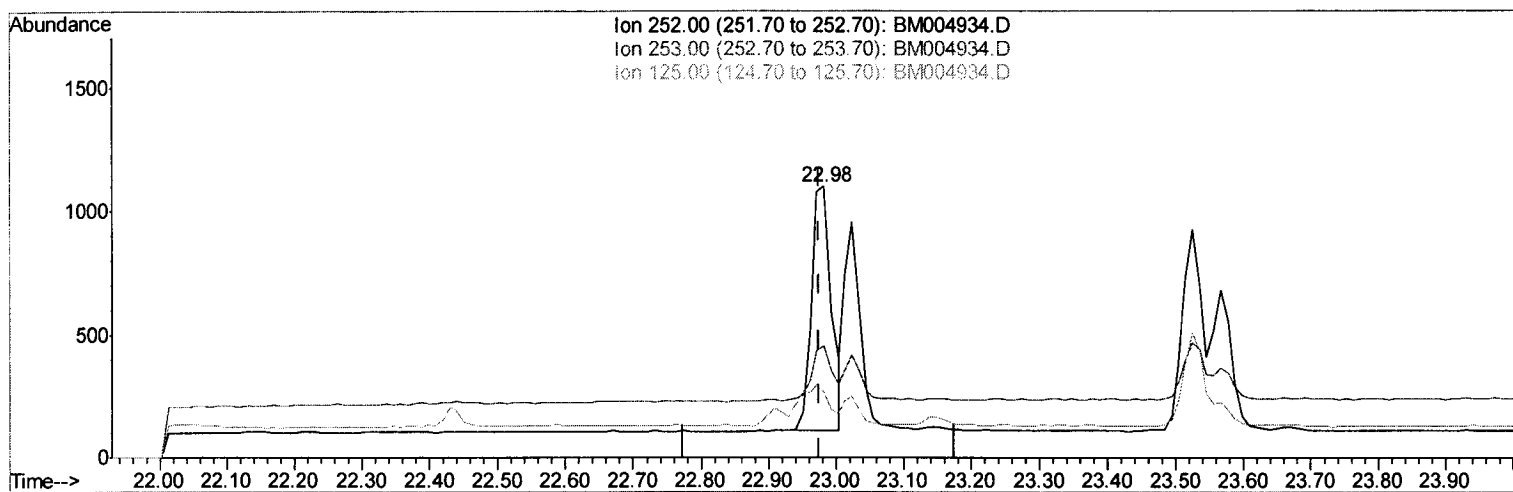

TIC: BM004934.D

(23) Benzo(b)fluoranthene

22.983min (+0.007) 0.11ng/ul m

response 2025

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	41.60
125.00	14.40	24.16
0.00	0.00	0.00

U.M
 04/22/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
Data File : BM004934.D
Acq On : 11 Apr 2016 12:31
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Manual Integrations
APPROVED

Sohil
4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 01:10:05 2016
Response via : Initial Calibration

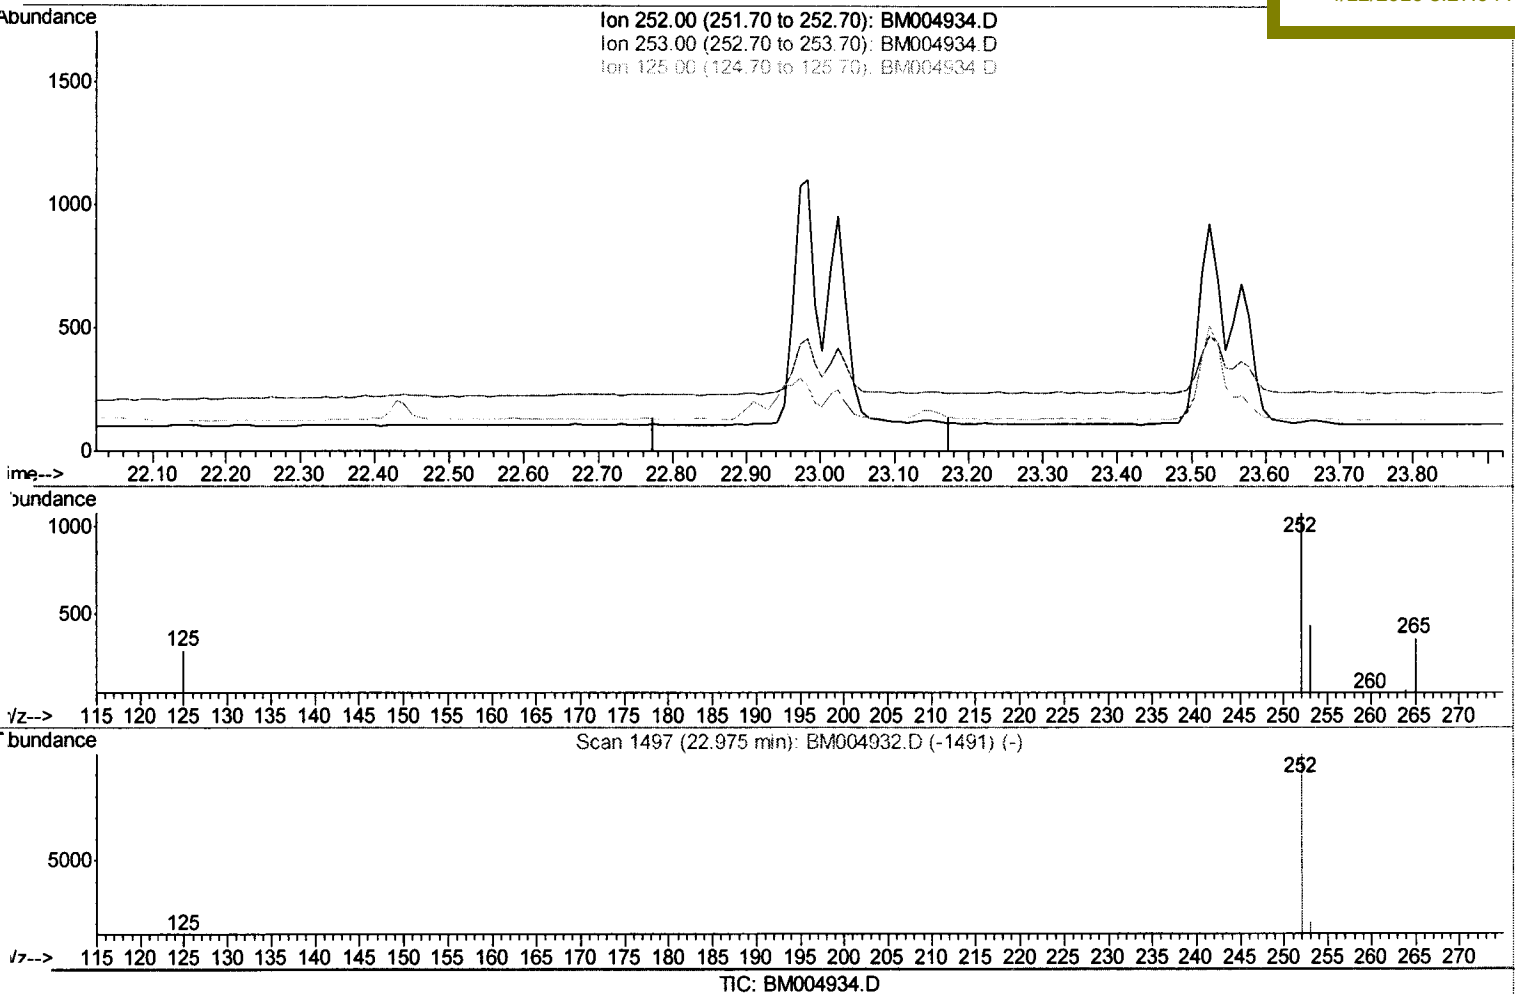

(23) Benzo(b)fluoranthene

22.975min (-22.975) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	22.70	0.00
125.00	14.40	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

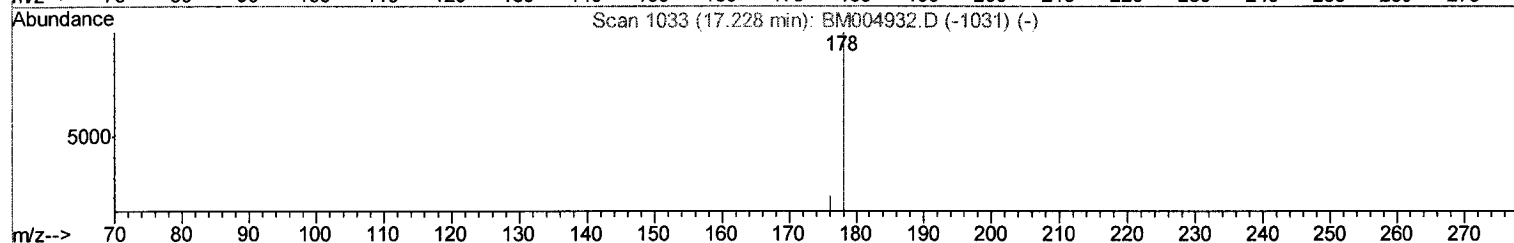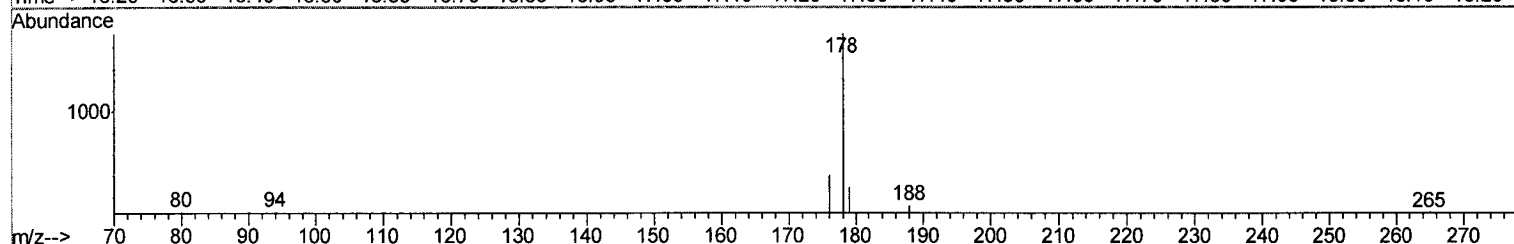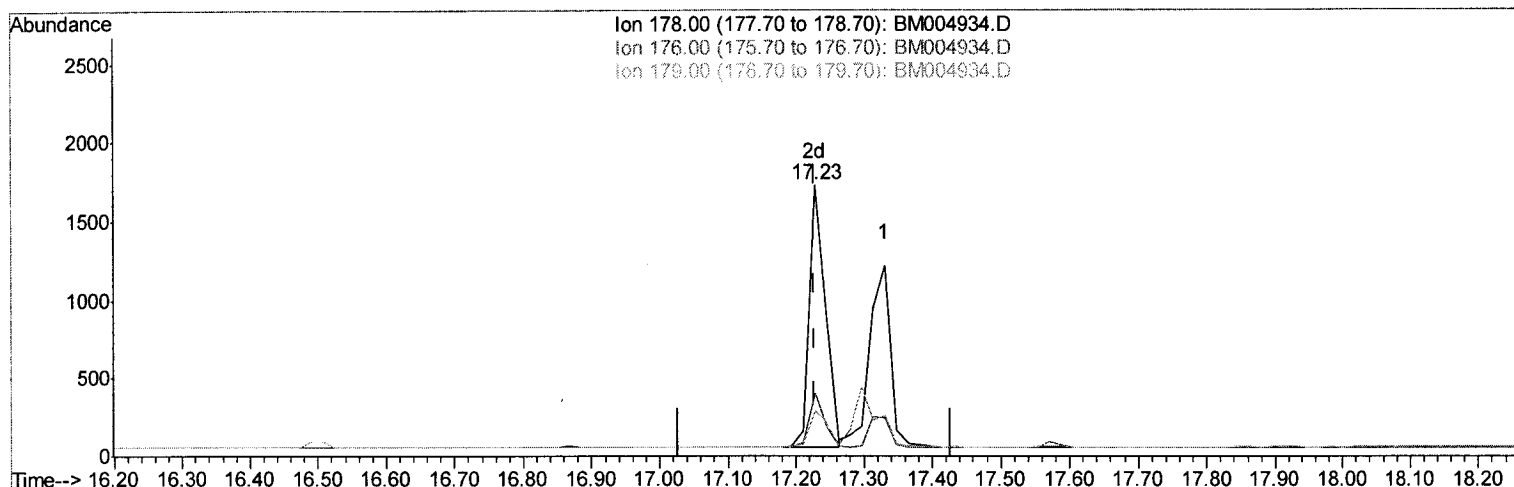

TIC: BM004934.D

(14) Phenanthrene

17.228min (+0.000) 0.14ng/ul m³

response 2736

Ion Exp% Act%

178.00 100 100

176.00 16.20 23.38#

179.00 17.70 16.61

0.00 0.00 0.00

U.M
 04/22/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

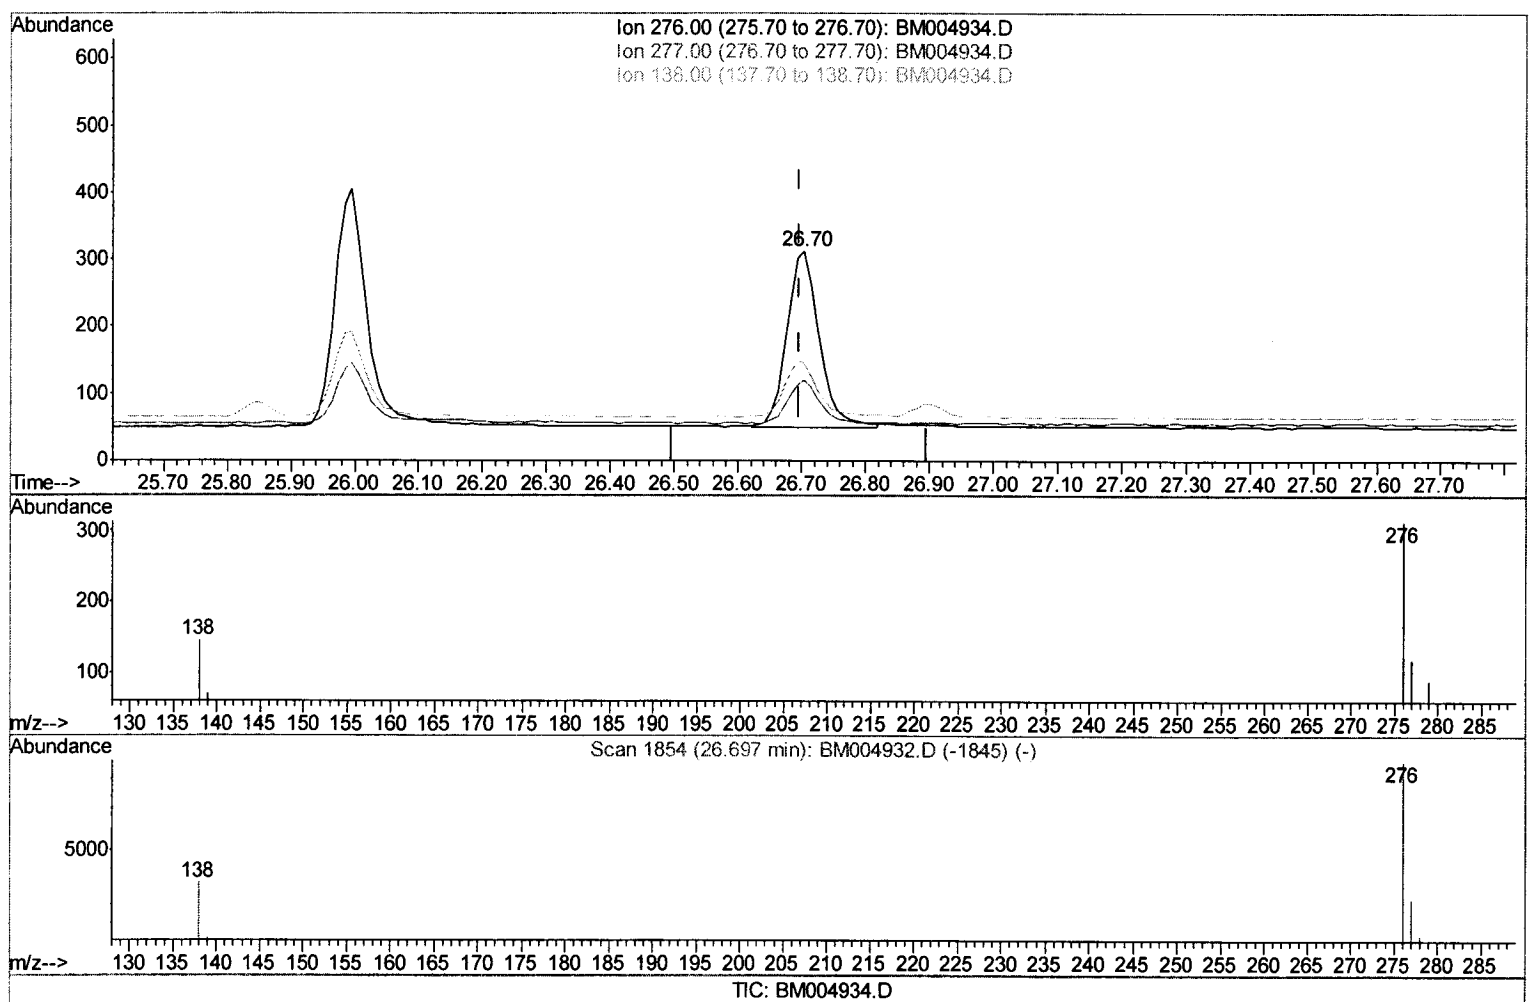

(28) Benzo(g,h,i)perylene

26.704min (+0.007) 0.07ng/ul m

response 923

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	38.14#
138.00	28.10	46.47#
0.00	0.00	0.00

U.M
 04/22/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

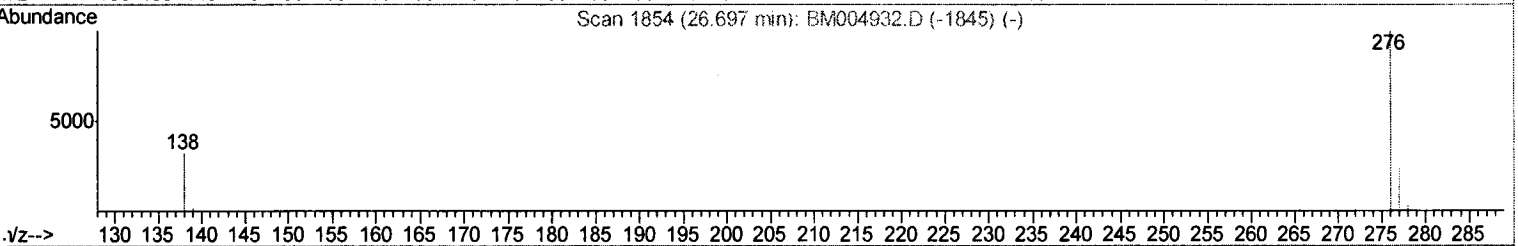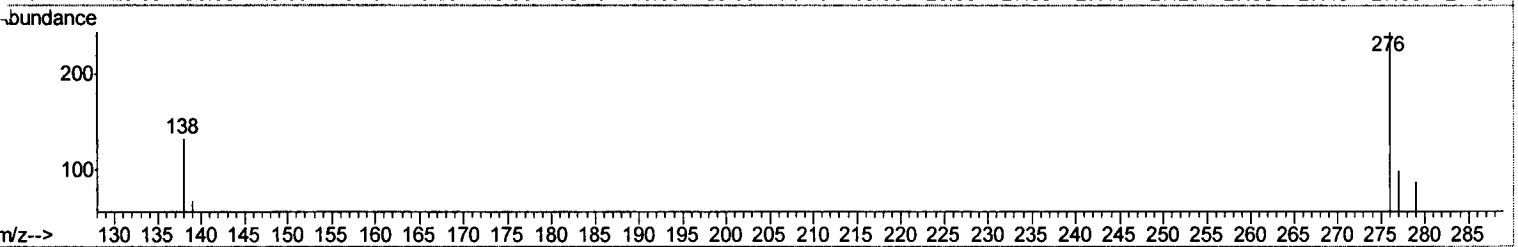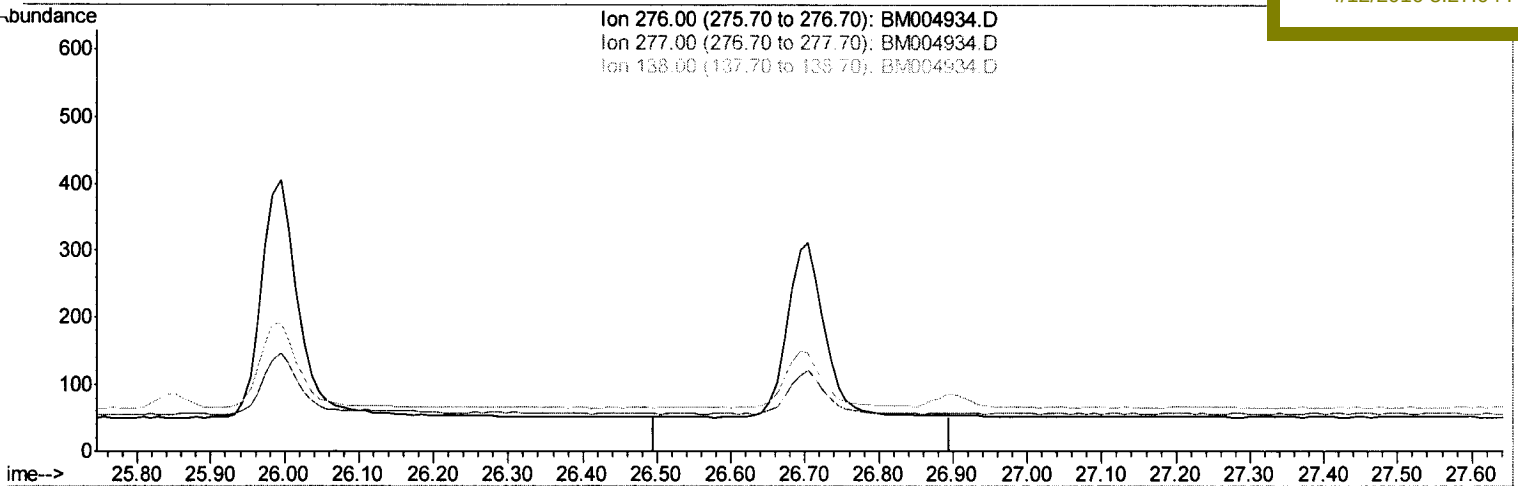

TIC: BM004934.D

(28) Benzo(g,h,i)perylene

26.697min (-26.697) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	23.60	0.00#
138.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

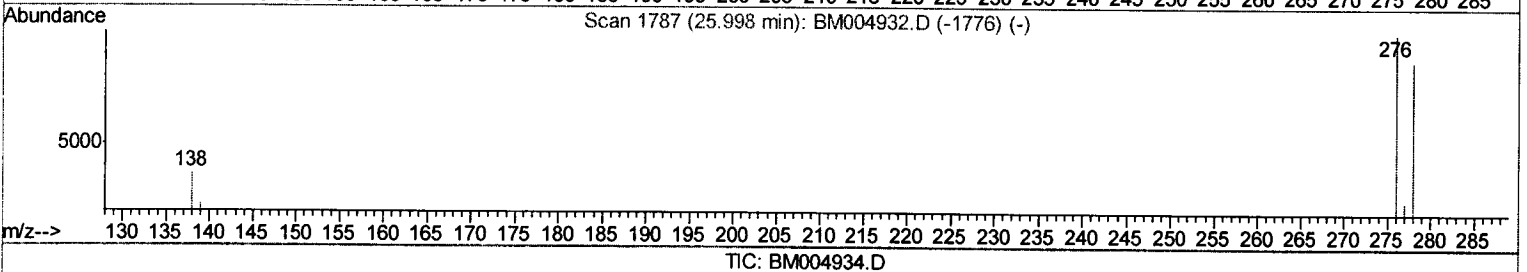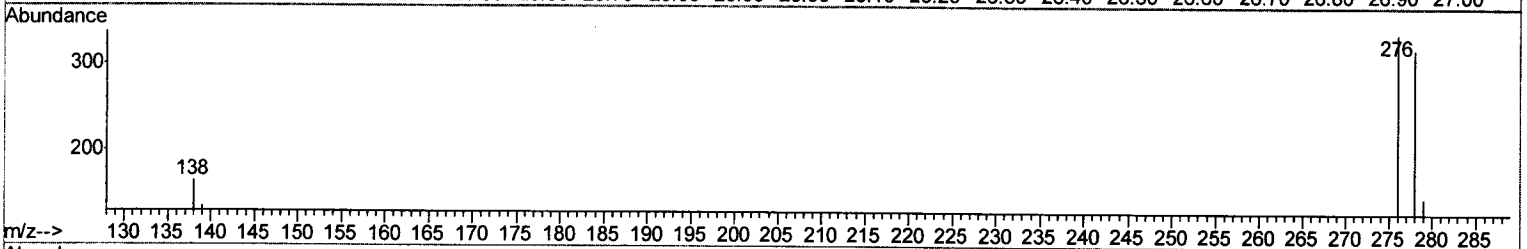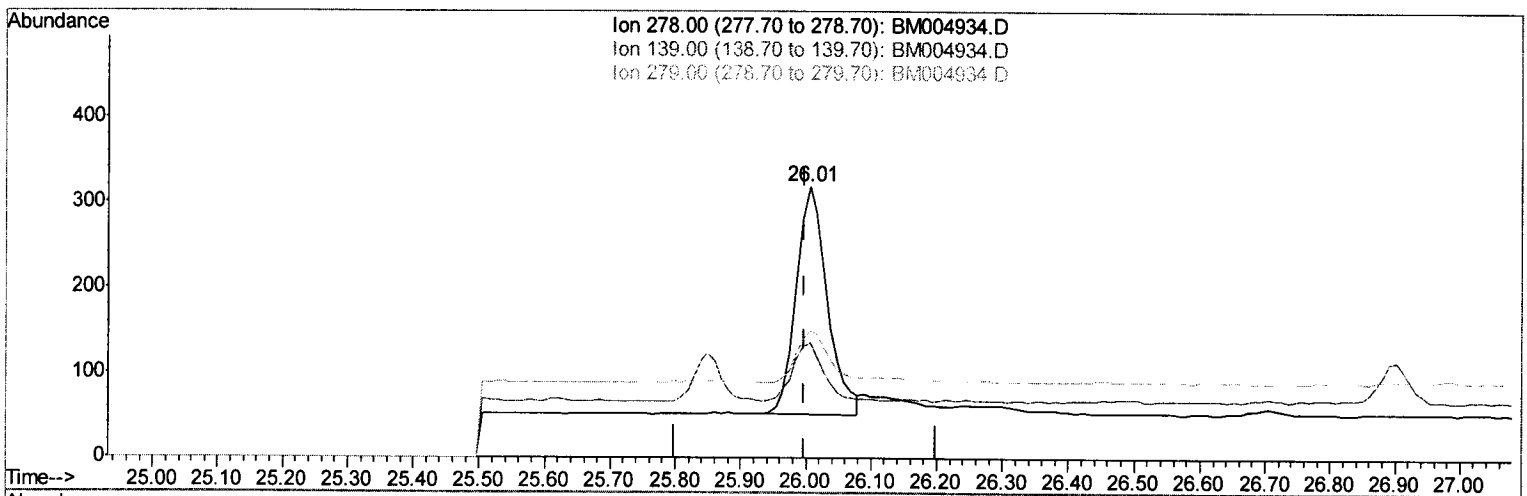

(27) Dibenzo(a,h)anthracene

26.006min (+0.007) 0.07ng/ul m

response 883

Ion Exp% Act%

278.00 100 100

139.00 20.50 42.63#

279.00 25.20 46.71#

0.00 0.00 0.00

> U.M
 04/22/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

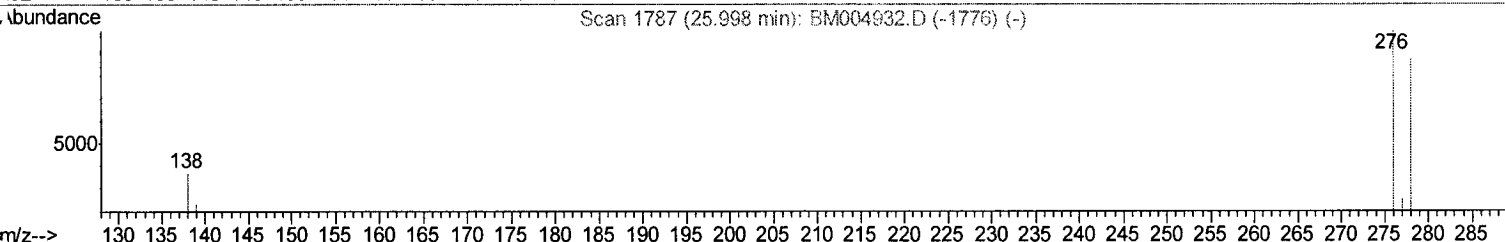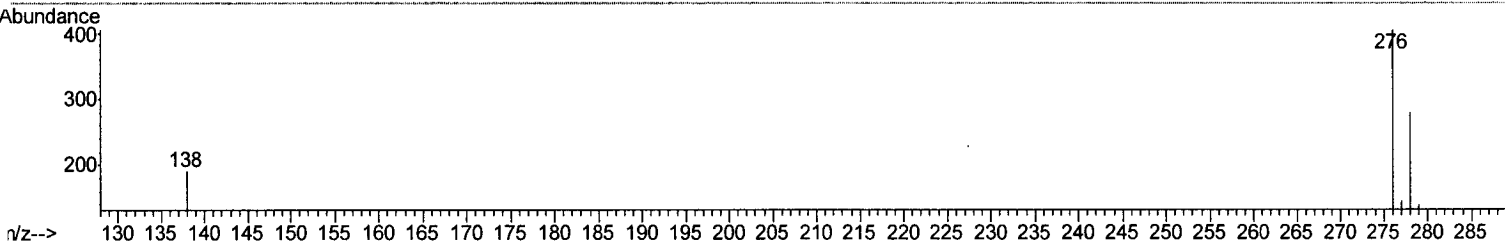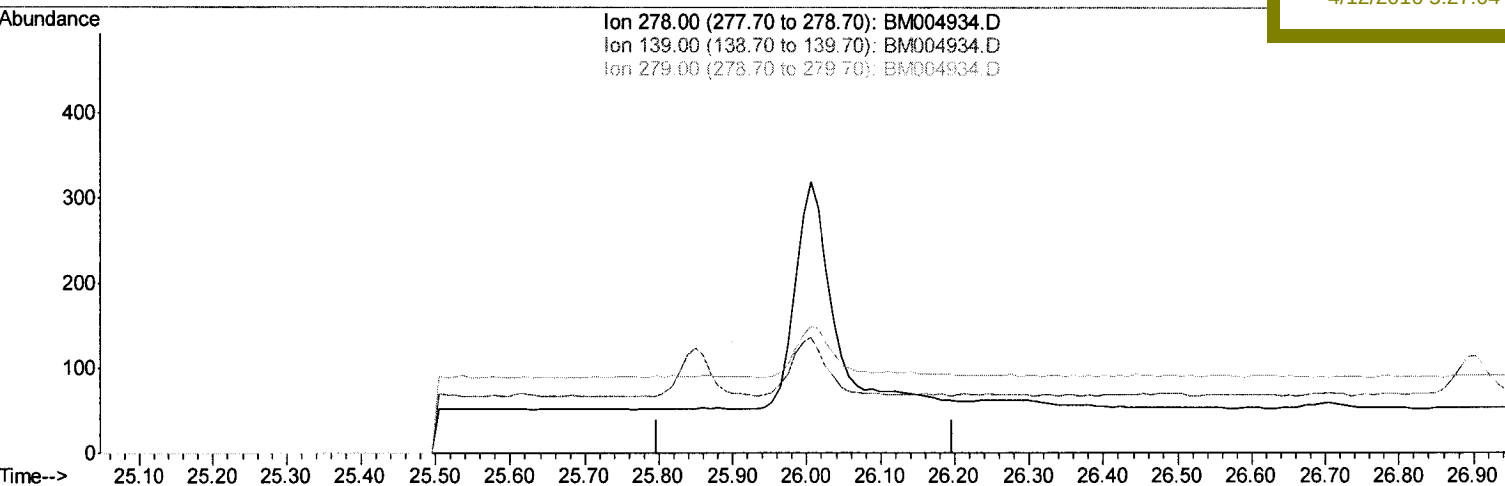

TIC: BM004934.D

(27) Dibenzo(a,h)anthracene

25.998min (-25.998) 0.00ng/ul

response 0

Ion	Exp%	Act%
278.00	100	0.00
139.00	20.50	0.00#
279.00	25.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

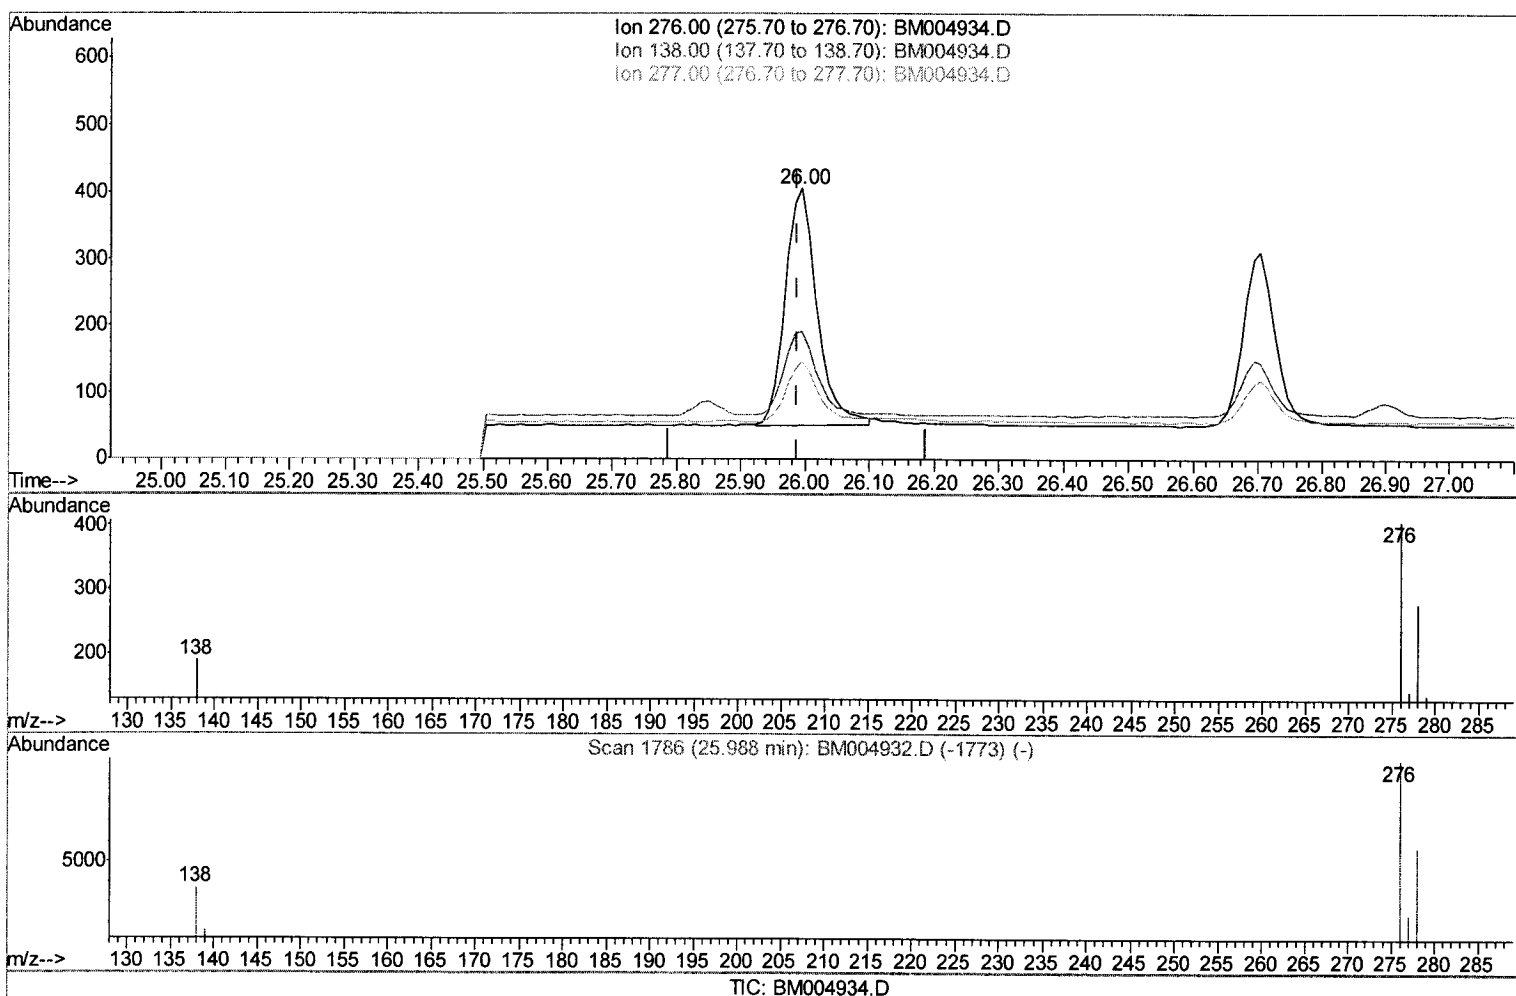

(26) Indeno(1,2,3-cd)pyrene

25.995min (+0.007) 0.08ng/ul m

response 1222

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	0.00#
277.00	24.80	0.00#
0.00	0.00	0.00

U.M
 04/22/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
Data File : BM004934.D
Acq On : 11 Apr 2016 12:31
Operator : UM/SJ
Sample : H2275-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T75

Manual Integrations
APPROVED

Sohil
4/12/2016 5:27:04 PM

Quant Time: Apr 12 01:21:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 01:10:05 2016
Response via : Initial Calibration

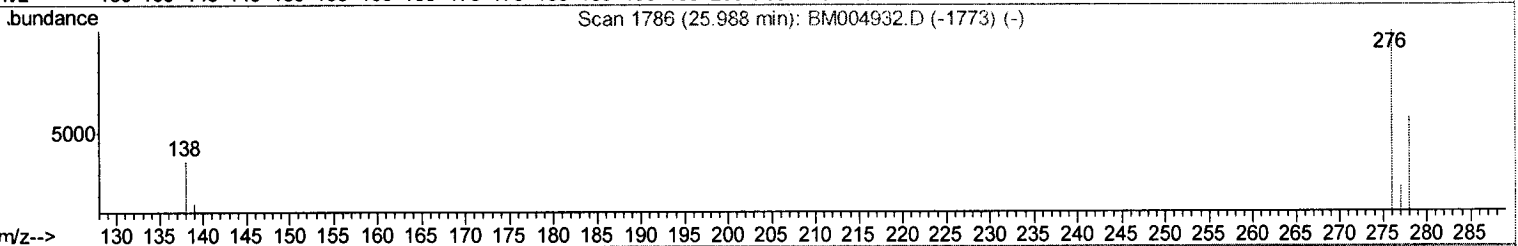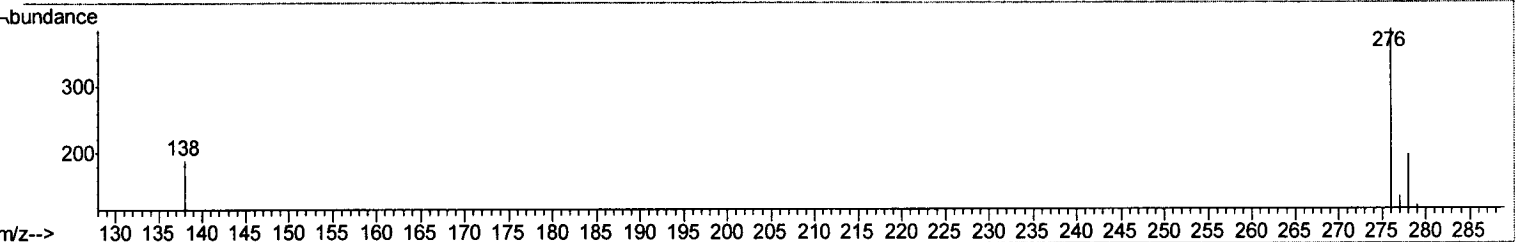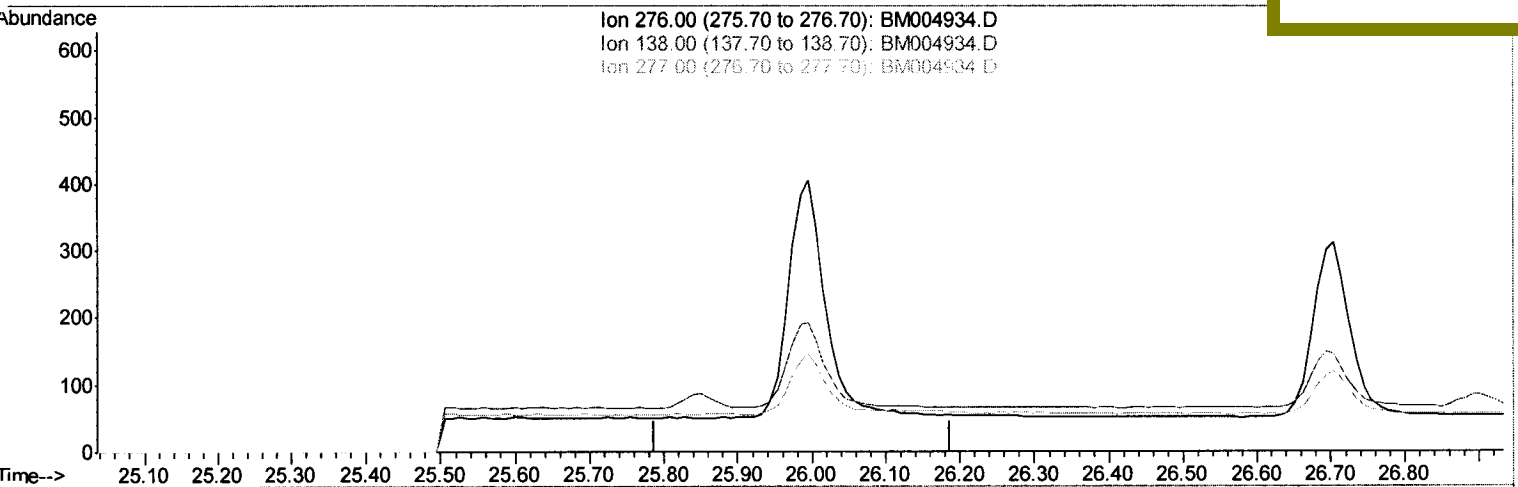

TIC: BM004934.D

(26) Indeno(1,2,3-cd)pyrene

25.988min (-25.988) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
138.00	20.40	0.00#
277.00	24.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041116\
 Data File : BM004934.D
 Acq On : 11 Apr 2016 12:31
 Operator : UM/SJ
 Sample : H2275-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T75

Quant Time: Apr 12 01:21:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 01:10:05 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2016 5:27:04 PM

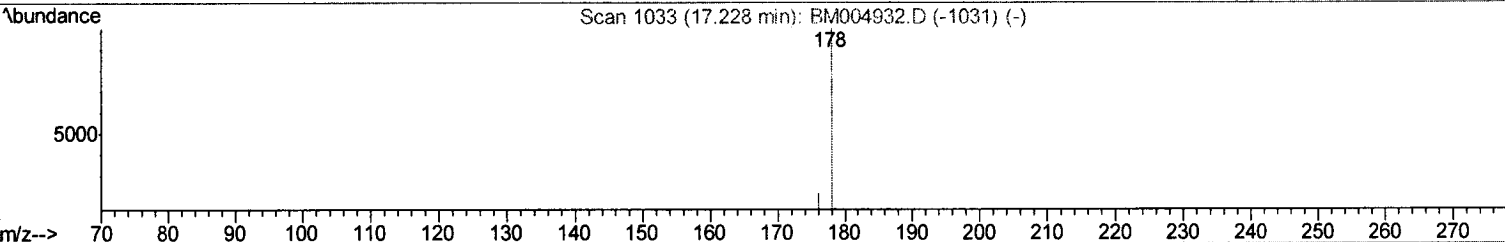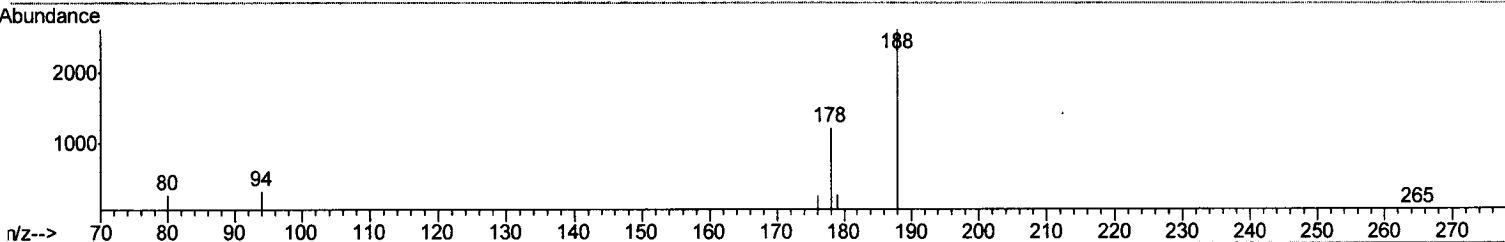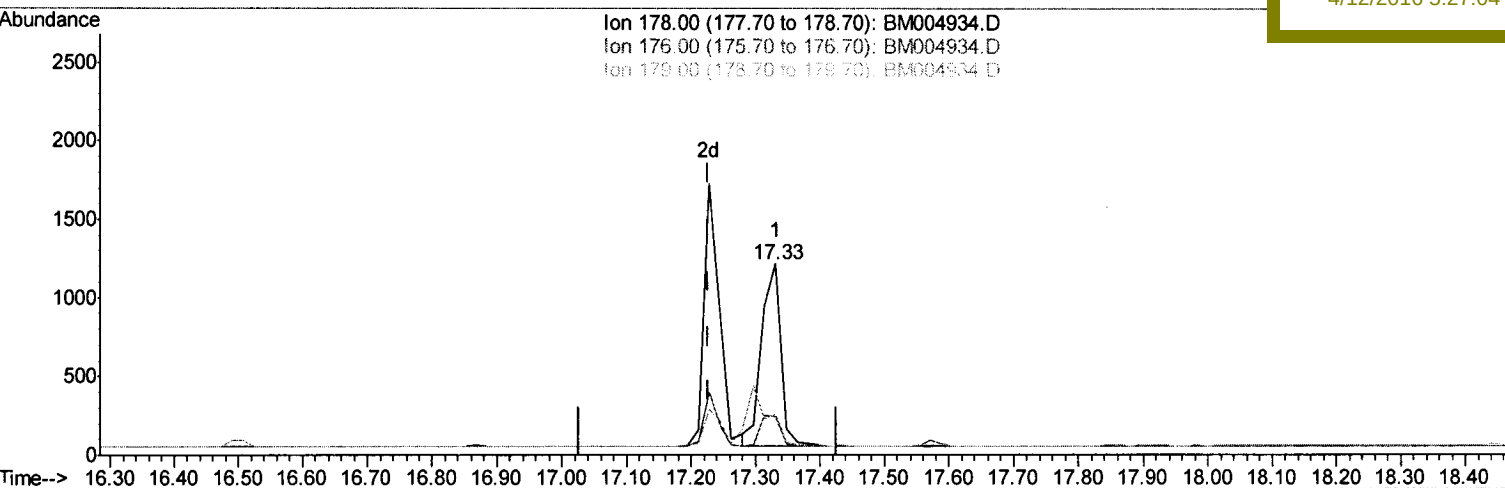

TIC: BM004934.D

(14) Phenanthrene

17.331min (+0.103) 0.12ng/ul

response 2415

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	19.85#
179.00	17.70	21.66#
0.00	0.00	0.00