

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM041116\  
 Data File : BM004937.D  
 Acq On : 11 Apr 2016 14:19  
 Operator : UM/SJ  
 Sample : SSTDCCC0.4EC  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 LabSampleID :  
 SSTD0.440

Manual Integrations  
 APPROVED

Sohil  
 4/12/2016 5:27:32 PM

Quant Time: Apr 12 01:14:37 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM032516.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Apr 12 01:10:05 2016  
 Response via : Initial Calibration

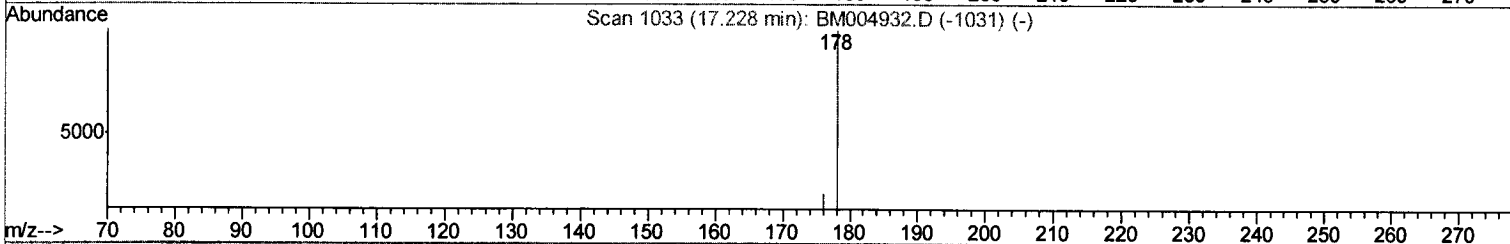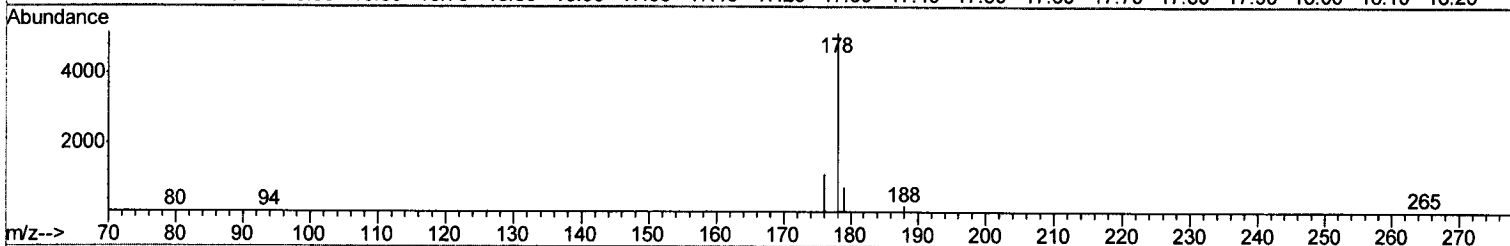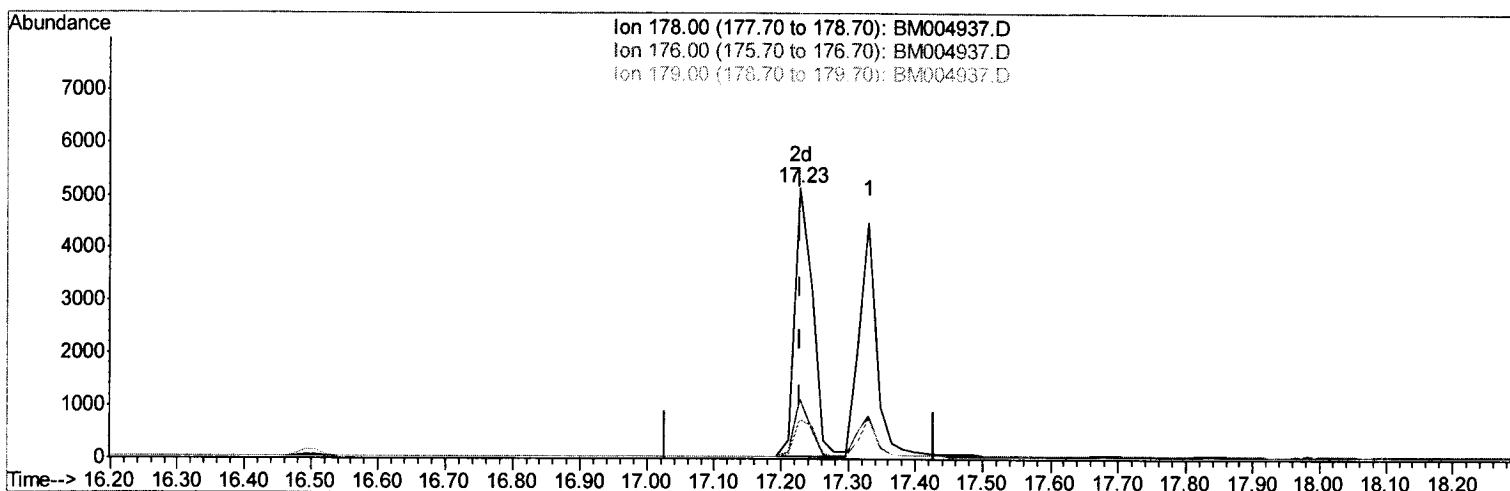

TIC: BM004937.D

(14) Phenanthrene

17.228min (-0.000) 0.41ng/ul m

response 9308

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 178.00 | 100   | 100    |
| 176.00 | 16.20 | 22.07# |
| 179.00 | 17.70 | 14.76  |
| 0.00   | 0.00  | 0.00   |


U-M  
 04/22/16

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM041116\  
Data File : BM004937.D  
Acq On : 11 Apr 2016 14:19  
Operator : UM/SJ  
Sample : SSTDCCC0.4EC  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_M  
LabSampleId :  
SSTD0.440

Manual Integrations  
APPROVED

Sohil  
4/12/2016 5:27:32 PM

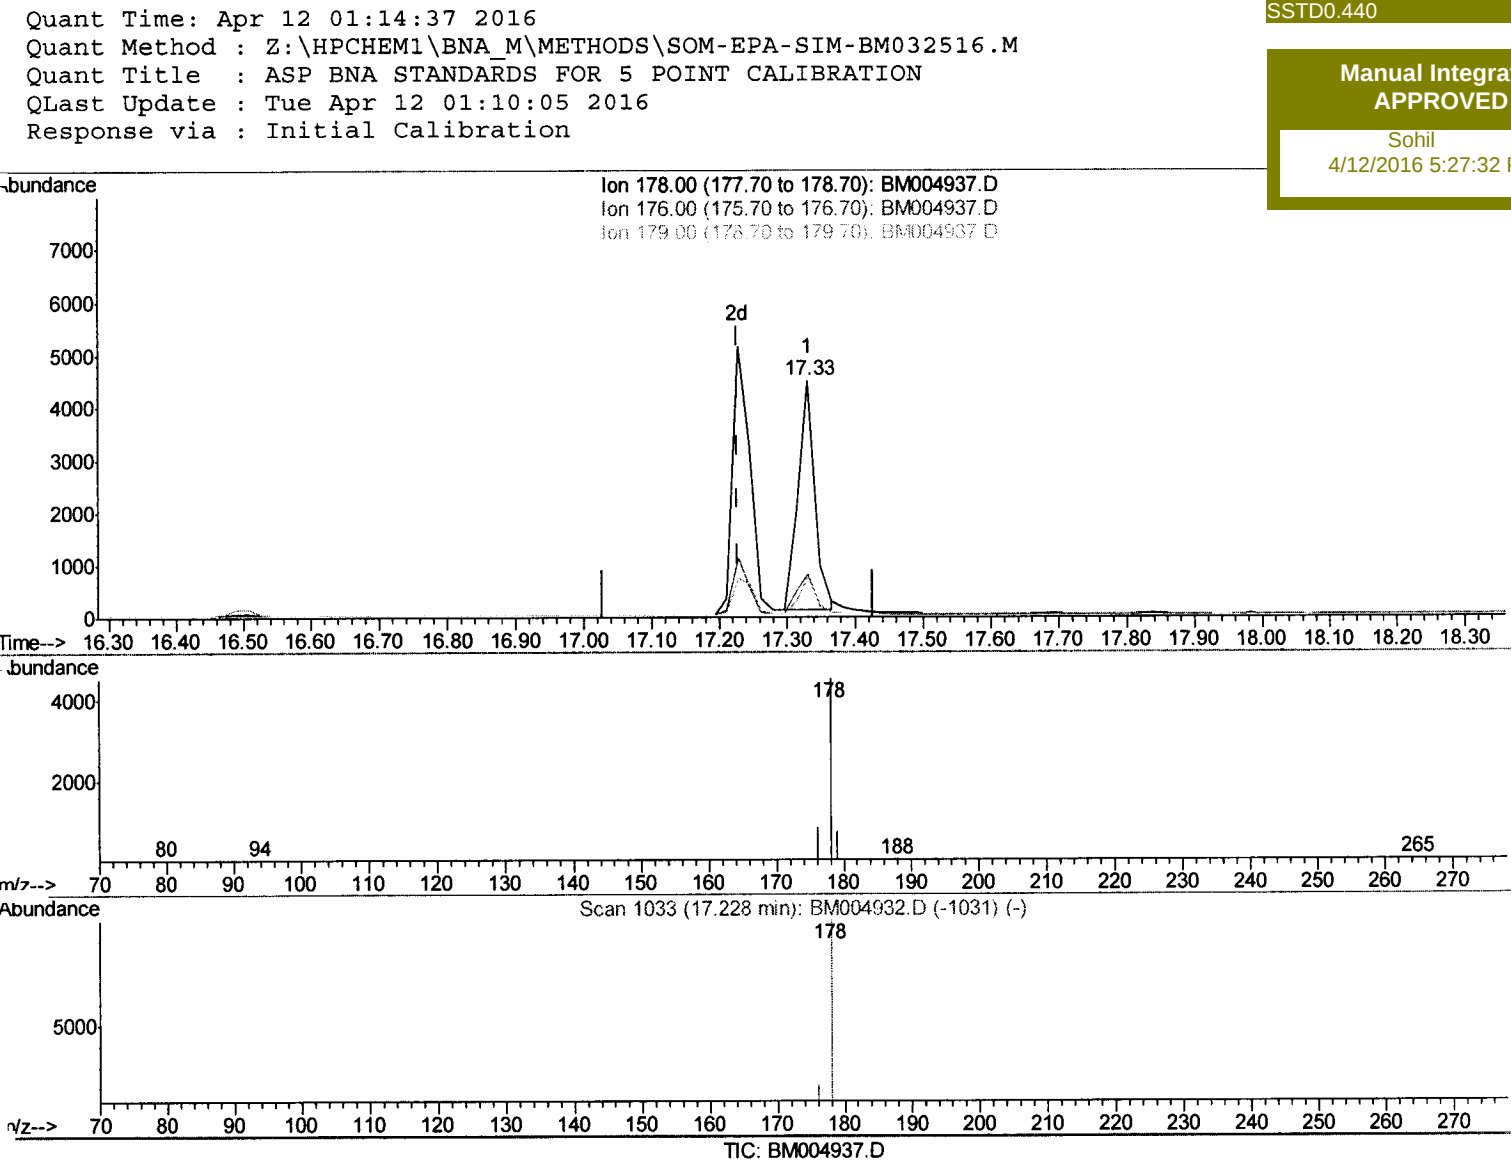

(14) Phenanthrene

17.331min (+0.103) 0.33ng/ul

response 7487

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 178.00 | 100   | 100   |
| 176.00 | 16.20 | 18.42 |
| 179.00 | 17.70 | 16.98 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM041116\  
 Data File : BM004937.D  
 Acq On : 11 Apr 2016 14:19  
 Operator : UM/SJ  
 Sample : SSTDCCC0.4EC  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 LabSampleID :  
 SSTD0.440

Manual Integrations  
 APPROVED

Sohil  
 4/12/2016 5:27:32 PM

Quant Time: Apr 12 01:33:57 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM032516.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Apr 12 01:10:05 2016  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.82  | 152  | 1518     | 0.40 | ng/ul | 0.00     |
| 4) Naphthalene-d8         | 10.61 | 136  | 6172     | 0.40 | ng/ul | 0.00     |
| 8) Acenaphthene-d10       | 14.45 | 164  | 3487     | 0.40 | ng/ul | 0.00     |
| 12) Phenanthrene-d10      | 17.19 | 188  | 8033     | 0.40 | ng/ul | 0.00     |
| 18) Chrysene-d12          | 21.39 | 240  | 8078     | 0.40 | ng/ul | 0.00     |
| 22) Perylene-d12          | 23.67 | 264  | 6677     | 0.40 | ng/ul | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|-----------------------------|-------|------|----------|------|-------|----------|
| 2) 1,4-Dioxane-d8           | 3.32  | 96   | 1420     | 2.08 | ng/uL | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.21 | 152  | 3123     | 0.36 | ng/ul | 0.00     |
| 16) Fluoranthene-d10        | 19.23 | 212  | 7542     | 0.40 | ng/ul | 0.00     |

| Target Compounds           | R.T.  | QIon | Response | Conc | Units  | Qvalue |
|----------------------------|-------|------|----------|------|--------|--------|
| 3) 1,4-Dioxane             | 3.35  | 88   | 1726     | 2.07 | ng/ul# | 23     |
| 5) Naphthalene             | 10.66 | 128  | 5920     | 0.40 | ng/ul# | 95     |
| 7) 2-Methylnaphthalene     | 12.27 | 142  | 4120     | 0.39 | ng/ul  | 98     |
| 9) Acenaphthylene          | 14.16 | 152  | 5794     | 0.36 | ng/ul  | 98     |
| 10) Acenaphthene           | 14.50 | 153  | 4706     | 0.41 | ng/ul# | 77     |
| 11) Fluorene               | 15.51 | 166  | 5488     | 0.41 | ng/ul  | 97     |
| 13) Pentachlorophenol      | 16.85 | 266  | 524      | 0.26 | ng/ul  | 94     |
| 14) Phenanthrene           | 17.23 | 178  | 9308m    | 0.41 | ng/ul  |        |
| 15) Anthracene             | 17.33 | 178  | 7996     | 0.37 | ng/ul  | 98     |
| 17) Fluoranthene           | 19.25 | 202  | 10562    | 0.41 | ng/ul  | 96     |
| 19) Pyrene                 | 19.62 | 202  | 10931    | 0.40 | ng/ul  | 98     |
| 20) Benzo(a)anthracene     | 21.37 | 228  | 9554     | 0.38 | ng/ul  | 95     |
| 21) Chrysene               | 21.42 | 228  | 9798     | 0.41 | ng/ul  | 95     |
| 23) Benzo(b)fluoranthene   | 22.98 | 252  | 9668     | 0.43 | ng/ul  | 93     |
| 24) Benzo(k)fluoranthene   | 23.02 | 252  | 8663     | 0.42 | ng/ul# | 96     |
| 25) Benzo(a)pyrene         | 23.57 | 252  | 8364     | 0.41 | ng/ul# | 94     |
| 26) Indeno(1,2,3-cd)pyrene | 25.98 | 276  | 8142     | 0.43 | ng/ul# | 83     |
| 27) Dibenzo(a,h)anthracene | 26.01 | 278  | 6504     | 0.43 | ng/ul# | 92     |
| 28) Benzo(g,h,i)perylene   | 26.69 | 276  | 6908     | 0.44 | ng/ul# | 92     |

U.M  
 04/22/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

(QT Reviewed)

```
Data Path   : Z:\HPCHEM1\BNA_M\DATA\BM041116\  
Data File  : BM004937.D  
Acq On     : 11 Apr 2016   14:19  
Operator   : UM/SJ  
Sample     : SSTDCCC0.4EC  
Misc       :  
ALS Vial   : 2      Sample Multiplier: 1
```

**Instrument :**  
BNA\_M  
**LabSampleId :**  
SSTD0.440

## Manual Integrations

Sohil  
4/12/2016 5:27:32 PM

Quant Time: Apr 12 01:33:57 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM032516.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 12 01:10:05 2016  
Response via : Initial Calibration

