

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034607.D
 Acq On : 11 Apr 2022 12:49
 Operator : CG/JU
 Sample : N2266-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ66

Manual Integrations
 APPROVED

Reviewed By :Jagrut
 Upadhyay

04/13/2022
 Supervised By :Yogesh
 Patel

Quant Time: Apr 12 02:54:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	96677	20.000	ng/u1	0.00
20) Naphthalene-d8	10.689	136	391892	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.524	164	228798	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.265	188	444146	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.442	240	416722m	20.000	ng/u1	0.00
88) Perylene-d12	23.824	264	484154	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	12146m	4.480	ng/uL	0.00
4) Pyridine-d5	3.690	84	59942	9.161	ng/u1	0.01
7) Phenol-d5	7.043	99	37455	4.655	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	157776	29.425	ng/u1	0.00
11) 2-Chlorophenol-d4	7.407	132	137752	22.146	ng/u1	0.00
15) 4-Methylphenol-d8	8.590	113	79480	12.645	ng/u1	0.00
21) Nitrobenzene-d5	9.042	128	86500m	30.033	ng/u1	0.00
24) 2-Nitrophenol-d4	9.766	143	84653	28.230	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.307	165	137505	24.353	ng/u1	0.00
31) 4-Chloroaniline-d4	10.825	131	186153	23.897	ng/u1	0.00
46) Dimethylphthalate-d6	13.936	166	537032	32.484	ng/u1	0.00
49) Acenaphthylene-d8	14.219	160	633326	29.805	ng/u1	0.00
54) 4-Nitrophenol-d4	14.766	143	4363m	1.731	ng/u1	0.05
60) Fluorene-d10	15.513	176	476771	33.372	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	68828	25.385	ng/u1	0.00
73) Anthracene-d10	17.365	188	754526	35.632	ng/u1	0.00
81) Pyrene-d10	19.654	212	957100	42.080	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.665	264	867785	35.632	ng/u1	0.00

Target Compounds Qvalue
 35) 4-Chloro-3-methylphenol 11.989 107 24279m 4.197 ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034607.D
Acq On : 11 Apr 2022 12:49
Operator : CG/JU
Sample : N2266-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ66


Quant Time: Apr 12 02:54:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration


Manual Integrations
APPROVED

Reviewed By :Jagrut
Upadhyay

04/13/2022
Supervised By :Yogesh
Patel


04/14/2022

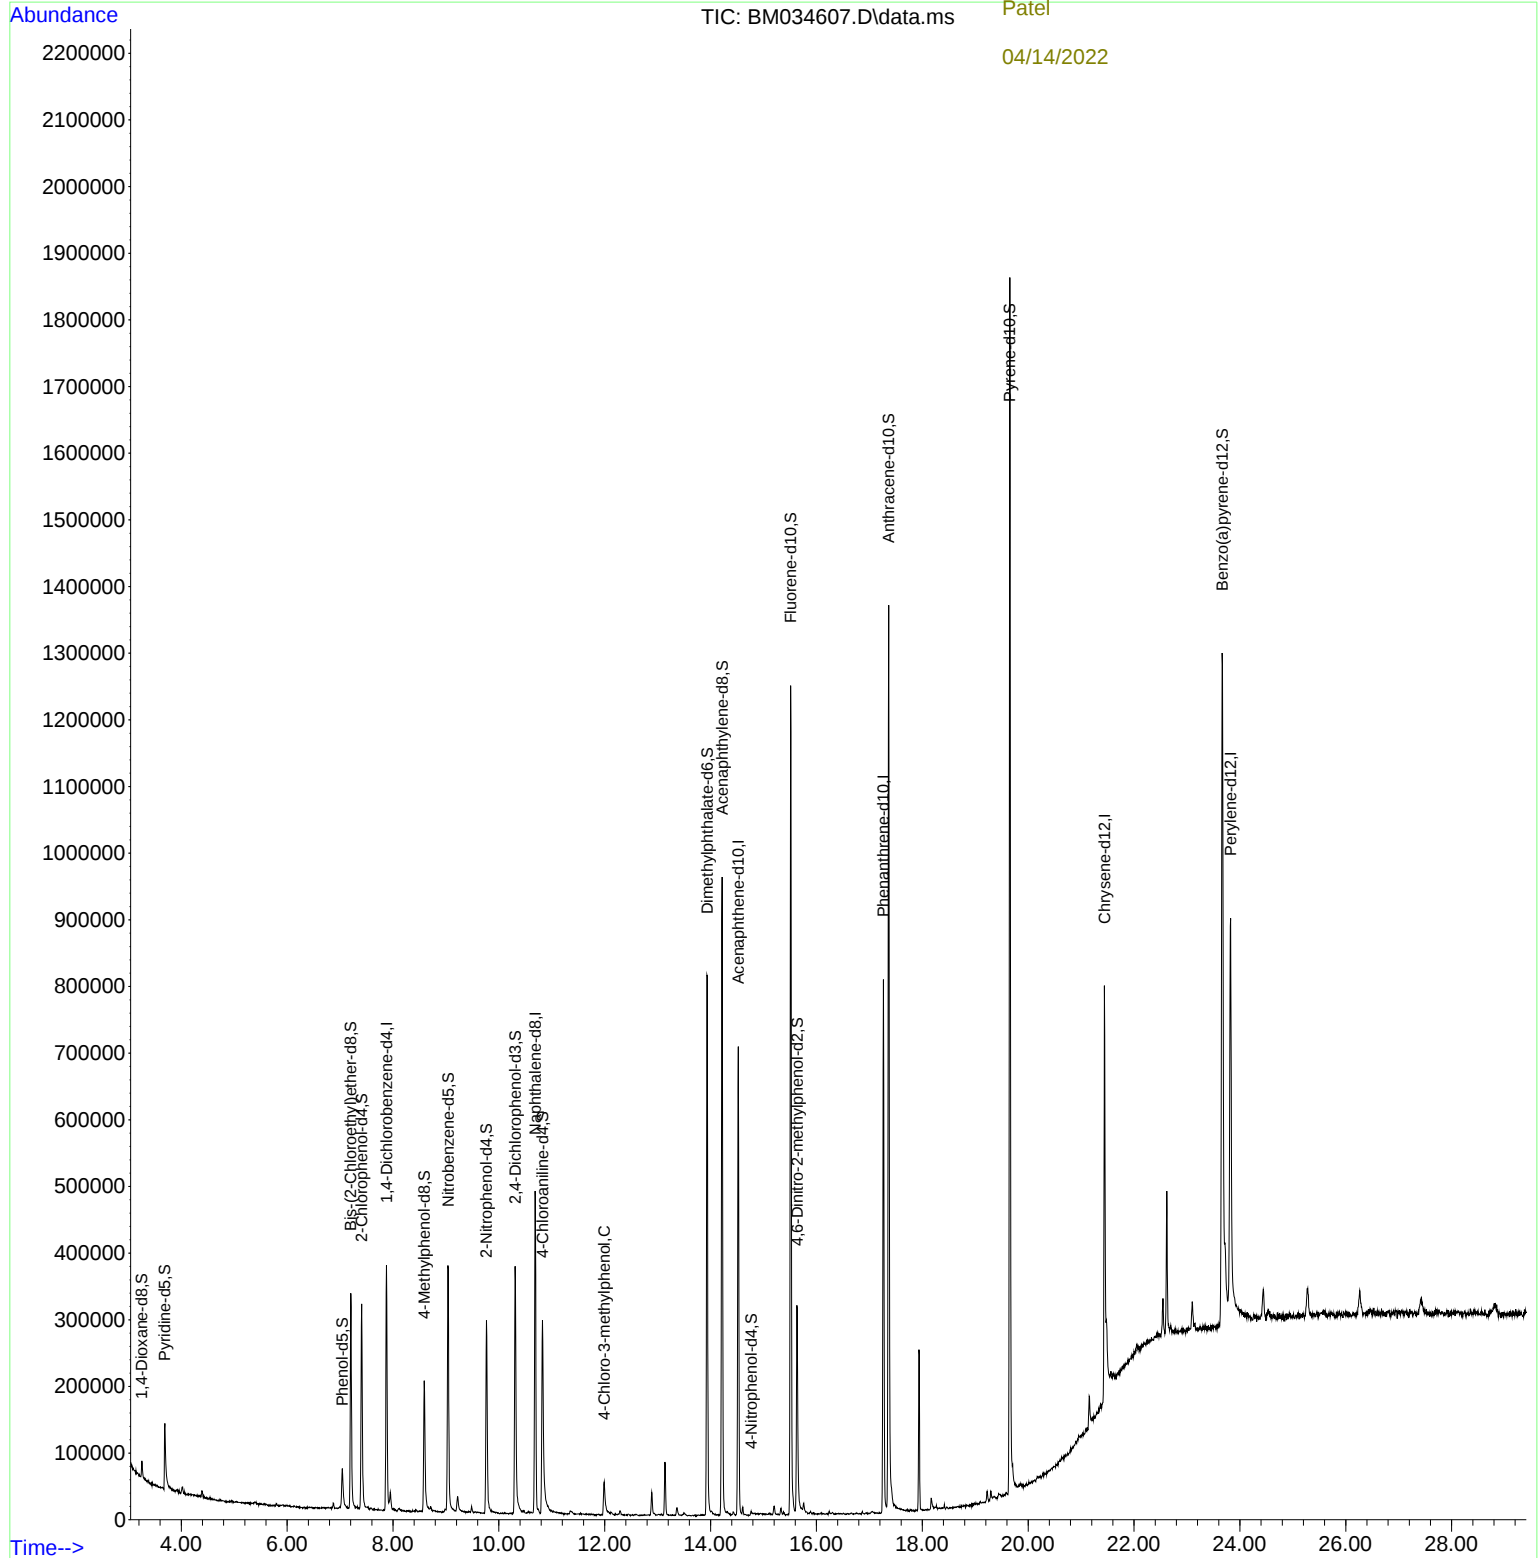

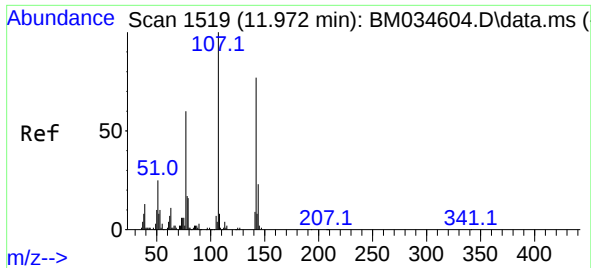

#35
 4-Chloro-3-methylphenol
 Concen: 4.197 ng/ul m
 RT: 11.989 min Scan# 1
 Delta R.T. 0.012 min
 Lab File: BM034607.D
 Acq: 11 Apr 2022 12:49

Instrument :
 BNA_M
 ClientSampleId :
 YAZ66

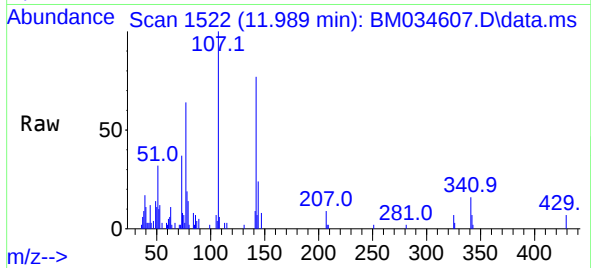

Tgt Ion:	107	Resp:	24279
Ion	Ratio	Lower	Upper
107	100		
144	23.9	23.0	34.4
142	77.1	69.8	104.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut
 Upadhyay

04/13/2022
 Supervised By :Yogesh
 Patel

04/14/2022

