

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034606.D
 Acq On : 11 Apr 2022 12:13
 Operator : CG/JU
 Sample : N2319-10DL 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.231	29	33	35	rBV5	17073	22077	1.49%	0.132%
2	3.290	40	43	50	rVB	102224	129033	8.68%	0.773%
3	3.702	110	113	122	rBV	31906	64001	4.31%	0.384%
4	4.561	255	259	265	rVB2	26508	38319	2.58%	0.230%
5	5.908	484	488	494	rVB7	7563	12114	0.82%	0.073%
6	6.872	649	652	655	rVB4	4118	4747	0.32%	0.028%
7	7.043	676	681	692	rBV2	30252	70555	4.75%	0.423%
8	7.202	703	708	723	rBV	176462	308217	20.74%	1.847%
9	7.407	736	743	756	rVB3	187012	354270	23.84%	2.123%
10	7.878	816	823	832	rBV	404635	683763	46.02%	4.098%
11	8.031	846	849	850	rBV2	2554	2759	0.19%	0.017%
12	8.596	939	945	956	rBV	95065	194503	13.09%	1.166%
13	8.878	992	993	995	rVV2	1556	1625	0.11%	0.010%
14	9.043	1014	1021	1033	rBV	188444	362516	24.40%	2.173%
15	9.196	1038	1047	1059	rBV	164999	354599	23.87%	2.125%
16	9.331	1068	1070	1078	rVB8	4460	9635	0.65%	0.058%
17	9.484	1092	1096	1103	rVB4	7576	11574	0.78%	0.069%
18	9.631	1118	1121	1122	rBV3	1721	1517	0.10%	0.009%
19	9.766	1138	1144	1158	rBV	143027	277304	18.66%	1.662%
20	10.007	1183	1185	1190	rVB4	1941	2388	0.16%	0.014%
21	10.054	1190	1193	1194	rBV2	1571	1594	0.11%	0.010%
22	10.160	1209	1211	1217	rVB5	1758	2301	0.15%	0.014%
23	10.254	1225	1227	1230	rVB4	1351	1600	0.11%	0.010%
24	10.307	1230	1236	1251	rBV	187264	380439	25.61%	2.280%
25	10.601	1283	1286	1289	rVB5	2413	2481	0.17%	0.015%
26	10.684	1293	1300	1314	rVV	540662	936366	63.02%	5.612%
27	10.831	1318	1325	1346	rBV	103946	297702	20.04%	1.784%
28	10.960	1346	1347	1350	rVB3	2571	1658	0.11%	0.010%
29	11.272	1397	1400	1403	rBV3	1611	2618	0.18%	0.016%
30	11.331	1406	1410	1412	rBV4	2046	2040	0.14%	0.012%
31	11.378	1415	1418	1422	rVB4	1262	1682	0.11%	0.010%
32	11.543	1441	1446	1448	rBV5	1799	1899	0.13%	0.011%
33	11.578	1450	1452	1453	rVB2	2546	1546	0.10%	0.009%
34	11.625	1455	1460	1462	rBV5	1430	2118	0.14%	0.013%
35	11.725	1475	1477	1479	rVV3	1878	1695	0.11%	0.010%
36	11.895	1502	1506	1510	rVB7	1046	1927	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034606.D
 Acq On : 11 Apr 2022 12:13
 Operator : CG/JU
 Sample : N2319-10DL 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	11.937	1510	1513	1516	rBV5	1537	1741	0.12%	0.010%
38	12.048	1529	1532	1533	rBV2	2098	1775	0.12%	0.011%
39	12.119	1538	1544	1547	rBV4	2939	4047	0.27%	0.024%
40	12.313	1570	1577	1580	rBV5	2689	5680	0.38%	0.034%
41	12.884	1672	1674	1677	rBV4	1392	1601	0.11%	0.010%
42	12.948	1681	1685	1689	rVB5	1708	3010	0.20%	0.018%
43	13.025	1694	1698	1700	rBV4	1430	2023	0.14%	0.012%
44	13.148	1716	1719	1722	rVB5	1361	1543	0.10%	0.009%
45	13.360	1748	1755	1761	rBV6	5421	8468	0.57%	0.051%
46	13.601	1791	1796	1801	rBV8	1459	3394	0.23%	0.020%
47	13.931	1846	1852	1862	rBV	454360	709837	47.78%	4.254%
48	14.019	1865	1867	1870	rVB4	3199	3230	0.22%	0.019%
49	14.119	1880	1884	1885	rBV3	1240	1628	0.11%	0.010%
50	14.219	1894	1901	1913	rBV	499356	785570	52.87%	4.708%
51	14.436	1933	1938	1942	rVB6	1799	2643	0.18%	0.016%
52	14.525	1946	1953	1966	rBV	775353	1160964	78.14%	6.958%
53	14.772	1990	1995	1996	rBV5	2591	3601	0.24%	0.022%
54	14.983	2029	2031	2039	rVB7	3581	5665	0.38%	0.034%
55	15.060	2039	2044	2051	rVB7	2858	5178	0.35%	0.031%
56	15.119	2051	2054	2055	rBV2	2002	1599	0.11%	0.010%
57	15.136	2055	2057	2062	rVB5	1101	1546	0.10%	0.009%
58	15.183	2062	2065	2069	rBV5	1309	1629	0.11%	0.010%
59	15.325	2086	2089	2090	rVV3	1625	2068	0.14%	0.012%
60	15.342	2090	2092	2094	rVB3	1627	1501	0.10%	0.009%
61	15.466	2111	2113	2115	rBV3	1342	1537	0.10%	0.009%
62	15.513	2115	2121	2136	rVV	660883	1041213	70.08%	6.240%
63	15.636	2136	2142	2154	rVV	151833	277244	18.66%	1.662%
64	15.754	2159	2162	2166	rVV5	9626	17102	1.15%	0.102%
65	15.783	2166	2167	2170	rVV3	4709	4553	0.31%	0.027%
66	15.819	2172	2173	2176	rVB3	3178	1969	0.13%	0.012%
67	15.860	2178	2180	2183	rVV4	1491	1609	0.11%	0.010%
68	15.954	2195	2196	2201	rVB4	1711	1681	0.11%	0.010%
69	16.054	2210	2213	2214	rBV2	2321	1964	0.13%	0.012%
70	16.236	2241	2244	2251	rVV8	3323	6615	0.45%	0.040%
71	16.307	2252	2256	2260	rVV7	3393	5603	0.38%	0.034%
72	16.495	2286	2288	2289	rBV2	2294	1528	0.10%	0.009%
73	16.613	2306	2308	2312	rBV4	1706	2022	0.14%	0.012%
74	16.689	2317	2321	2324	rBV5	2836	3807	0.26%	0.023%
75	16.825	2339	2344	2345	rBV5	1775	2405	0.16%	0.014%
76	16.883	2349	2354	2357	rBV7	2720	3927	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034606.D
 Acq On : 11 Apr 2022 12:13
 Operator : CG/JU
 Sample : N2319-10DL 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

77	17.048	2377	2382	2386	rVV6	4842	10779	0.73%	0.065%
78	17.136	2395	2397	2402	rVV6	2892	2999	0.20%	0.018%
79	17.266	2412	2419	2430	rBV	872656	1301971	87.63%	7.803%
80	17.366	2430	2436	2453	rVB	708018	1132788	76.24%	6.789%
81	17.766	2502	2504	2507	rVB4	3198	3399	0.23%	0.020%
82	17.860	2516	2520	2525	rVB3	6754	11467	0.77%	0.069%
83	18.013	2545	2546	2550	rBV4	2024	3072	0.21%	0.018%
84	18.166	2567	2572	2573	rBV2	29441	36197	2.44%	0.217%
85	18.189	2573	2576	2582	rVB2	37246	55139	3.71%	0.330%
86	18.654	2653	2655	2657	rBV3	2649	2341	0.16%	0.014%
87	18.713	2663	2665	2666	rVB2	3334	1892	0.13%	0.011%
88	18.836	2683	2686	2687	rBV3	2973	3716	0.25%	0.022%
89	19.224	2748	2752	2755	rBV4	12062	14730	0.99%	0.088%
90	19.295	2761	2764	2766	rBV2	11385	14085	0.95%	0.084%
91	19.324	2766	2769	2773	rVV5	15284	19788	1.33%	0.119%
92	19.654	2819	2825	2842	rBV	1016305	1485760	100.00%	8.904%
93	21.442	3124	3129	3146	rBV	820307	1418391	95.47%	8.500%
94	23.665	3501	3507	3513	rBV2	537629	1104583	74.34%	6.620%
95	23.818	3527	3533	3546	rVB2	632780	1422977	95.77%	8.528%




Sum of corrected areas: 16685976

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034606.D
Acq On : 11 Apr 2022 12:13
Operator : CG/JU
Sample : N2319-10DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

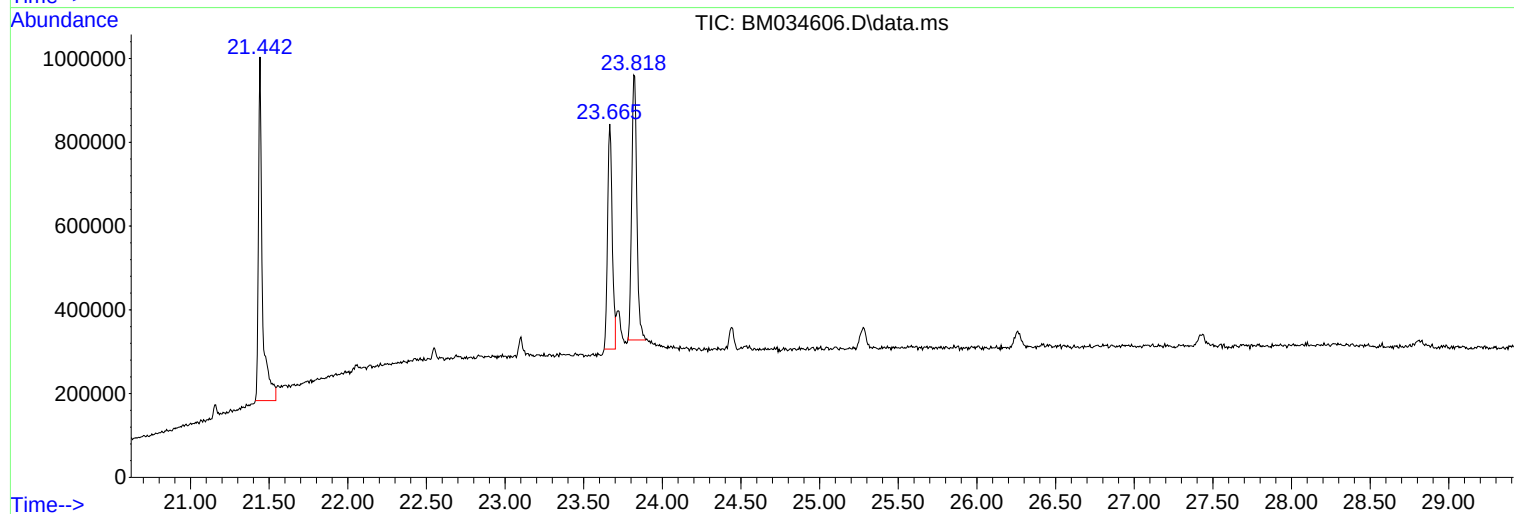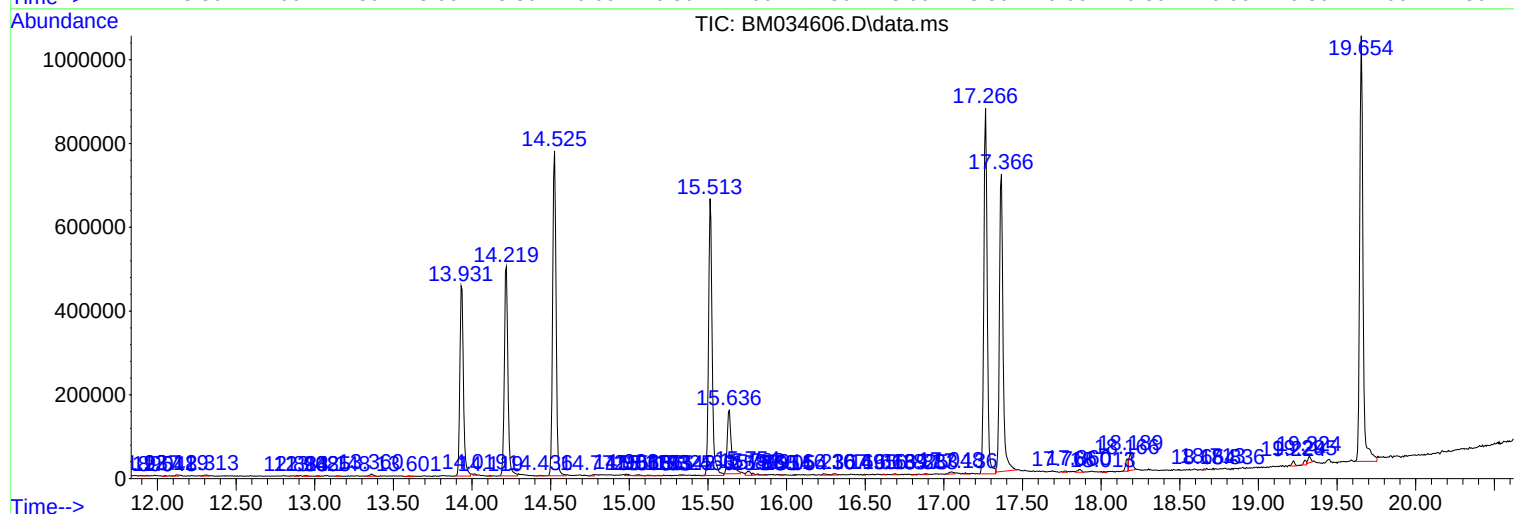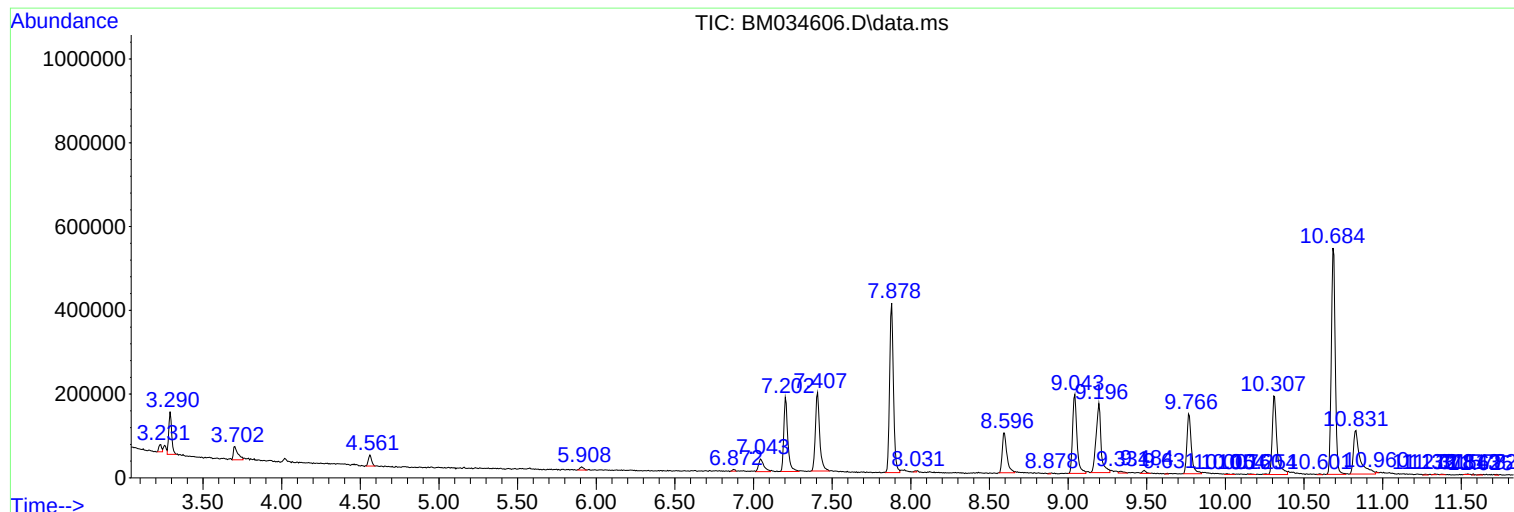

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034606.D
Acq On : 11 Apr 2022 12:13
Operator : CG/JU
Sample : N2319-10DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H8DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanoic acid, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.196	10.37 ng/ul	354599	1,4-Dichlorobenzene-d4	7.878

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	78
2			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	78
3			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	78
4			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	72
5			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	72

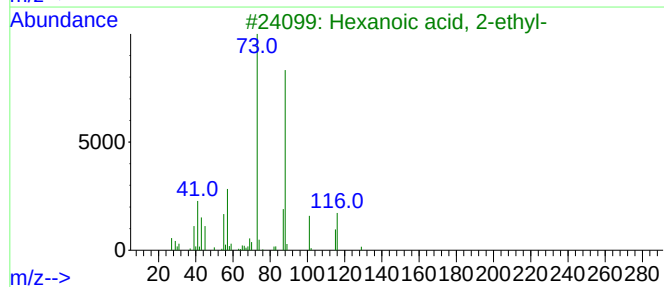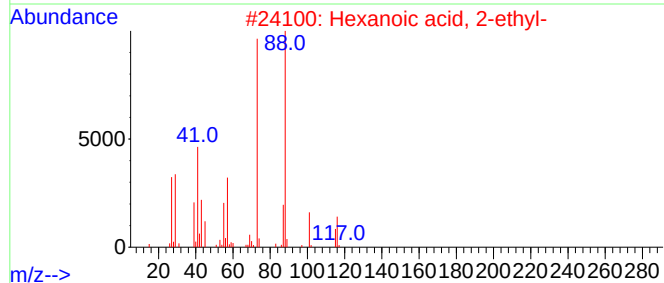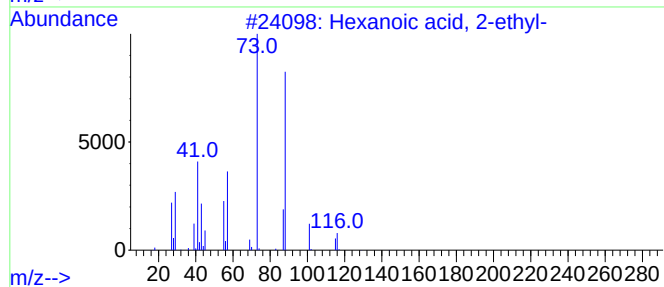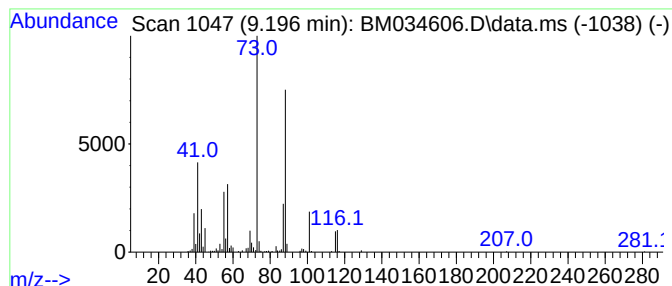

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034606.D
Acq On : 11 Apr 2022 12:13
Operator : CG/JU
Sample : N2319-10DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanoic acid, ...	9.196	10.4	ng/ul	354599	1	7.878	683763	20.0