

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034609.D
 Acq On : 11 Apr 2022 14:38
 Operator : CG/JU
 Sample : N2338-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.255	34	37	43	rVB	33294	48167	1.45%	0.168%
2	3.684	108	110	125	rBV	146646	240619	7.26%	0.838%
3	4.019	164	167	172	rVB3	11049	17178	0.52%	0.060%
4	5.166	358	362	370	rVB3	15074	25648	0.77%	0.089%
5	7.037	674	680	694	rBV	91509	186771	5.63%	0.650%
6	7.201	702	708	726	rBV	443383	723478	21.82%	2.520%
7	7.407	736	743	758	rBV	419331	737639	22.25%	2.569%
8	7.507	758	760	766	rVB6	6776	8265	0.25%	0.029%
9	7.878	816	823	834	rBV	376331	653075	19.70%	2.275%
10	8.231	879	883	890	rVB3	10862	20148	0.61%	0.070%
11	8.589	938	944	960	rBV	293579	548597	16.55%	1.911%
12	9.036	1014	1020	1038	rBV	514872	897622	27.07%	3.126%
13	9.484	1093	1096	1101	rVB2	11244	15513	0.47%	0.054%
14	9.766	1137	1144	1157	rBV	391521	704332	21.24%	2.453%
15	10.307	1227	1236	1254	rBV	513155	949483	28.64%	3.307%
16	10.554	1274	1278	1282	rVB5	2826	3640	0.11%	0.013%
17	10.683	1293	1300	1309	rBV	522839	879971	26.54%	3.065%
18	10.825	1317	1324	1351	rBV	400791	899937	27.14%	3.134%
19	11.989	1518	1522	1524	rVB4	4036	5046	0.15%	0.018%
20	12.301	1571	1575	1581	rBV6	4969	11730	0.35%	0.041%
21	13.366	1752	1756	1764	rVB7	5454	10786	0.33%	0.038%
22	13.930	1846	1852	1865	rBV	1072225	1610785	48.58%	5.610%
23	14.019	1865	1867	1872	rVV5	6380	11213	0.34%	0.039%
24	14.218	1894	1901	1914	rBV	1269825	1881625	56.75%	6.553%
25	14.524	1945	1953	1963	rBV	747741	1089111	32.85%	3.793%
26	14.760	1985	1993	1999	rBV9	8838	27534	0.83%	0.096%
27	14.948	2019	2025	2027	rVB4	1971	3438	0.10%	0.012%
28	15.383	2096	2099	2102	rVB3	2876	3350	0.10%	0.012%
29	15.513	2115	2121	2136	rBV	1635777	2415210	72.84%	8.412%
30	15.630	2136	2141	2153	rBV	477310	766214	23.11%	2.669%
31	15.754	2159	2162	2167	rVB	15433	22663	0.68%	0.079%
32	16.301	2252	2255	2259	rVB6	4254	6064	0.18%	0.021%
33	17.059	2377	2384	2393	rBV8	3360	7944	0.24%	0.028%
34	17.265	2413	2419	2429	rBV	851835	1219626	36.78%	4.248%
35	17.365	2430	2436	2453	rVV	1827292	2736955	82.55%	9.532%
36	17.948	2531	2535	2537	rBV5	4515	4996	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034609.D
 Acq On : 11 Apr 2022 14:38
 Operator : CG/JU
 Sample : N2338-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	18.171	2568	2573	2583	rBV5	22023	45152	1.36%	0.157%
38	18.995	2711	2713	2715	rBV3	3420	3358	0.10%	0.012%
39	19.224	2748	2752	2758	rBV3	22266	35746	1.08%	0.124%
40	19.295	2760	2764	2770	rBV	19349	33212	1.00%	0.116%
41	19.448	2786	2790	2797	rBV9	11893	24518	0.74%	0.085%
42	19.589	2812	2814	2817	rVB4	6518	6151	0.19%	0.021%
43	19.653	2819	2825	2832	rBV	2422394	3315672	100.00%	11.548%
44	21.153	3077	3080	3091	rBV4	63244	98939	2.98%	0.345%
45	21.442	3125	3129	3135	rBV	648866	1059595	31.96%	3.690%
46	23.671	3501	3508	3526	rBV	1420980	3207076	96.72%	11.169%
47	23.824	3528	3534	3552	rVB2	660436	1489103	44.91%	5.186%


Sum of corrected areas: 28712895

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034609.D
Acq On : 11 Apr 2022 14:38
Operator : CG/JU
Sample : N2338-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

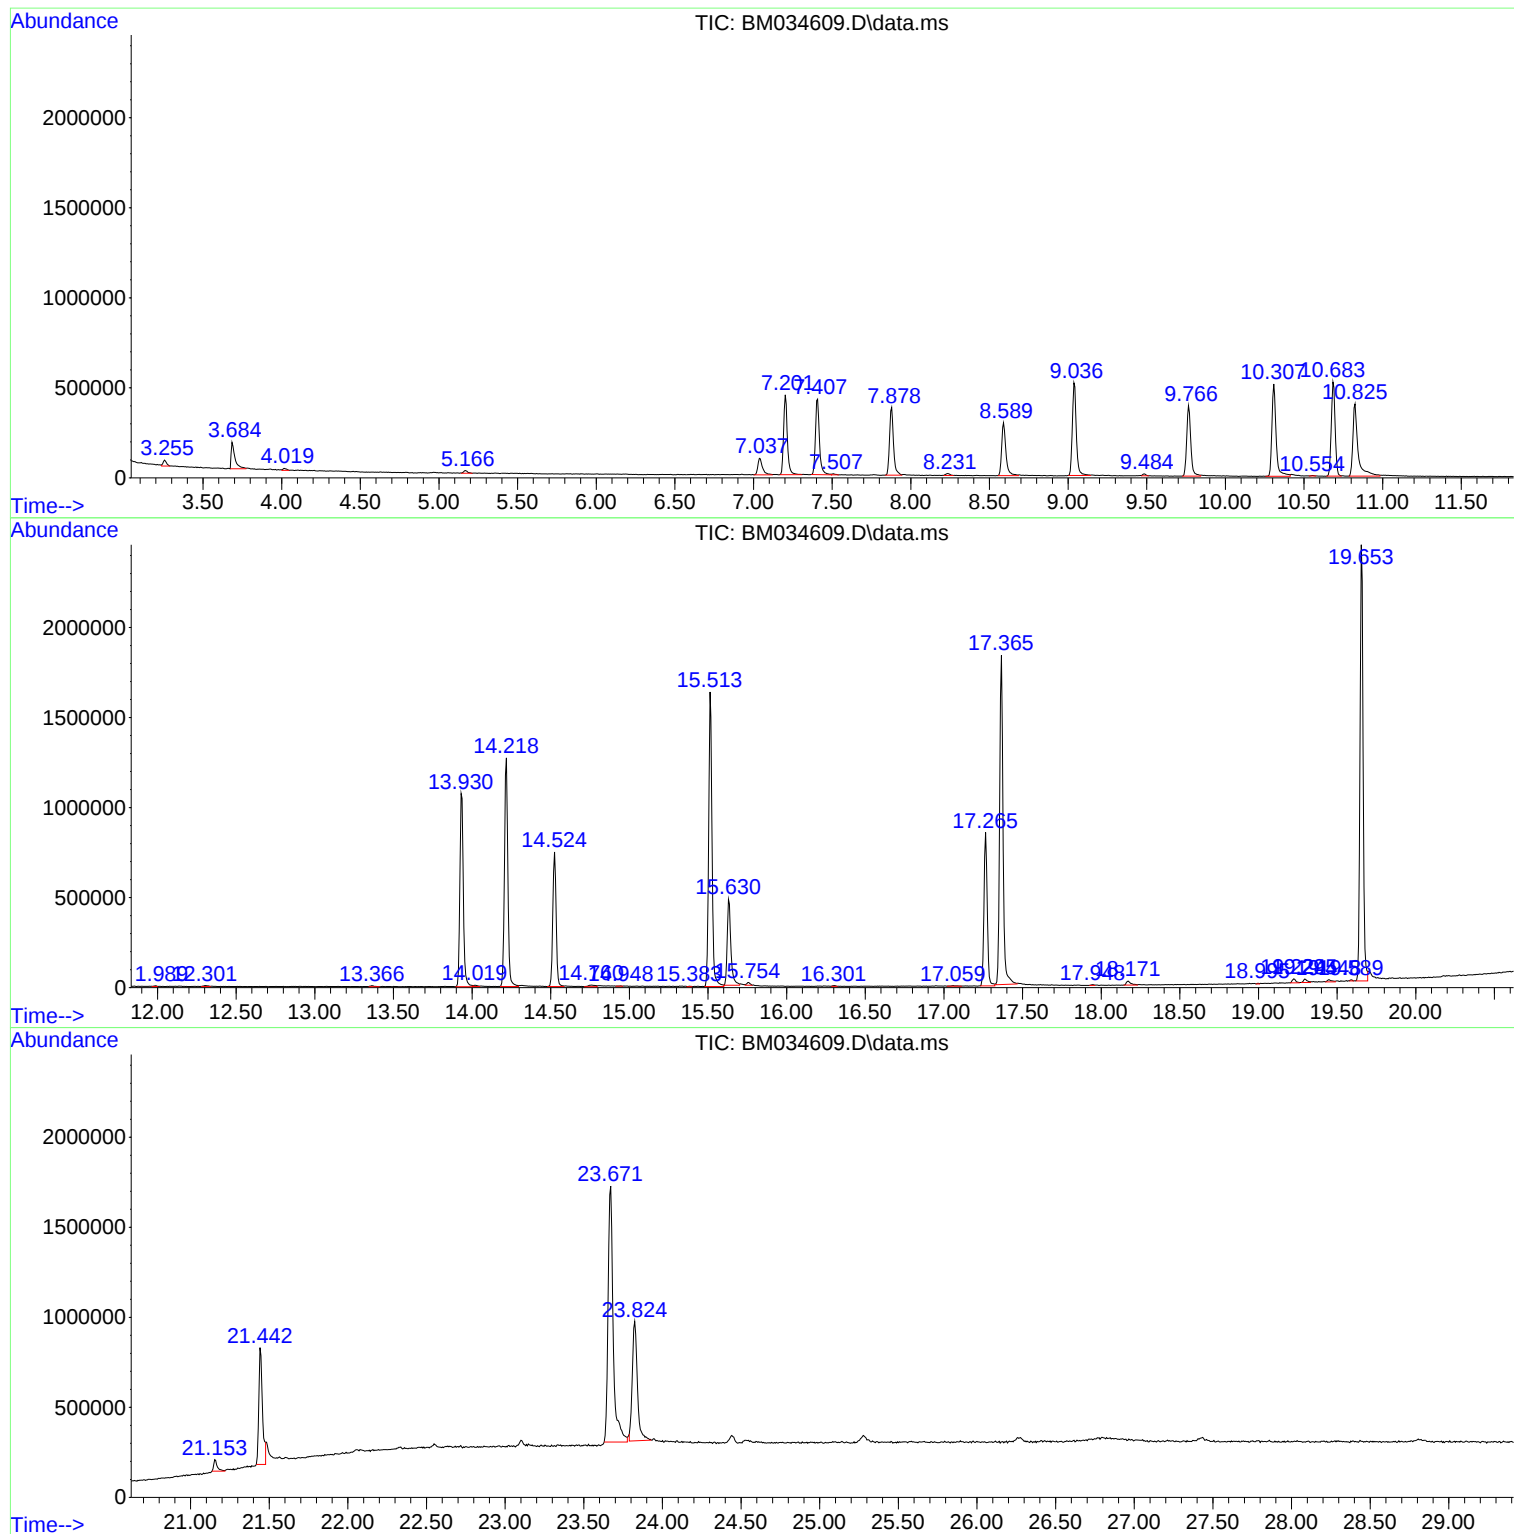

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034609.D
Acq On : 11 Apr 2022 14:38
Operator : CG/JU
Sample : N2338-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034609.D
Acq On : 11 Apr 2022 14:38
Operator : CG/JU
Sample : N2338-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------