

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034610.D
 Acq On : 11 Apr 2022 15:15
 Operator : CG/JU
 Sample : N2338-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.254	34	37	44	rVB2	31981	44787	1.47%	0.162%
2	3.684	108	110	128	rBV	127759	230188	7.58%	0.834%
3	7.042	675	681	690	rBV	95930	181258	5.97%	0.657%
4	7.201	702	708	719	rBV	423259	699323	23.02%	2.533%
5	7.407	736	743	756	rBV	420101	722067	23.76%	2.616%
6	7.878	816	823	840	rBV	368090	652610	21.48%	2.364%
7	8.236	880	884	890	rVB6	3894	8423	0.28%	0.031%
8	8.589	938	944	958	rBV	297374	542231	17.85%	1.964%
9	9.042	1013	1021	1039	rBV	488582	896959	29.52%	3.249%
10	9.483	1090	1096	1102	rBV5	6223	10227	0.34%	0.037%
11	9.766	1137	1144	1160	rBV	385191	676146	22.25%	2.449%
12	10.307	1229	1236	1250	rBV	482227	899357	29.60%	3.258%
13	10.554	1275	1278	1281	rVB4	3230	4388	0.14%	0.016%
14	10.689	1294	1301	1313	rVB	488175	845027	27.81%	3.061%
15	10.824	1317	1324	1347	rBV	359719	844616	27.80%	3.060%
16	12.142	1542	1548	1552	rBV6	1437	3213	0.11%	0.012%
17	12.307	1569	1576	1577	rBV4	5095	7686	0.25%	0.028%
18	13.366	1751	1756	1758	rBV3	3501	5012	0.16%	0.018%
19	13.936	1846	1853	1865	rBV	1054355	1567433	51.58%	5.678%
20	14.024	1865	1868	1870	rVB4	3763	4957	0.16%	0.018%
21	14.218	1892	1901	1914	rBV	1215932	1830497	60.24%	6.631%
22	14.524	1943	1953	1963	rBV	708690	1040635	34.25%	3.770%
23	14.765	1987	1994	1997	rBV7	8750	19767	0.65%	0.072%
24	15.330	2086	2090	2092	rBV4	3395	3715	0.12%	0.013%
25	15.512	2115	2121	2135	rBV	1524104	2319840	76.35%	8.404%
26	15.630	2135	2141	2159	rVV	433968	737519	24.27%	2.672%
27	15.754	2159	2162	2172	rVB3	17118	32200	1.06%	0.117%
28	16.301	2251	2255	2263	rBV8	4271	6414	0.21%	0.023%
29	17.265	2413	2419	2429	rBV	816945	1160350	38.19%	4.203%
30	17.365	2429	2436	2454	rVV	1677378	2561865	84.31%	9.280%
31	17.777	2503	2506	2509	rVB4	2861	3464	0.11%	0.013%
32	17.801	2509	2510	2516	rBV5	2183	3521	0.12%	0.013%
33	17.948	2530	2535	2544	rVB	24368	33309	1.10%	0.121%
34	18.106	2560	2562	2565	rBV4	2486	3535	0.12%	0.013%
35	18.165	2567	2572	2581	rBV	63861	114480	3.77%	0.415%
36	18.424	2614	2616	2619	rBV4	2265	3245	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
 Data File : BM034610.D
 Acq On : 11 Apr 2022 15:15
 Operator : CG/JU
 Sample : N2338-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	18.795	2674	2679	2680	rBV5	3038	5372	0.18%	0.019%
38	19.224	2748	2752	2756	rBV2	22506	30832	1.01%	0.112%
39	19.300	2760	2765	2769	rBV2	17144	27500	0.91%	0.100%
40	19.447	2786	2790	2796	rBV6	12333	27810	0.92%	0.101%
41	19.653	2819	2825	2832	rBV	2193876	3038545	100.00%	11.007%
42	21.153	3076	3080	3088	rBV	221185	352691	11.61%	1.278%
43	21.441	3125	3129	3134	rBV	606534	948565	31.22%	3.436%
44	23.671	3501	3508	3526	rBV2	1332429	3005113	98.90%	10.886%
45	23.824	3528	3534	3555	rVB2	628616	1448525	47.67%	5.247%


Sum of corrected areas: 27605217

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034610.D
Acq On : 11 Apr 2022 15:15
Operator : CG/JU
Sample : N2338-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

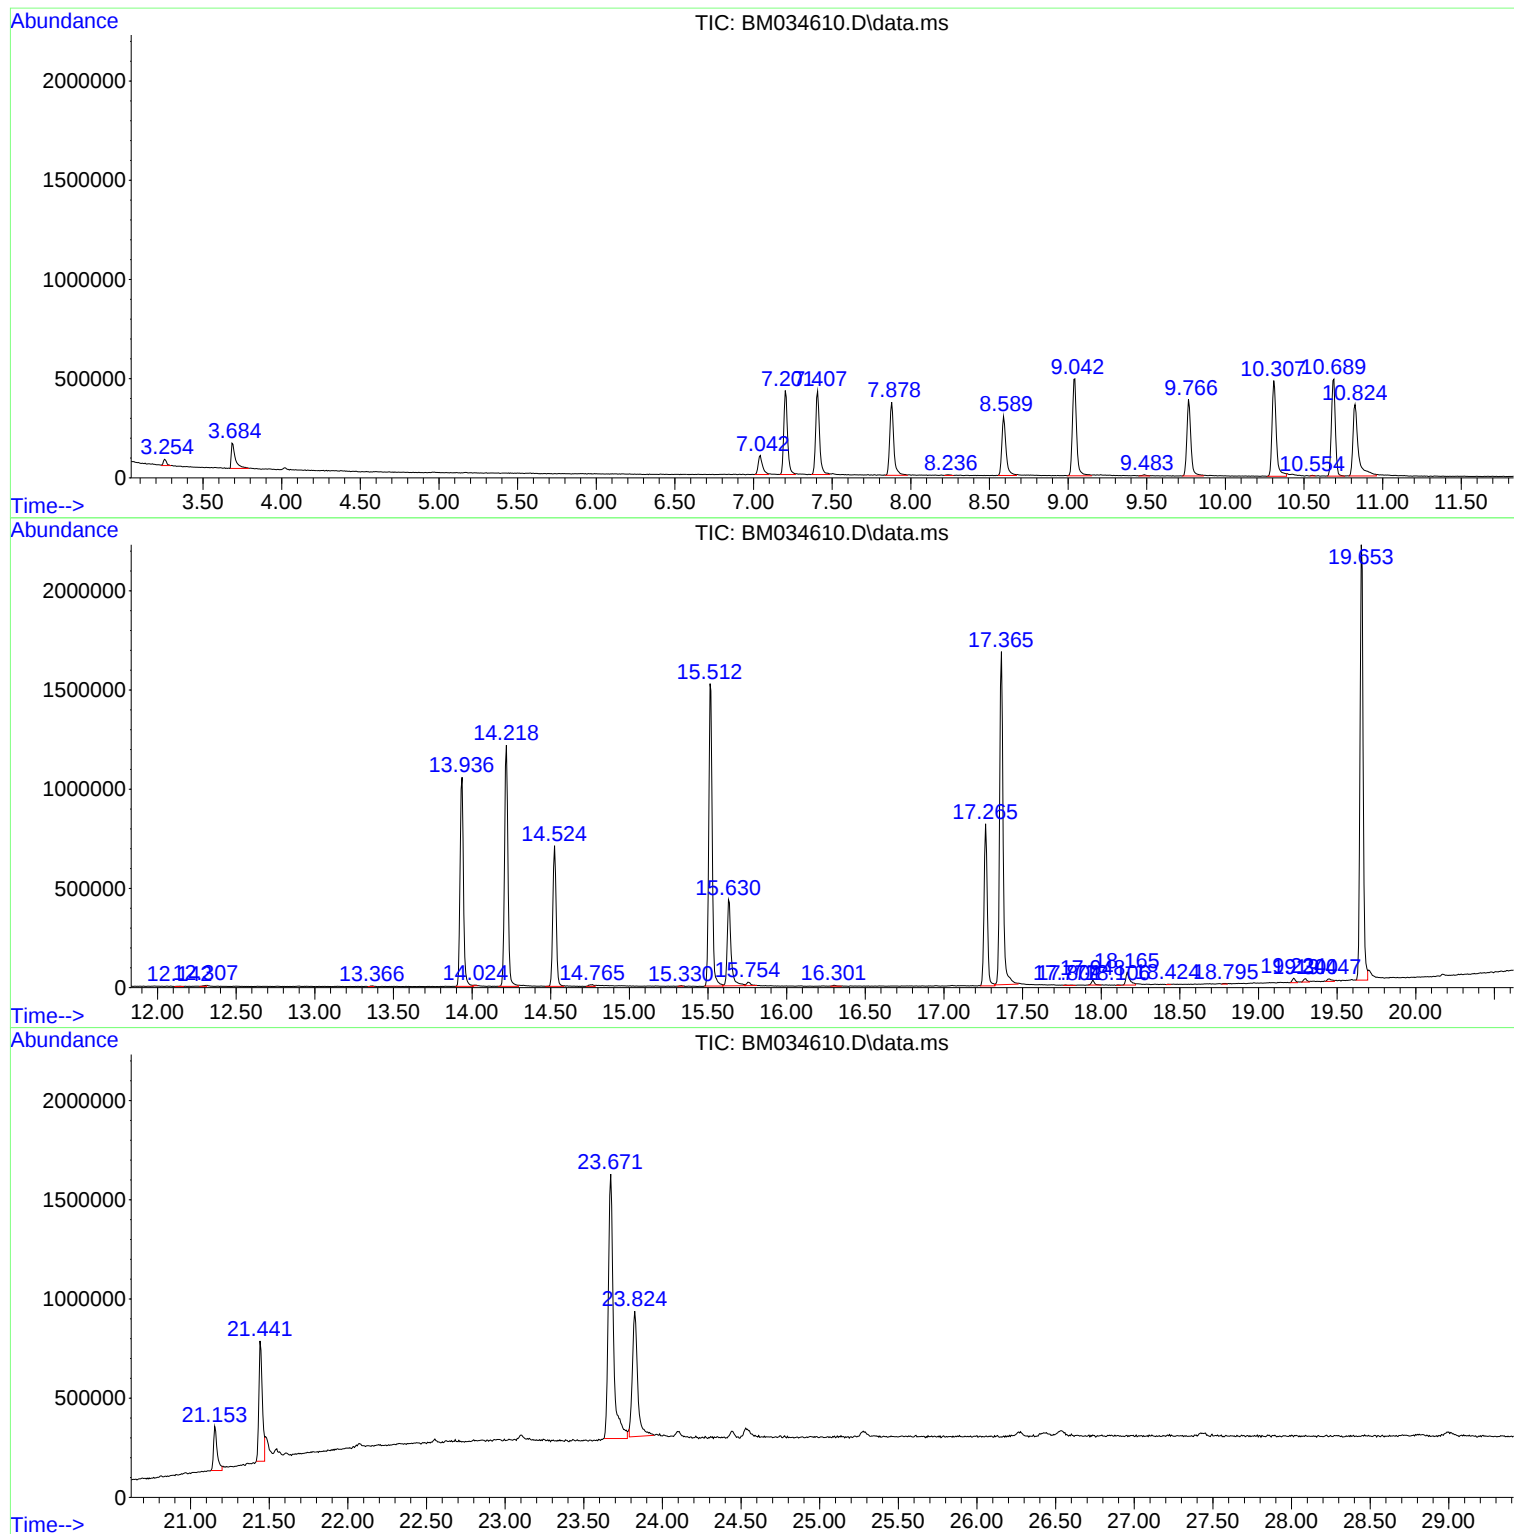

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034610.D
Acq On : 11 Apr 2022 15:15
Operator : CG/JU
Sample : N2338-06
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
C0J91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.153	7.44 ng/ul	352691	Chrysene-d12		21.442	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Nonadecene		266	C19H38	018435-45-5	95
2	Dichloroacetic acid, heptadecyl ...		366	C19H36Cl2O2	1000282-98-2	95
3	Trichloroacetic acid, hexadecyl ...		386	C18H33Cl3O2	074339-54-1	94
4	Pentafluoropropionic acid, tetra...		360	C17H29F5O2	006222-06-6	94
5	1-Hexacosene		364	C26H52	018835-33-1	94

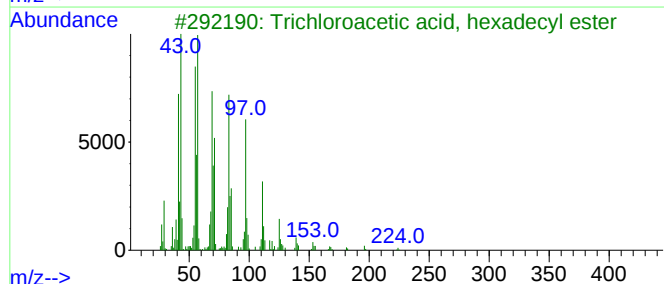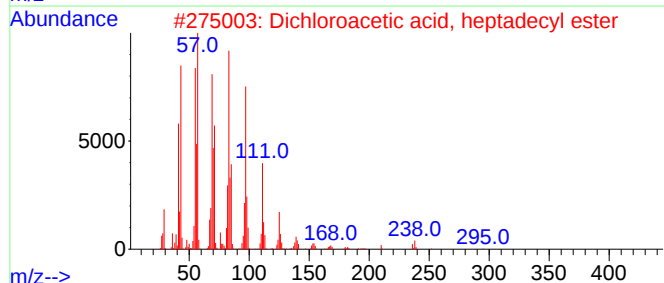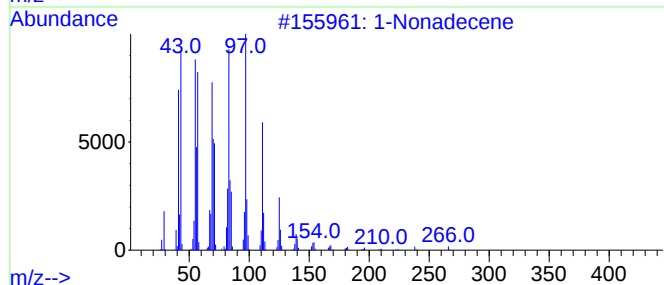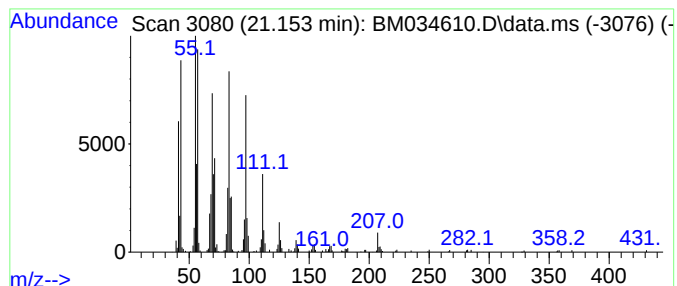

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041122\
Data File : BM034610.D
Acq On : 11 Apr 2022 15:15
Operator : CG/JU
Sample : N2338-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.153	7.4	ng/u1	352691	5	21.442	948565	20.0