
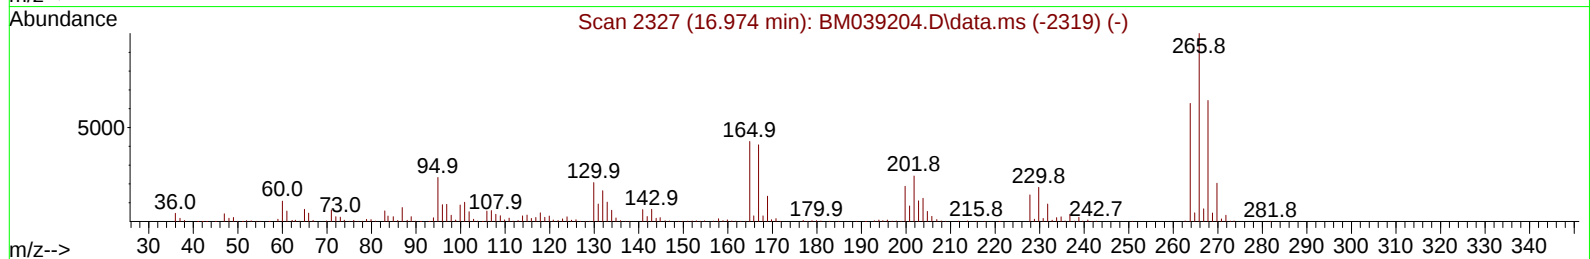
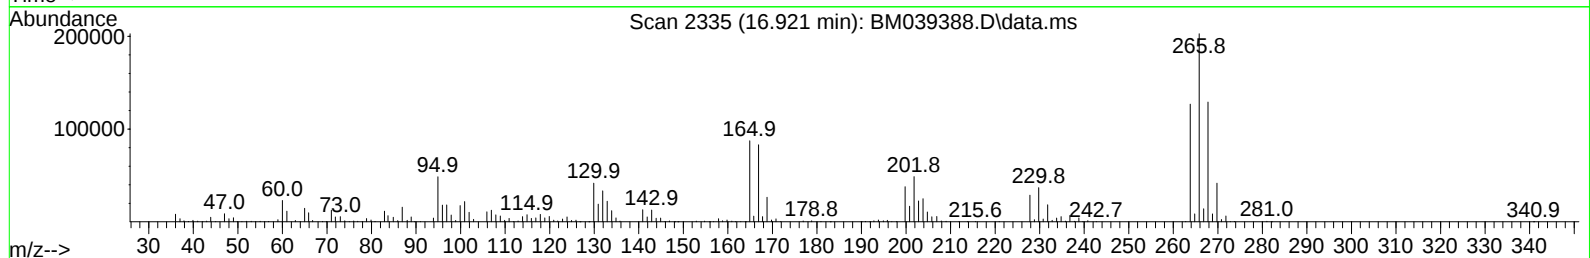


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041123\  
Data File : BM039388.D  
Acq On : 11 Apr 2023 10:48  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 05:30:21 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM032923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 11 16:05:42 2023  
Response via : Initial Calibration

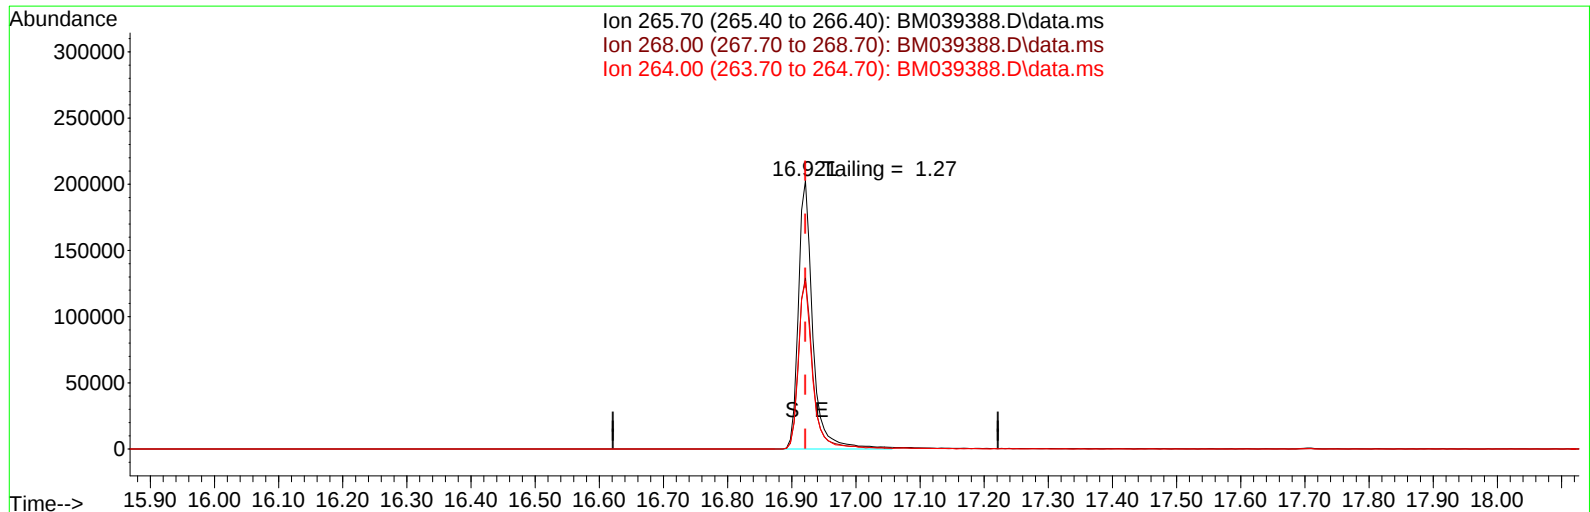

TIC: BM039388.D\data.ms

**(70) Pentachlorophenol (C)**




**16.921min ( 0.000) 715803.19 ng**

**response 321125**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.30  | 63.69  |
| 264.00 | 62.80  | 62.57  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041123\  
Data File : BM039388.D  
Acq On : 11 Apr 2023 10:48  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 05:30:21 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM032923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 11 16:05:42 2023  
Response via : Initial Calibration

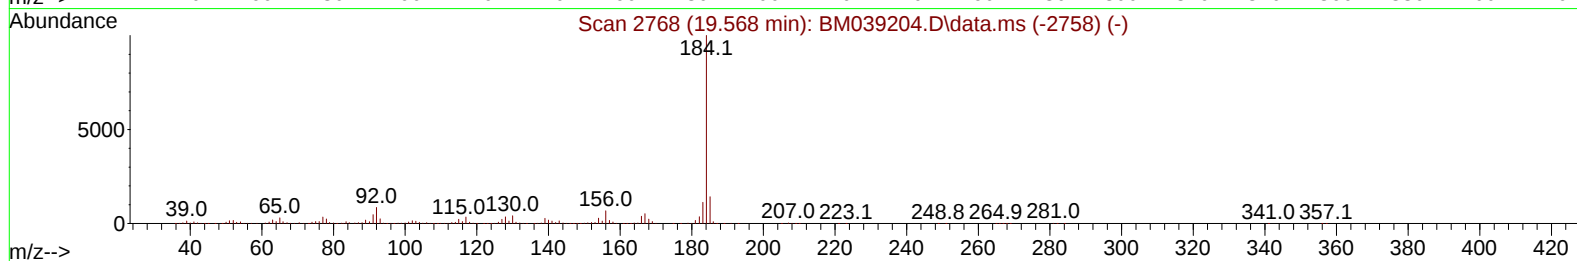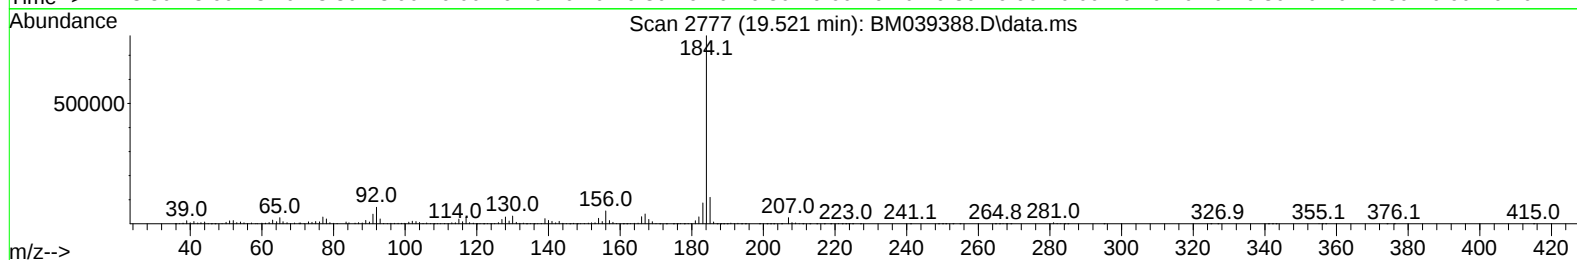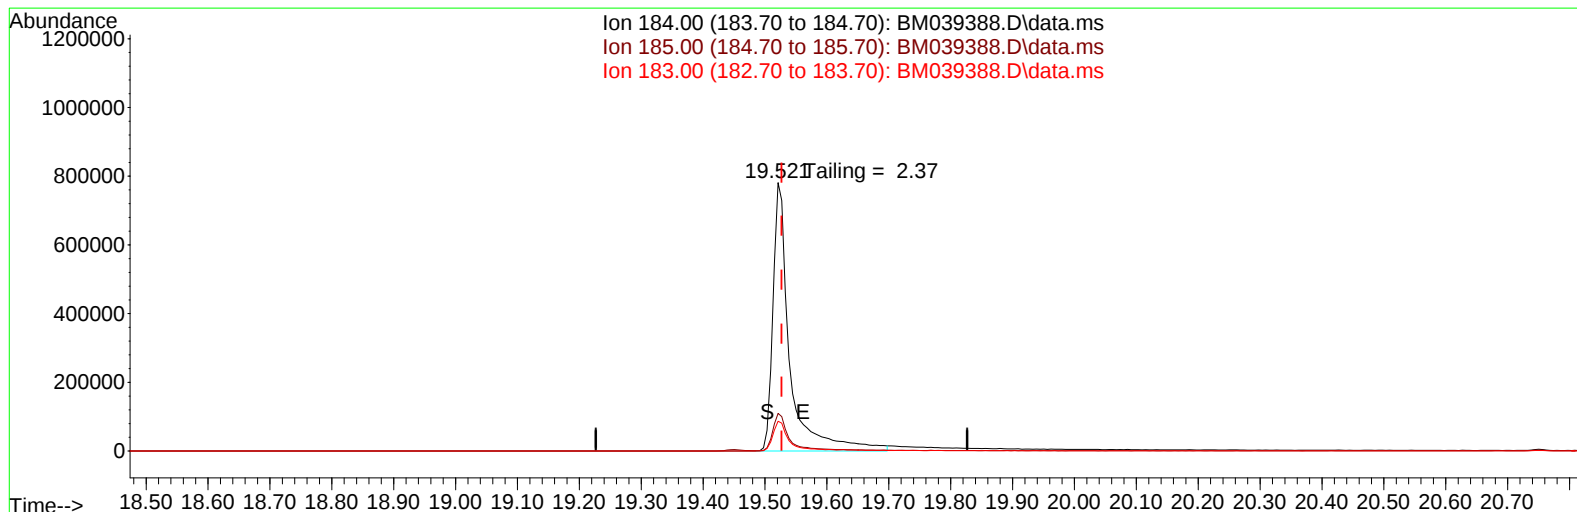

TIC: BM039388.D\data.ms

**(77) Benzidine****19.521min (-0.006) 30991.46 ng****response 1567857**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.03  |
| 183.00 | 11.20  | 11.12  |
| 0.00   | 0.00   | 0.00   |