
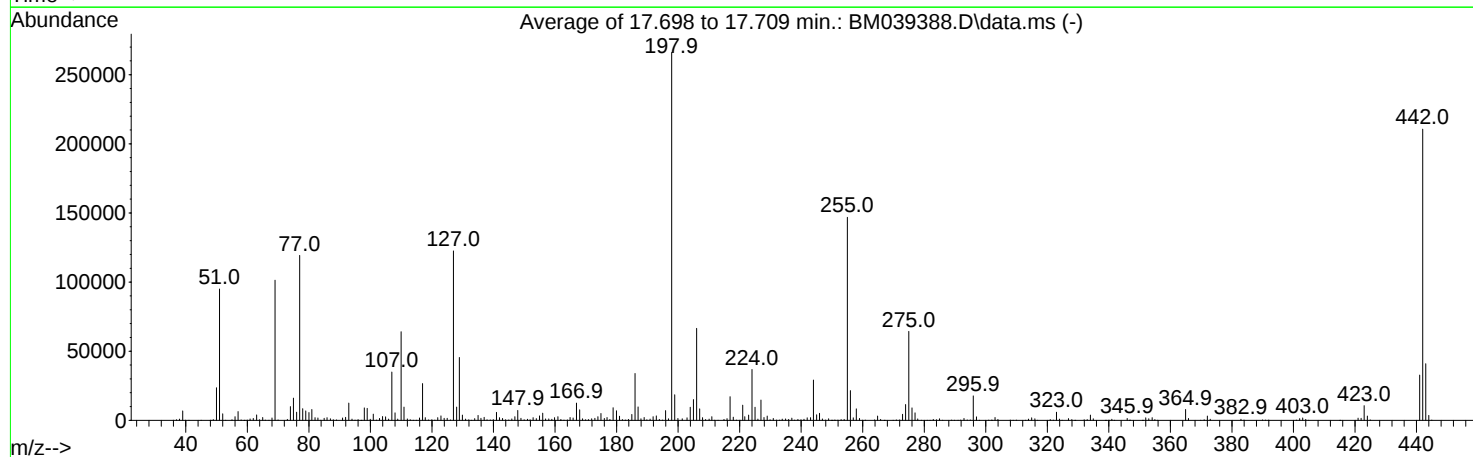


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041123\
 Data File : BM039388.D
 Acq On : 11 Apr 2023 10:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 11 16:05:42 2023

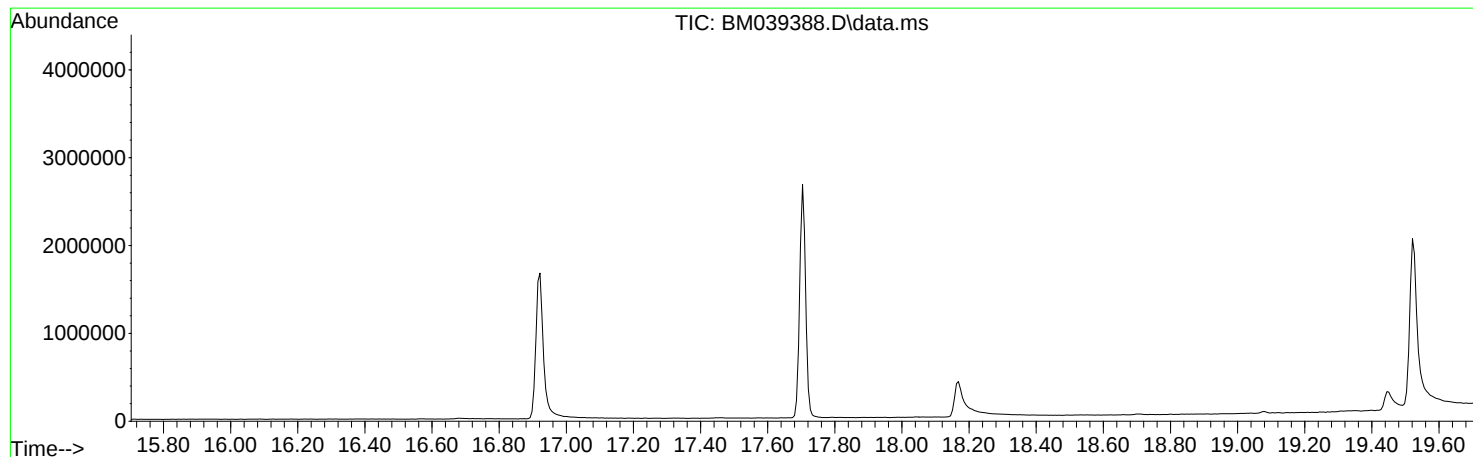




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	95017	PASS
68	69	0.00	2	1.7	1696	PASS
69	198	0.00	100	38.1	101373	PASS
70	69	0.00	2	0.4	390	PASS
127	198	10	80	46.1	122560	PASS
197	198	0.00	2	0.4	1108	PASS
198	198	100	100	100.0	266069	PASS
199	198	5	9	6.9	18488	PASS
275	198	10	60	24.2	64309	PASS
365	198	1	100	2.9	7824	PASS
441	198	0.01	100	12.3	32728	PASS
442	442	50	100	100.0	210624	PASS
443	442	15	24	19.5	41021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041123\
 Data File : BM039388.D
 Acq On : 11 Apr 2023 10:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 12 05:30:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 11 16:05:42 2023
 Response via : Initial Calibration

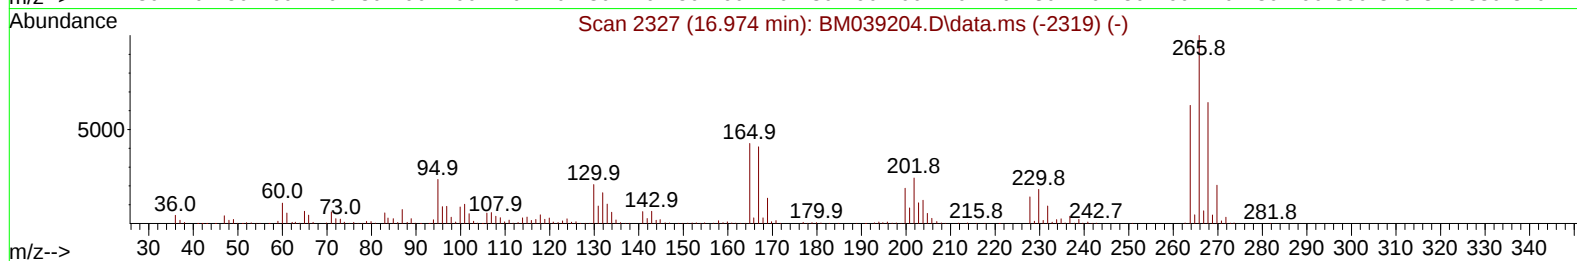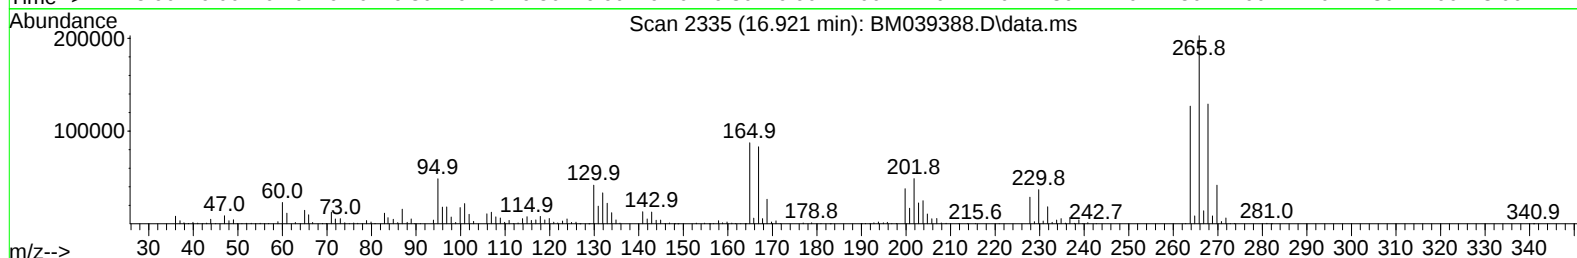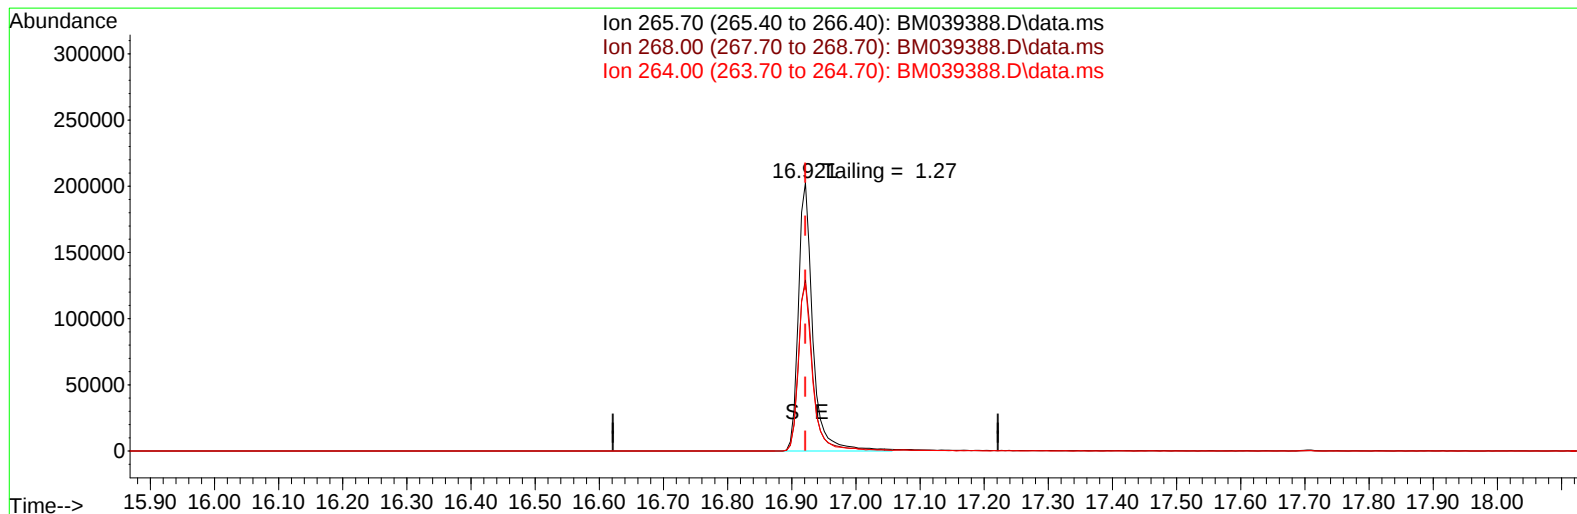

TIC: BM039388.D\data.ms

(70) Pentachlorophenol (C)

16.921min (0.000) 715803.19 ng




response 321125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.69
264.00	62.80	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041123\
Data File : BM039388.D
Acq On : 11 Apr 2023 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 12 05:30:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 11 16:05:42 2023
Response via : Initial Calibration

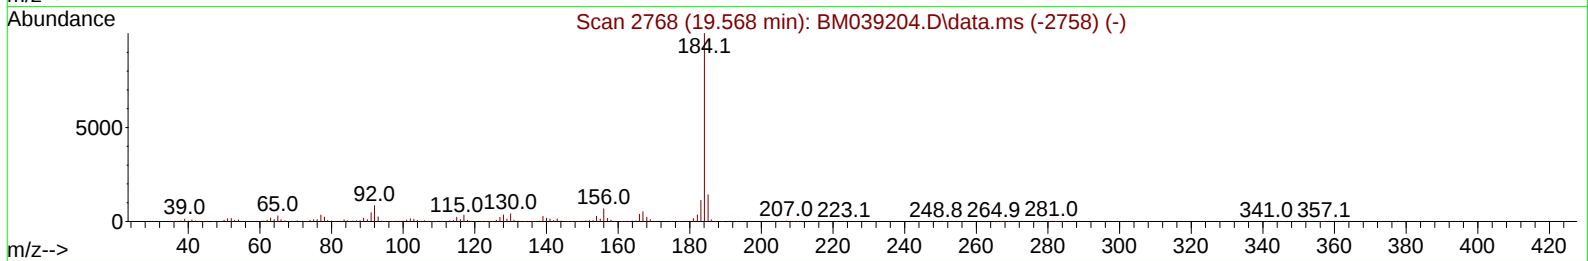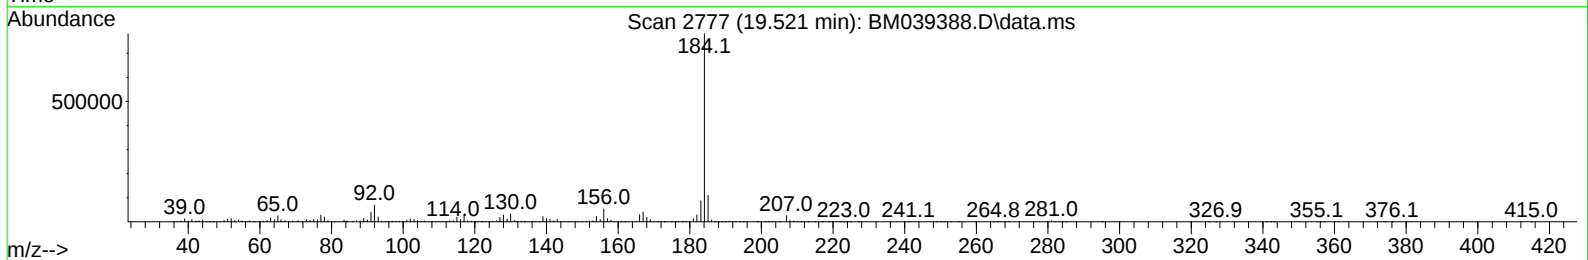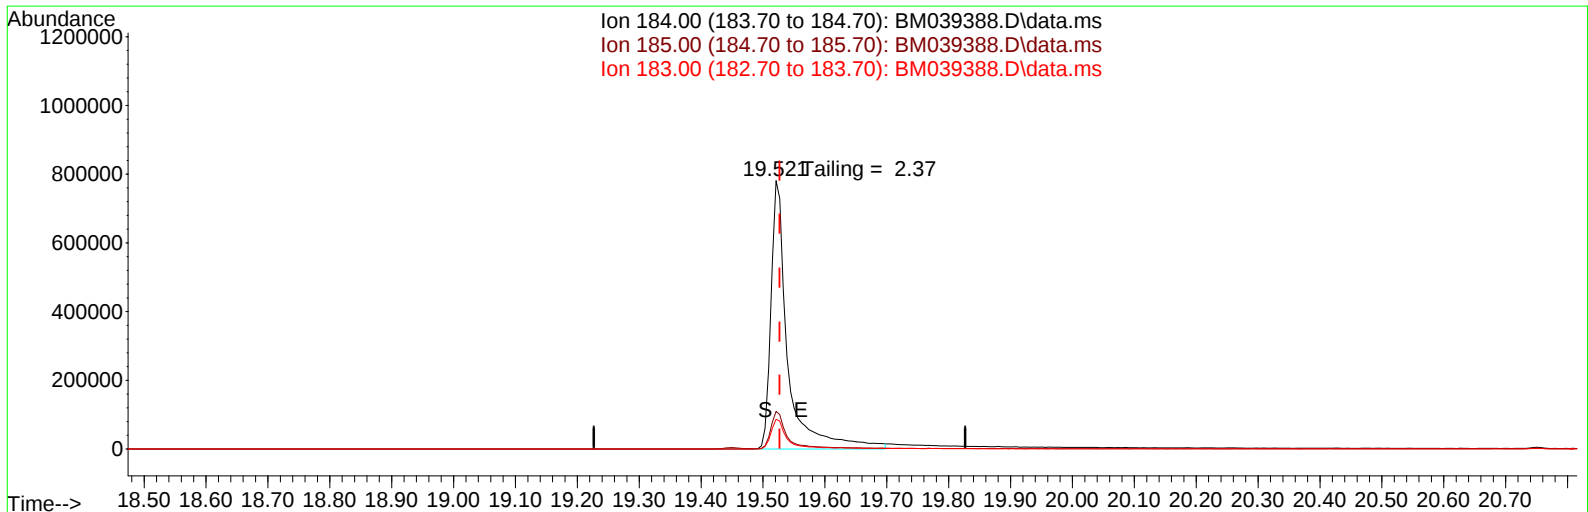

TIC: BM039388.D\data.ms

(77) Benzidine

19.521min (-0.006) 30991.46 ng

response 1567857

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.03
183.00	11.20	11.12
0.00	0.00	0.00

Date	Instrument Name	DFTPP Data File
4/11/2023	BNA_M	<u>BM039388.D</u>
Compound Name	Response	Retention Time
DDT	946486	20.75
DDD	16837	20.362
DDE	979	19.803
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17816	964302	1.85

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP