

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047938.D
 Acq On : 12 Apr 2022 04:00
 Operator : SY/MD
 Sample : N2293-02ME
 Misc : 7.71g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :

BNA_M




ClientSampleId :

SSTD0.4024

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:08:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

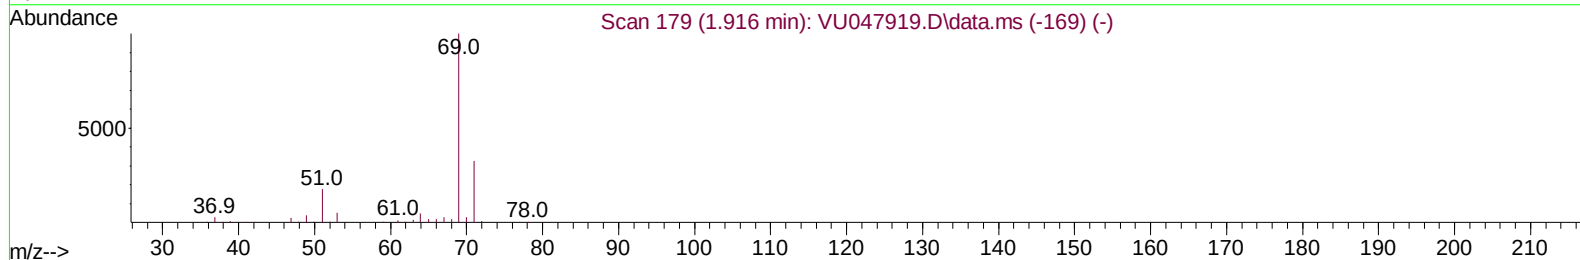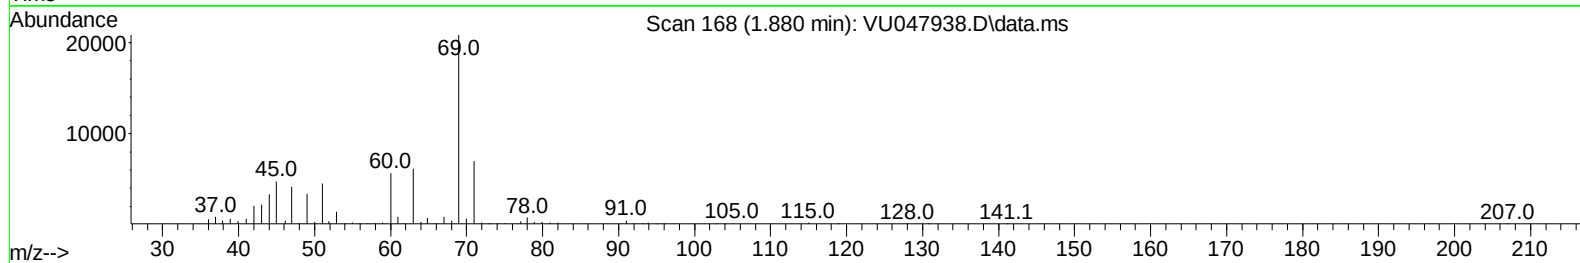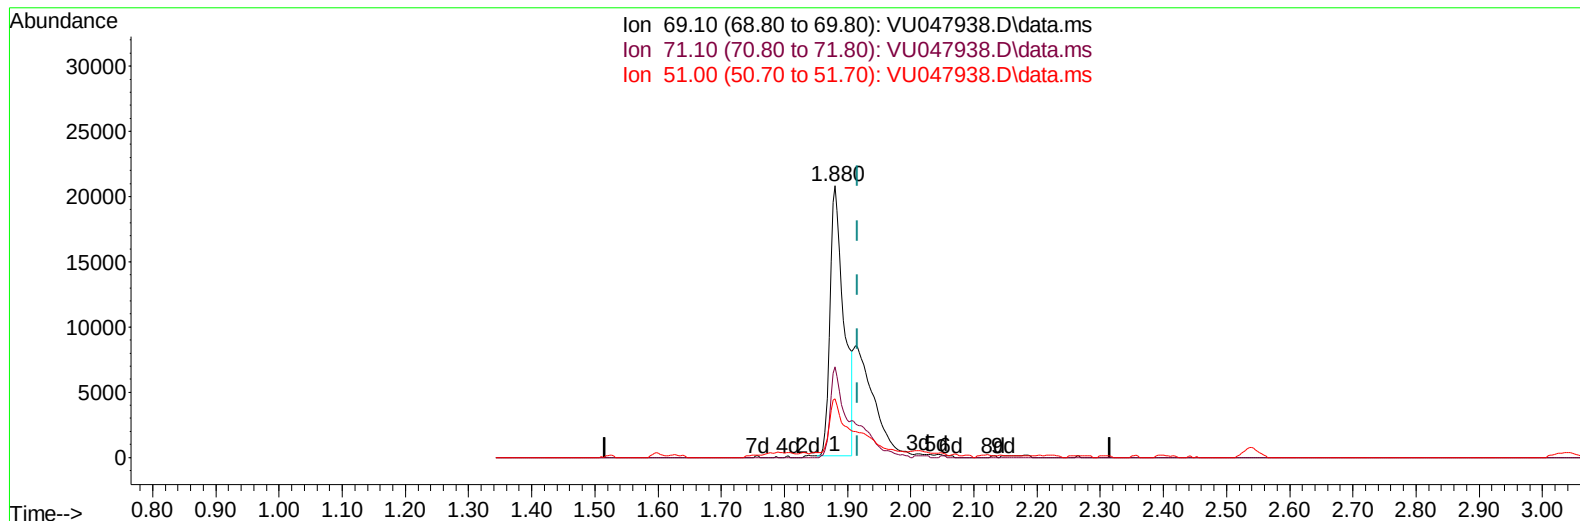

TIC: VU047938.D\data.ms

(7) Chloroethane-d5 (S)

1.880min (-0.035) 12.29 ug/L

response 31300

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	31.22
51.00	24.50	33.52#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047938.D
 Acq On : 12 Apr 2022 04:00
 Operator : SY/MD
 Sample : N2293-02ME
 Misc : 7.71g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :

BNA_M




ClientSampleId :

SSTD0.4024

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 12 05:08:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

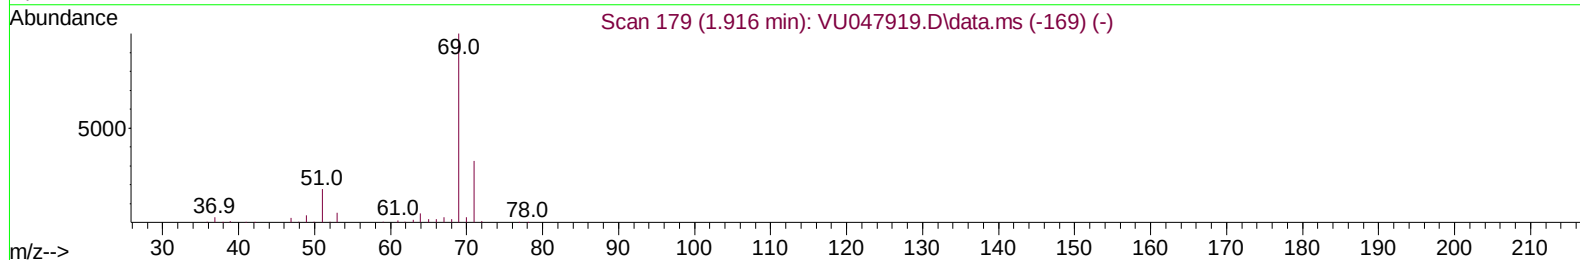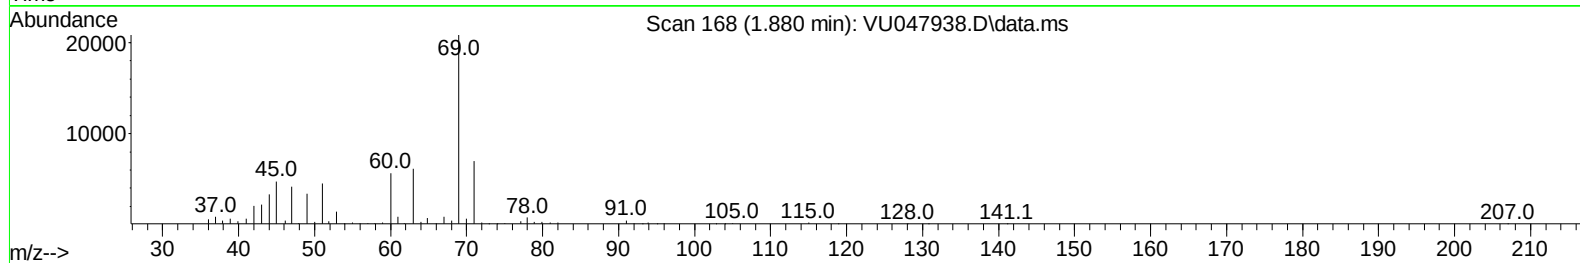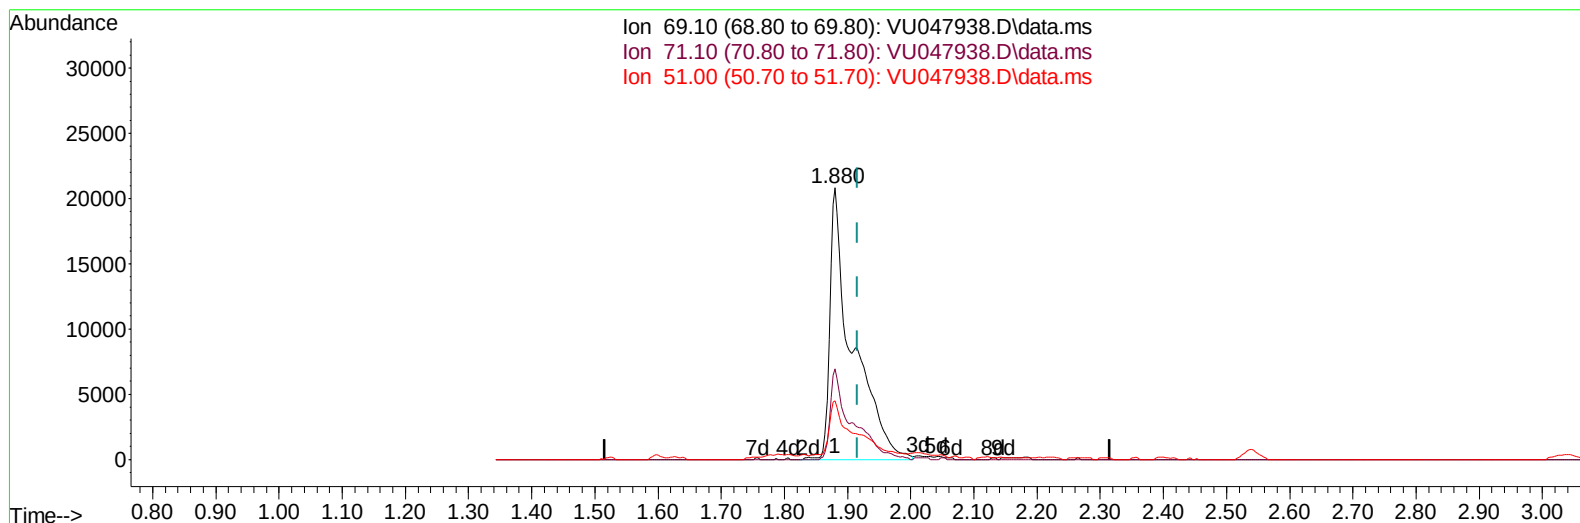

TIC: VU047938.D\data.ms

(7) Chloroethane-d5 (S)

1.880min (-0.035) 20.20 ug/L m

response 51449

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	18.99#
51.00	24.50	20.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034619.D
Acq On : 12 Apr 2022 13:18
Operator : CG/JU
Sample : SST0.424
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD0.4024

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 12 15:03:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 14:58:22 2022
Response via : Initial Calibration

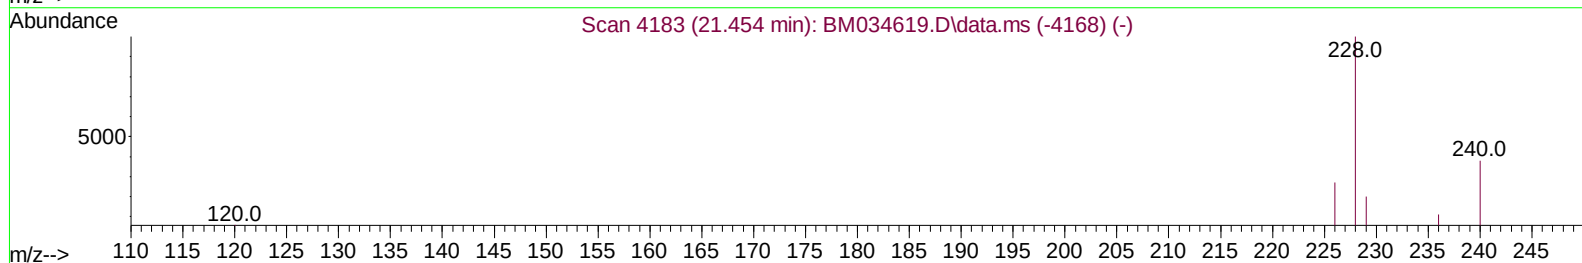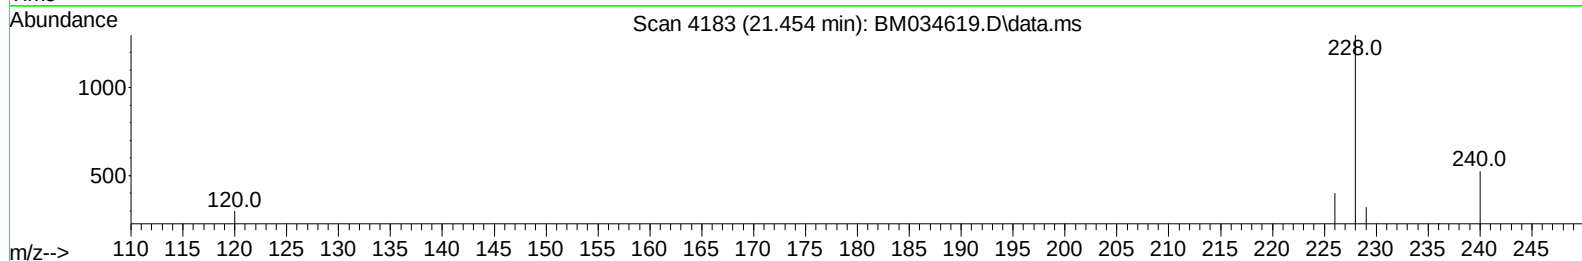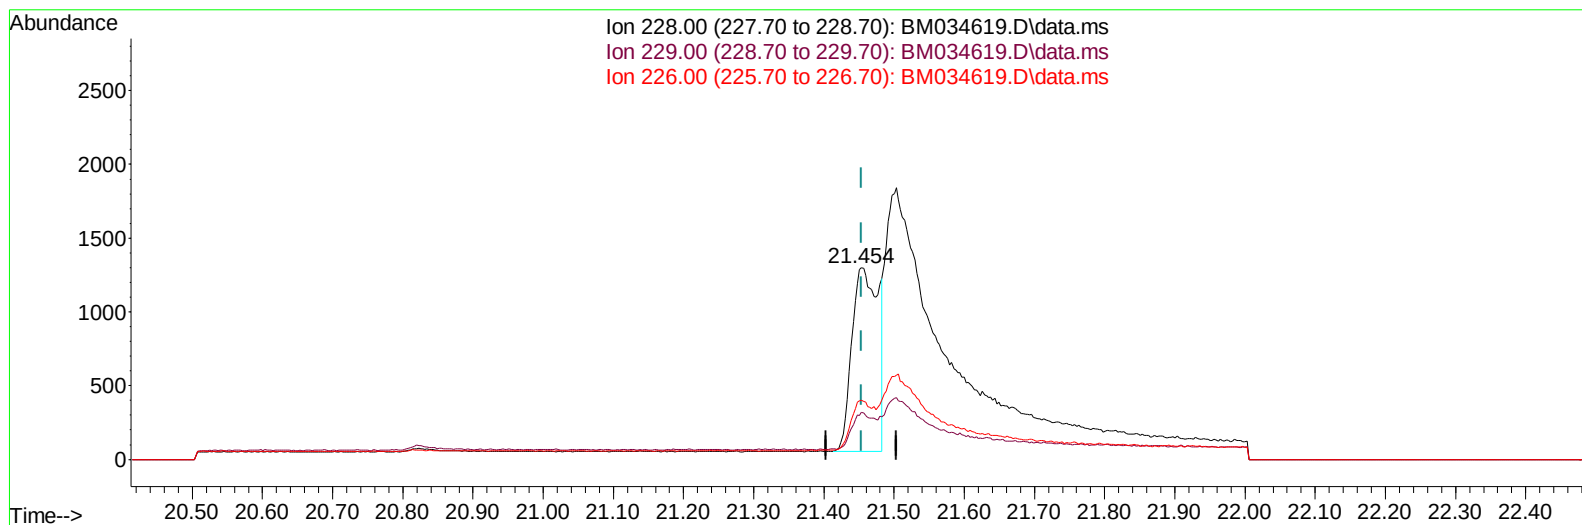

TIC: BM034619.D\data.ms

(21) Benzo(a)anthracene

21.454min (0.000) 0.42 ng/u1

response 3288

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	24.73
226.00	29.00	30.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034619.D
 Acq On : 12 Apr 2022 13:18
 Operator : CG/JU
 Sample : SST0.424
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST0.4024

Manual IntegrationsAPPROVED

Quant Time: Apr 12 15:03:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 14:58:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

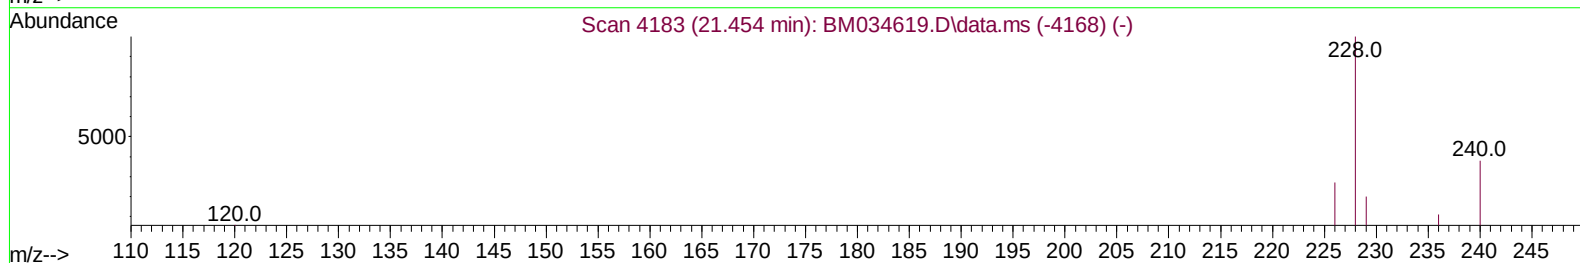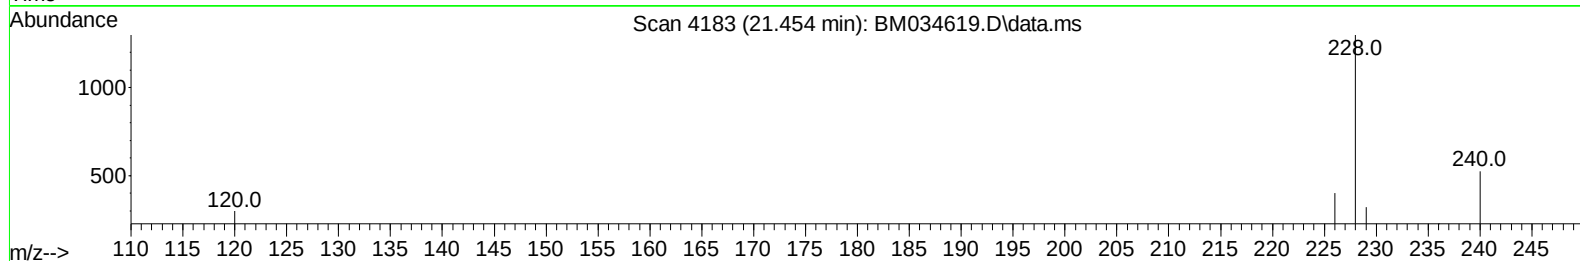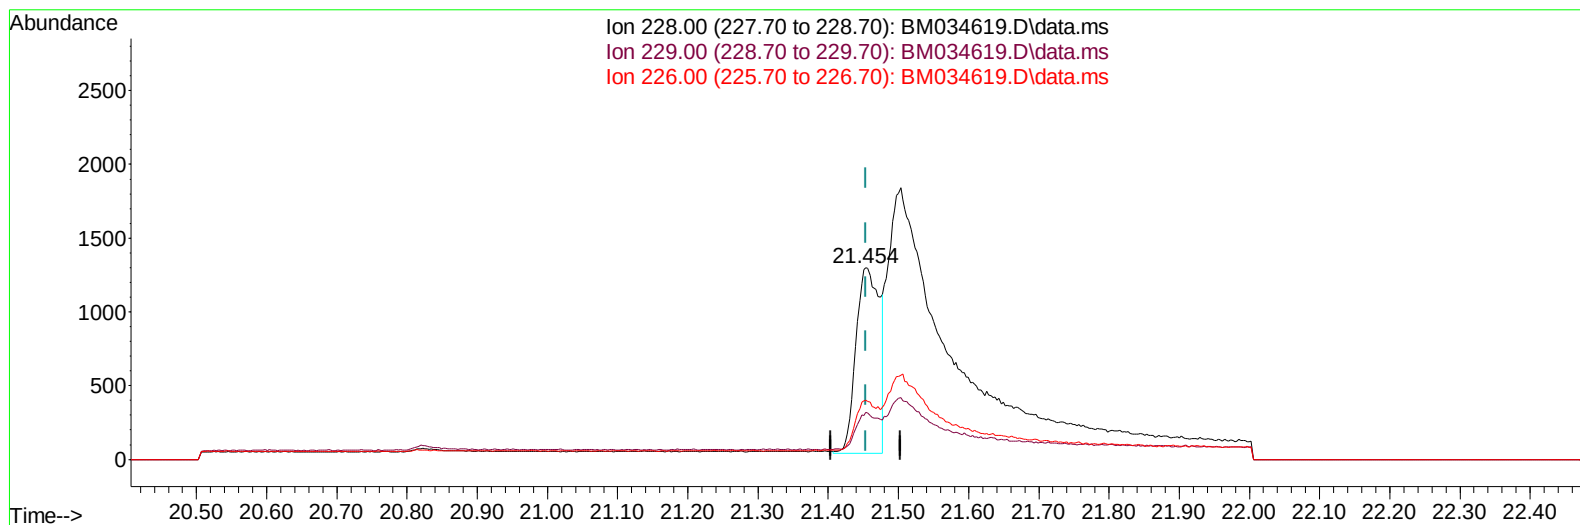

TIC: BM034619.D\data.ms

(21) Benzo(a)anthracene

21.454min (0.000) 0.38 ng/ul m

response 2948

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	24.73
226.00	29.00	30.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034619.D
Acq On : 12 Apr 2022 13:18
Operator : CG/JU
Sample : SST0.424
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD0.4024

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 12 15:03:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 14:58:22 2022
Response via : Initial Calibration

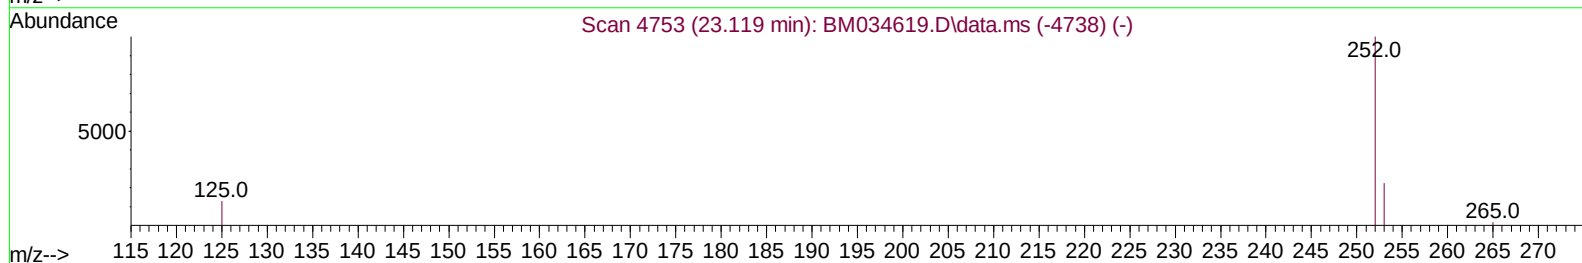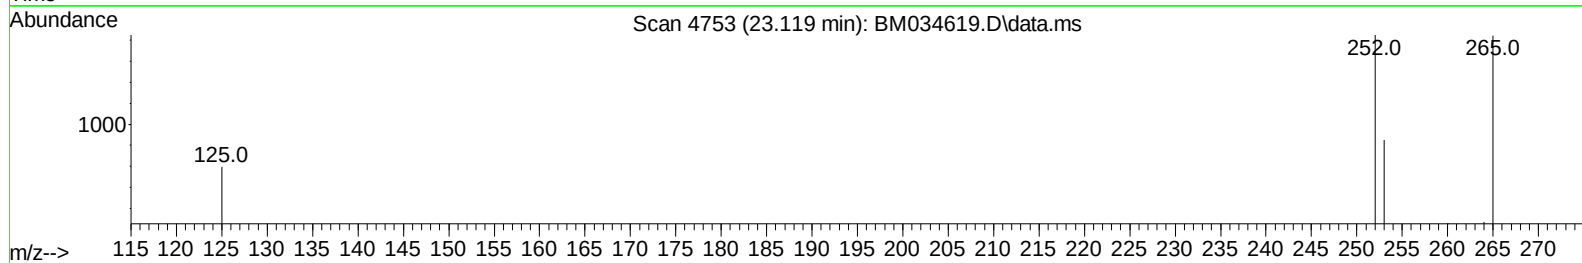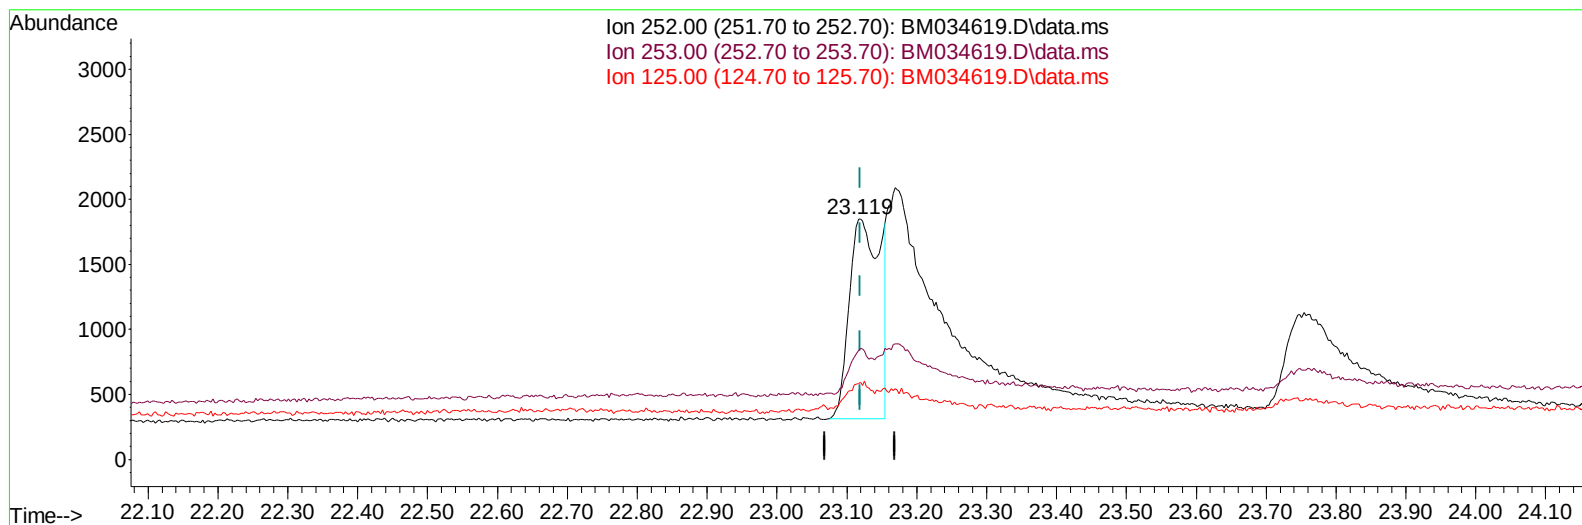

TIC: BM034619.D\data.ms

(24) Benzo(b)fluoranthene

23.119min (+ 0.000) 0.50 ng/u1

response 4722

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.10	46.11
125.00	14.40	32.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034619.D
 Acq On : 12 Apr 2022 13:18
 Operator : CG/JU
 Sample : SST0.424
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST0.4024

Manual IntegrationsAPPROVED

Quant Time: Apr 12 15:03:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 14:58:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

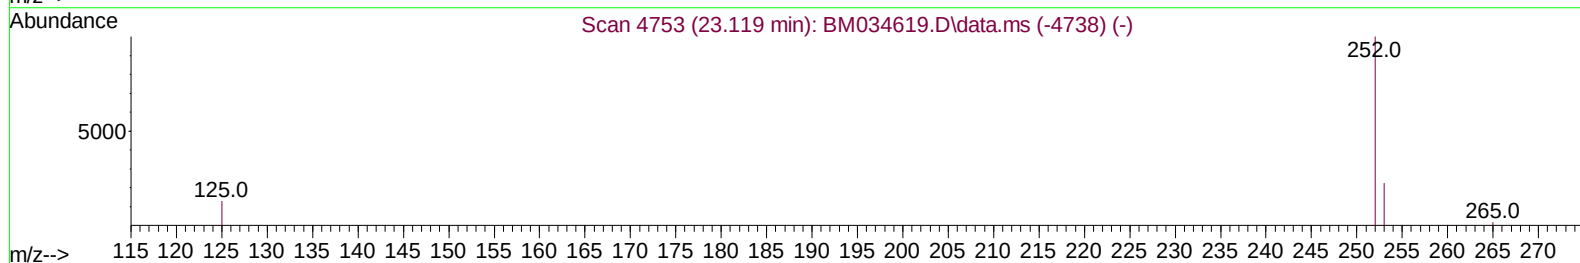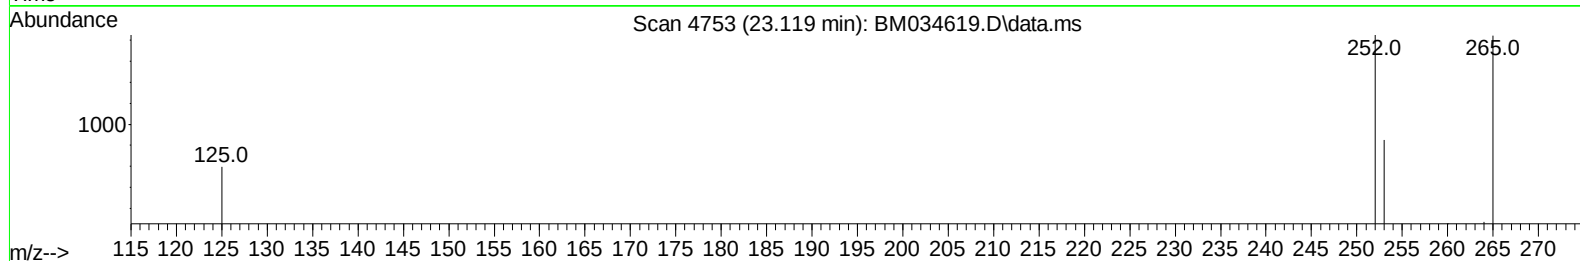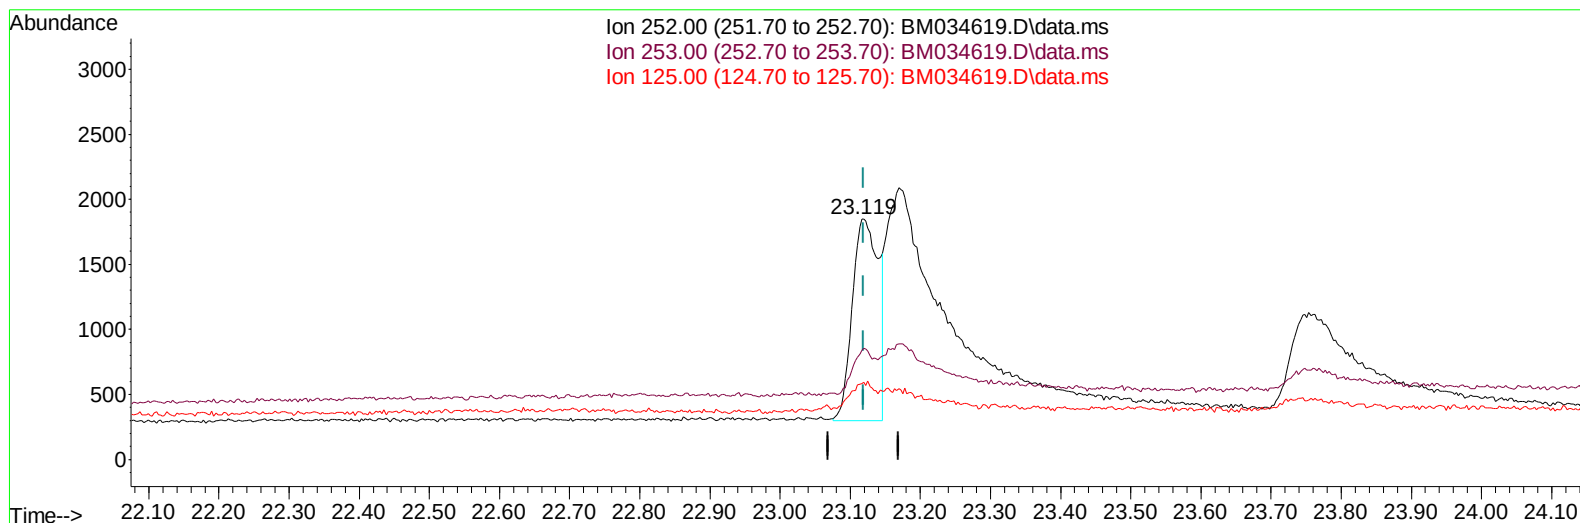

TIC: BM034619.D\data.ms

(24) Benzo(b)fluoranthene

23.119min (+ 0.000) 0.43 ng/ul m

response 4047

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.10	46.11
125.00	14.40	32.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034619.D
 Acq On : 12 Apr 2022 13:18
 Operator : CG/JU
 Sample : SST00.424
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST00.4024

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 12 15:03:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 14:58:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.914	152	1547	0.400	ng/ul	0.00
4) Naphthalene-d8	10.705	136	4922	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.534	164	2535	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.284	188	3868	0.400	ng/ul	0.00
17) Chrysene-d12	21.468	240	3586	0.400	ng/ul	# 0.00
23) Perylene-d12	23.844	264	2893	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	1259	0.486	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	2705	0.419	ng/ul	0.00
18) Fluoranthene-d10	19.308	212	4479	0.426	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.290	88	1205	0.466	ng/ul#	71
5) Naphthalene	10.754	128	5826	0.379	ng/ul	93
7) 2-Methylnaphthalene	12.382	142	3518	0.419	ng/ul	99
8) 1-Methylnaphthalene	12.591	142	3515	0.416	ng/ul	98
10) Acenaphthylene	14.256	152	4938	0.421	ng/ul	93
11) Acenaphthene	14.594	153	3956	0.417	ng/ul	96
12) Fluorene	15.589	166	4013	0.410	ng/ul	98
14) Pentachlorophenol	16.946	266	657	0.401	ng/ul	98
15) Phenanthrene	17.326	178	5212	0.415	ng/ul	98
16) Anthracene	17.423	178	4126	0.433	ng/ul	100
19) Fluoranthene	19.336	202	6352	0.422	ng/ul	97
20) Pyrene	19.699	202	7527	0.428	ng/ul#	95
21) Benzo(a)anthracene	21.454	228	2948m	0.378	ng/ul	
22) Chrysene	21.503	228	3963	0.430	ng/ul	97
24) Benzo(b)fluoranthene	23.119	252	4047m	0.428	ng/ul	
25) Benzo(k)fluoranthene	23.169	252	3767	0.446	ng/ul#	81
26) Benzo(a)pyrene	23.754	252	4707	0.426	ng/ul#	61
27) Indeno(1,2,3-cd)pyrene	26.347	276	6063	0.456	ng/ul#	94
28) Dibenzo(a,h)anthracene	26.387	278	4345	0.449	ng/ul#	58
29) Benzo(g,h,i)perylene	27.095	276	6703	0.465	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034619.D
 Acq On : 12 Apr 2022 13:18
 Operator : CG/JU
 Sample : SST00.424
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST00.4024

Manual IntegrationsAPPROVED

Quant Time: Apr 12 15:03:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 14:58:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

