




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034624.D
 Acq On : 12 Apr 2022 16:43
 Operator : CG/JU
 Sample : PB144046BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK046

Manual IntegrationsAPPROVED

Quant Time: Apr 13 01:58:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

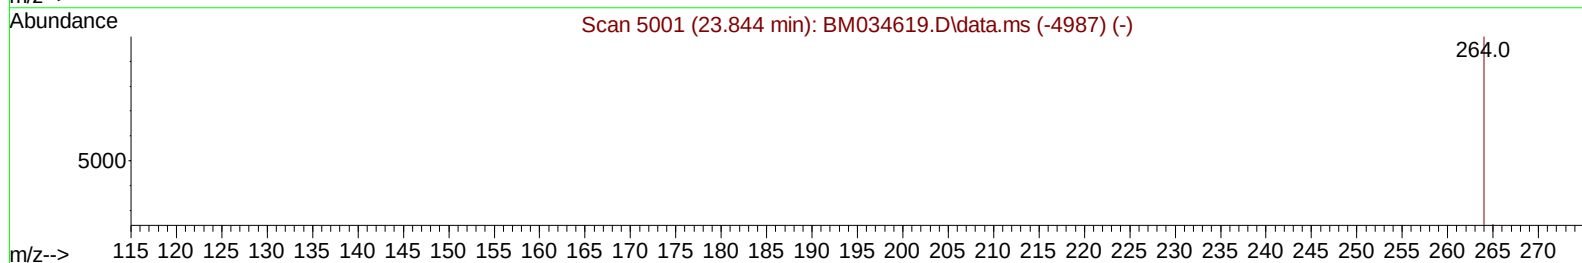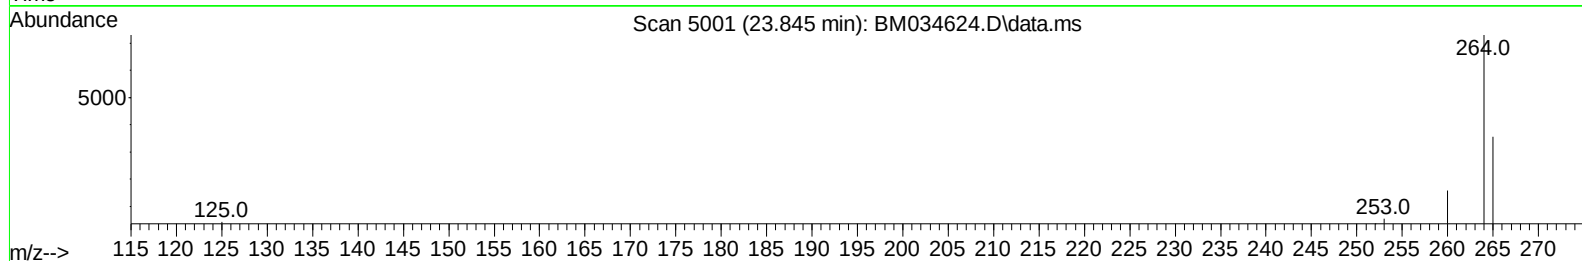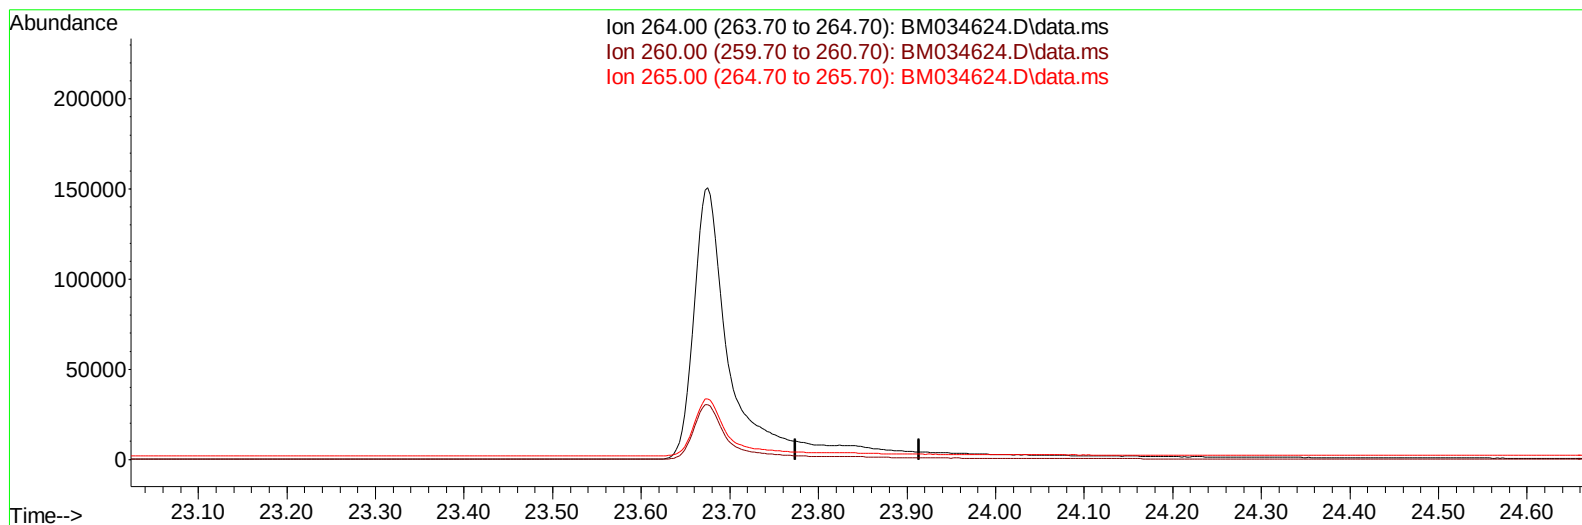

TIC: BM034624.D\data.ms

(23) Perylene-d12 (I)

23.844min (-23.844) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034624.D
 Acq On : 12 Apr 2022 16:43
 Operator : CG/JU
 Sample : PB144046BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK046

Manual IntegrationsAPPROVED

Quant Time: Apr 13 01:58:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

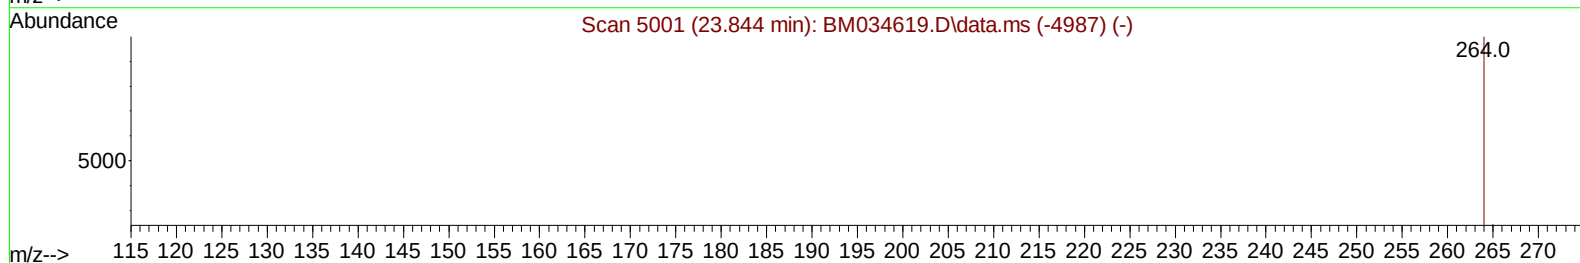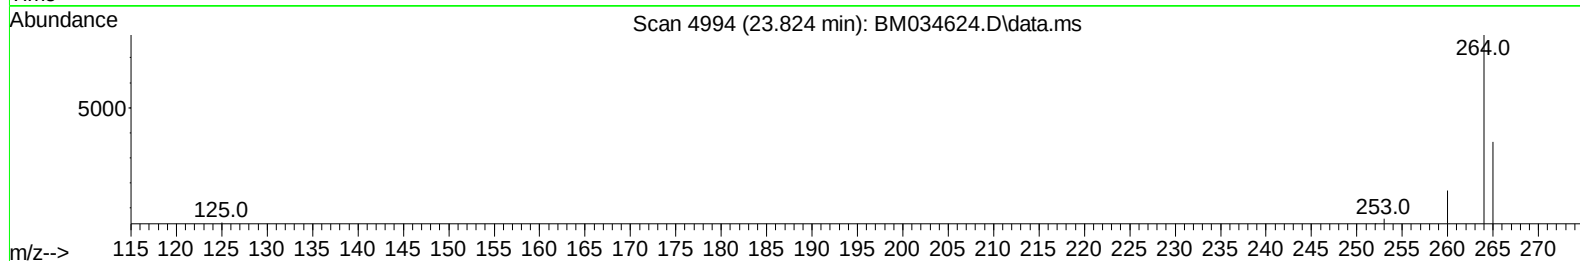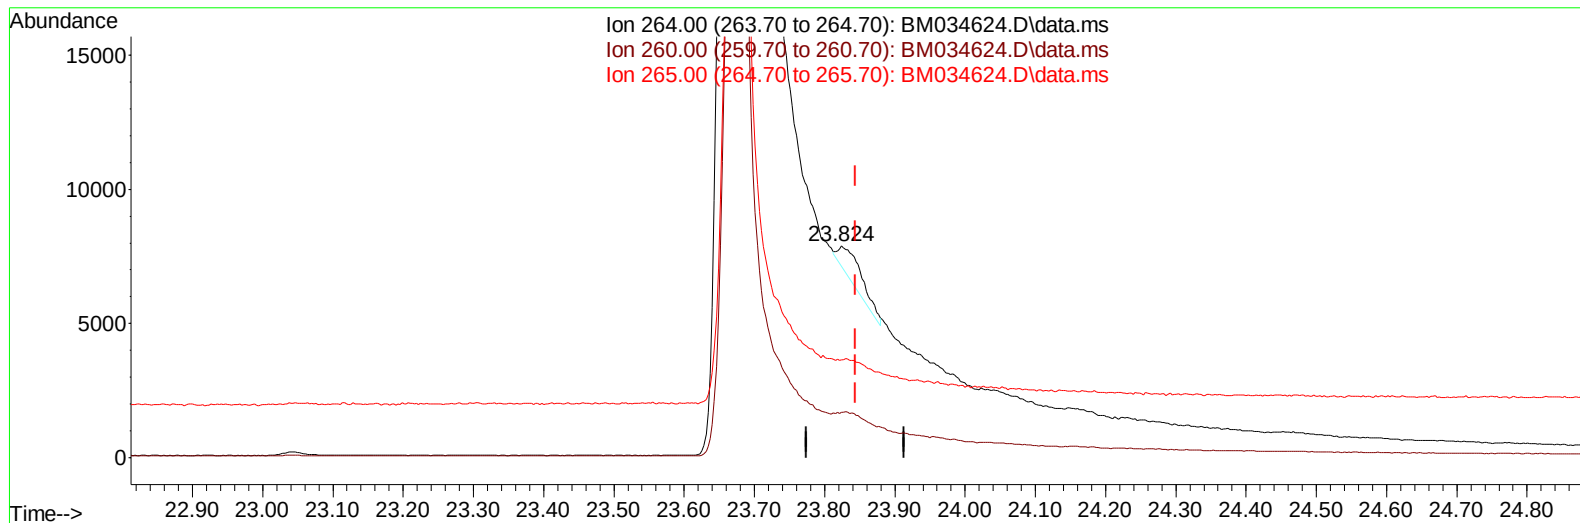

TIC: BM034624.D\data.ms

(23) Perylene-d12 (I)

23.824min (-0.020) 0.40 ng/ul m

response 2389

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.34#
265.00	95.30	46.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034624.D
 Acq On : 12 Apr 2022 16:43
 Operator : CG/JU
 Sample : PB144046BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK046

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 01:58:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.884	152	1978	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.694	136	5456	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.529	164	2984	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	5404	0.400	ng/ul	-0.01
17) Chrysene-d12	21.489	240	4179	0.400	ng/ul	# 0.02
23) Perylene-d12	23.824	264	2389m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	16336	4.764	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	2347	0.325	ng/ul	0.01
18) Fluoranthene-d10	19.299	212	4484	0.369	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034624.D
Acq On : 12 Apr 2022 16:43
Operator : CG/JU
Sample : PB144046BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK046

Manual IntegrationsAPPROVED

Quant Time: Apr 13 01:58:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

