




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034636.D
 Acq On : 13 Apr 2022 00:45
 Operator : CG/JU
 Sample : N2319-14MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

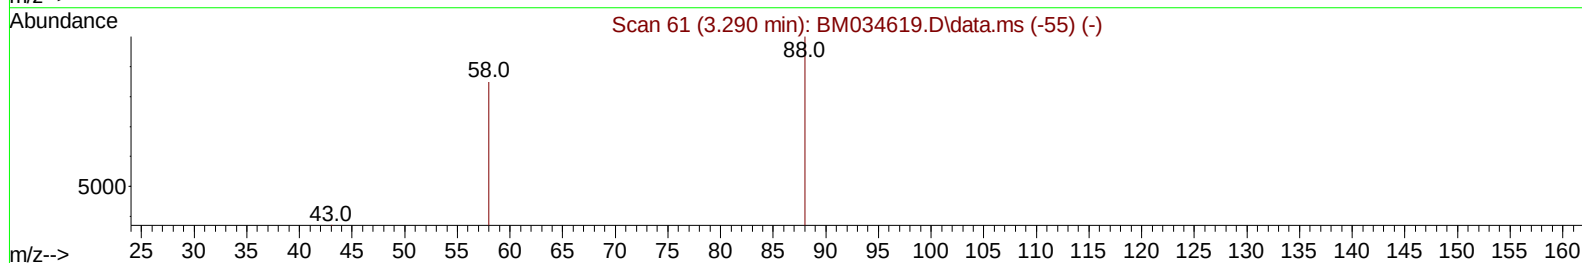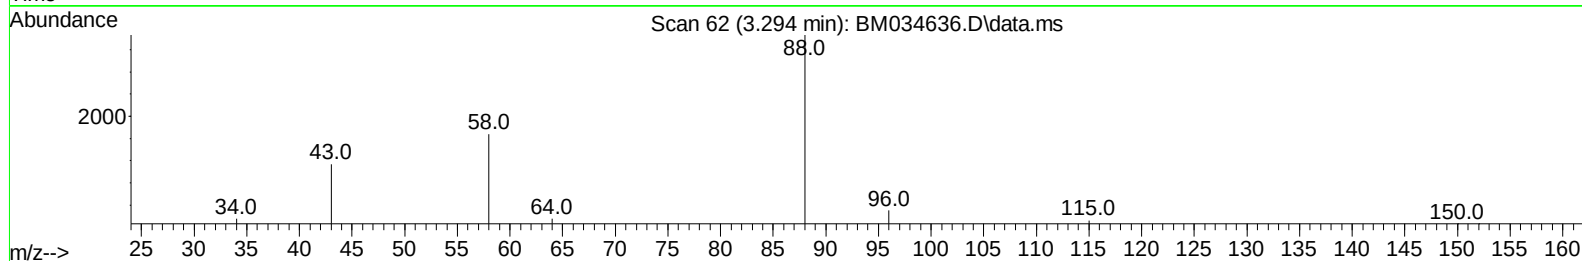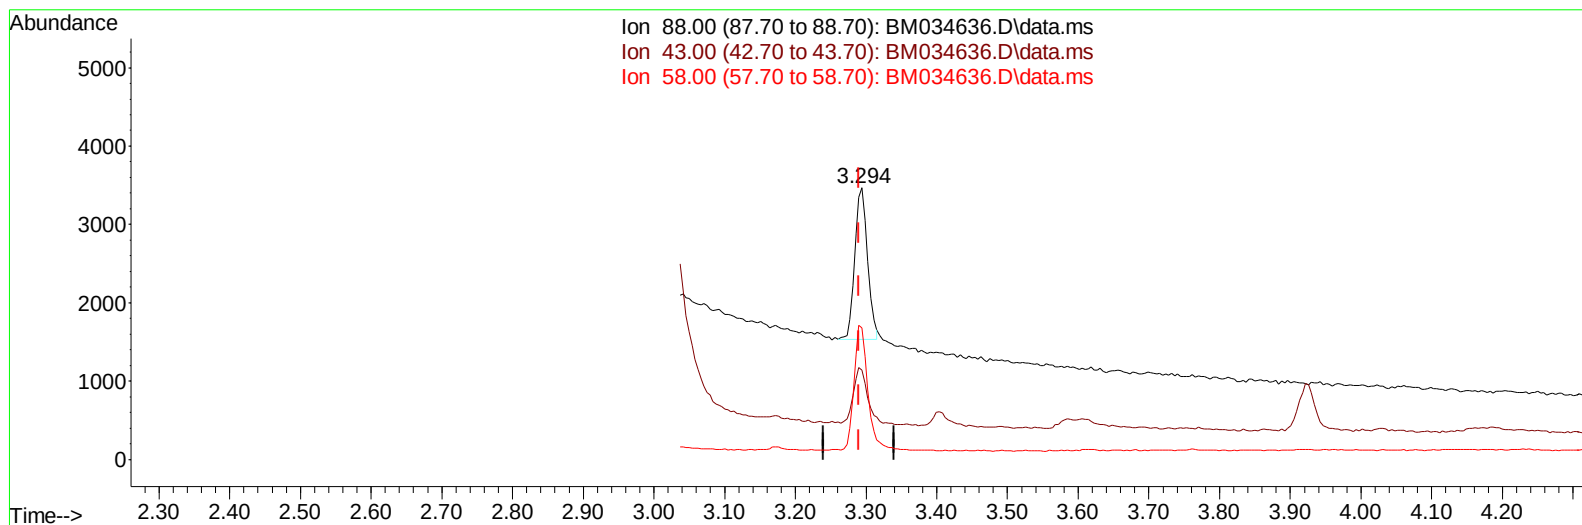

TIC: BM034636.D\data.ms

(2) 1,4-Dioxane

3.294min (+ 0.004) 0.81 ng/uL

response 2406

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	62.10	32.83#
58.00	65.60	48.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034636.D
 Acq On : 13 Apr 2022 00:45
 Operator : CG/JU
 Sample : N2319-14MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

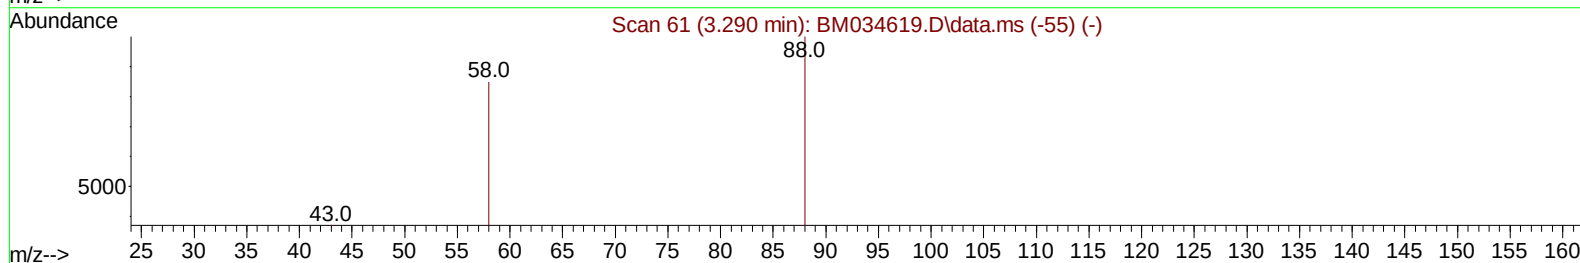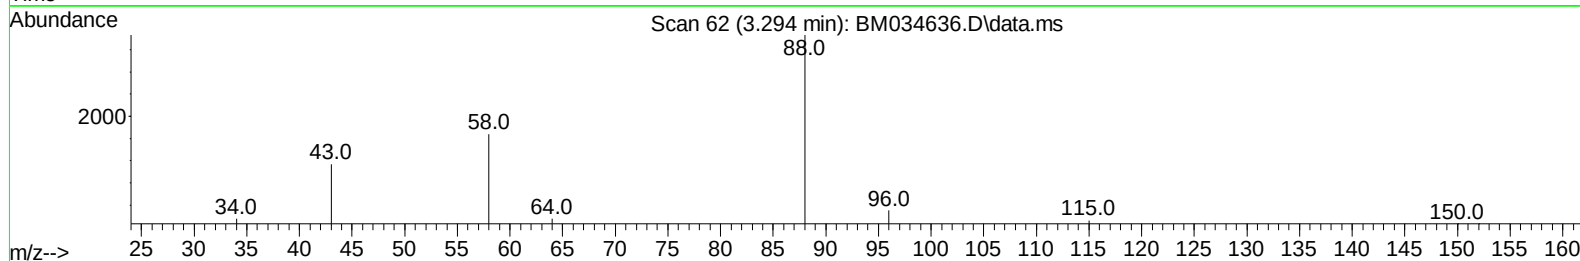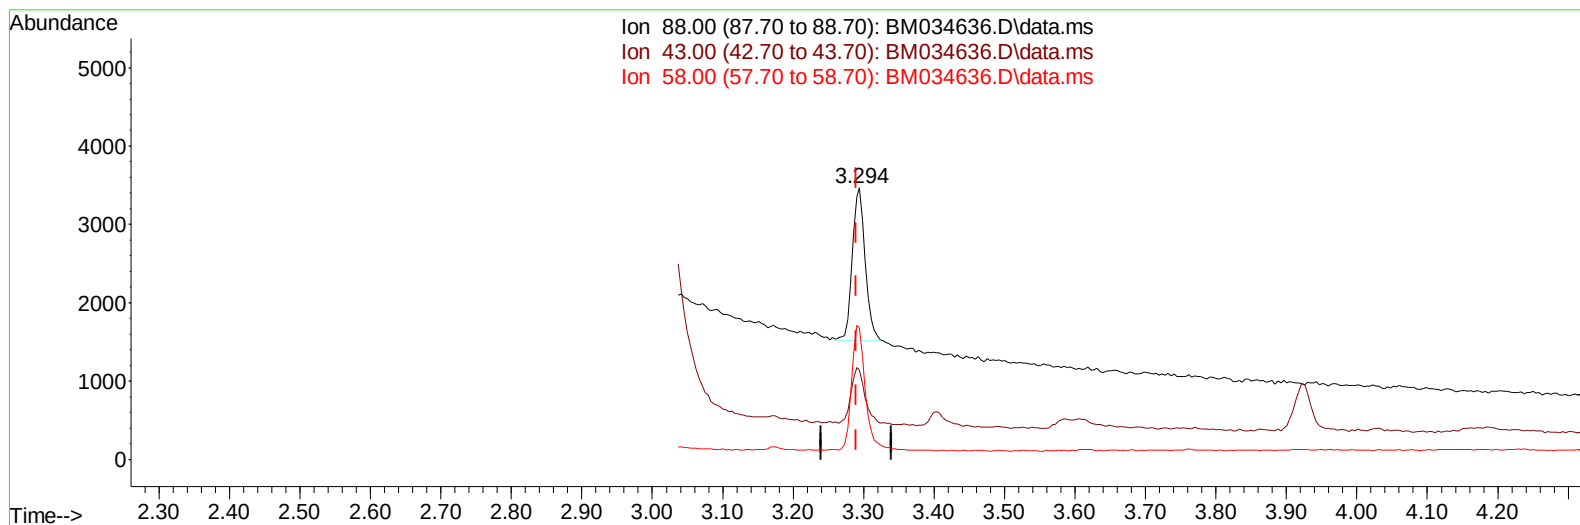

TIC: BM034636.D\data.ms

(2) 1,4-Dioxane

3.294min (+ 0.004) 0.83 ng/ul m

response 2477

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	62.10	32.83#
58.00	65.60	48.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034636.D
 Acq On : 13 Apr 2022 00:45
 Operator : CG/JU
 Sample : N2319-14MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

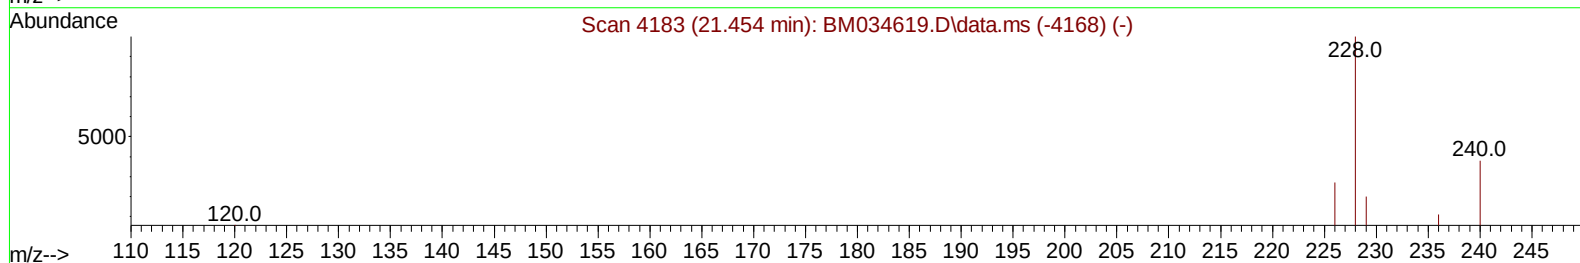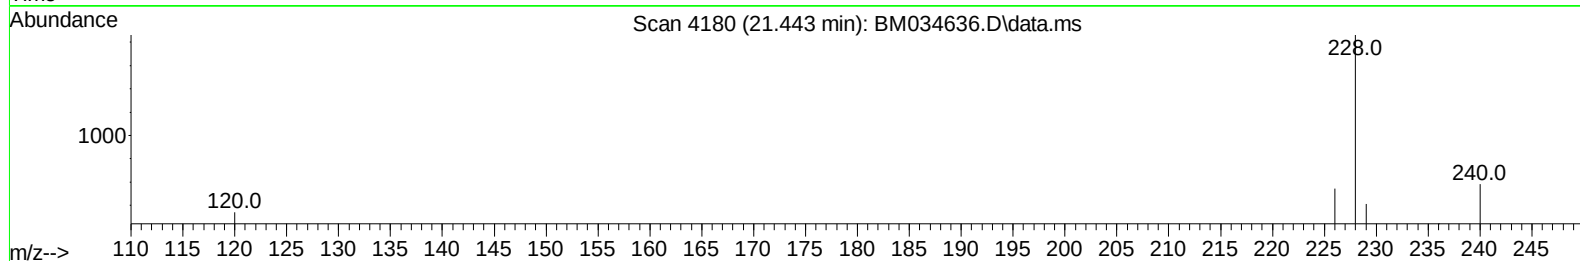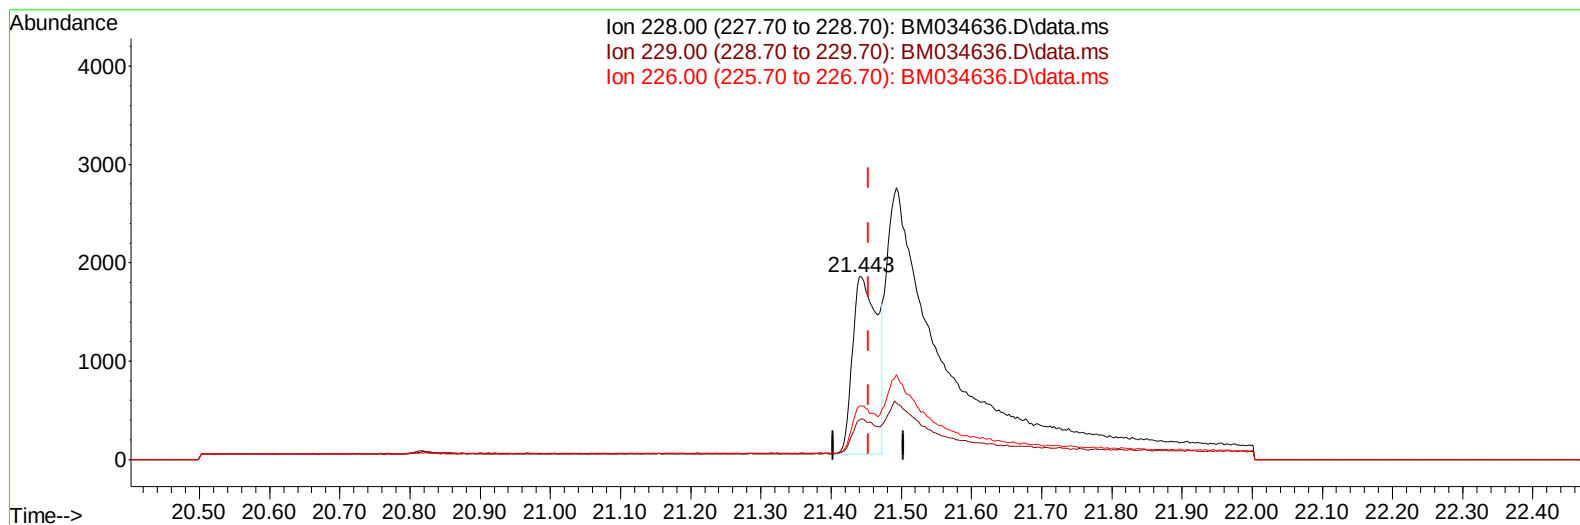

TIC: BM034636.D\data.ms

(21) Benzo(a)anthracene

21.443min (-0.010) 0.45 ng/u1

response 4451

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	22.08
226.00	29.00	29.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034636.D
Acq On : 13 Apr 2022 00:45
Operator : CG/JU
Sample : N2319-14MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

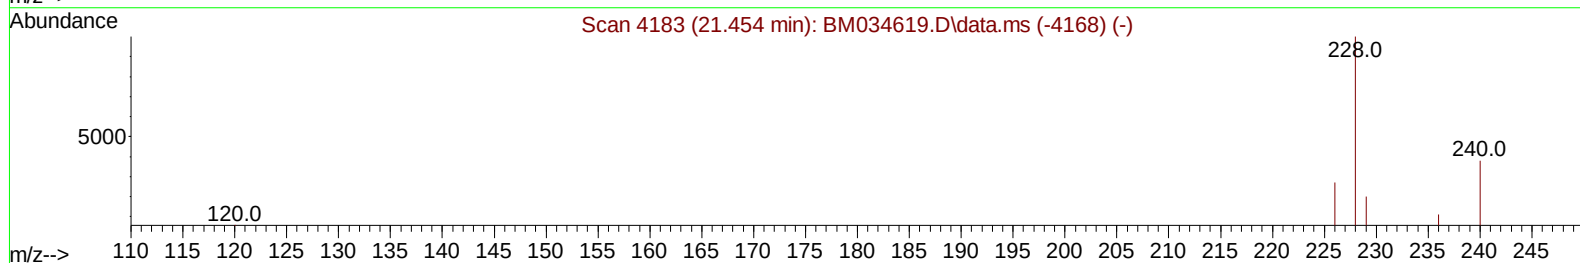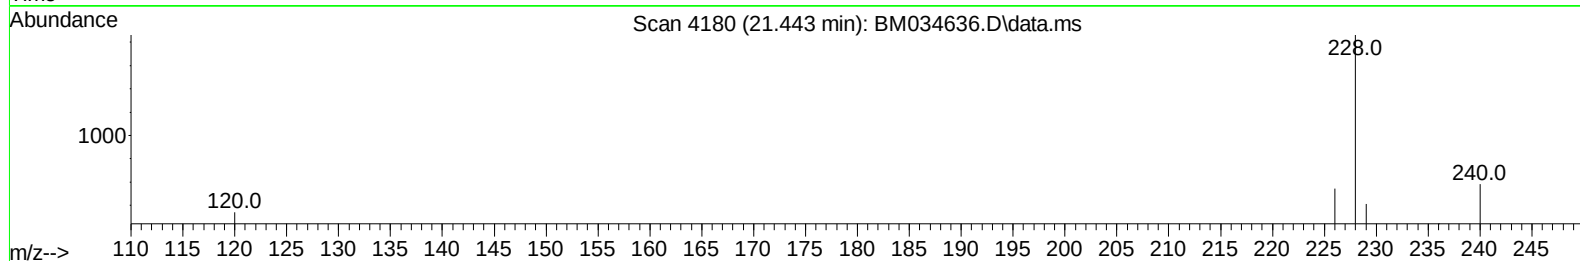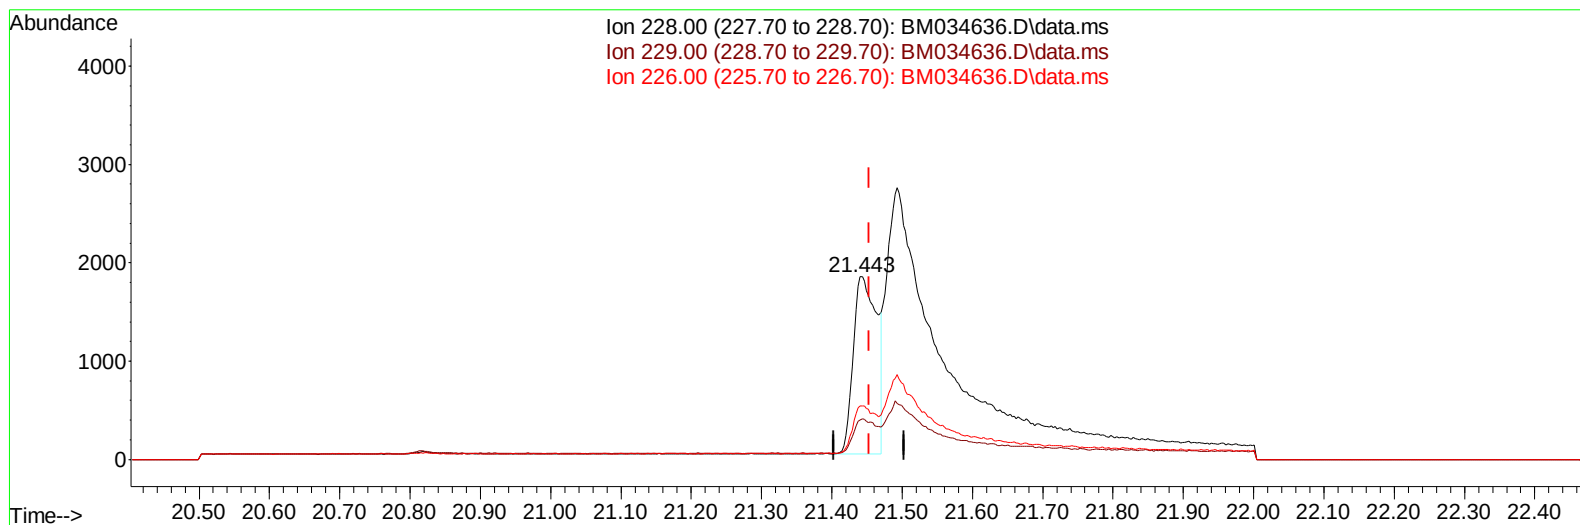

TIC: BM034636.D\data.ms

(21) Benzo(a)anthracene

21.443min (-0.010) 0.43 ng/ul m

response 4193

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	22.08
226.00	29.00	29.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034636.D
 Acq On : 13 Apr 2022 00:45
 Operator : CG/JU
 Sample : N2319-14MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

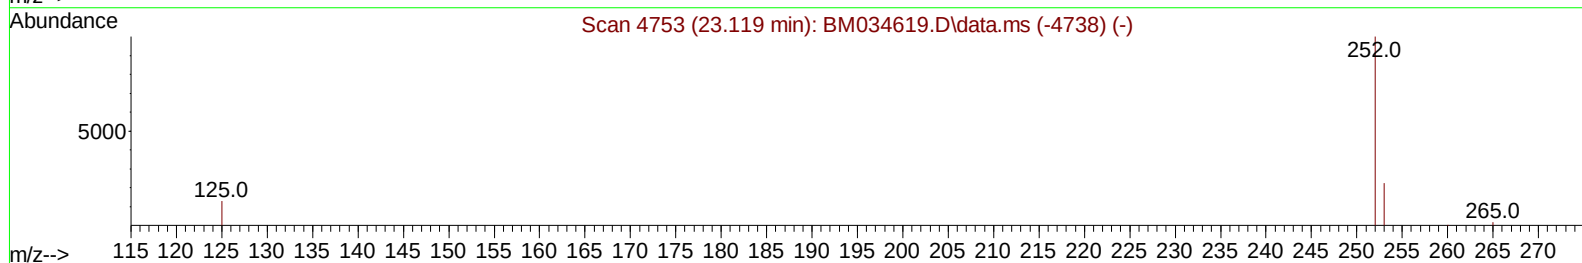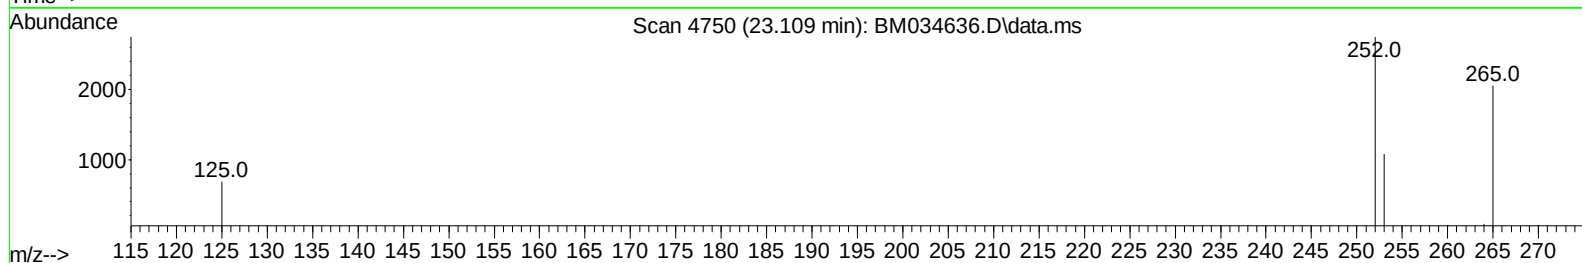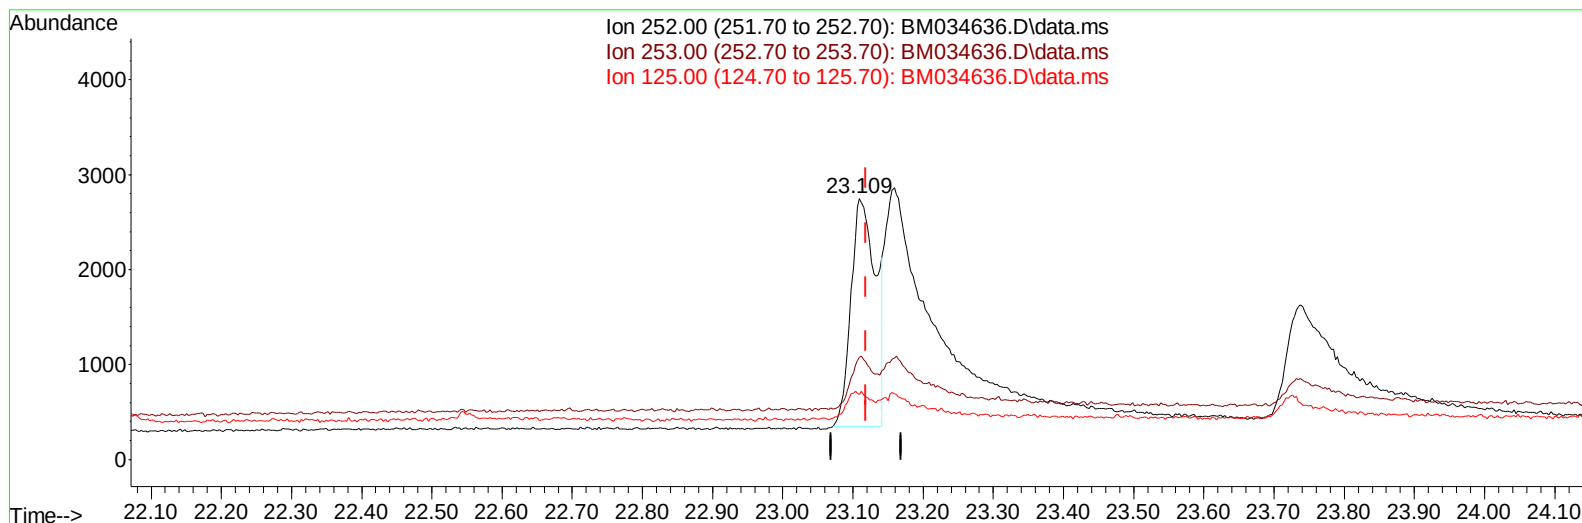

TIC: BM034636.D\data.ms

(24) Benzo(b)fluoranthene

23.109min (-0.010) 0.48 ng/u1

response 5935

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.10	39.21
125.00	14.40	24.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034636.D
 Acq On : 13 Apr 2022 00:45
 Operator : CG/JU
 Sample : N2319-14MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

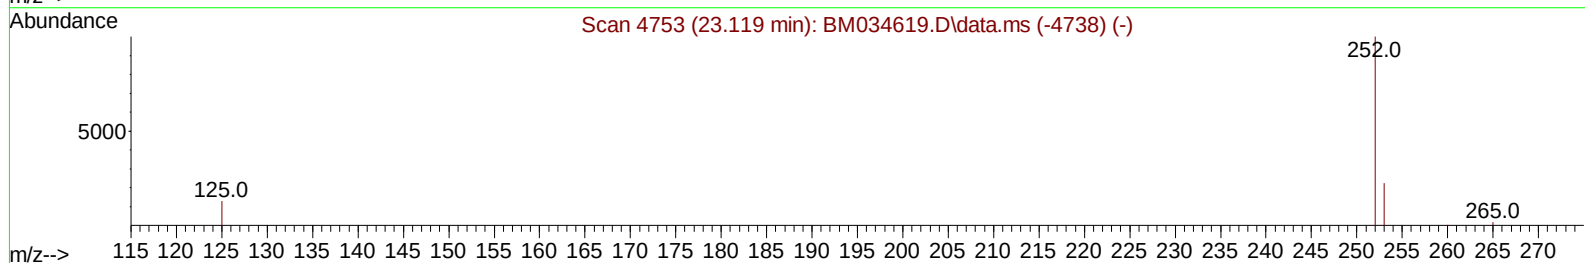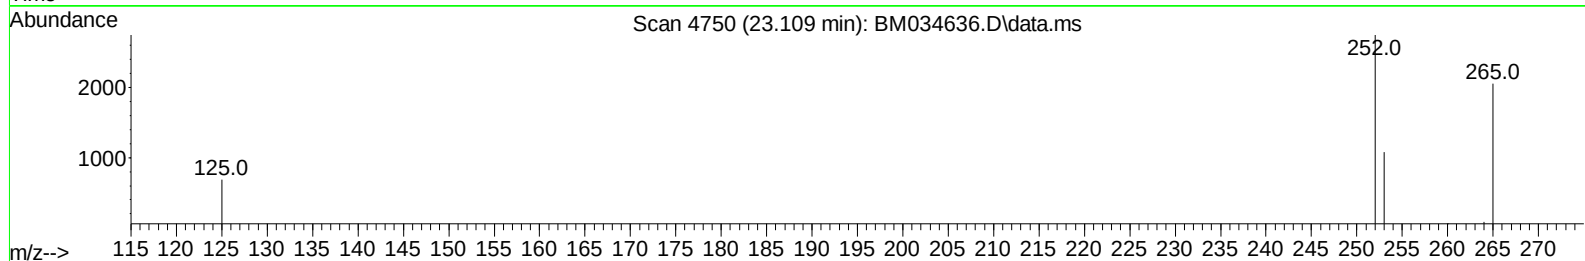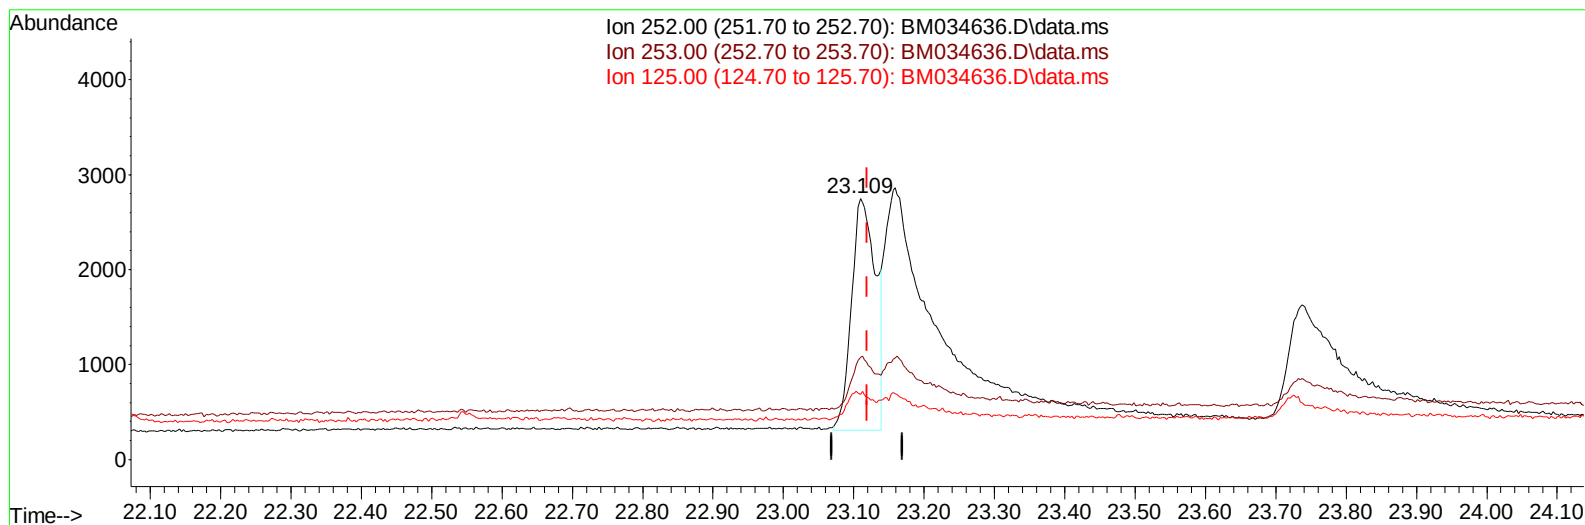

TIC: BM034636.D\data.ms

(24) Benzo(b)fluoranthene

23.109min (-0.010) 0.47 ng/ul m

response 5780

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.10	39.21
125.00	14.40	24.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034636.D
 Acq On : 13 Apr 2022 00:45
 Operator : CG/JU
 Sample : N2319-14MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.897	152		1739	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.705	136		5741	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.530	164		3250	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.280	188		5088	0.400	ng/ul	0.00
17) Chrysene-d12	21.458	240		4704	0.400	ng/ul	#-0.01
23) Perylene-d12	23.840	264		3747	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.256	96		4959	1.645	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152		2932	0.385	ng/ul	0.00
18) Fluoranthene-d10	19.299	212		6911	0.505	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.294	88		2477m	0.830	ng/ul	
5) Naphthalene	10.755	128		6159	0.371	ng/ul	93
7) 2-Methylnaphthalene	12.377	142		3625	0.366	ng/ul	99
8) 1-Methylnaphthalene	12.586	142		3715	0.370	ng/ul	99
10) Acenaphthylene	14.252	152		5943	0.389	ng/ul	92
11) Acenaphthene	14.594	153		4268	0.350	ng/ul	96
12) Fluorene	15.584	166		4669	0.372	ng/ul	98
14) Pentachlorophenol	16.938	266		1588	0.805	ng/ul	97
15) Phenanthrene	17.322	178		6885	0.419	ng/ul	98
16) Anthracene	17.424	178		3475	0.277	ng/ul	100
19) Fluoranthene	19.332	202		8907	0.458	ng/ul	98
20) Pyrene	19.694	202		10394	0.453	ng/ul#	95
21) Benzo(a)anthracene	21.443	228		4193m	0.427	ng/ul	
22) Chrysene	21.493	228		5705	0.460	ng/ul	99
24) Benzo(b)fluoranthene	23.109	252		5780m	0.470	ng/ul	
25) Benzo(k)fluoranthene	23.159	252		5369	0.435	ng/ul#	88
26) Benzo(a)pyrene	23.738	252		6661	0.471	ng/ul#	73
27) Indeno(1,2,3-cd)pyrene	26.325	276		8073	0.430	ng/ul#	95
28) Dibenzo(a,h)anthracene	26.359	278		5946	0.437	ng/ul#	76
29) Benzo(g,h,i)perylene	27.073	276		9094	0.445	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034636.D
Acq On : 13 Apr 2022 00:45
Operator : CG/JU
Sample : N2319-14MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1MS

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

