




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034637.D
Acq On : 13 Apr 2022 01:21
Operator : CG/JU
Sample : N2319-15MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

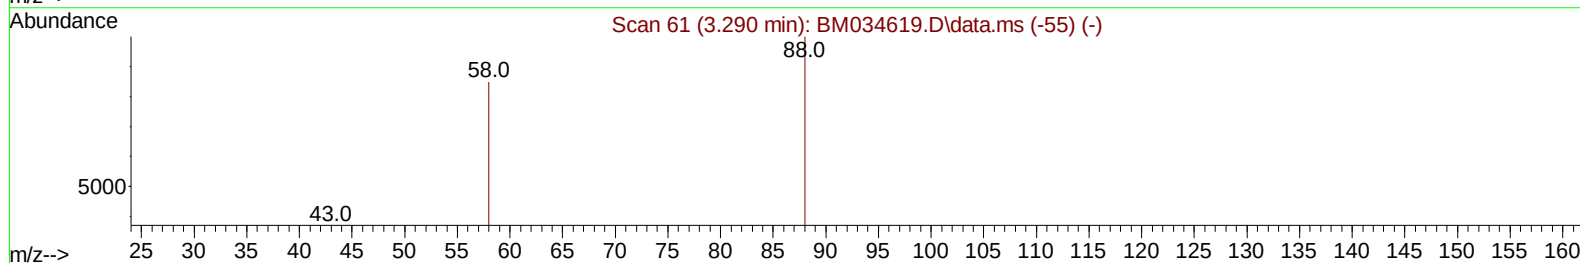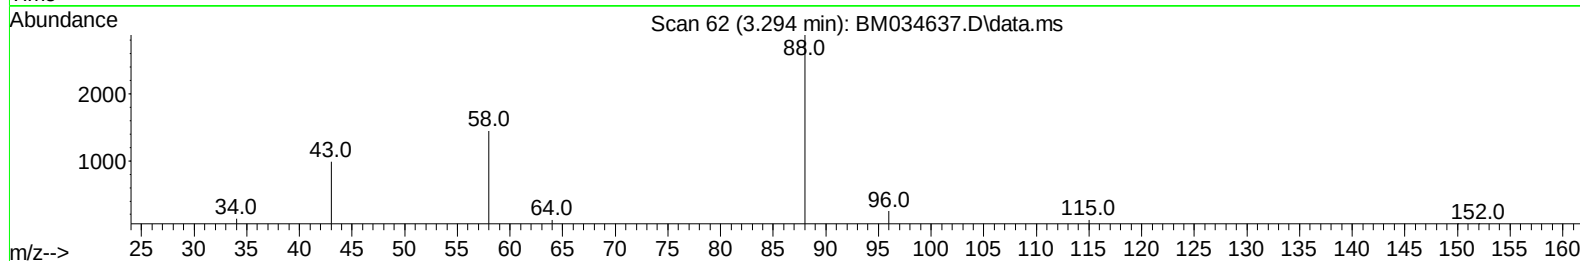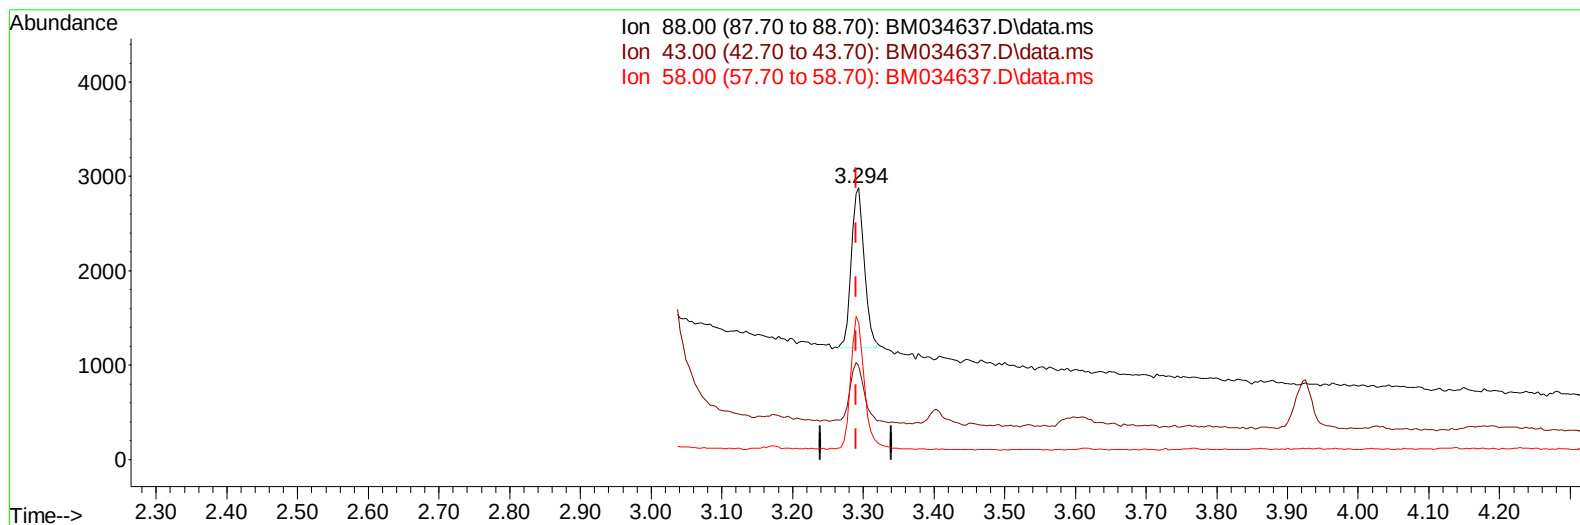

TIC: BM034637.D\data.ms

(2) 1,4-Dioxane

3.294min (+ 0.004) 0.87 ng/uL

response 2164

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	62.10	34.42#
58.00	65.60	50.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034637.D
 Acq On : 13 Apr 2022 01:21
 Operator : CG/JU
 Sample : N2319-15MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

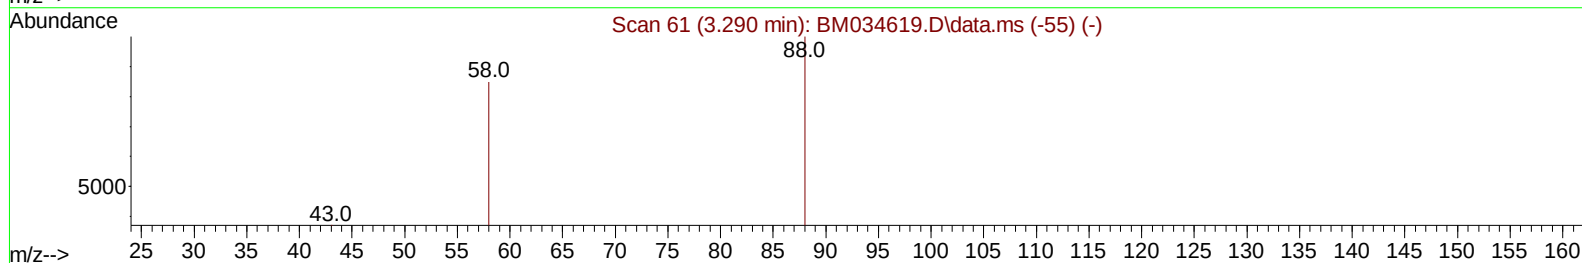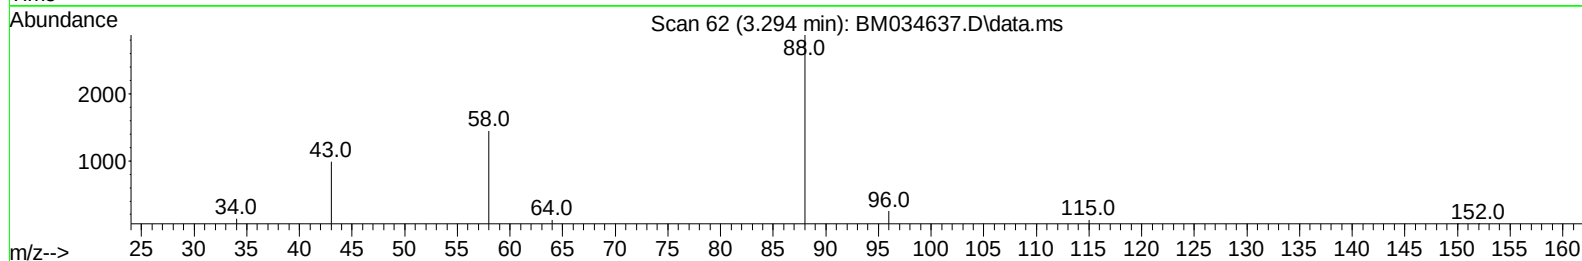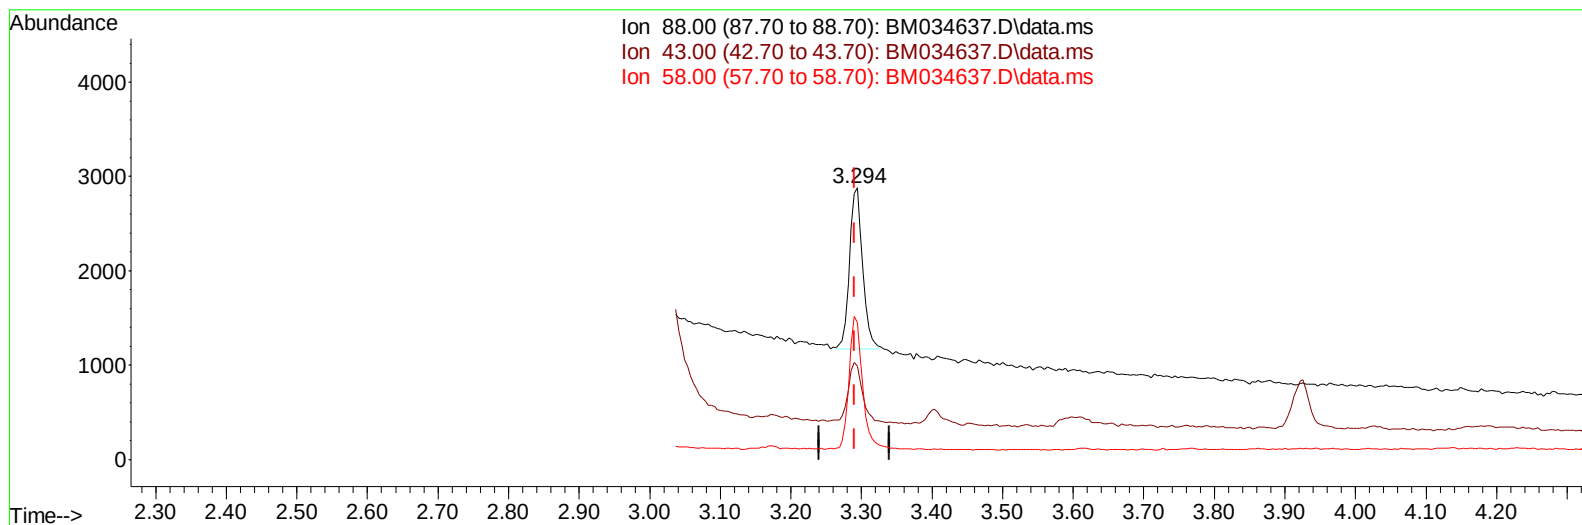

TIC: BM034637.D\data.ms

(2) 1,4-Dioxane

3.294min (+ 0.004) 0.88 ng/ul m

response 2198

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	62.10	34.42#
58.00	65.60	50.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034637.D
 Acq On : 13 Apr 2022 01:21
 Operator : CG/JU
 Sample : N2319-15MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

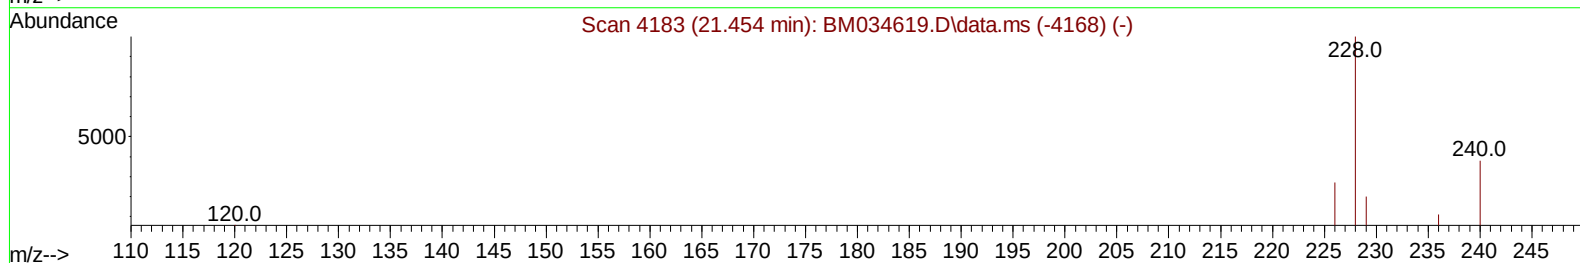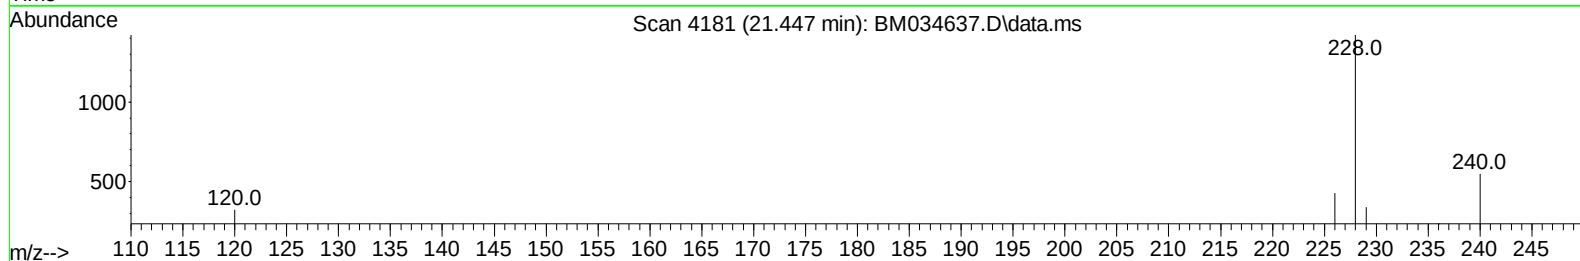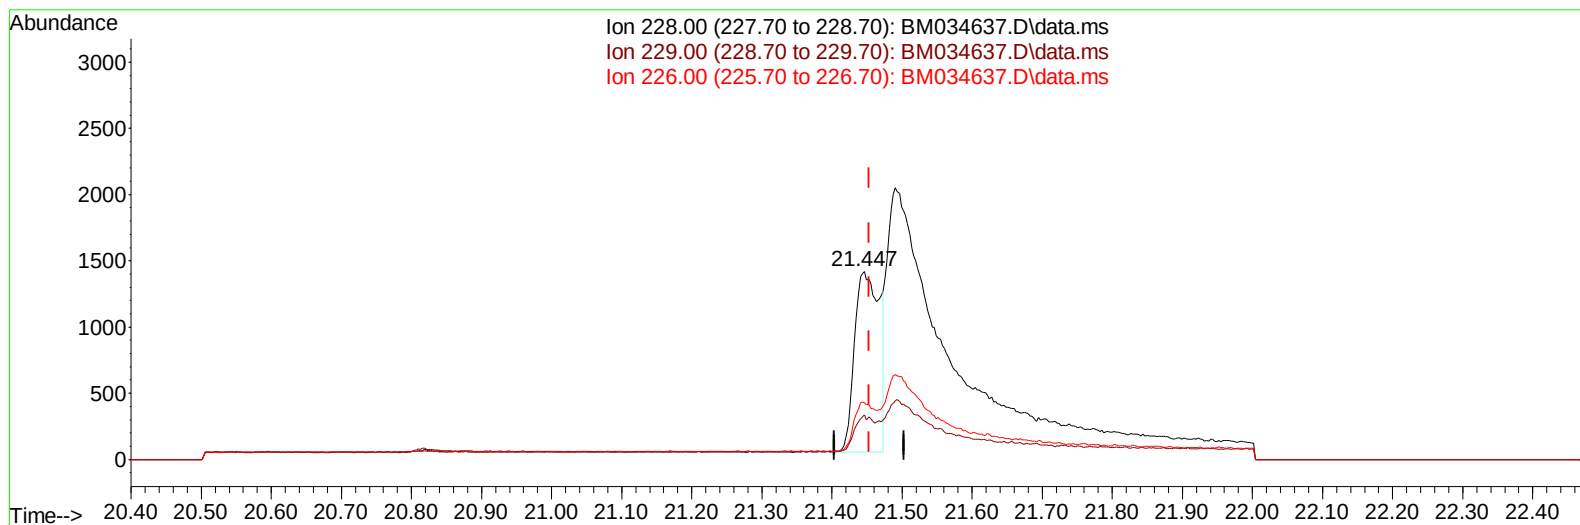

TIC: BM034637.D\data.ms

(21) Benzo(a)anthracene

21.447min (-0.007) 0.44 ng/u1

response 3394

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	23.79
226.00	29.00	30.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034637.D
 Acq On : 13 Apr 2022 01:21
 Operator : CG/JU
 Sample : N2319-15MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

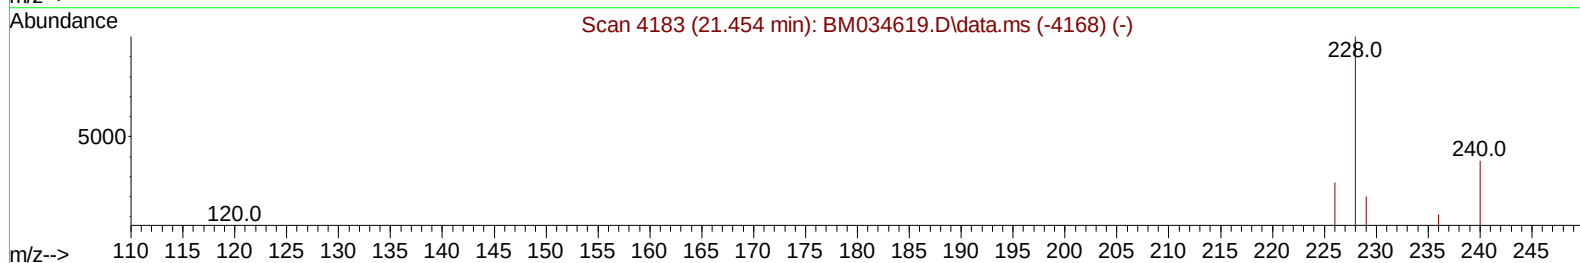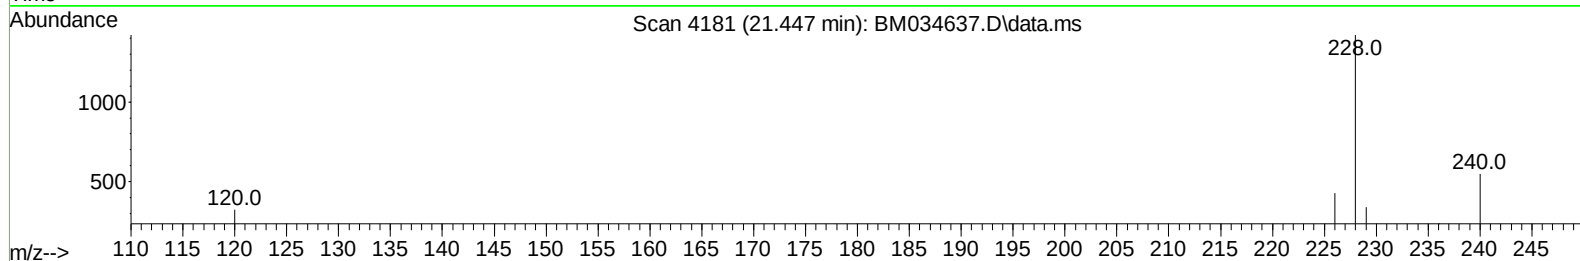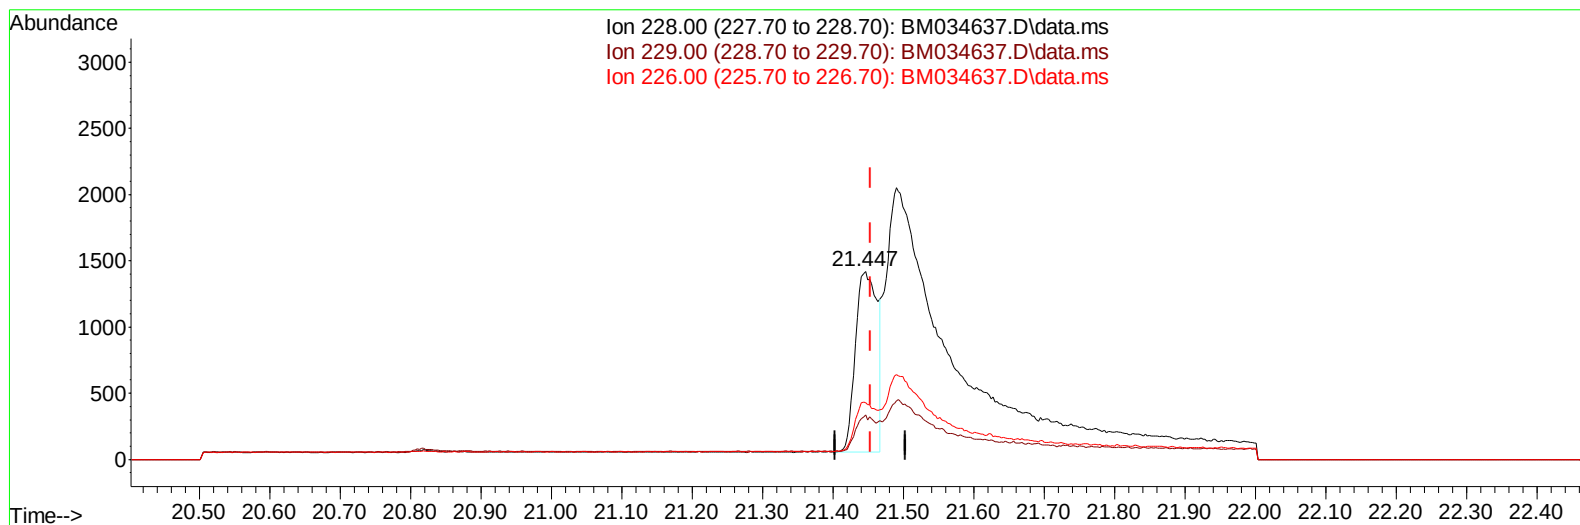

TIC: BM034637.D\data.ms

(21) Benzo(a)anthracene

21.447min (-0.007) 0.39 ng/ul m

response 2983

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	23.79
226.00	29.00	30.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034637.D
 Acq On : 13 Apr 2022 01:21
 Operator : CG/JU
 Sample : N2319-15MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

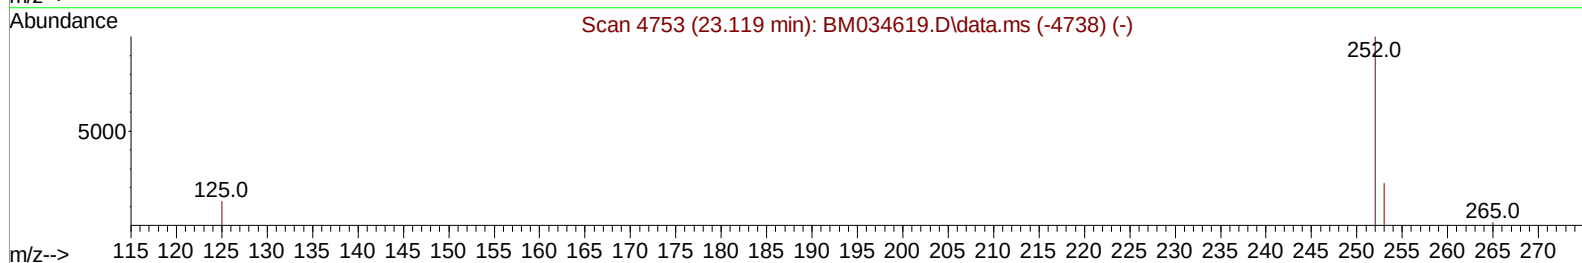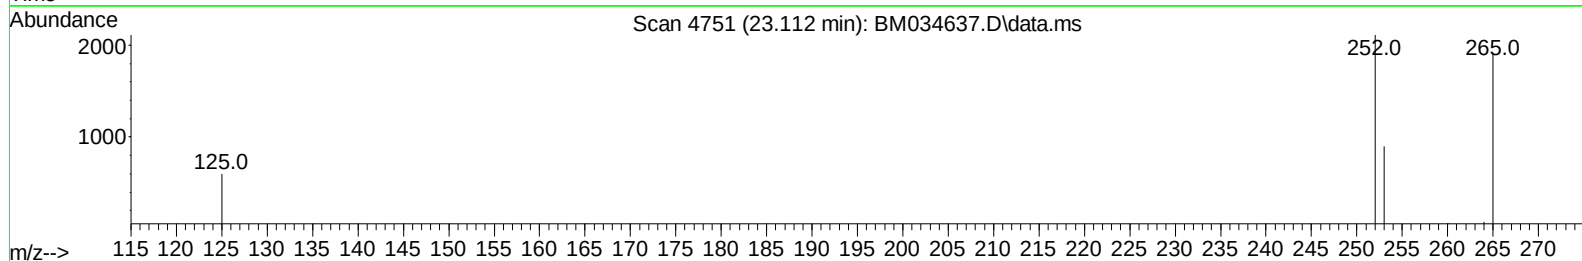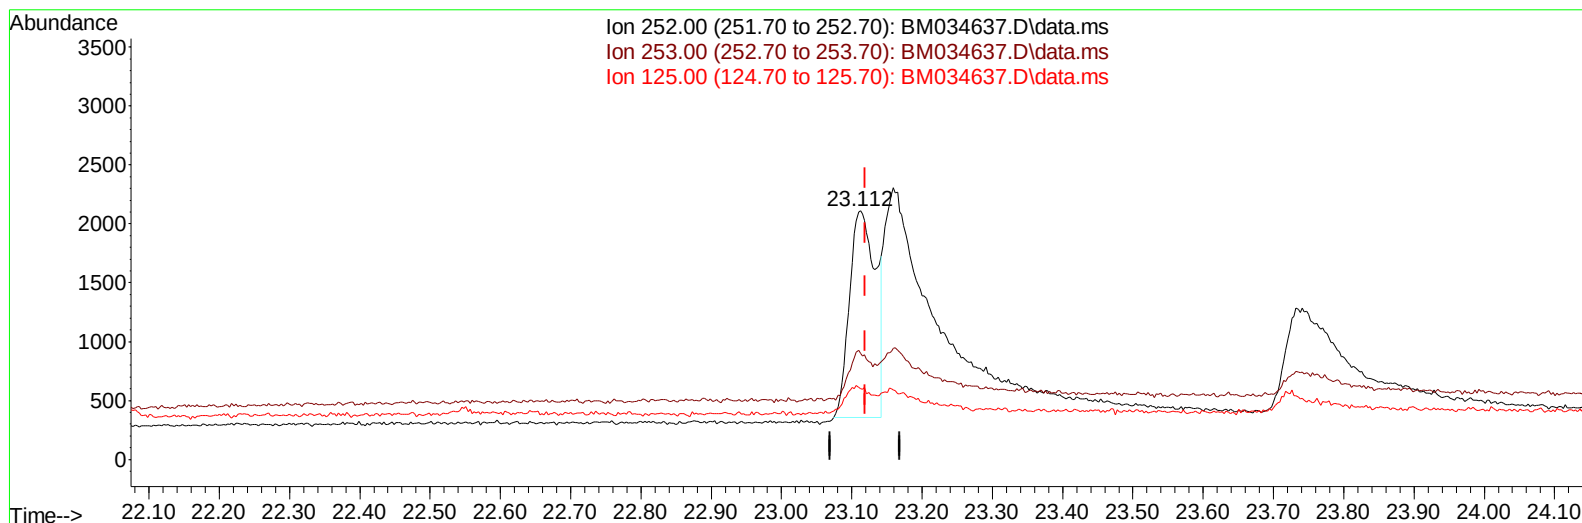

TIC: BM034637.D\data.ms

(24) Benzo(b)fluoranthene

23.112min (-0.007) 0.47 ng/u1

response 4564

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.10	42.70
125.00	14.40	28.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034637.D
 Acq On : 13 Apr 2022 01:21
 Operator : CG/JU
 Sample : N2319-15MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

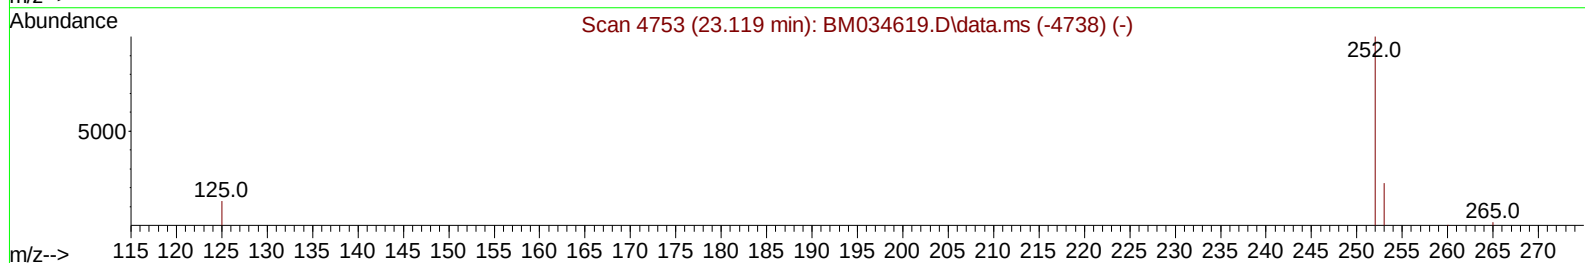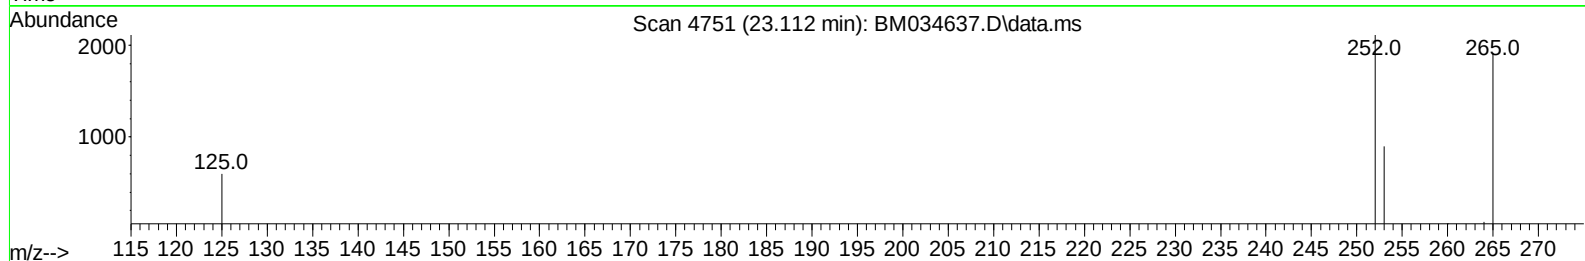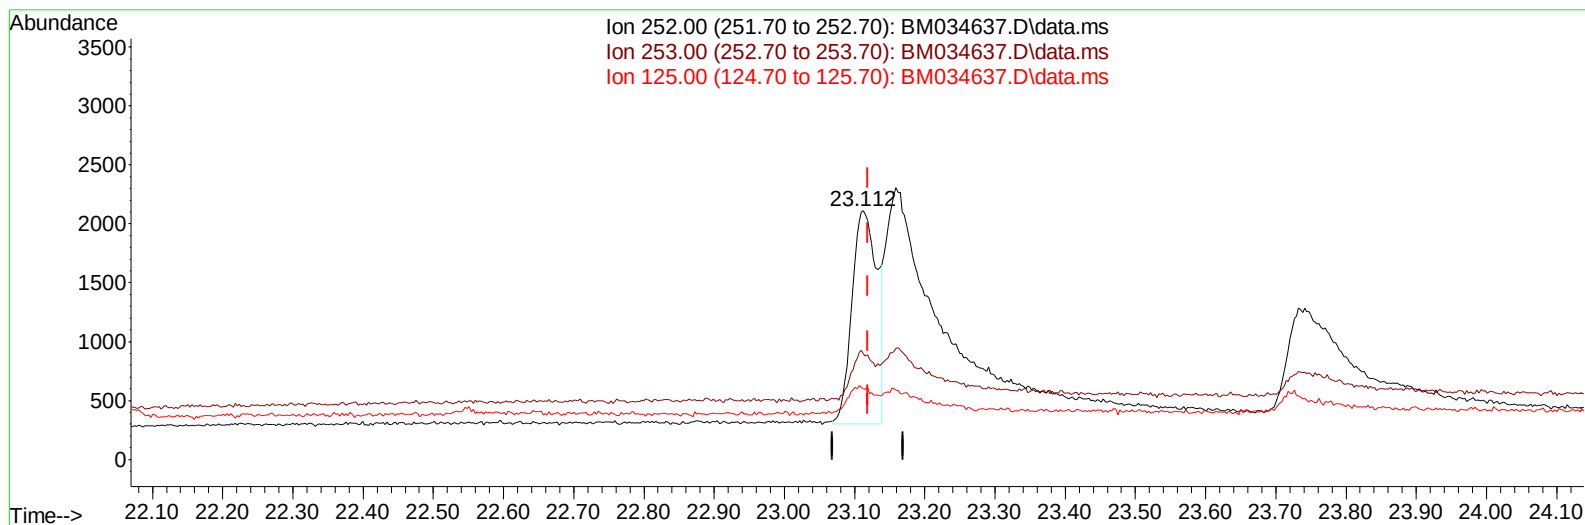

TIC: BM034637.D\data.ms

(24) Benzo(b)fluoranthene

23.112min (-0.007) 0.47 ng/ul m

response 4556

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.10	42.70
125.00	14.40	28.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034637.D
 Acq On : 13 Apr 2022 01:21
 Operator : CG/JU
 Sample : N2319-15MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1MSD

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 05:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.905	152		1453	0.400	ng/ul	0.00
4) Naphthalene-d8	10.709	136		4792	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.533	164		2516	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.283	188		3911	0.400	ng/ul	0.00
17) Chrysene-d12	21.458	240		3707	0.400	ng/ul	# 0.00
23) Perylene-d12	23.843	264		2941	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.256	96		4209	1.671	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152		2401	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.302	212		5460	0.506	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.294	88		2198m	0.881	ng/ul	
5) Naphthalene	10.759	128		5032	0.363	ng/ul	96
7) 2-Methylnaphthalene	12.381	142		2881	0.348	ng/ul	97
8) 1-Methylnaphthalene	12.584	142		3040	0.363	ng/ul	99
10) Acenaphthylene	14.255	152		4822	0.408	ng/ul	93
11) Acenaphthene	14.593	153		3427	0.363	ng/ul	96
12) Fluorene	15.587	166		3689	0.380	ng/ul	97
14) Pentachlorophenol	16.937	266		1235	0.814	ng/ul	98
15) Phenanthrene	17.321	178		5470	0.433	ng/ul	99
16) Anthracene	17.422	178		2639	0.273	ng/ul	93
19) Fluoranthene	19.330	202		7145	0.466	ng/ul	96
20) Pyrene	19.693	202		8330	0.460	ng/ul#	93
21) Benzo(a)anthracene	21.447	228		2983m	0.385	ng/ul	
22) Chrysene	21.490	228		4493	0.459	ng/ul	98
24) Benzo(b)fluoranthene	23.112	252		4556m	0.472	ng/ul	
25) Benzo(k)fluoranthene	23.159	252		4537	0.469	ng/ul#	83
26) Benzo(a)pyrene	23.732	252		5450	0.491	ng/ul#	63
27) Indeno(1,2,3-cd)pyrene	26.325	276		6739	0.458	ng/ul#	95
28) Dibenzo(a,h)anthracene	26.366	278		5029	0.471	ng/ul#	65
29) Benzo(g,h,i)perylene	27.077	276		7701	0.480	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034637.D
Acq On : 13 Apr 2022 01:21
Operator : CG/JU
Sample : N2319-15MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:11:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

