




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034642.D
Acq On : 13 Apr 2022 04:22
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:42:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

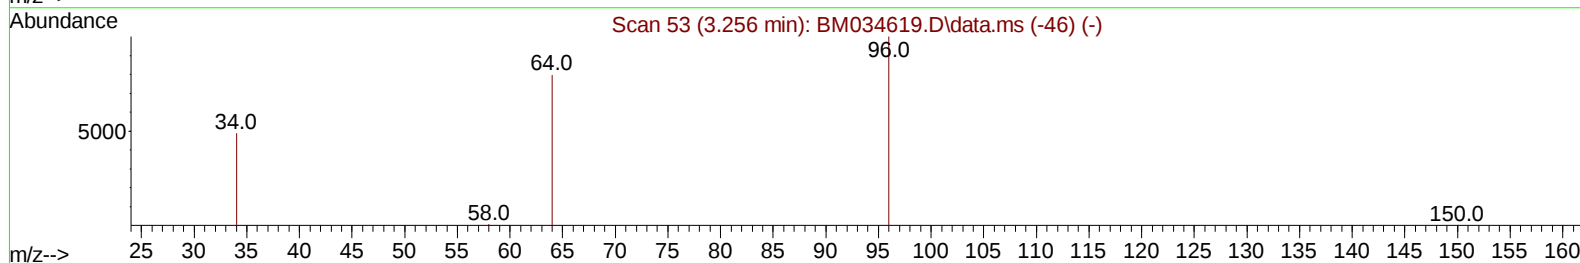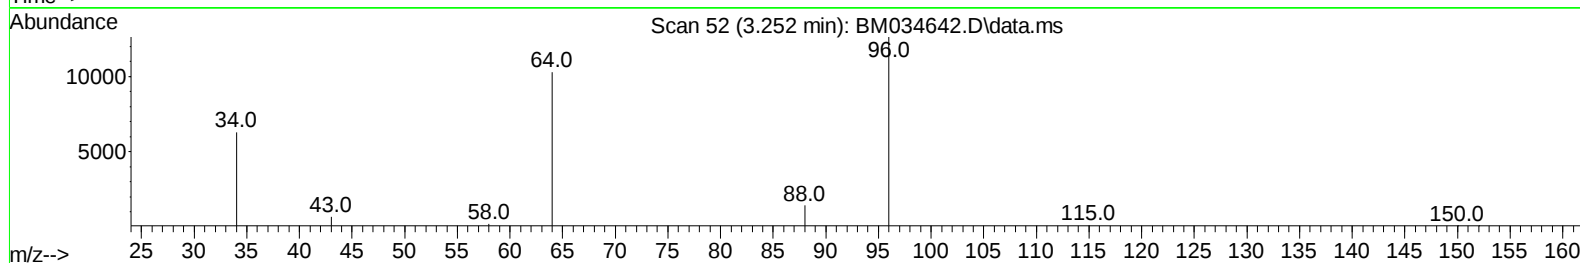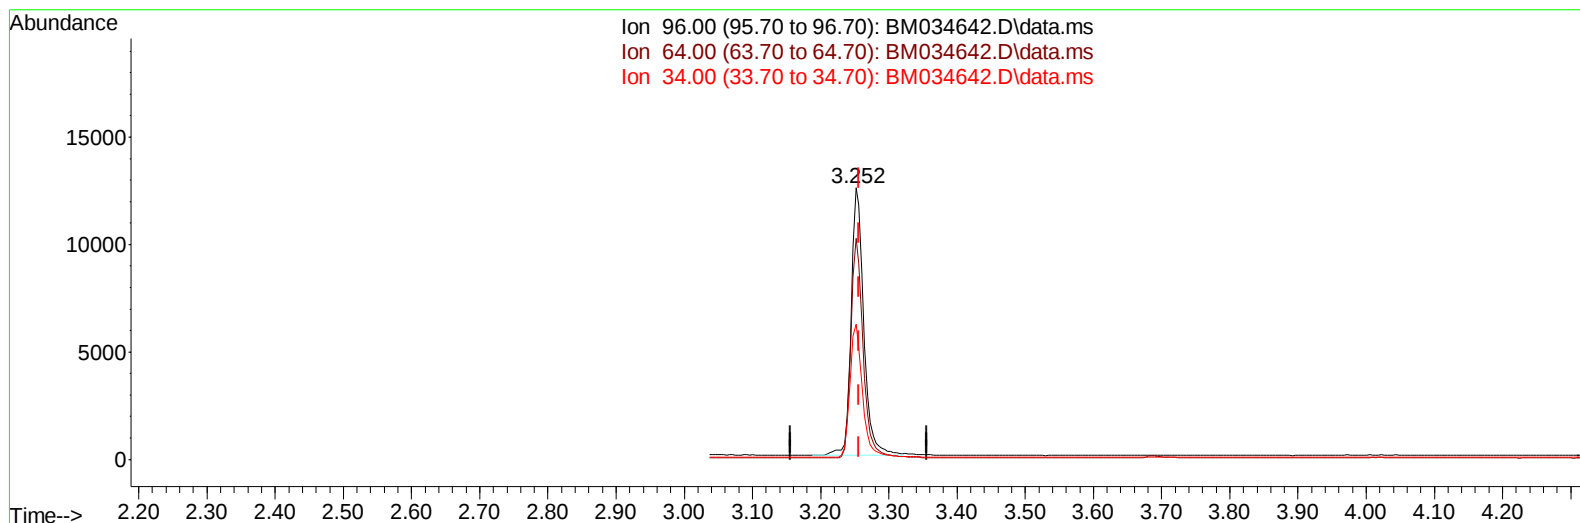

TIC: BM034642.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.252min (-0.004) 4.04 ng/u1

response 16030

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	81.51
34.00	243.00	49.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034642.D
Acq On : 13 Apr 2022 04:22
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:42:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

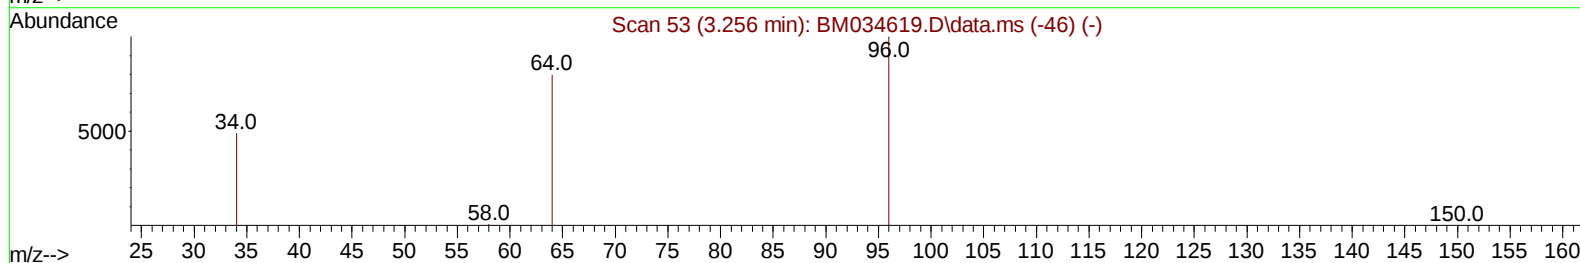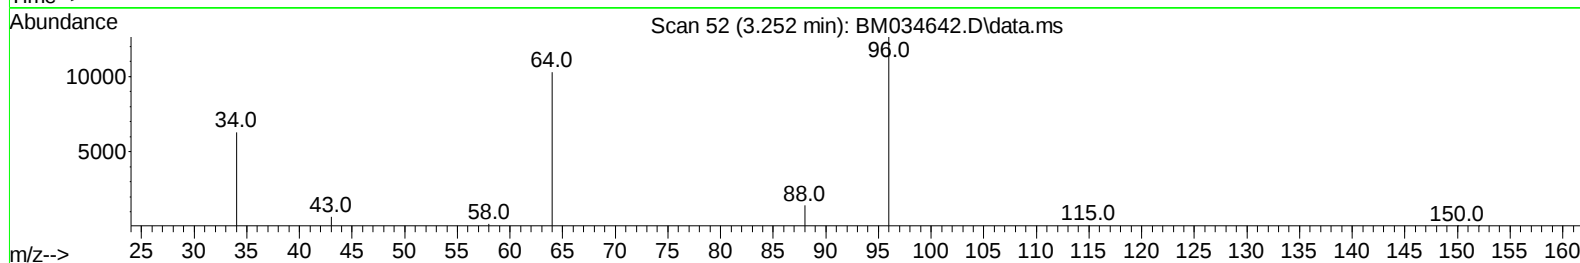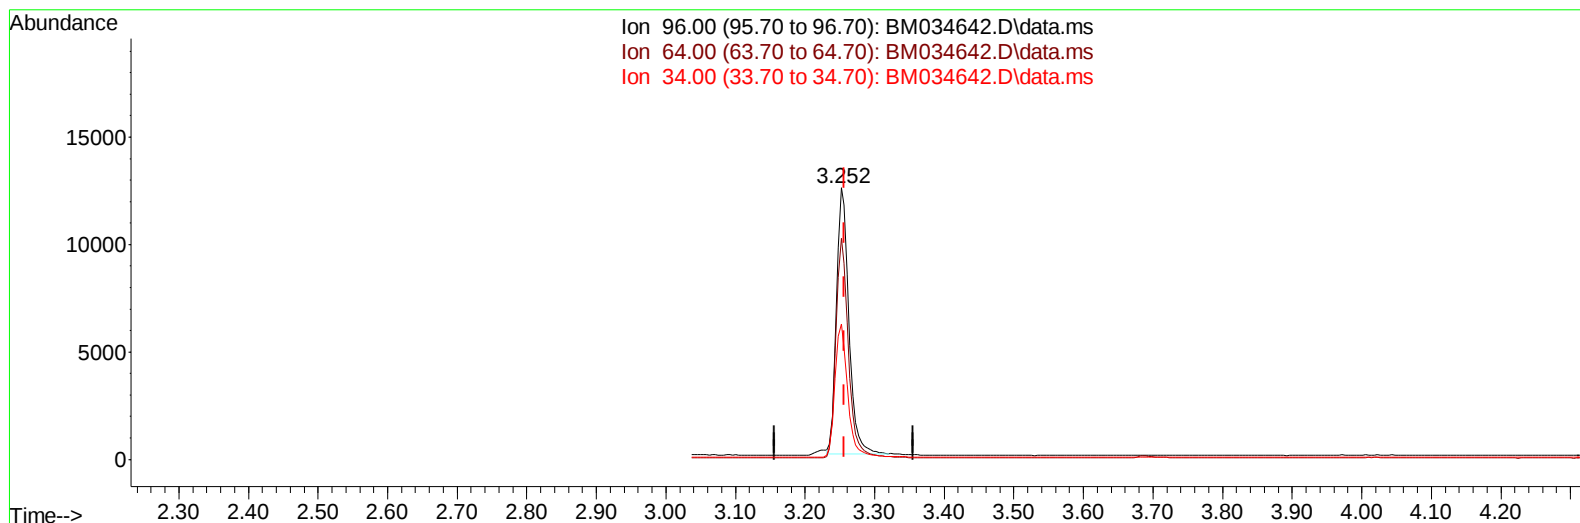

TIC: BM034642.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.252min (-0.004) 3.89 ng/ul m

response 15434

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	81.51
34.00	243.00	49.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034642.D
Acq On : 13 Apr 2022 04:22
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:42:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

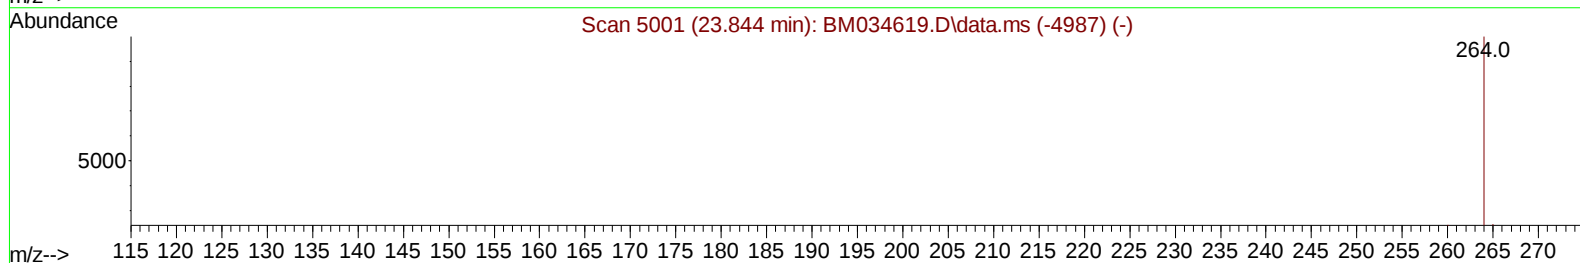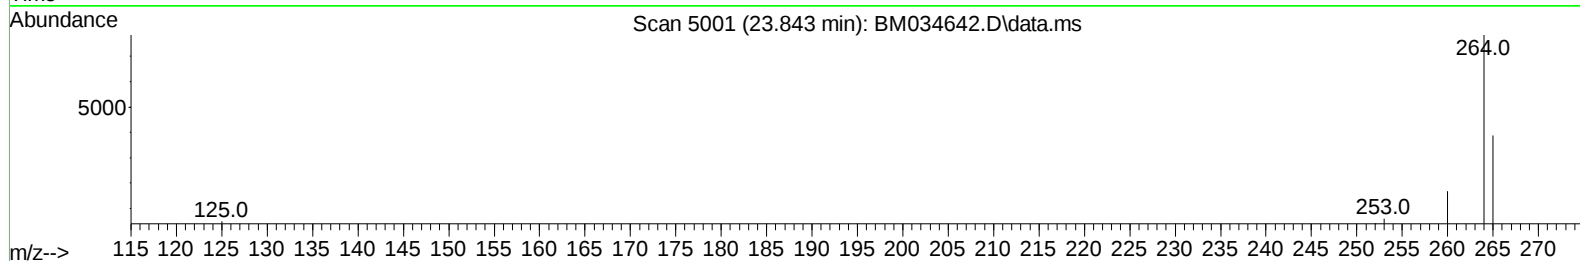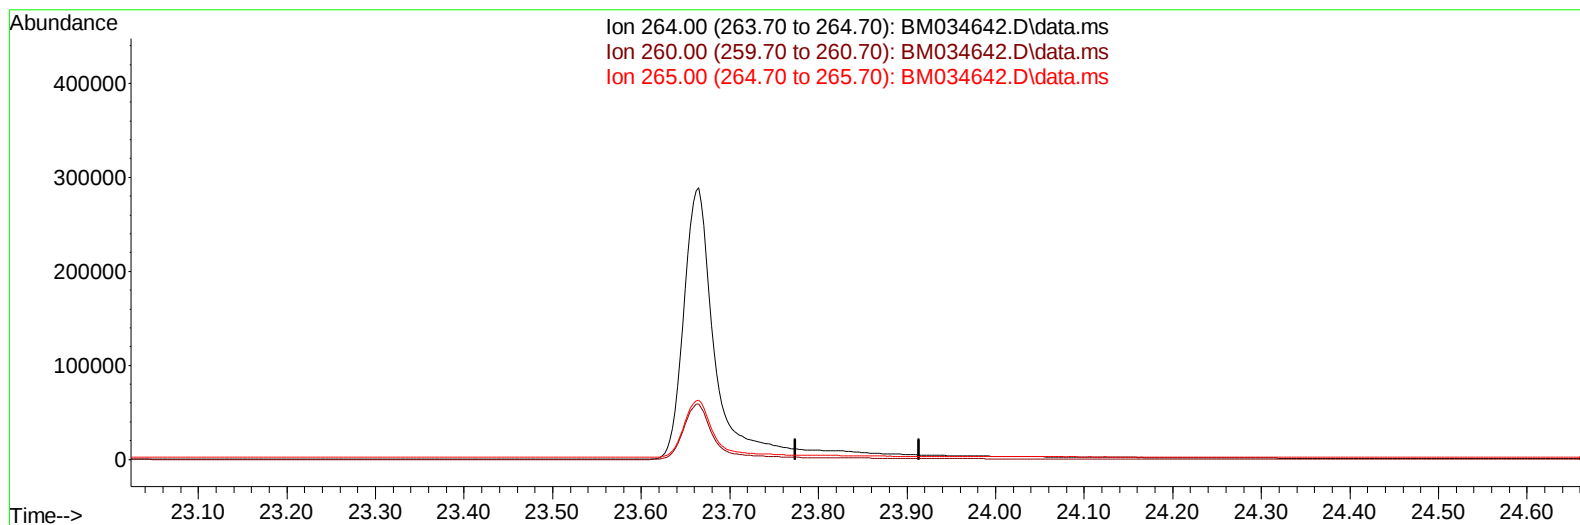

TIC: BM034642.D\data.ms

(23) Perylene-d12 (I)

23.844min (-23.844) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034642.D
 Acq On : 13 Apr 2022 04:22
 Operator : CG/JU
 Sample : N2319-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2G7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:42:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

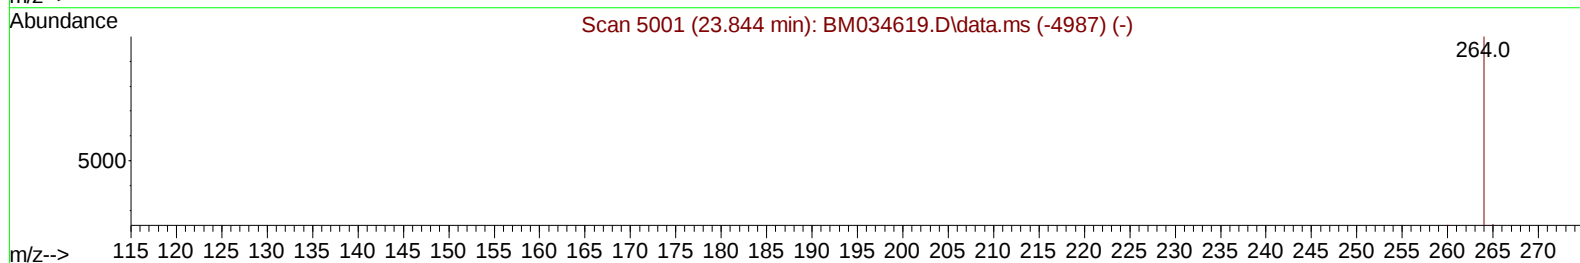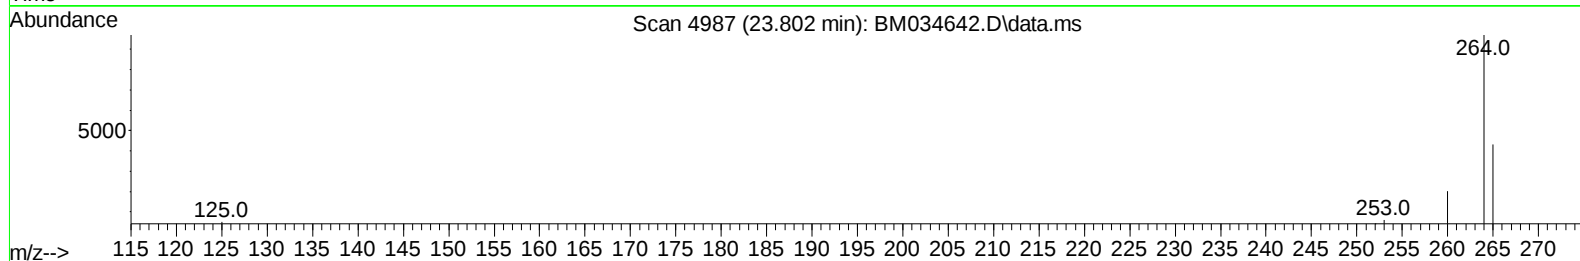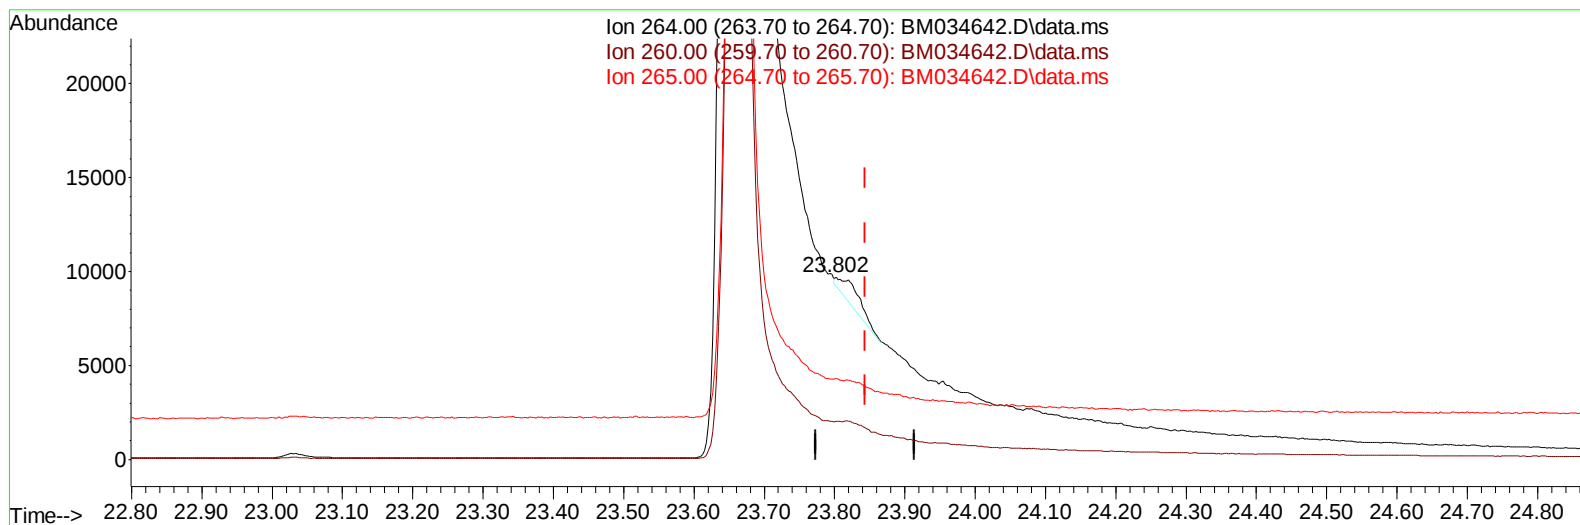

TIC: BM034642.D\data.ms

(23) Perylene-d12 (I)

23.802min (-0.042) 0.40 ng/ul m

response 2215

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	20.82#
265.00	95.30	44.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034642.D
 Acq On : 13 Apr 2022 04:22
 Operator : CG/JU
 Sample : N2319-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2G7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 05:42:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.880	152		2286	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.689	136		6388	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.525	164		3561	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.267	188		6651	0.400	ng/ul	-0.02
17) Chrysene-d12	21.478	240		5006	0.400	ng/ul	# 0.01
23) Perylene-d12	23.802	264		2215m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.252	96		15434m	3.895	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152		3484	0.412	ng/ul	0.00
18) Fluoranthene-d10	19.294	212		7936	0.545	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034642.D
Acq On : 13 Apr 2022 04:22
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 05:42:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

