




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034649.D
 Acq On : 13 Apr 2022 09:11
 Operator : CG/JU
 Sample : PB143960BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK960

Manual IntegrationsAPPROVED

Quant Time: Apr 14 04:13:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

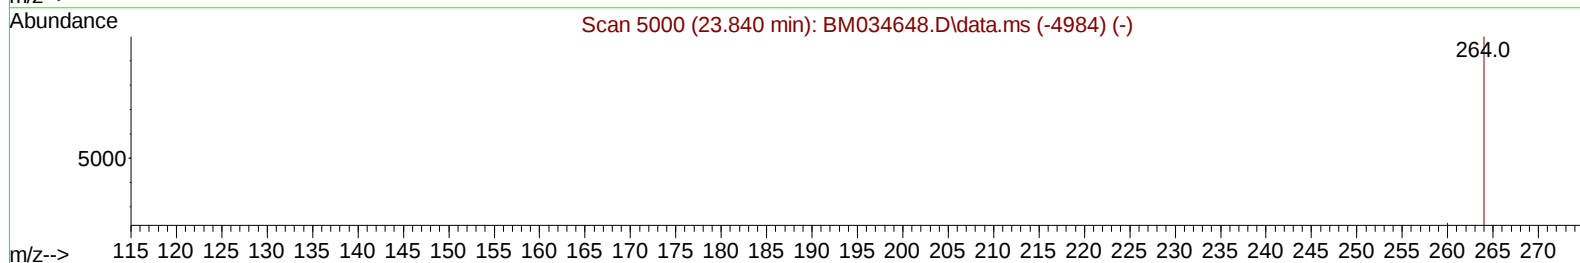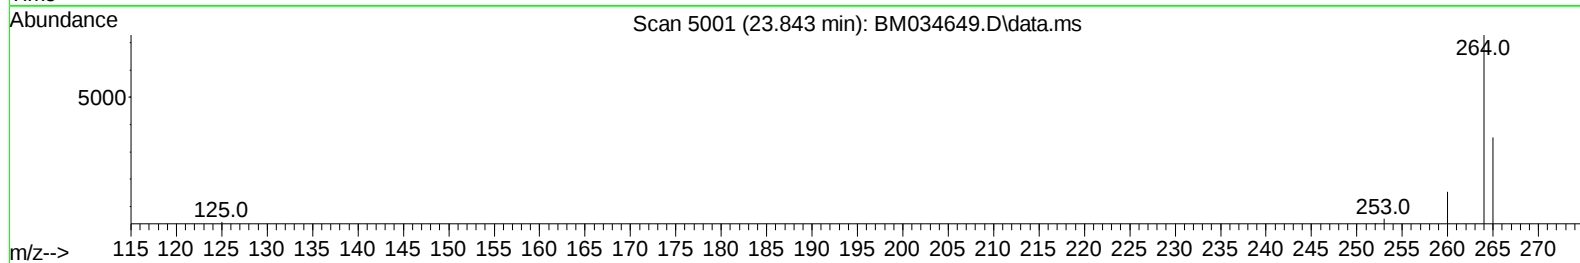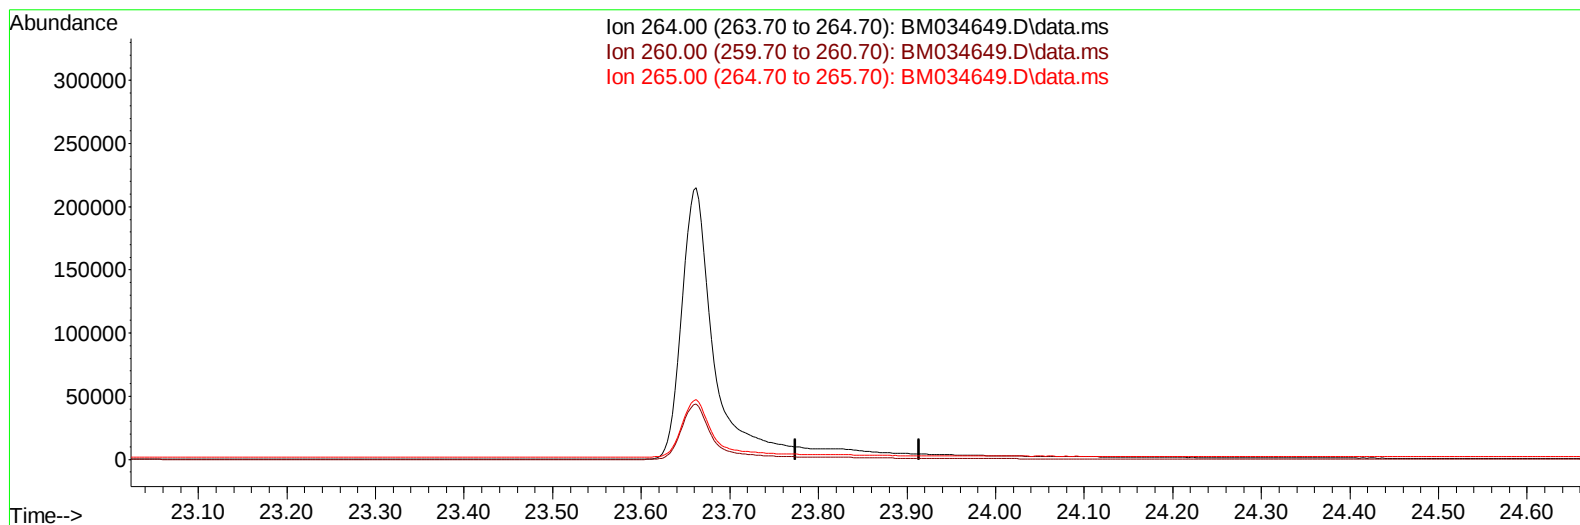

TIC: BM034649.D\data.ms

(23) Perylene-d12 (I)

23.844min (-23.844) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034649.D
 Acq On : 13 Apr 2022 09:11
 Operator : CG/JU
 Sample : PB143960BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK960

Manual IntegrationsAPPROVED

Quant Time: Apr 14 04:13:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

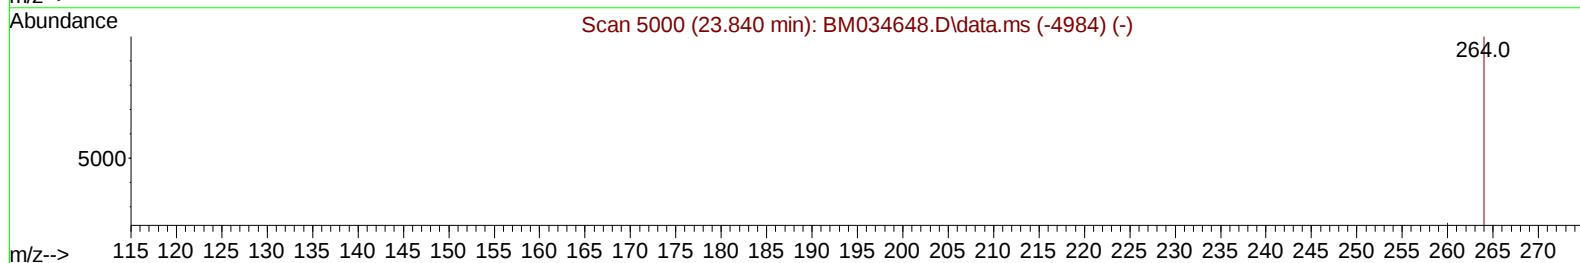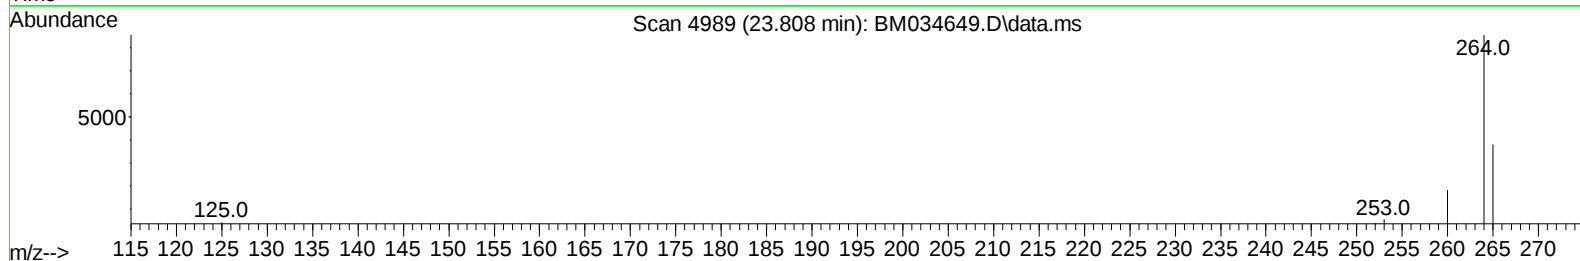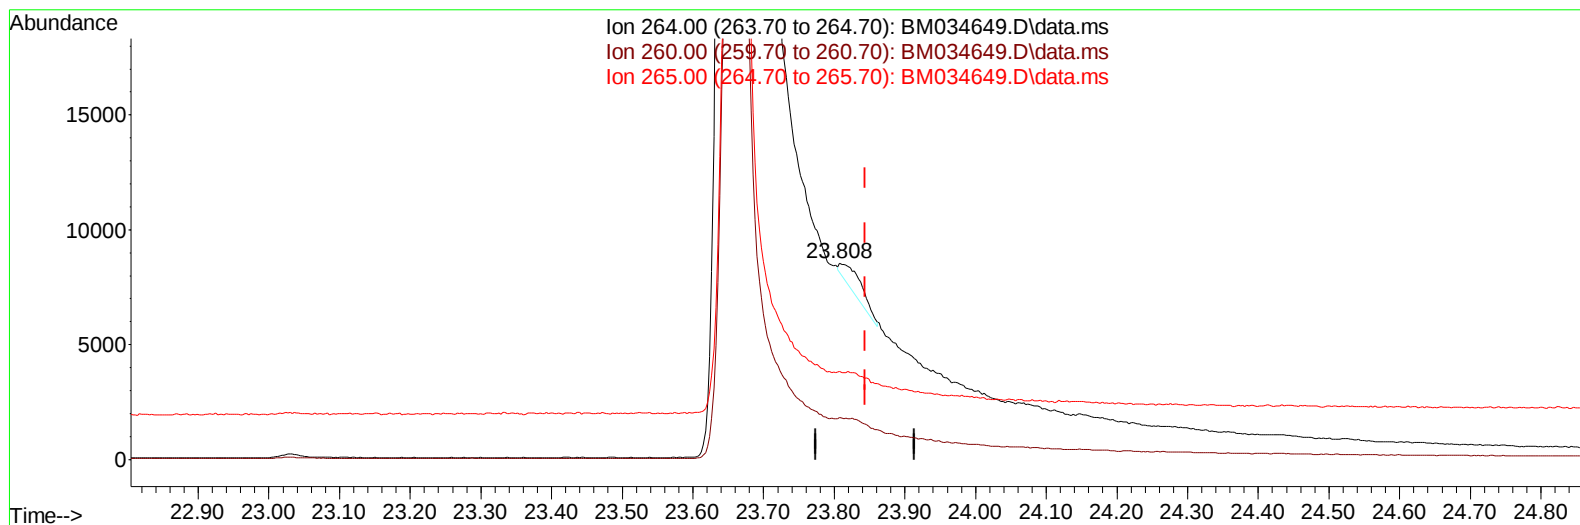

TIC: BM034649.D\data.ms

(23) Perylene-d12 (I)

23.808min (-0.036) 0.40 ng/ul m

response 1915

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.52#
265.00	95.30	44.68#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034649.D
 Acq On : 13 Apr 2022 09:11
 Operator : CG/JU
 Sample : PB143960BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK960

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 14 04:13:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.880	152		2302	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.683	136		6399	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.520	164		3564	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.263	188		6368	0.400	ng/ul	-0.02
17) Chrysene-d12	21.478	240		4414	0.400	ng/ul	# 0.01
23) Perylene-d12	23.808	264		1915m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.248	96		21873	5.481	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.311	152		3062	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.294	212		5984	0.466	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034649.D
Acq On : 13 Apr 2022 09:11
Operator : CG/JU
Sample : PB143960BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK960

Manual IntegrationsAPPROVED

Quant Time: Apr 14 04:13:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
Supervised By :Yogesh Patel 04/14/2022

