

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034625.D
 Acq On : 12 Apr 2022 17:27
 Operator : CG/JU
 Sample : N2289-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 01:03:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.888	152	1867	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.688	136	5317	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.529	164	2944	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.271	188	5528m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.483	240	4516	0.400	ng/ul	# 0.01
23) Perylene-d12	23.827	264	1787m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	13982	4.320	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	2830	0.402	ng/ul	0.00
18) Fluoranthene-d10	19.299	212	6549	0.498	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.290	88	550m	0.172	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\  
Data File : BM034625.D  
Acq On    : 12 Apr 2022   17:27  
Operator  : CG/JU  
Sample    : N2289-01  
Misc      :  
ALS Vial  : 10    Sample Multiplier: 1
```


Instrument :
BNA_M
ClientSampleId :
BFFC6

Manual Integrations

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022


Quant Time: Apr 13 01:03:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

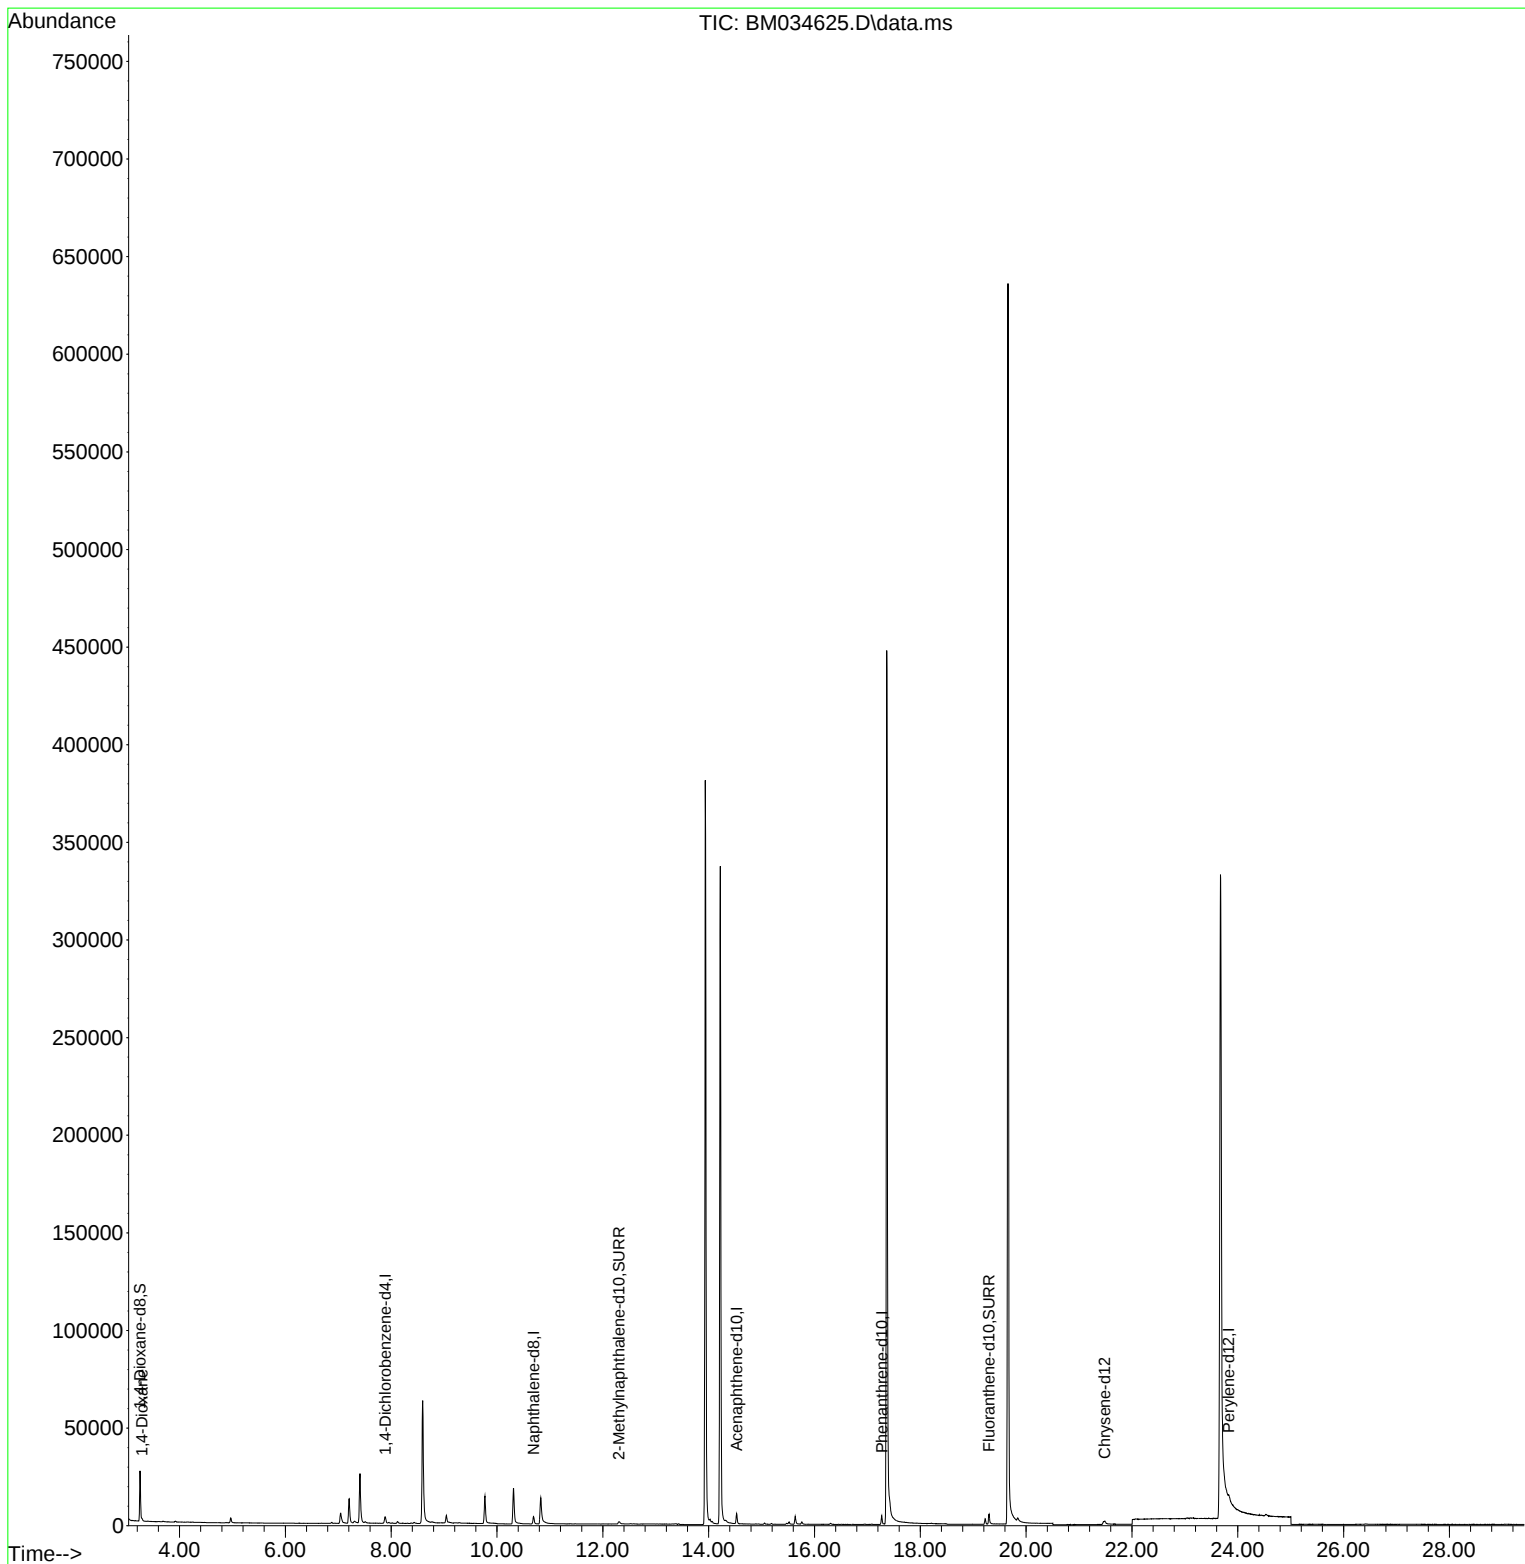

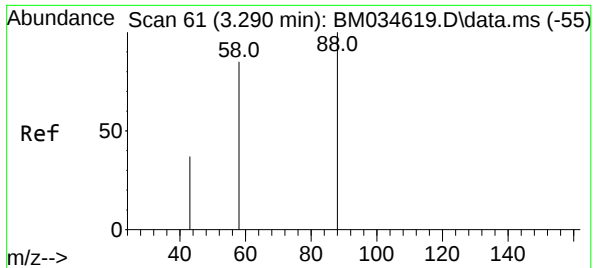

#2
 1,4-Dioxane
 Concen: 0.172 ng/ul m
 RT: 3.290 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM034625.D
 Acq: 12 Apr 2022 17:27

Instrument :
 BNA_M
 ClientSampleId :
 BFFC6

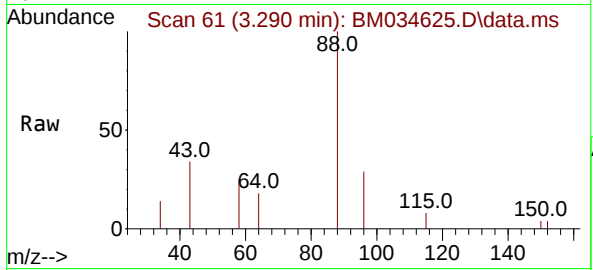

Tgt Ion: 88 Resp: 550

Ion	Ratio	Lower	Upper
88	100		
43	34.1	49.7	74.5
58	25.2	52.5	78.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

