

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034627.D
 Acq On : 12 Apr 2022 18:40
 Operator : CG/JU
 Sample : N2319-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 04:55:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.888	152	2027	0.400	ng/u1	-0.03
4) Naphthalene-d8	10.693	136	5740	0.400	ng/u1	#-0.01
9) Acenaphthene-d10	14.533	164	3125	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.270	188	5687m	0.400	ng/u1	-0.01
17) Chrysene-d12	21.484	240	4596	0.400	ng/u1	# 0.02
23) Perylene-d12	23.802	264	3738m	0.400	ng/u1	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	14216	4.046	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.315	152	3214	0.422	ng/u1	0.00
18) Fluoranthene-d10	19.297	212	7006	0.524	ng/u1	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.294	88	3650m	1.049	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034627.D
Acq On : 12 Apr 2022 18:40
Operator : CG/JU
Sample : N2319-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H4




Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 04:55:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

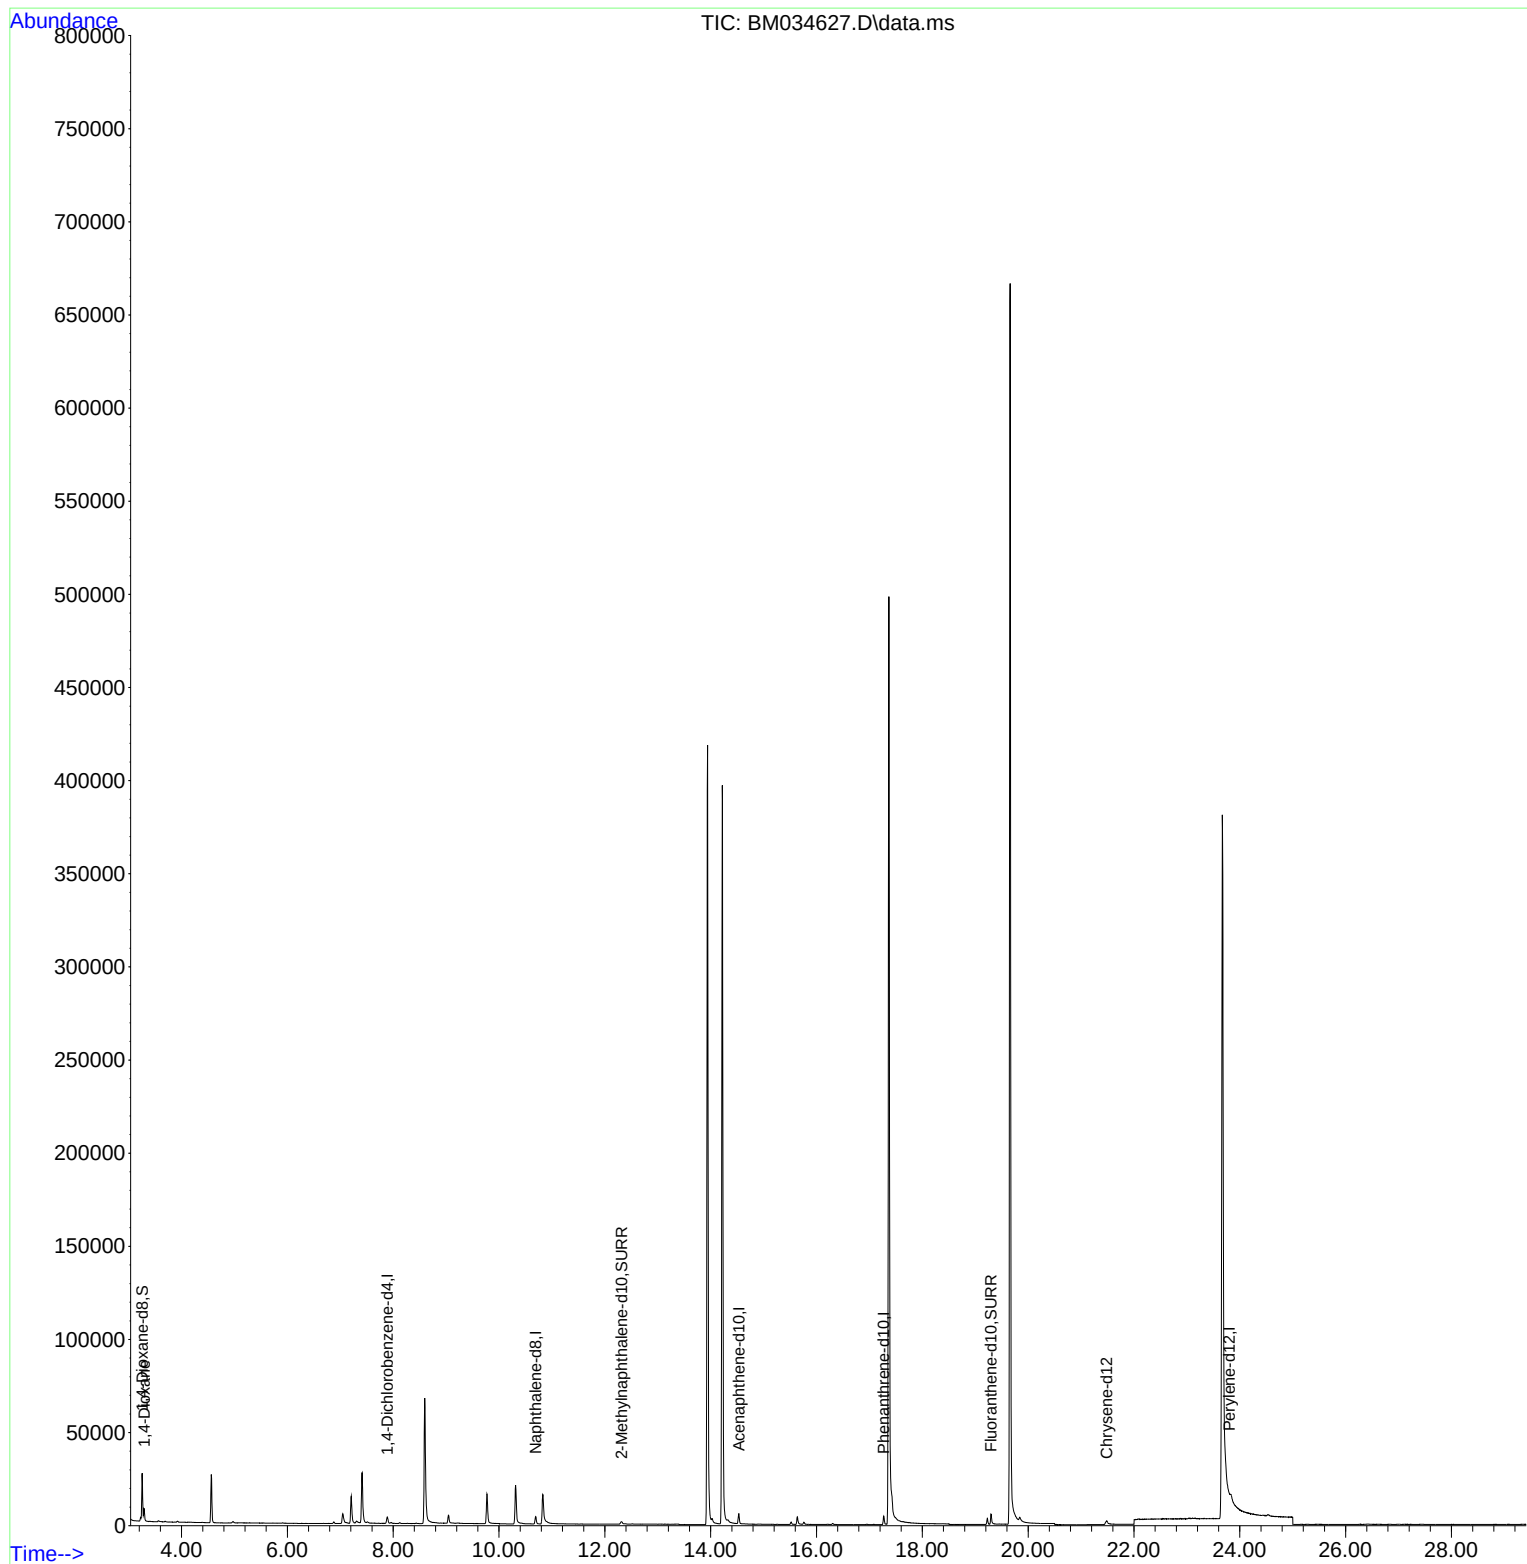

Abundance Scan 61 (3.290 min): BM034619.D\data.ms (-55)

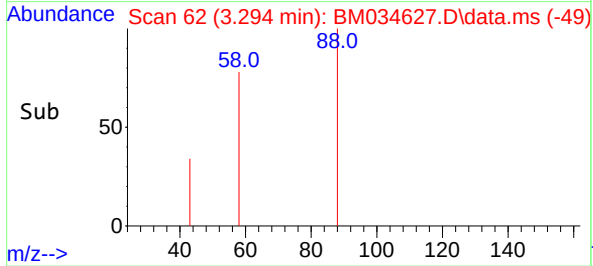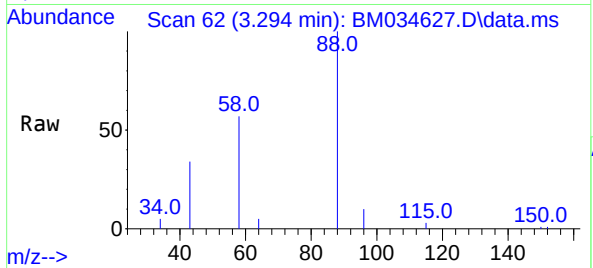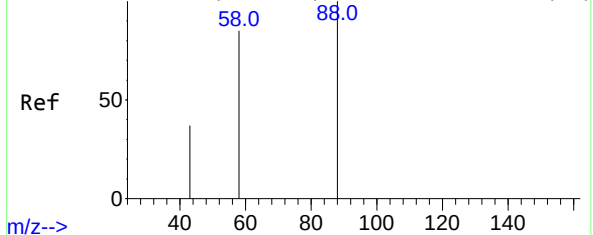

#2
1,4-Dioxane
Concen: 1.049 ng/ul m
RT: 3.294 min Scan# 61
Delta R.T. 0.004 min
Lab File: BM034627.D
Acq: 12 Apr 2022 18:40

Instrument :
BNA_M
ClientSampleId :
YB2H4

Tgt Ion: 88 Resp: 3650
Ion Ratio Lower Upper
88 100
43 33.6 49.7 74.5
58 56.8 52.5 78.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

